

## DIAMOND-AF STUDY

Study Title: A Randomized Controlled Clinical Evaluation of the **DiamondTemp™** System for the Treatment of Paroxysmal Atrial Fibrillation

Sponsor:

**Advanced Cardiac Therapeutics (ACT)**  
2880 Lakeside Drive, Suite 250  
Santa Clara, CA 95054 USA  
+1 (408) 755-1500

Protocol No:

TP00599

Investigational Device:

**DiamondTemp Ablation System**  
(Inclusive of the DiamondTemp Ablation Catheter, DiamondTemp Catheter-to-RFG Cable, DiamondTemp GenConnect Cable, DiamondTemp RF Generator, DiamondTemp Irrigation Pump and DiamondTemp Irrigation Tubing Set)

Revision Number:

C

Effective Date:

08/31/2017

## 1. STUDY CONTACT INFORMATION

### Sponsor Contacts

**Bryan Wylie**  
Director, Clinical Affairs (US)

**Jean Maurice Dussartre, M.D.**  
Director, Clinical Affairs (EU)

**Patty Hevey**  
Vice President, Clinical Affairs

### Coordinating Principal Investigators, US

**Tom McElderry, MD, FACC, FHRS**  
Section Chief, Cardiac Electrophysiology

**William Maddox, M.D., FACC, FHRS**  
Assistant Professor, Electrophysiology

University of Alabama Birmingham (UAB)  
930B Faculty Office Tower  
510 20<sup>th</sup> Street South  
Birmingham, AL 35294

### Coordinating Principal Investigator, OUS

**Josef Kautzner, MUDr., CSc., FESC**  
Director, Electrophysiology  
Institut klinické a experimentální medicíny (IKEM)  
Vitebsk 1958/9  
140 21 Prague 4

**Steering Committee**

*Including Coordinating  
Principal Investigators*

**Andrea Natale, M.D., FACC, FHRS**

Director, Electrophysiology

Texas Cardiac Arrhythmia Institute at St. David's Medical Center

**Frank Cuoco, M.D., MBA**

Director, Electrophysiology

Medical University of South Carolina (MUSC)

**OUS Contract Research  
Organizations (CRO)**

**High Tech Med Consult**

Firmlova 1322/4e

15500 Prague 5, Czech Republic

Phone: +402 777 671 069

**MERC srl**

Via Elia Capriolo, 41

25122 Brescia, Italy

Phone: +39 030 2754021

**Data Management /  
Biostatistics**

**Advanced Research Associates**

Data Management / Biostatistics

2350 Mission College Blvd., Suite 825

Santa Clara, CA 94054

Phone: +1 (650) 810-1190

**Electronic Data  
Capture (EDC)**

**Medrio**

345 California Street, Suite 325

San Francisco, CA 94104

Phone: +1 (415) 963-3700

**ECG Core Lab**

**HeartcoR Solutions, LLC**

Event Monitor, ECG Core Lab

2403 Harnish Drive #201

Algonquin, IL 60102

Project Manager: Madalina Andreescu, BS, CRA, CCT

Phone: +1 (224) 333-3318

### Investigator Protocol Signature Page and Agreement

I have read this Investigational Plan and agree to adhere to the requirements. I will share this Investigational Plan and all pertinent information to all site personnel involved in this study. I will discuss this material with them and ensure they are fully informed regarding the study products and the conduct of the study.

I agree to conduct the study as outlined in the Investigational Plan, in accordance with the signed clinical study agreement and to the ethical principles stated in the latest version of the Declaration of Helsinki (2013), the applicable guidelines for good clinical practices, MEDDEV 2.7/4 (Guidelines on Clinical investigations: A Guide for Manufacturers and Notified Bodies) and 2.7/3 (Clinical investigations: Serious Adverse Event reporting), ISO 14155:2011 (Clinical Investigation of Medical Devices for Human Subjects – Good Clinical Practice) or the applicable local and international regulations, whichever provide the greater protection of the individual.

I agree to provide all the information requested in the Case Report Forms presented to me by the Sponsor in a manner to assure completeness, legibility and accuracy. I agree to actively enroll patients into this study.

I also agree that all information provided to me by the Sponsor, including pre-clinical data, protocols, Case Report Forms, and any verbal and written information, will be kept strictly confidential and confined to the clinical personnel involved in conducting the study. It is recognized that this information may be relayed in confidence to the Institutional Review Board / Ethics Committee.

In addition, no reports or information about the study or its progress will be provided to anyone not involved in the study other than the Sponsor, the Institutional Review Board / Ethics Committee, the core labs, or the Data Safety Monitoring Board. Any such submission will indicate that the material is confidential.

---

Investigator Signature

---

Date

---

Investigator Printed Name

---

Date

---

Sponsor Signature

---

Date

---

Sponsor Printed Name

---

Date

## 2. REVISION HISTORY

Revision Level	DCO	Description of Change	Reason for Change	Effective Date
A	0426	Initial Release	N/A	08/25/2017
B	0429	a. Update section 7.1, Proposed Intended Use of the Investigational Device to include: accessories (DiamondTemp Cable-to-RFG Cable, DiamondTemp GenConnect Cable, DiamondTemp Irrigation Pump/Tubing Set); removed ablation, RF, and three dimensional descriptors. b. Update SAE rates for 7 and 30 day follow up	a. Clarification of statement; no change to intent. b. Reflects updated results.	08/29/2017
C	0438	Updated Table 4, Summary of Procedural Data, in Section 5.	Reflects updated results.	08/31/2017

### 3. PROTOCOL SUMMARY

Objective	The objective of this study is to demonstrate the safety and effectiveness of the DiamondTemp Ablation System for the treatment of drug refractory, recurrent, symptomatic paroxysmal atrial fibrillation.
Test Device	<p>DiamondTemp Ablation System consists of:</p> <ul style="list-style-type: none"> <li>• DiamondTemp Ablation Catheter</li> <li>• DiamondTemp Catheter-to RFG Cable</li> <li>• DiamondTemp GenConnect Cable</li> <li>• DiamondTemp Generator with Footswitch</li> <li>• DiamondTemp Irrigation Pump</li> <li>• DiamondTemp Irrigation Tubing Set</li> </ul> <p>The investigational device will be used with commonly available:</p> <ul style="list-style-type: none"> <li>• EP recording systems</li> <li>• Cardiac stimulators</li> <li>• EnSite™ Velocity™ or Precision™ Cardiac Mapping System</li> </ul>
Control Device	<p>St. Jude Medical (Abbott) Ablation System</p> <ul style="list-style-type: none"> <li>○ TactiCath™ Quartz Contact Force Ablation Catheter</li> <li>○ AMPERE™ RF Ablation Generator and Cables or equivalent</li> <li>○ COOL POINT™ Irrigation Pump and Tubing or equivalent</li> </ul> <p>The control device will be used with commonly available:</p> <ul style="list-style-type: none"> <li>• EP Recording Systems</li> <li>• Cardiac Stimulators</li> <li>• EnSite™ Velocity™ or Precision™ Cardiac Mapping System</li> </ul>
Study Design	The DIAMOND-AF study is a prospective, single-blind, 1:1 randomized, controlled trial being performed at multiple centers in the United States, Canada and Europe.
Planned Subject Sample Size	A maximum of 350 subjects will be enrolled and randomized in this study.
Planned Number of Global Investigational Sites	<p>Subjects will be enrolled at up to 30 investigational sites in the United States (US) and outside of the US (OUS).</p> <p>A minimum of 50% of the data will be generated from sites within the US.</p>
Ablation Procedure	The primary focus of the ablation procedure is to create a series of point-by-point radiofrequency (RF) lesions encircling the left and right PVs to achieve electrical pulmonary vein isolation (PVI) from the rest of the left atrium (LA).

	<p>Investigators may use their preferred approach to obtain PVI, such as antral or wide area circumferential ablation (WACA) targeting PVs individually or PV pairs ipsilaterally.</p> <p>PVI must be confirmed by entrance block at least 20 minutes following the last ablation around the respective PV. Targeting non-PV foci and complex fractionated electrograms (CFAE) is not recommended in this investigation. If the investigator identifies additional focal or macro-reentrant atrial sites to be clinically relevant to AF and requiring ablation, the ablation location will be documented.</p>
Primary Safety Endpoint	<p>The primary safety endpoint is defined as freedom from a composite of serious adverse events (SAE) occurring within 7-days post-index ablation procedure or hospital discharge, whichever occurs later, as adjudicated by an independent Clinical Events Committee (CEC) for relatedness to the procedure or device.</p> <p>The primary safety device- or procedure-related SAEs composite will be the combined rate of the following events:</p> <ul style="list-style-type: none"><li>• Atrioesophageal fistula</li><li>• Cardiac tamponade / perforation</li><li>• Cardiovascular-related death post-ablation</li><li>• Bleeding complication</li><li>• Myocardial infarction</li><li>• Pericarditis</li><li>• Phrenic nerve paralysis</li><li>• Pulmonary edema</li><li>• Stroke or transient ischemic attack (TIA)</li><li>• Thromboembolism</li><li>• Vagal nerve injury</li><li>• Vascular access complications</li></ul>

Primary Effectiveness Endpoint	<p>The primary effectiveness endpoint is defined as freedom from documented symptomatic atrial fibrillation (AF) episodes following the blanking period (3-month follow-up post-ablation procedure) through the end of the effectiveness evaluation period (12-month follow-up post-ablation procedure).</p> <p>An effectiveness failure is defined by any of the following events during the effectiveness evaluation period (3-month through 12-month follow-up visits post ablation):</p> <ul style="list-style-type: none"> <li>• Documented episodes of AF lasting <math>\geq</math> 30 seconds in duration as evidenced by electrocardiographic data</li> <li>• A repeat ablation procedure to treat AF</li> <li>• Use of a new or modification to existing Class I-IV anti-arrhythmic drug (AAD) regimen to treat AF recurrence</li> </ul>
Secondary Endpoints	<p>Secondary endpoints to characterize the performance of the DiamondTemp Ablation System, relative to the control device, will include:</p> <ul style="list-style-type: none"> <li>• Freedom from a composite of SAE occurring within 30-days post-index ablation procedure as adjudicated by an independent CEC for relatedness to the procedure or device.</li> <li>• Freedom from documented symptomatic and asymptomatic atrial tachycardia (AT) and atrial flutter (AFL)* episodes following the blanking period through 12-month follow-up post-ablation procedure.</li> <li>• Freedom from documented asymptomatic AF episodes through the effectiveness evaluation period lasting <math>\geq</math> 30 seconds in duration by electrocardiogram (ECG) or ECG monitoring system.</li> <li>• Rate of acute procedural success, defined as confirmation of electrical isolation of PVs via assessment of entrance block at least 20 minutes following the last ablation around the respective PV.</li> <li>• Rate of occurrence of electrically reconnected PVs following a 20-minute waiting period assessed by entrance block at index procedure.</li> <li>• Accumulated changes in QOL using the AF QOL Survey (AFEQT Questionnaire) from baseline through 6 and 12 months following ablation procedure.</li> <li>• Neurological changes measured using the NIH stroke scale between baseline and post-ablation (pre-discharge visit) and at 12 months post-ablation procedure.</li> </ul>

	<ul style="list-style-type: none"> <li>• Total procedure time (minutes), defined as time of first assigned ablation catheter insertion into the vasculature to time of last procedural ablation catheter removed.</li> <li>• Time to achieve initial PVI at index procedure (minutes), defined as time of delivery of first RF ablation with the assigned ablation catheter until confirmation of PVI.</li> <li>• Total treatment device time (minutes), defined as time of delivery of first RF ablation with the assigned ablation treatment catheter to removal of the treatment catheter.</li> <li>• Mean cumulative RF time (minutes).</li> <li>• Mean duration of RF ablations (seconds).</li> <li>• Total number of RF ablations per procedure.</li> <li>• Total fluid infused through the assigned ablation catheter (mL).</li> <li>• Total fluoroscopy time (minutes).</li> <li>• Number of re-hospitalizations due to atrial fibrillation recurrence after blanking period.</li> </ul> <p><i>*Occurrence and/or ablation of cavotricuspid isthmus (CTI)-dependent AFL, as confirmed by entrainment maneuvers during EP testing at any time during this study is not a primary effectiveness failure because it is not considered an iatrogenic arrhythmia following a left atrial ablation procedure for AF.</i></p>
Inclusion Criteria	<ol style="list-style-type: none"> <li>1. Above eighteen (18) years of age or of legal age to give informed consent specific to state and national law.</li> <li>2. Patients with a history of symptomatic, paroxysmal atrial fibrillation (PAF) who have had <math>\geq 2</math> episodes of PAF reported within the 12 months prior to index ablation procedure.</li> <li>3. At least one episode of PAF <math>\geq 30</math> seconds in duration documented by electrocardiographic data.</li> <li>4. Failure or intolerance of at least one Class I-IV anti-arrhythmic AAD for treatment of PAF.</li> <li>5. Suitable candidate for intra-cardiac mapping and ablation of arrhythmia.</li> <li>6. Patient agrees to comply with study procedures and be available (geographically stable) for follow-up visits for at least 12 months after enrollment.</li> <li>7. Patient is willing and able to provide written consent.</li> </ol>

Exclusion Criteria	<p><i>At time of enrollment and/or prior to procedure:</i></p> <ol style="list-style-type: none"><li>1. AF secondary to electrolyte imbalance, thyroid disease or reversible or non-cardiac cause.</li><li>2. LA diameter &gt; 5.5 cm.</li><li>3. Left ventricular ejection fraction (LVEF) &lt; 35%.</li><li>4. Currently NYHA Class III or IV or exhibits uncontrolled heart failure.</li><li>5. Body Mass Index (BMI) &gt; 40 kg/m<sup>2</sup>.</li><li>6. LA ablation, septal closure device or mitral valve surgical procedure at any time prior to enrollment.</li><li>7. Presence of intramural thrombus, tumor or abnormality that precludes vascular access, catheter introduction or manipulation.</li><li>8. Coagulopathy, bleeding diathesis or suspected procoagulant state</li><li>9. Sepsis, active systemic infection or fever (&gt;100.5 °F / 38 °C) within a week prior to the ablation procedure.</li><li>10. Significant restrictive or obstructive pulmonary disease or chronic respiratory condition.</li><li>11. Renal failure requiring dialysis or renal compromise that in the investigator's judgement would increase risk to the patient or deem the patient inappropriate to participate in the study.</li><li>12. Known allergies or intolerance to anticoagulant and antiplatelet therapies to be used in conjunction with the study or contrast sensitivity that cannot be adequately pre-treated prior to the ablation procedure.</li><li>13. Positive pregnancy test results for female patients of childbearing potential or breast feeding.</li><li>14. Enrollment in a concurrent clinical study that in the judgement of the investigator would impact study outcomes.</li><li>15. Acute or chronic medical condition that in the judgment of the investigator would increase risk to the patient or deem the patient inappropriate to participate in the study.</li><li>16. Life expectancy &lt; 12 months based on medical history or the medical judgement of the investigator.</li></ol> <p><i>Within 1 month of enrollment or just prior to procedure:</i></p> <ol style="list-style-type: none"><li>17. Documented LA thrombus upon imaging.</li><li>18. Creatinine &gt;2.5mg/dl or creatinine clearance &lt;30mL/min.</li></ol> <p><i>Within 3 months of enrollment:</i></p> <ol style="list-style-type: none"><li>19. Regularly prescribed amiodarone.</li></ol>
--------------------	--

	<p>20. Significant gastrointestinal (GI) bleed.</p> <p>21. Myocardial infarction (MI), unstable angina, cardiac surgery or coronary intervention.</p> <p><i>Within 6 months of enrollment:</i></p> <p>22. Coronary artery bypass graft (CABG) procedure.</p> <p>23. ICD, CRT leads or pacemaker implant procedure.</p> <p>24. Documented stroke, CVA, TIA or suspected neurological event.</p> <p><i>Within 12 months of enrollment:</i></p> <p>25. An episode of AF lasting &gt;7 days in duration.</p>																						
Follow-up Visit Schedule	<table border="1"> <thead> <tr> <th>Subject Visit Description</th><th>Timeframe / Visit Window</th></tr> </thead> <tbody> <tr> <td>Enrollment and Screening</td><td>Within 60 days of ablation procedure</td></tr> <tr> <td>Ablation Procedure (Index)</td><td>Day 0; follow-up visit windows determined by ablation procedure completion date</td></tr> <tr> <td>Pre-Discharge</td><td>Prior to discharge from hospital following ablation procedure</td></tr> <tr> <td>7 days Follow-Up (Phone)</td><td><math>7 \pm 3</math> days</td></tr> <tr> <td>1 Month Follow-Up (Phone or Clinic)</td><td><math>30 \pm 14</math> days</td></tr> <tr> <td>3 Month Follow-Up</td><td><math>90 \pm 21</math> days</td></tr> <tr> <td>6 Month Follow-Up</td><td><math>180 \pm 28</math> days</td></tr> <tr> <td>12 Month Follow-up</td><td><math>365 \pm 45</math> days</td></tr> <tr> <td>Unscheduled Visits</td><td>As needed/necessary</td></tr> <tr> <td>Repeat Ablation Procedure</td><td>Within 90 days of ablation procedure (follow-up visit schedule does not restart)</td></tr> </tbody> </table>	Subject Visit Description	Timeframe / Visit Window	Enrollment and Screening	Within 60 days of ablation procedure	Ablation Procedure (Index)	Day 0; follow-up visit windows determined by ablation procedure completion date	Pre-Discharge	Prior to discharge from hospital following ablation procedure	7 days Follow-Up (Phone)	$7 \pm 3$ days	1 Month Follow-Up (Phone or Clinic)	$30 \pm 14$ days	3 Month Follow-Up	$90 \pm 21$ days	6 Month Follow-Up	$180 \pm 28$ days	12 Month Follow-up	$365 \pm 45$ days	Unscheduled Visits	As needed/necessary	Repeat Ablation Procedure	Within 90 days of ablation procedure (follow-up visit schedule does not restart)
Subject Visit Description	Timeframe / Visit Window																						
Enrollment and Screening	Within 60 days of ablation procedure																						
Ablation Procedure (Index)	Day 0; follow-up visit windows determined by ablation procedure completion date																						
Pre-Discharge	Prior to discharge from hospital following ablation procedure																						
7 days Follow-Up (Phone)	$7 \pm 3$ days																						
1 Month Follow-Up (Phone or Clinic)	$30 \pm 14$ days																						
3 Month Follow-Up	$90 \pm 21$ days																						
6 Month Follow-Up	$180 \pm 28$ days																						
12 Month Follow-up	$365 \pm 45$ days																						
Unscheduled Visits	As needed/necessary																						
Repeat Ablation Procedure	Within 90 days of ablation procedure (follow-up visit schedule does not restart)																						

---

## TABLE OF CONTENTS

<b>1. STUDY CONTACT INFORMATION .....</b>	<b>2</b>
<b>2. REVISION HISTORY .....</b>	<b>5</b>
<b>3. PROTOCOL SUMMARY .....</b>	<b>6</b>
<b>4. INTRODUCTION.....</b>	<b>15</b>
4.1. ATRIAL FIBRILLATION (AF) AND CLINICAL NEED .....	15
4.2. PRIOR CLINICAL EVIDENCE FOR RF ABLATION TO TREAT PAF.....	16
<b>5. SUMMARY OF FIRST-IN-HUMAN CLINICAL STUDY (TRAC-AF).....</b>	<b>17</b>
5.1. TRAC-AF STUDY DESIGN.....	17
5.2. INVESTIGATIONAL DEVICE.....	17
5.3. TRAC-AF CLINICAL ENDPOINTS .....	18
5.4. STUDY ELIGIBILITY CRITERIA.....	18
5.5 STUDY RESULTS .....	19
5.6. CONCLUSION FROM CLINICAL STUDY .....	23
<b>6. TACTICATH CONTROL DEVICE.....</b>	<b>23</b>
6.1. INDICATIONS FOR USE.....	23
6.2. PRODUCT CLASSIFICATION, CODE, REGULATION.....	24
6.3. CONTROL DEVICE DESCRIPTION .....	24
6.4. TACTICATH QUARTZ CONTACT FORCE ABLATION CATHETER .....	24
6.5. TACTISYS QUARTZ EQUIPMENT.....	25
6.6. ADDITIONAL REQUIRED EQUIPMENT .....	25
<b>7. DIAMONDTEMP INVESTIGATIONAL DEVICE .....</b>	<b>25</b>
7.1. PROPOSED INTENDED USE OF THE INVESTIGATIONAL DEVICE .....	25
7.2. PRODUCT CLASSIFICATION, CODE, REGULATION.....	26
7.3. INVESTIGATIONAL DEVICE DESCRIPTION.....	26
7.4. DIAMONDTEMP ABLATION CATHETER .....	27
7.5. DIAMONDTEMP RF GENERATOR .....	27
7.6. DIAMONDTEMP IRRIGATION PUMP .....	28
7.7. DIAMONDTEMP TUBING SET.....	29
7.8. DIAMONDTEMP FOOTSWITCH .....	29
7.9. DIAMOND TEMP CABLES .....	29
7.10. MAPPING SYSTEM AND EP RECORDING SYSTEM COMPATIBILITY .....	30

---

<b>8. STUDY PROTOCOL AND METHODS .....</b>	<b>30</b>
8.1. STUDY OBJECTIVE .....	30
8.2. STUDY DESIGN.....	30
8.3. PRIMARY SAFETY ENDPOINTS.....	32
8.4. PRIMARY EFFECTIVENESS ENDPOINTS .....	34
8.5. SECONDARY ENDPOINTS.....	34
8.6. SAMPLE SIZE JUSTIFICATION.....	35
8.7. STATISTICAL ANALYSIS .....	35
8.8. SITE TRAINING .....	36
<b>9. SUBJECT SELECTION .....</b>	<b>36</b>
9.1. CRITERIA FOR ELIGIBILITY .....	36
9.2. STUDY INCLUSION CRITERIA.....	36
9.3. STUDY EXCLUSION CRITERIA .....	36
<b>10. SUBJECT ACCOUNTABILITY .....</b>	<b>38</b>
10.1. POINT OF ENROLLMENT .....	38
10.2. SUBJECT STATUS AND CLASSIFICATION.....	38
10.3. SUBJECT WITHDRAWAL .....	39
<b>11. STUDY METHODS.....</b>	<b>39</b>
11.1. ENROLLMENT AND VISIT SCHEDULE.....	39
11.2. SCREENING EVALUATION.....	41
11.3. BASELINE EVALUATION.....	41
11.4. PRE-ABLATION TESTING AND REQUIREMENTS .....	42
11.5. ABLATION PROCEDURE.....	42
11.6. PRE-DISCHARGE FOLLOW-UP VISIT .....	47
11.7. SEVEN DAY FOLLOW-UP PHONE CALL .....	48
11.8. ONE MONTH FOLLOW-UP PHONE CALL OR CLINIC VISIT .....	48
11.9. REPEAT ABLATION PROCEDURE (IF APPLICABLE) .....	48
11.10. THREE MONTH FOLLOW-UP VISIT .....	49
11.11. SIX MONTH FOLLOW-UP VISIT.....	49
11.12. TWELVE MONTH FOLLOW-UP VISIT.....	49
11.13. UNSCHEDULED VISITS .....	50
11.14. SUBJECT LOST TO FOLLOW-UP.....	50
11.15. EXTENDED FOLLOW-UP PERIOD (IF APPLICABLE) .....	50
11.16. STUDY COMPLETION .....	50
<b>12. STUDY CONDUCT .....</b>	<b>51</b>
12.1. STATEMENT OF COMPLIANCE .....	51
12.2. REGULATORY CONSIDERATIONS.....	51

12.3. INVESTIGATOR RESPONSIBILITIES .....	51
12.4. CONFIDENTIALITY AND DATA PROTECTION.....	52
12.5. INSURANCE .....	52
12.6. PROTOCOL AMENDMENTS.....	52
12.7. ADVERSE EVENT REPORTING.....	52
12.8. DEVICE DEFICIENCY REPORTING .....	54
12.9. PROTOCOL DEVIATIONS .....	55
12.10 INVESTIGATIONAL DEVICE ACCOUNTABILITY .....	55
12.11. DOCUMENTATION .....	56
12.12. RECORD RETENTION .....	57
<b>13. POTENTIAL RISKS AND BENEFITS.....</b>	<b>57</b>
13.1. ANTICIPATED ADVERSE EVENTS.....	57
13.2. RISK MINIMIZATION .....	59
13.3. BENEFITS .....	60
<b>14. MONITORING .....</b>	<b>61</b>
14.1 STUDY MONITOR .....	61
14.2. MONITORING PROCEDURES.....	61
14.3. ECG CORE LAB .....	62
14.4 DATA SAFETY MONITORING BOARD.....	62
14.5. CLINICAL EVENTS COMMITTEE.....	62
14.6. STEERING COMMITTEE.....	63
<b>15. SUSPENSION OR TERMINATION .....</b>	<b>63</b>
15.1. PREMATURE TERMINATION OF THE STUDY .....	63
15.2. TERMINATION OF PARTICIPATION .....	63
<b>16. PUBLICATION AND REPORTING POLICY .....</b>	<b>64</b>
<b>17. REIMBURSEMENT AND COMPENSATION FOR SUBJECTS .....</b>	<b>64</b>
<b>18. ABBREVIATIONS AND DEFINITIONS .....</b>	<b>65</b>
18.1. TABLE OF DEFINITIONS .....	65
18.2. TABLE OF ABBREVIATIONS .....	70
<b>19. BIBLIOGRAPHY .....</b>	<b>72</b>

## 4. INTRODUCTION

### 4.1. Atrial Fibrillation (AF) and Clinical Need

Atrial fibrillation (AF) is the most common clinically-significant cardiac arrhythmia. It is a major public health concern in the United States, affecting an estimated 2.3 million people in North America and 4.5 million people in Europe<sup>[1]</sup>. It has been projected that the prevalence of AF will increase 2.5 fold during the next 50 years in the United States<sup>[2]</sup>. AF is associated with increased cardiovascular morbidity and mortality and the prevalence increases over time due to the aging population and an increase in age-specific occurrence of AF<sup>[3-5]</sup>.

Symptoms of AF vary with the ventricular rate, underlying functional status, duration of AF, presence and degree of structural heart disease, and individual patient perception; however, most patients with AF complain of palpitations, angina, dyspnea, fatigue, or dizziness. AF also significantly impairs quality of life, with up to two-thirds of patients reporting it is disruptive and debilitating to their lives<sup>[6-8]</sup>. AF is an abnormal heart rhythm that has been classified as recurrent when two or more episodes are detected. If these episodes of AF last less than seven days and terminate spontaneously, then it is classified as paroxysmal AF (PAF). PAF accounts for approximately 40 to 45 percent of AF cases.<sup>[4, 9]</sup>

AF is a sustained arrhythmia characterized by rapid and disorganized atrial activation leading to impaired atrial function, which can be diagnosed on an ECG by lack of a P-wave and irregular QRS complexes. The disorganized atrial activation appears as “fibrillatory” waves activating the atria at a rate generally between 350 and 600 beats/min and the syncytial contraction of the atria is replaced by irregular atrial twitches. While AF can occur in isolation, it may also be associated with other arrhythmias such as atrial flutter or atrial tachycardia.

The electrophysiological mechanisms responsible for AF may include rapid focal tachyarrhythmia in the pulmonary veins (PVs) and/or other atrial regions with fibrillatory conduction, multiple reentrant wavelet conduction initiated by premature atrial complexes (PACs) and/or atrial tachyarrhythmia, and/or formation of stable or unstable reentrant circuits of very short cycle lengths that generate fibrillatory conduction<sup>[10, 11]</sup>.

Of all electrophysiological mechanisms responsible for AF, of significant interest are the PVs which have been identified to play a critical role in triggering and maintaining AF. Haissaguerre and colleagues have demonstrated that in most AF patients, the focus is in one of the PVs<sup>[12]</sup>.

The choice of therapy for AF is influenced by patient preference, associated structural heart disease, severity of symptoms and whether the AF is classified as recurrent paroxysmal, recurrent persistent or permanent. Although AF can be problematic to manage medically due to its progressive nature, there are multiple therapies in current use for the treatment of AF, and many of these therapies are sub-optimal for most patients. Treatment options include medical management, pacing, cardioversion, implantable devices, surgery and ablation therapy to eliminate the arrhythmia<sup>[4, 13]</sup>.

Of all therapeutic strategies for AF one of interest is radiofrequency catheter ablation (RFCA) as a potential curative treatment. RFCA for the treatment of AF is a commonly

performed procedure for symptomatic patients in whom medications are either ineffective or not tolerated [4, 9, 14]. RFCA restores normal sinus rhythm by delivering RF energy through a catheter at targeted focal sites to disrupt abnormal electrical activity. The most common catheter ablation approach to treat AF is to electrically isolate the PVs (PVI). Other approaches used include WACA and CFAE ablation. Additional focal or macroreentrant atrial sites may be ablated but the approach varies from center to center.

Despite significant improvements in catheter ablation strategies to treat AF in recent years, Neuzil and colleagues report that refractory recurrence of arrhythmia remains a continuing concern with recurrence rates of AF after RFCA still remaining relatively high (20-55%) [15] and perhaps attributed to lack of transmural lesions during PVI [16]. Technological innovations in RFCA include multi-electrode ablation catheters, high resolution ablation catheters, force-sensing technologies and navigation technologies.

#### 4.2. Prior Clinical Evidence for RF Ablation to Treat PAF

Ablation has become the standard of care in many centers due to the superiority of catheter ablation to AADs. The first two classes of devices to seek and achieve FDA approval for ablation of PAF were an irrigated RF catheter (ThermoCool, Biosense Webster) and a cryoballoon ablation catheter (ArticFront, Medtronic). The prospective randomized studies for these devices demonstrated the safety and efficacy and the superiority of catheter ablation over drug therapy in drug refractory patients. [17, 18]

Subsequent approval studies of new ablation technologies have been either compared with a previously-approved device with the same indications for use in a randomized, controlled non-inferiority study or, in the case of a second-generation RF ablation catheter, compared with predefined performance goals in a single-arm study.

Recently, two catheters have been developed to measure real-time contact force during ablation, a concept where force is one of the primary factors determining lesion size. One catheter uses three optical fibers to measure the micro-deformation of a deformable body in the catheter tip (TactiCath, St Jude Medical, Incorporated), which correlates with tip force [19-21]. The second catheter uses a small spring between the ablation tip electrode and the catheter shaft, with a tiny magnetic transmitter in the tip and magnetic sensors to measure microdeflection of the spring (ThermoCool SmartTouch, Biosense Webster, Inc.), corresponding to tip force [22-24].

The TactiCath catheter was evaluated in the FDA investigational study, TOCCASTAR clinical trial [25]. In this prospective, randomized clinical trial, 300 patients with PAF were randomized to ablation with the TactiCath catheter or to the non-contact force sensing ThermoCool ablation catheter. No difference in efficacy was observed, with success rates of 67.8% and 69.4% in the contact force (CF) and control arms, respectively. When the CF arm was stratified into optimal CF and non-optimal CF groups, effectiveness was 75.9% vs 58.1%, respectively. There was no difference in the rate of complications in the two groups. Cardiac tamponade occurred in one subject in each group.

The ThermoCool SmartTouch catheter was evaluated in a multicenter, prospective, randomized clinical trial performed for FDA approval [24]. The outcomes were compared with the ThermoCool IDE trial [18], in which 170 subjects were enrolled. The 12-month

freedom from AF/AT/AFL in SMART-AF was 72.5% at 1-year follow-up, compared with 66% efficacy for the ThermoCool non-contact force catheter. The average CF per procedure was 18 grams. Four subjects experienced cardiac tamponade. A post hoc analysis revealed that when the CF was between investigator-selected working ranges >80% of the time, outcomes were 4.25 times more likely to be successful.

## 5. SUMMARY OF FIRST-IN-HUMAN CLINICAL STUDY (TRAC-AF)

ACT conducted a multi-center First-In-Human clinical study, TRAC-AF, across four European centers to establish evidence of clinical safety and effectiveness of the DiamondTemp Ablation System to treat patients with drug refractory, recurrent, symptomatic paroxysmal atrial fibrillation (PAF).

TRAC-AF (DiamondTemp TempeRAture-Controlled and Contact Sensing RF Ablation Clinical Trial for Atrial Fibrillation, NCT02821351) study was a prospective, multi-center, single-arm feasibility study initiated in 2016 and conducted at four European investigational sites.

Enrollment was performed in two phases. Phase 1 included enrollment of 38 subjects from January through March of 2016 and Phase 2 included enrollment of an additional 34 subjects from June through July 2017. A total of 72 patients were enrolled in the study and 70 subjects were treated with the study device and analyzed. Enrollment is now closed and all subjects in both phases have completed 7-day and 30-day follow-up visits. Subjects in the first phase have completed 12-month follow-up visits and are now exited from the study.

All primary study endpoints have been met through 30 days follow up. Assessments of primary safety events resulted in four (4) SAEs (5.7%) through the 7-day safety endpoint and five (5) SAEs (7.1%) through the 30-day safety endpoint. The primary effectiveness endpoint of acute procedural success was achieved in 100% of subjects.

Once all subjects in the second phase have completed the 12-month follow-up a final clinical study report will be generated. The focus of this report is on subject follow up through 30-days.

### 5.1. TRAC-AF Study Design

Subjects with symptomatic PAF who were refractory or intolerant to at least 1 anti-arrhythmic drug (AAD; class I-IV) were screened for enrollment. Subjects that met the study eligibility criteria and signed the informed consent form (ICF) were enrolled and treated in accordance with the protocol and the HRS/EHRA/ECAS Expert Consensus Statement on Catheter and Surgical Ablation of Atrial Fibrillation [14, 26]. Subjects received ablation using the investigational device which required electrical isolation of all clinical relevant pulmonary veins.

### 5.2 Investigational Device

The investigational device in this clinical study is the DiamondTemp Ablation System. The investigational device was used with a commonly available EP recording system, cardiac stimulator and mapping device, the EnSite™ Velocity™ or Precision™ Cardiac Mapping System (St. Jude Medical). There were no control devices in this study.

### 5.3. TRAC-AF Clinical Endpoints

The primary endpoint events for this trial used to assess the safety and effectiveness of the DiamondTemp Ablation System for the treatment of drug refractory, recurrent, symptomatic PAF are as follows:

#### Primary Safety Endpoint

The safety of the DiamondTemp Ablation System was assessed by evaluating the nature and frequency of serious adverse events (SAEs) and serious adverse device effects (SADEs) during the time of the ablation procedure and within 7 days afterwards.

#### Long Term Primary Safety

The long-term safety of the DiamondTemp System was assessed by evaluating the nature and frequency of serious adverse events (SAE) and SADEs at 30 days post-procedure.

#### Primary Effectiveness Endpoint

The effectiveness of the DiamondTemp System was evaluated post-ablation by demonstration of acute procedural success, defined as isolation of clinically relevant pulmonary veins by demonstration of block or isolation of signals confirmed after delivery of the ablation treatment.

#### Secondary Endpoints

The chronic safety of the DiamondTemp System was assessed by evaluating the nature and frequency of adverse events (AE) and adverse device effects (ADE) at 90 days, 6 months and 12 months post-procedure.

### 5.4. Study Eligibility Criteria

Subjects presenting with drug refractory, paroxysmal atrial fibrillation requiring treatment and clinically indicated for standard of care pulmonary vein isolation ablation treatment were eligible for screening and potential enrollment in the study. Enrollment was confirmed once the subject signed informed consent, had echocardiographic assessment to confirm final eligibility and the study device was introduced into the subject's vasculature.

Subjects had to meet all of the defined inclusion and none of the defined exclusion criteria to be eligible for enrollment in this study.

#### Inclusion Criteria

1. Suitable candidate for intra-cardiac mapping and ablation for arrhythmias
2. History of recurrent symptomatic PAF with  $\geq 2$  episodes reported within the 365 days (12) months prior to enrollment
3. At least 1 episode of AF documented by Holter monitor, rhythm strip, trans-telephonic monitor (TTM), or 12-lead ECG prior to enrollment
4. Refractory to at least one Class I-IV anti-arrhythmic drug (AAD)
5. Eighteen (18) years of age or above

### Exclusion Criteria

1. Previous left atrial ablation procedure
2. Intracardiac thrombus, tumor or other abnormality that precludes catheter introduction and placement
3. Known severe cerebrovascular disease or history of cerebrovascular event (within 1 month)
4. Patients with severely impaired kidney function as measured by a Cockcroft-Gault Glomerular Filtration Rate (GFR)3 with a GFR  $\leq$  29. Active gastrointestinal bleeding
5. Active infection or fever ( $>100.5$  F/38 °C)
6. Sepsis
7. Cardiac surgery within the past two months.
8. Short life expectancy ( $<1$  yr.) due to other illnesses, such as cancer or pulmonary, hepatic, or renal disease Significant anemia (hemoglobin  $< 8.0$  mg/dL)
9. Severe uncontrolled systemic hypertension (systolic pressure  $> 240$  mm Hg within the last 30 days)
10. Documented anaphylaxis during previous exposure to angiographic contrast media
11. Uncontrolled congestive heart failure (NYHA1 Class III or IV)
12. Unstable angina or acute myocardial infarction within the past three months
13. Bleeding, clotting disorders, or known thrombosis
14. Severe Peripheral vascular disease
15. Uncontrolled diabetes
16. Heart valve replacement
17. Mitral clip (E-valve)
18. Women who are of childbearing potential who are currently pregnant or not willing to use contraception for the duration of the study
19. Active participation in another investigational protocol currently or the last 30 days
20. Unable or unwilling to take anti-coagulants
21. Unwilling or unable to comply with any protocol or follow up requirements

### **5.5 Study Results**

#### Study Accountability and Disposition

Study enrollment is closed and all subjects in both phases have completed 7-day and 30-day follow-up. Additionally, subjects in the first phase have completed their 12-month follow-up visits and are now exited from the study. Subjects were followed for 7 and 30 days after the index ablation procedure to assess primary safety and effectiveness endpoints. The last subject's 30-day visit was completed on 17 August 2017. **Table 1** provides a summary of the subject disposition for the study. Although a total of seventy-two (72) subjects met the definition for enrollment, analysis of the study results was conducted on seventy (70 subjects).

**Table 1. Subject Accountability and Disposition**

Subject Accountability	Number
Subjects enrolled in study	72
Subjects who did not have PVI attempted with study device (excluded from the analysis)	2
Analyzable Population	70

Baseline subject demographics for the analyzable subjects are described in **Table 2**. The mean age for subjects in this cohort was  $60.5 \pm 9.8$  years, with a higher incidence of subjects being of males (N=42) vs. females (N=28). Overall the characteristics of the subjects enrolled in the study were representative of the patient population usually undergoing RF ablation for the treatment of paroxysmal atrial fibrillation.

Study Population Demographics

**Table 2. Subject Demographics (n=70)**

Characteristic	Measurement	Results		
Age at Ablation Procedure (years)	Mean $\pm$ SD	60.5	$\pm$	9.8
	Range	35	-	76
Gender [N] (%)	Female	28	(40%)	
	Male	42	(60%)	
Height (cm)	Mean $\pm$ SD	173.8	$\pm$	11.7
	Range	115.0	-	194.0
Weight (kg)	Mean $\pm$ SD	91.3	$\pm$	17.5
	Range	59.0	-	140.0
Resting Heart Rate (bpm)	Mean $\pm$ SD	72.2	$\pm$	17.6
	Range	47.0	-	135.0
Resting Systolic BP (mmHg)	Mean $\pm$ SD	142.5	$\pm$	17.6
	Range	110.0	-	135.0
Resting Diastolic BP (mmHg)	Mean $\pm$ SD	82.6	$\pm$	10.1
	Range	60.0	-	110.0
Hemoglobin (g/l)	Mean $\pm$ SD	140.0	$\pm$	33.5
	Range	13.1	-	176.0
Creatinine (umol/l)	Mean $\pm$ SD	88.5	$\pm$	17.8
	Range	54.0	-	140.1
GFR (ml/min/1.73m <sup>2</sup> )	Mean $\pm$ SD	77.1	$\pm$	19.0
	Range	34.0	-	128.0
LVEF % <sup>i</sup>	Mean $\pm$ SD	61.2%	$\pm$	7.2%
	Range	25.0%	-	72.0%
LA diameter, cm <sup>ii</sup>	Mean $\pm$ SD	6.6	$\pm$	9.5
	Range	2.9	-	46.0

<sup>i</sup> LVEF not recorded on four subjects

<sup>ii</sup> LA diameter not recorded on 14 subjects

The medical history of each subject was assessed including history of atrial fibrillation, cardiovascular disease, non-cardiovascular disease and cardiac surgery at time of the screening visit. **Table 3** lists the pre-existing conditions recorded during the screening visits.

**Table 3. Medical History, (N=70)**

PAF History	N (%)
History of Prior Ablation Treatment	0 (0)
Refractory to Anti-Arrhythmic Drugs	70 (100)
Duration of AF (Mean±SD, years) <sup>1</sup>	2.6 ± 2.4
Medical History	
History of Smoking	21 (30)
Diabetes Mellitus Type II	8 (11.4)
Previous Stroke or TIA	6 (8.6)
Previous Myocardial Infarction	3 (4.3)
Coronary Artery Bypass Grafting (CABG)	0 (0)
Concurrent Medical Conditions	
Hepatic Disease	9 (12.9)
Pulmonary disease	17 (24.3)
Other Relevant Cardiac Diseases	
Hypertension	38 (54.3)
Hypertrophic Cardiomyopathy	0 (0)
Coronary Artery Disease	0 (0)

<sup>1</sup>Onset date of PAF not collected in first phase subjects; data only available on 30 subjects.

#### Study Procedural Results

Pulmonary vein isolation (PVI) was achieved by point-by-point, wide antral ablation encircling each pair of ipsilateral PV's supported by the EnSite Velocity or Precision to collect electrical map of the atrium and assist the navigation of the DiamondTemp to each ablation site. The investigational device was used with the market-approved EnSite Velocity/Precision in 70/70 (100%) of the subjects. A summary of procedural data is listed in **Table 4**.

**Table 4. Summary of Procedural Data, (N=70)**

Procedure Data (n=70)	Measurement	Results
Mode of Operation	Temperature Control	
Programmed Infusion Rate (ml/min)	Standby Flow Rate – 2 ml/min Therapeutic Flow Rate – 8 ml/min	
No. of RF Applications <sup>¥</sup>		4662
Ablation Duration <sup>†</sup> (sec)	Mean ± SD	17.5 ± 2.4
	Range	10.2 - 22.4
Average Power <sup>†</sup> (W)	Mean ± SD	36.2 ± 2.7
	Range	31.7 - 41.9
Max Power* (W)	Mean ± SD	50.8 ± 0.4
	Range	50.2 - 53.1
Temperature Set-Point <sup>†</sup> (°C)	Mean ± SD	58.1 ± 1.7
	Range	51.5 - 60
Max Temperature <sup>†</sup> (°C)	Mean ± SD	65.0 ± 3.5
	Range	56.8 - 73.8
Average Temperature <sup>†</sup> (°C)	Mean ± SD	48.2 ± 1.8
	Range	43.3 - 52.5
Max Impedance <sup>†</sup> (Ω)	Mean ± SD	134.7 ± 31.2
	Range	94 - 239
Average Impedance <sup>†</sup> (Ω)	Mean ± SD	96.1 ± 11.3
	Range	74.9 - 118.9
Total RF Ablation Time <sup>†</sup> (min)	Mean ± SD	19.8 ± 8.6
	Range	8.5 - 41.8
Total Procedure Time (mean)	Mean ± SD	2:42 ± 1:23
	Range	1:25 - 12:15
Total Fluoroscopy Time <sup>‡</sup> (mins)	Mean ± SD	9.38 ± 6.38
	Range	0:03 - 18:00
Total fluid vol. <sup>§</sup> (ablation procedure)	Mean ± SD	322.6 ± 99
	Range	152 - 531

<sup>¥</sup>RF application count includes all ablations (PVI + atrial tachycardia, etc.)

<sup>†</sup> These values were generated from the generator, not the database.

<sup>‡</sup> Fluoroscopic time not recorded on two subjects.

<sup>§</sup> Fluid volume not collected on one subject.

Once electrical isolation was achieved, ablation in the targeted veins was considered complete. Documentation of entrance block into the PVs (PVI) was required for each vein ablated. PVI was confirmed by either testing with an adenosine bolus (n=36 or 51% of subjects) or confirming PVI after a minimum of 20 minutes (n=34 or 49% of subjects) after the last RF application.

#### Primary Endpoint Results

All primary study endpoints have been met through 30 days. Assessments of primary safety events resulted in a total of four (4) SAEs (5.7%) through the 7-day safety endpoint and five (5) SAEs (7.1%) through the 30-day safety endpoint, as adjudicated by an independent CEC (**Table 5**). The primary effectiveness endpoint of acute procedural success was achieved in 100% of subjects.

**Table 5. Summary of Primary Safety Endpoint (Analyzable Population)**

Event	DiamondTemp N=70	Timing
	Subjects (%)	
Pericardial Effusion	1 (1.4%)	Prior to 7 days
Transient Ischemic Attack*	1 (1.4%)	Prior to 7 days
Hospitalization for AF recurrence	1 (1.4%)	Prior to 7 days
Hospitalization for chest pain	1 (1.4%)	Prior to 7 days
Supraventricular Tachycardia	1 (1.4%)	Prior to 30 days
<b>Total SAEs through 7 days</b>	<b>4 (5.7%)</b>	
<b>Total SAEs through 30 days</b>	<b>5 (7.1%)</b>	

\* Pending final adjudication

#### Long Term Interim Safety Analysis

The chronic safety of the DiamondTemp System is assessed in TRAC-AF by evaluating the nature and frequency of all serious adverse events at 90 days, 6 months and 12 months post procedure, as adjudicated by the CEC.

To date this additional safety information is only available for the first phase of subjects were treated from January through March of 2016 and that have completed and exited the study. The second phase of subjects have reached 30-day follow-up and have been analyzed together with the first cohort through the 30-day follow-up as outlined in this report. All subjects will be analyzed together at each additional follow-up interval (90 days, 6 months and 12 months) and will be reported in the final study report.

#### **5.6. Conclusion from Clinical Study**

The objective of this First-In-Human study was to substantiate the safety and effectiveness of the DiamondTemp Ablation System use to ablate cardiac tissue in patients with paroxysmal atrial fibrillation. The study endpoints achieved the efficacy performance goal demonstrating 100% effectiveness by confirming PVI isolation in all subjects treated as intended under this study protocol. The safety profile demonstrated in this study indicates the DiamondTemp System can be used safely in cardiac ablation procedures in this patient population, with no incidences of acute serious adverse device-related events (SADEs) and a 5.7% to 7.1% safety endpoint rate through 7 and 30 days, respectively.

The safety results observed in these seventy (70) subjects treated with the DiamondTemp System up to 30 days are well within the recommendations of the published literature and documented safety and efficacy rates of catheter ablation for PAF<sup>[27]</sup>.

## **6. TACTICATH CONTROL DEVICE**

### **6.1. Indications for Use**

The TactiCath Quartz Contact Force Ablation Catheter is indicated for use in cardiac electrophysiological mapping and for the treatment of drug refractory recurrent symptomatic

paroxysmal atrial fibrillation, when used in conjunction with a compatible radiofrequency generator and three-dimensional mapping system.

TactiSys Quartz Equipment and accessories are indicated for use in conjunction with a TactiCath Quartz Contact Force Ablation Catheter. TactiSys Quartz Equipment allows the visualization of the force information coming from the catheter tip.

## 6.2. Product Classification, Code, Regulation

Device Name: TactiCath Quartz Contact Force Ablation Catheter  
Classification: Catheter, Percutaneous, Cardiac Ablation, for Treatment of Atrial Fibrillation  
Product Code: OAE  
Device Class: 3  
Submission Type: PMA (P130026, Approved)

## 6.3. Control Device Description

The TactiCath Quartz Contact Force Ablation System is comprised of the following components:

- TactiCath Quartz Contact Force Ablation Catheter
- TactiSys Quartz CF Equipment hardware inclusive of:
  - TactiSys Quartz Unit
  - TactiSoft Software
  - TactiSys Quartz RF Cable
  - TactiSys Quartz Ethernet Cable
  - Equipotential Cable
  - Mains Cord and Adapter
- Optional Accessories:
  - TactiSys Quartz Mount
  - TactiSys Analog Output Cable
  - TactiSys Quartz Integration Module

## 6.4. TactiCath Quartz Contact Force Ablation Catheter

TactiCath Quartz Contact Force Ablation Catheter (TactiCath) is a sterile, 7F steerable, open-irrigated, multi-electrode RF ablation catheter with a deflectable tip incorporating a force sensor and a thermocouple temperature sensor. The catheter is designed to facilitate electrophysiology mapping of the heart chambers and to transmit RF current to the catheter tip electrode for intracardial ablation. The deflectable distal section of the catheter shaft includes four platinum-iridium electrodes (three ring electrodes and one tip electrode) and is available in 65 mm or 75 mm length, with a total usable length of 115 cm. At the proximal

end of the catheter, a saline port is used to deliver isotonic saline solution to irrigate and cool the tip electrode and ablation site, through a 0.7 mm diameter catheter lumen and six small holes on the distal electrode tip. The catheter features a tri-axial optical force sensor embedded in the tip section which transmits contact force information to the TactiSys Quartz Equipment.

### **6.5. TactiSys Quartz Equipment**

The contact force visualization equipment associated with TactiCath is comprised of the TactiSys Quartz (TactiSys) unit (hardware and associated cables) and TactiSoft (stand-alone software). The TactiSys unit is a non-sterile active signal and data processing unit that interconnects the TactiCath catheter to an external RF generator and collects data from the catheter to compute contact force and related information transmitted from the catheter. The optical measurement system, which is compatible with the force sensing technology incorporated in the TactiCath catheter, is comprised of three optical sensor analyzer modules. The TactiSoft software displays the contact force information transmitted from the catheter through an Ethernet connection on a dedicated, properly configured computer.

### **6.6. Additional Required Equipment**

The following devices are required in addition to the TactiCath Quartz System to perform catheter ablation procedures:

- AMPERE Generator (St. Jude Medical) or Stockert Generator (Biosense Webster)
- Cool Point Irrigation Pump (St. Jude Medical) or CoolFlow Irrigation Pump (Biosense Webster)
- Electrophysiology recording system and cardiac stimulators
- Dedicated Personal Computer with display screen to run TactiSoft software
- St. Jude EnSite Velocity or Precision Cardiac Mapping System

Optional accessories include choice of RF cable, Ethernet cables available in different lengths, an analog output cable, a mount and an integration module (Ethernet - switch) that will allow the integration of contact force information with third party equipment (e.g. integration in the screen of 3D mapping system for enhanced electrophysiology laboratory set-up).

## **7. DIAMONDTEMP INVESTIGATIONAL DEVICE**

### **7.1. Proposed Intended Use of the Investigational Device**

The DiamondTemp Catheter is indicated for use in cardiac electrophysiological mapping (stimulation and recording) and for treatment of drug refractory, recurrent, symptomatic paroxysmal atrial fibrillation when used in conjunction with the DiamondTemp Generator and accessories (DiamondTemp Cable-to-RFG Cable, DiamondTemp GenConnect Cable, DiamondTemp Irrigation Pump/Tubing Set) and compatible mapping system.

## 7.2. Product Classification, Code, Regulation

Device Name: DiamondTemp Ablation Catheter  
Classification: Catheter, Percutaneous, Cardiac Ablation, for Treatment of Atrial Fibrillation  
Product Code: OAE  
Device Class: 3  
Submission Type: PMA


## 7.3. Investigational Device Description

The ACT DiamondTemp Ablation System investigational device includes:

- DiamondTemp Catheter
- DiamondTemp Catheter-to RFG Cable
- DiamondTemp GenConnect Cable
- DiamondTemp RF Generator
- DiamondTemp Irrigation Pump
- DiamondTemp Irrigation Tubing Set
- DiamondTemp Footswitch (optional)

The DiamondTemp Ablation System can be used with the St. Jude EnSite Velocity or Precision Cardiac Mapping System and commonly available EP recording systems and cardiac stimulators.

A representative DiamondTemp Ablation System is illustrated in **Figure 1**.

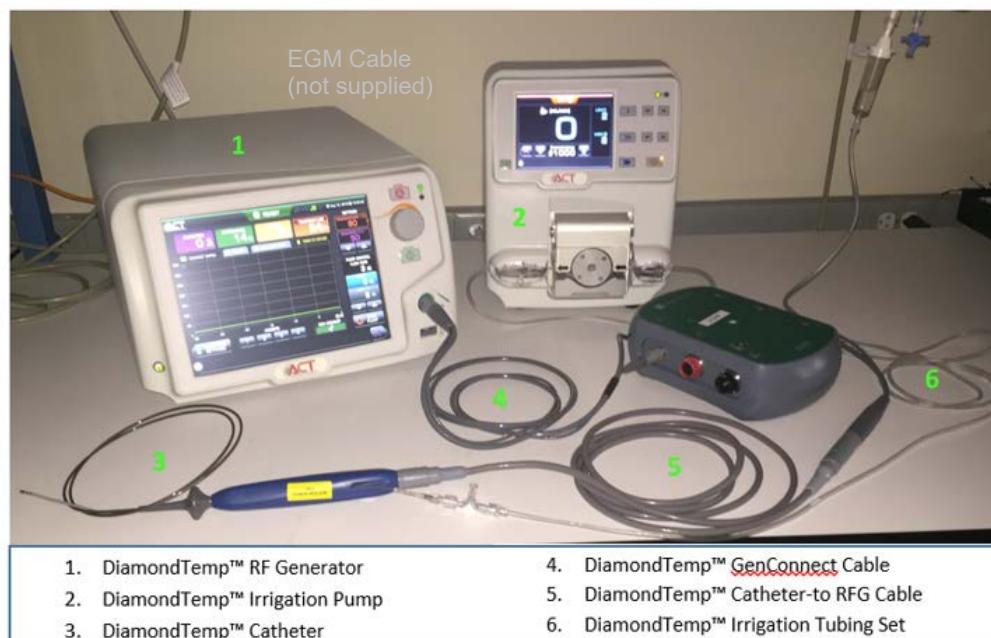

**Figure 1. DiamondTemp Ablation System**


*Key features of the DiamondTemp System:*

- The DiamondTemp System allows for cardiac mapping, pacing and ablation when connected to the St. Jude EnSite Velocity or Precision Mapping System and commercially-available cardiac stimulators and recording systems.
- The DiamondTemp Catheter design, materials and composite tip geometry allow for the recording of local electrograms at the ablation site.
- Six thermocouples at the DiamondTemp Catheter tip provide surface temperature feedback.
- The DiamondTemp Generator modulates power to maintain catheter-tissue interface temperature at a set point optimal for creating an effective lesion without char or thrombus formation.
- The DiamondTemp Generator displays the ablation parameters and the composite temperature recorded from the thermocouples.

All investigational devices for use in the clinical study are identified with model, lot or serial number and will be tracked for dispositioning throughout the study. For the DiamondTemp Ablation Catheter and DiamondTemp Catheter-to-RFG Cable, in addition to the model and lot number, a unique serial number will be used. System Accessories used in the clinical study will be identified by lot and/or serial number.

#### 7.4. DiamondTemp Ablation Catheter

The DiamondTemp Ablation Catheter (DiamondTemp Catheter) is a sterile, single use, externally-irrigated cardiac ablation catheter, 110 cm in length, designed to deliver RF energy at the catheter tip electrode for mapping and cardiac ablation. The DiamondTemp Ablation Catheter (**Figure 2**) is a 7.5F uni-directional, externally irrigated catheter designed to deliver RF energy to composite tip electrode of the catheter for mapping and cardiac ablation. The distal tip and ring electrodes are designed to record electrocardiogram (EGM) signals for mapping and deliver stimulus for pacing. RF emission from the composite tip is similar to commercially-available, externally-irrigated catheters

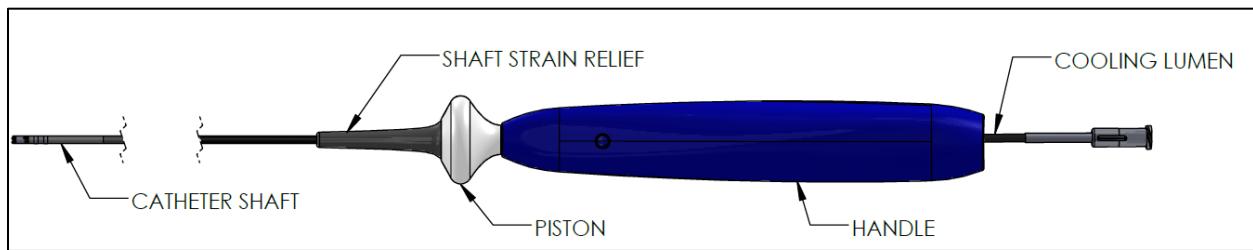

**Figure 2. DiamondTemp Ablation Catheter**

#### 7.5. DiamondTemp RF Generator

The DiamondTemp RF Generator (**Figure 3**) is a temperature-controlled RF generator and provides power to the DiamondTemp Catheter at approximately 460 kHz. It has a universal AC power supply and provides isolated communication ports to the

DiamondTemp Irrigation Pump and serial output to an external monitor which can mirror the RF Generator front panel information (**Figure 3b**) such as temperature, power and impedance curves resulting during RF delivery.



**Figure 3. DiamondTemp RF Generator (a) and Front Panel Display (b)**

#### 7.6. DiamondTemp Irrigation Pump

The DiamondTemp Irrigation Pump (**Figure 4**) is a peristaltic pump designed to deliver normal saline (0.9%, with heparin 1 IU/ml) when used in conjunction with the DiamondTemp Irrigation Tubing Set. The Irrigation Pump can be controlled to deliver the prescribed therapeutic flow rate of 8 ml/min at all power levels up to 50 Watts. The DiamondTemp Irrigation Pump can also be controlled using the touch-screen display on the front panel of the DiamondTemp RF Generator or Irrigation Pump.



**Figure 4. DiamondTemp Irrigation Pump**

### 7.7 DiamondTemp Tubing Set

The DiamondTemp Tubing Set is a disposable, one-time use, one-piece tubing that connects the DiamondTemp Ablation Catheter to the DiamondTemp Irrigation Pump.

### 7.8. DiamondTemp Footswitch

The DiamondTemp Footswitch (**Figure 5**) is an optional accessory used for On/Off control of RF power delivery. Pressing the footswitch turns RF energy ON. Releasing the footswitch terminates delivery of RF energy.



**Figure 5. DiamondTemp Footswitch**

### 7.9. Diamond Temp Cables

#### DiamondTemp Catheter-to-RFG Cable

The DiamondTemp Catheter-to-RFG Cable (**Figure 6**) is 2.4 meters in length, supplied sterile, and contains no latex. The cable distal end has a 19-pin connector that connects to the DiamondTemp Catheter. The cable proximal end, identified by a green band, has a 26-pin connector that connects to either the DiamondTemp RF Generator or to the DiamondTemp GenConnect Cable when a mapping system is used.



**Figure 6. DiamondTemp Catheter-to-RFG Cable**

### **DiamondTemp GenConnect Cable**

The DiamondTemp GenConnect Cable (**Figure 7**) is 2 meters in length and has 4 connectors. The cable connects the DiamondTemp Catheter-to-RFG Cable to a commercially-available mapping system (e.g. St. Jude EnSite Velocity or Precision) GenConnect Box (Maestro/EPT) and to the DiamondTemp RF Generator. The cable is supplied non-sterile and contains no latex.



**Figure 7. DiamondTemp GenConnect Cable**

#### **7.10. Mapping System and EP Recording System Compatibility**

The DiamondTemp System is used with the St. Jude EnSite Velocity and Precision Cardiac Mapping Systems and commonly available EP recording systems and cardiac stimulators.

## **8. STUDY PROTOCOL AND METHODS**

### **8.1. Study Objective**

The objective of this study is to demonstrate the safety and effectiveness of the DiamondTemp Ablation System for the treatment of drug refractory, recurrent, symptomatic paroxysmal atrial fibrillation (PAF). The study will be considered successful if the investigative device is considered non-inferior to the control device for the primary safety and effectiveness endpoints.

### **8.2. Study Design**

The DIAMOND-AF study is a prospective, single-blind, 1:1 randomized, controlled trial being performed at multiple centers in the United States, Canada and Europe to evaluate the safety and effectiveness of the DiamondTemp Ablation System for the treatment of drug refractory, recurrent, symptomatic paroxysmal atrial fibrillation compared to the TactiCath Quartz Contact Force Ablation Catheter and compatible ablation system.

This study will enroll up to 350 subjects diagnosed with PAF at up to 30 investigational sites in the US, Canada and Europe. Investigational sites will have a principal investigator (PI) that is responsible for the conduct of a research study as well as sub-investigators. It is

anticipated that at least 50% of the randomized subjects will be enrolled at centers within the United States.

After providing consent, subjects will undergo screening and baseline tests. Subjects that meet the eligibility criteria will be randomly assigned to either treatment with the investigational or control device only after completion of all screening and eligibility procedures. A randomization module within the Electronic Data Capture (EDC) system will be used to randomize subjects 1:1 to one of two treatment groups using a blocked randomization stratified by site. Since full eligibility for the study may not be confirmable until pre-ablation procedure tests are performed, enrolled subjects will only count towards the enrollment ceiling if they receive treatment or treatment was attempted (e.g. the assigned treatment catheter was introduced into the vasculature).

The primary focus of the left atrial ablation procedure is to create a series of point-by-point RF lesions encircling the left and right PVs to achieve electrical PVI from the rest of the left atrium (LA). Investigators may use their preferred approach to obtain PVI, such as antral or WACA ablation targeting PVs segmentally or PV pairs ipsilaterally. PVI must be confirmed by entrance block at least 20 minutes following the last ablation around the respective PV. Targeting non-PV foci and complex fractionated electrograms is not recommended in this investigation. If the investigator identifies additional focal or macroreentrant atrial sites to be clinically relevant to AF and requiring ablation, the ablation location will be documented.

All subjects will be followed per protocol in relation to the date of the index ablation procedure. Follow up will be required prior to hospital discharge and at 7 days, 1 month, 3 months, 6 months and 12 months post-ablation.

Subjects will be given a cardiac event monitor (Sentinel Wireless ECG Recorder System or equivalent, HeartcoR Solutions, LLC.) at the hospital pre-discharge visit to be used throughout the duration of the study. If subject exhibits symptoms (e.g. palpitations, dizziness, tiredness, lightheadedness, shortness of breath, chest pain, fatigue, syncope) associated with AF recurrence at any time after the ablation procedure, they will be instructed to record their heart rhythm using their cardiac event monitor and to contact the site investigator. This data will be transmitted to and read at an ECG core lab. If a subject has an arrhythmia recurrence within the first 90 days after the ablation procedure (blanking period), one repeat ablation procedure is allowed per protocol. Investigators should make every attempt to schedule a repeat ablation procedure on or before day 90. The repeat ablation procedure must be performed with the assigned investigational or control catheter. Repeat ablation procedures performed with a catheter different than originally assigned will be a protocol deviation.

The duration of the study is projected to span approximately 36 months. The duration accounts for:

- Approximately 12-15 months to enroll all subjects in the trial;
- Approximately 12 -15 months subject participation from consent to end of 12-month follow-up visit window;

- Approximately 3-6 months to analyze, report on study results and close the study.

### 8.3. Primary Safety Endpoints

The primary safety endpoint is defined as freedom from a composite of serious adverse events (SAE) occurring within 7-days post-index ablation procedure or hospital discharge, whichever occurs later, as adjudicated by an independent CEC to be related to the procedure or device.

The primary safety device- or procedure-related SAE composite will be the combined rate of the following events in **Table 6**.

**Table 6. Primary SAE, Classification and Definition**

Primary SAE	Severity Classification / Definition <sup>[26]</sup>
Atrioesophageal fistula	Creation of direct communication between the left atrium and esophagus as documented by esophageal erosion combined with evidence of a fistulous connection to the atrium (e.g. air emboli, an embolic event or direct observation at the time of surgical repair). A CT or MRI scan is recommended to document event.
Bleeding complication	Major bleed that requires a transfusion or results in a $\geq 20\%$ fall in hematocrit
Cardiac tamponade / perforation	Significant pericardial effusion with hemodynamic compromise that requires elective or urgent pericardiocentesis or results in a 1-cm or more pericardial effusion as documented by echocardiography.
Death	Cardiovascular related death post ablation
Myocardial infarction	MI as it relates to AF ablation resulting in the presence of any one of the following criteria: <ul style="list-style-type: none"> <li>• ECG changes indicative of new ischemia that persist for <math>&gt; 1</math> hour</li> <li>• development of new pathological Q waves on an ECG</li> <li>• imaging evidence of new loss of viable myocardium or new regional wall motion abnormality</li> </ul>
Pericarditis	Pericarditis resulting in an effusion that leads to hemodynamic compromise, requires pericardiocentesis, prolongs hospitalization $> 48$ hours or persists for more than 30 days following procedure.
Phrenic nerve paralysis	Absence of phrenic nerve function assessed by a sniff test that persists $> 7$ days. A phrenic nerve paralysis is considered to be permanent when it is documented to be present $\geq 12$ months following ablation.
Pulmonary edema	Pulmonary alveolar fluid accumulation accompanied by typical symptoms (dyspnea), physical findings (rales, hypoxemia), radiologic findings, and response to diuretic therapy and requiring hospitalization.
Stroke post-ablation	Rapid onset of a focal or global neurological deficit with at least one of the following: change in level of consciousness, hemiplegia, hemiparesis, numbness or sensory loss affecting one side of the body, dysphasia or aphasia, hemianopia, amaurosis fugax that persists for $> 24$ hours as determined by the consulting neurologist and subsequent neuroimaging procedure (MRI or CT scan or cerebral angiography).
Thromboembolism	Occurrence of deep vein thrombosis or pulmonary embolism post ablation
Transient ischemic attack (TIA) post-ablation	Rapid onset of new focal neurological deficit with immediate symptom resolution (usually 1 to 2 hours), always within 24 hours as determined by consulting neurologist and neuroimaging without tissue injury.
Vagal nerve injury	Esophageal dysmotility or gastroparesis requiring or prolonging hospitalization following an ablation procedure
Vascular access complications	Resulting in development of a hematoma, an AV fistula or a pseudoaneurysm that requires intervention, such as surgical repair or transfusion, prolongs the hospital stay, or requires hospital admission.

#### 8.4. Primary Effectiveness Endpoints

The primary effectiveness endpoint is defined as freedom from documented symptomatic atrial fibrillation (AF) episodes following the blanking period (3-month follow-up post-ablation procedure) through the end of the effectiveness evaluation period (12-month follow-up post-ablation procedure).

An effectiveness failure is defined by any of the following events during the effectiveness evaluation period (3 through 12-month follow-up visits post ablation):

- Documented episodes of AF lasting  $\geq$  30 seconds in duration as evidenced by electrocardiographic data
- A repeat ablation procedure to treat AF
- Use of a new or modification to existing Class I-IV AAD regimen to treat AF recurrence

#### 8.5. Secondary Endpoints

Secondary endpoints to characterize the performance of the DiamondTemp Ablation System, relative to the control device, will include

- Freedom from a composite of SAE occurring within 30-days post-index ablation procedure as adjudicated by an independent CEC for relatedness to the procedure or device.
- Freedom from documented symptomatic and asymptomatic AT and AFL\* episodes following the blanking period through 12-month follow-up post-ablation procedure.
- Freedom from documented asymptomatic AF episodes through the effectiveness evaluation period lasting  $\geq$  30 seconds in duration by ECG or ECG monitoring system.
- Rate of acute procedural success, defined as confirmation of electrical isolation of PVs via assessment of entrance block at least 20 minutes following the last ablation around the respective PV.
- Rate of occurrence of electrically reconnected PVs following a 20-minute waiting period assessed by entrance block at index procedure.
- Accumulated changes in QOL using the AFEQT Questionnaire from baseline through 6 and 12 months following ablation procedure.
- Neurological changes measured using the NIH stroke scale between baseline and post-ablation (pre-discharge visit) and at 12 months post-ablation procedure.
- Total procedure time (minutes), defined as time of first assigned ablation catheter insertion into the vasculature to time of last procedural ablation catheter removed.
- Time to achieve initial PVI at index procedure (minutes), defined as time of delivery of first RF ablation with the assigned ablation catheter until confirmation of PVI via exit block following a 20-minute waiting period.
- Total treatment device time (minutes), defined as time of delivery of first RF ablation with the assigned ablation treatment catheter to removal of the treatment catheter.

- Mean cumulative RF Time (minutes).
- Mean duration of RF ablations (seconds).
- Total number of RF ablations per procedure.
- Total fluid infused through the assigned ablation catheter (mL).
- Total fluoroscopy time (minutes).
- Number of re-hospitalizations due to atrial fibrillation recurrence after blanking period.

\* *Occurrence and/or ablation of cavotricuspid isthmus (CTI)-dependent AFL, as confirmed by entrainment maneuvers during EP testing at any time during this study is not a primary effectiveness failure because it is not considered an iatrogenic arrhythmia following a left atrial ablation procedure for AF.*

## 8.6. Sample Size Justification

With a randomization ratio of 1:1 and an estimated attrition rate of 7-10%, 175 subjects per treatment group (total N=350) should yield sufficient power for both the primary safety and primary effectiveness endpoints. For primary safety, assuming a Control composite SAE rate of 9%, 159 subjects per group yields 80% power to detect a non-inferiority margin of 9% between treatment groups at a significance level of 0.025. Similarly, assuming a Control effectiveness rate of 65%, 159 subjects per group yields 80% power to detect a non-inferiority margin of -15% between treatment groups at a significance level of 0.025.

## 8.7. Statistical Analysis

Before database lock, the final SAP for clinical data will be prepared to provide full details of all planned analyses. The analyses presented here represent an outline of the intended methodology.

### Analysis Populations

Two analysis populations are defined in this study:

- ITT Population: all randomized subjects regardless of whether they receive study treatment, with analyses conducted according to the randomized treatment assignment.
- Safety Analysis Population: all randomized subjects in which treatment was at least attempted (assigned treatment catheter inserted into vasculature), with analyses conducted by actual treatment received.

### General Considerations

Descriptive summary statistics for continuous variables will include the number of subjects, mean, standard deviation or standard error, median, minimum, and maximum. Nominal categorical variables will be summarized using counts and percentages. Ordinal variables may be analyzed as if they were continuously scaled.

### Subject Disposition

The number and percentage of subjects who complete and discontinue as well as reasons for early discontinuation will be presented.

### Demographics and Baseline Characteristics

Demographic and baseline characteristics will be summarized descriptively. Treatment groups will be compared statistically to confirm that the randomization process generated two homogeneous groups prior to treatment.

## **8.8. Site Training**

Technical training with the DiamondTemp Ablation System will be provided by the Sponsor. Training will be documented and will include a review of the investigational plan, study procedures, CRF completion, instructions for use (IFU) and all study compliance requirements.

## **9. SUBJECT SELECTION**

### **9.1. Criteria for Eligibility**

Subjects included in the DIAMOND-AF study should be selected from the general patient population indicated for or currently scheduled for catheter ablation of PAF. Investigators are responsible for screening all potential subjects and selecting those who meet all inclusion and none of the exclusion criteria for the study.

### **9.2. Study Inclusion Criteria**

Candidates must meet ALL the following criteria to be enrolled in the DIAMOND-AF study:

1. Above eighteen (18) years of age or of legal age to give informed consent specific to state and national law.
2. Patients with a history of symptomatic, paroxysmal atrial fibrillation (PAF) who have had  $\geq 2$  episodes of PAF reported within the 12 months prior to index ablation procedure.
3. At least one episode of PAF  $\geq 30$  seconds in duration documented by electrocardiographic data.
4. Failure or intolerance of at least one Class I-IV AAD for treatment of PAF.
5. Suitable candidate for intra-cardiac mapping and ablation of arrhythmia.
6. Patient agrees to comply with study procedures and be available (geographically stable) for follow-up visits for at least 12 months after enrollment.
7. Patient is willing and able to provide written consent.

### **9.3. Study Exclusion Criteria**

Candidates will be excluded from the DIAMOND-AF study if any of the following conditions apply within the following timeframes:

*At time of enrollment and/or prior to procedure:*

1. AF secondary to electrolyte imbalance, thyroid disease or reversible or non-cardiac cause.
2. LA diameter > 5.5 cm.
3. LVEF < 35%.
4. Currently NYHA Class III or IV or exhibits uncontrolled heart failure.
5. BMI > 40 kg/m<sup>2</sup>.
6. LA ablation, septal closure device or mitral valve surgical procedure at any time prior to enrollment.
7. Presence of intramural thrombus, tumor or abnormality that precludes vascular access, catheter introduction or manipulation.
8. Coagulopathy, bleeding diathesis or suspected procoagulant state
9. Sepsis, active systemic infection or fever (>100.5°F / 38°C) within a week prior to the ablation procedure.
10. Significant restrictive or obstructive pulmonary disease or chronic respiratory condition.
11. Renal failure requiring dialysis or renal compromise that in the investigator's judgement would increase risk to the patient or deem the patient inappropriate to participate in the study.
12. Known allergies or intolerance to anticoagulant and antiplatelet therapies to be used in conjunction with the study or contrast sensitivity that cannot be adequately pre-treated prior to the ablation procedure.
13. Positive pregnancy test results for female patients of childbearing potential or breast feeding.
14. Enrollment in a concurrent clinical study that in the judgement of the investigator would impact study outcomes.
15. Acute or chronic medical condition that in the judgment of the investigator would increase risk to the patient or deem the patient inappropriate to participate in the study.
16. Life expectancy < 12 months based on medical history or the medical judgement of the investigator.

*Within 1 month of enrollment or just prior to procedure:*

17. Documented LA thrombus upon imaging.
18. Creatinine >2.5mg/dl or creatinine clearance <30mL/min.

*Within 3 months of enrollment:*

19. Regularly prescribed amiodarone.
20. Significant GI bleed.
21. MI, unstable angina, cardiac surgery or coronary intervention.

*Within 6 months of enrollment:*

22. CABG procedure.
23. ICD, CRT leads or pacemaker implant procedure.
24. Documented stroke, CVA, TIA or suspected neurological event.

*Within 12 months of enrollment:*

25. An episode of AF lasting >7 days in duration.

## 10. SUBJECT ACCOUNTABILITY

### 10.1. Point of Enrollment

Since full eligibility for the study may not be confirmed without pre-ablation procedure testing (e.g. echocardiography, pregnancy test, creatinine), consented subjects will be considered enrolled and count towards the maximum enrollment ceiling once they are randomized, final eligibility is confirmed and the assigned treatment catheter has been introduced into the vasculature (regardless of treatment).

### 10.2. Subject Status and Classification

The following classifications will be applied to all subjects:

- **Screening Failure:** A subject who has consented (signed ICF) but is found to not meet eligibility criteria through medical file review and/or screening procedures to confirm eligibility. Screening failures do not count against the maximum study enrollment ceiling and there are no follow-up requirements. If screening failure occurs after randomization but prior to insertion of the assigned treatment catheter, the screening failure will be documented.
- **Intent-to-Treat:** Includes all subjects who sign ICF, meet eligibility criteria, are randomized into one of the two study groups and have the assigned treatment catheter inserted into the vasculature or any other RF ablation procedure attempted. These subjects will count against the maximum study enrollment ceiling regardless of any deviation from the protocol or subsequent withdrawal from study. All intent-to-treat subjects will be followed for a minimum of 30 days post-procedure. Exit from the study will be documented. The primary safety and effectiveness endpoints analysis will be used to demonstrate the non-inferiority of the DiamondTemp treatment to the control.
- **Treatment-Per-Protocol:** A subject who is successfully treated per the study protocol with the assigned randomized treatment catheter. These subjects are followed in accordance with the follow-up schedule and are included in all analyses of safety and effectiveness.

The statistical analysis for each classification will be documented in the Statistical Analysis Plan (SAP).

### **10.3. Subject Withdrawal**

All subjects enrolled in the clinical study (including those withdrawn from the clinical study or lost to follow-up) will be accounted for and documented. If a subject withdraws from the clinical study, the reason(s) will be documented. Reasons for withdrawal may include physician discretion, subject choice to withdraw consent, loss to follow-up or death. While study withdrawal is discouraged, subjects may withdraw from the study at any time, with or without reason, and without prejudice to further treatment.

All applicable case report forms up to the point of subject withdrawal must be completed. For subjects who are “lost-to-follow-up” the investigator/center should have at least three documented attempts to contact the subject prior to withdrawal from the study. No additional data may be collected after a subject has been withdrawn from the study or withdraws his/her consent, for whatever reason. All open adverse events should be closed or documented as chronic. Data collected up to the point of subject withdrawal may be used.

## **11. STUDY METHODS**

### **11.1. Enrollment and Visit Schedule**

Enrollment of subjects will occur at the clinical sites only after the appropriate local and national study approvals, “Approval to Enroll” documentation from the Sponsor and written informed consent from subjects have been obtained. **Table 7** summarizes the study follow-up and testing schedule:

**Table 7. Follow up and Testing Schedule**

Assessments/ Activities	Baseline Evaluation	Ablation Procedure	Blanking Period (Ablation procedure – 3 months post procedure)				Effectiveness Evaluation Period (3 months -12 months post procedure)		
			Pre- Discharge	7-Day Follow- Up (± 3 days)	1- Month Follow- Up (± 14 days)	Repeat Ablation Procedure	3- Month Follow- Up (±21 days)	6- Month Follow- up (± 28 days)	12- Month Follow- up (± 45 days)
Eligibility Screening	<b>X</b>								
Informed Consent	<b>X</b>								
Patient Demographics	<b>X</b>								
Medical History	<b>X</b>								
Limited Physical Exam (vitals)	<b>X</b>		<b>X</b>				<b>X<sup>A</sup></b>	<b>X</b>	<b>X</b>
12-lead ECG		<b>X</b>	<b>X</b>				<b>X<sup>A</sup></b>	<b>X</b>	<b>X</b>
TEE or TTE	<b>X<sup>B</sup></b>								
TEE, TTE or ICE		<b>X<sup>C</sup></b>					<b>X<sup>C</sup></b>		
NIH Stroke Scale	<b>X</b>		<b>X</b>				<b>X<sup>A</sup></b>		<b>X</b>
Procedural Data		<b>X</b>					<b>X<sup>A</sup></b>		
Event Monitor Recording			<b>X<sup>D</sup></b>	<b>X<sup>D</sup></b>	<b>X<sup>D</sup></b>			<b>X</b>	<b>X</b>
24 hr. Holter Monitor									<b>X</b>
Cardiac Medication Changes	<b>X</b>	<b>X</b>	<b>X</b>	<b>X</b>	<b>X</b>	<b>X<sup>A</sup></b>	<b>X</b>	<b>X</b>	<b>X</b>
Protocol Deviations	<b>X</b>	<b>X</b>	<b>X</b>	<b>X</b>	<b>X</b>	<b>X<sup>A</sup></b>	<b>X</b>	<b>X</b>	<b>X</b>
Adverse Events	<b>X</b>	<b>X</b>	<b>X</b>	<b>X</b>	<b>X</b>	<b>X<sup>A</sup></b>	<b>X</b>	<b>X</b>	<b>X</b>
AF Quality of Life Survey (AFEQT)	<b>X</b>						<b>X<sup>A</sup></b>		<b>X</b>

<sup>A</sup> Only required if a repeat ablation procedure performed. 1 repeat ablation procedure is allowed during Blanking Period.

<sup>B</sup> TEE only required if subject does not have imaging data to determine LA diameter, LVEF for eligibility within 180d of ablation procedure

<sup>C</sup> TTE, TEE or ICE required pre-procedure to rule out LA thrombus if CHA2DS2-VASc score is ≥ 2, if LA diameter ≥4.6 or if pre-procedure anticoagulation requirements are not met

<sup>D</sup> Event monitor recording only required if subject is experiencing symptoms during blanking period

## 11.2. Screening Evaluation

Investigators and research staff at each site are responsible for conducting screening evaluations and obtaining patient medical history to identify patients that meet eligibility requirements per the study inclusion and exclusion criteria. Sites should maintain a subject screening log to document patients evaluated for enrollment into the study that did not consent. A reason for ineligibility or not providing consent should be provided. Patients who meet general eligibility for consideration in the study will sign an informed consent and undergo a baseline evaluation.

## 11.3. Baseline Evaluation

After eligible subjects have signed an informed consent form and before the scheduled interventional procedure, subjects will undergo a baseline evaluation. This evaluation may be conducted up to 45 days prior to the interventional procedure or on the same day. The evaluation will include but is not limited to the following:

- Medical History and Physical Exam:
  - Subject Demographics
  - Limited Physical Assessment
    - Height and weight
    - Resting blood pressure
    - Resting heart rate
  - Medical History
    - History and documentation of PAF
    - NYHA score
    - CHA<sub>2</sub>DS<sub>2</sub>-VASc score
    - Cardiovascular or other medical history as it pertains to eligibility criteria
  - Medication History
    - Class I-IV AAD history, current doses and/or failure or intolerance
    - Other: cardiac, diuretic, and anticoagulation medications
- Baseline Tests
  - Transesophageal or transthoracic echocardiography (TEE or TTE) \*
    - to determine LA diameter and % LVEF
    - to rule out LA thrombus pre-ablation procedure\*\*
  - Pregnancy test for women of child bearing potential
- Baseline Assessments
  - NIH Stroke Scale administration\*\*\*
  - AF Quality of Life Survey (AFEQT Questionnaire version 1.0)

\* Only required if subject does not have imaging data within 180 days of procedure to determine LA diameter, LVEF for eligibility

\*\* Only required pre-procedure if CHA<sub>2</sub>DS<sub>2</sub>-VASc score is  $\geq 2$ , if LA diameter  $\geq 4.6$  or if pre-procedure anticoagulation requirements are not met

\*\*\* NIH Stroke Scale must be administered by staff certified to conduct assessment

#### 11.4. Pre-Ablation Testing and Requirements

- Echocardiogram (TEE or TTE or ICE) must be performed prior to ablation in the following instances:
  - To confirm LA diameter and LVEF
    - if not available within 180 days of the ablation procedure
  - To rule out LA thrombus\* in subjects if:
    - Not currently and adequately anticoagulated for 3 weeks or longer
      - If subject is on an oral anticoagulant (OAC) they should be taking it regularly for 21 days prior to ablation
      - If a subject is on warfarin prior to ablation, they should have a therapeutic International Normalized Ratio (INR)  $> 2$
    - CHA<sub>2</sub>DS<sub>2</sub>-VASc score is  $\geq 2$
    - LA diameter  $\geq 4.6$  cm

*\*ICE may be considered to rule out LA thrombus in subjects contraindicated for TEE*

If a thrombus is observed on echo, the subject no longer meets eligibility criteria. The subject can be anticoagulated for 30 days until confirmation is received that the clot has resolved but if the clot persists, the subject will not meet eligibility for the study.

- Discontinuation of AADs prior to the procedure is left to the discretion and practice of the investigator and investigational site best practices.
  - Regular amiodarone use must be discontinued 3 months prior to the ablation procedure and not restarted after the ablation procedure.
- Performance of the ablation procedure on uninterrupted anti-coagulation therapy (e.g. warfarin or OACs) is strongly recommended.
  - For subjects anticoagulated with a OAC prior to AF catheter ablation, it is reasonable to hold one to two doses of the OAC prior to AF ablation with re-initiation post-ablation.
- Women of child bearing potential will be required to verify entrance criteria prior to procedure by providing documentation of a negative pregnancy test conducted within 7 days prior to enrollment.

#### 11.5. Ablation Procedure

##### Pre-procedural Preparation

Subjects that meet the eligibility and pre-ablation requirements will be prepped for the ablation procedure with the ablation system to which they are randomized.

The procedures will follow standard hospital practice but should, at a minimum, include the following:

1. Prep and sedate subject per institutional standard practice.

- a. Method of sedation will be recorded (i.e. conscious sedation or general anesthesia).
- b. Placement of an esophageal temperature probe is strongly recommended.
  - i. Deviation of the esophageal temperature probe is allowed if standard practice at the institution.
  - c. Place Ensite Velocity or Precision patches on subject per IFU.
  - d. Place commercially available Dispersive Indifferent Electrode (DIP) patch.
2. Gain vascular access per lab protocol via the femoral veins and/or right or left internal jugular or subclavian veins by insertion of sheaths.
3. Any commercially available 8.5F, fixed or steerable, sheath may be used.
  - a. A steerable sheath is recommended to be used with the DiamondTemp Ablation Catheter.
4. Aspirate and flush sheaths with heparinized saline to remove air prior to introduction into the body and catheter insertion.
  - a. Sheaths (fixed or steerable) should be continuously infused with heparinized saline at 1-2ml/min throughout the procedure.
5. Complete a single or double transseptal puncture to access the LA.
6. A heparin loading dose should be administered just prior to transseptal puncture (recommended) or immediately following. A standard heparin infusion through catheter and sheaths should be given to maintain anticoagulation and activated clotting times (ACT)  $\geq 300$  seconds throughout the ablation procedure.
  - a. ACT must be  $\geq 300$  seconds prior to first ablation.
  - b. ACT levels should be checked every 20-30 minutes during the ablation procedure.
  - c. If ACT is  $<300$  seconds during ablation procedure, more heparin should be administered.
7. Insert and place multi-electrode diagnostic catheters under fluoroscopic guidance.
  - a. Placement of intracardiac catheters will be per standard lab practice but must include a coronary sinus (CS) catheter and a multi-electrode circular catheter for PV mapping and verification of PV isolation and entrance block.
8. Create a 3D anatomical map of the left atrium and location of the PVs with a multielectrode catheter using Ensite Velocity or Precision system.
  - a. RF applications and location will be added to the map during the procedure.
9. A pre-ablation EGM/12 lead ECG documenting the subject's rhythm at the beginning of the procedure will be collected.
10. All peri-procedural AEs must be recorded on the AE CRF and reported to the Sponsor. All device issues, malfunction or deficiencies with the investigational or control devices must be reported on the Device Deficiency CRF. The use of a replacement (back-up) device should be indicated on the Procedure CRF.

### **TactiCath Quartz Contact Force Ablation Catheter Set-up**

The TactiCath Quartz Contact Force Ablation Catheter and TactiSys Quartz Equipment hardware should be prepped and deployed following the operator's manual, IFUs and physician training. General recommended ablation parameters taken directly from the TactiCath IFU are listed in **Table 8**. Please refer to the TactiCath Quartz Catheter IFU for more information.

**Table 8. TactiCath Recommended RF Application Parameters**

General recommendations:

	<b>Atrial ablation</b>
Recommended power range	10 W to 30 W*
Contact Force	Target 20 g with a minimum of 10 g <sup>1,2</sup>
Temperature monitoring	37 to 50 °C**
Irrigation flow rate during RF application	17 to 30 ml/min

\* Power levels exceeding 30 Watts may be used when transmural lesions cannot be achieved at lower energy levels. For power settings > 30 Watts, the recommended irrigation flow rate is 30 ml/min.

**Warning:** Application of higher power is associated with a higher likelihood of audible steam pop occurrence. High power should only be used in special circumstances and only when good contact force cannot be achieved.

**Warning:** Contact force in excess of 70 g may not improve the characteristics of lesion formation and may increase the risk for perforation during manipulation of the catheter.

\*\* The temperature displayed on the generator does not represent tissue temperature or electrode tissue interface temperature.

Additional recommendation:

For isthmus dependent flutter ablation, power applications exceeding 30 Watts and up to 50 Watts maximum should only be used if conduction block cannot be achieved at lower power levels.

### **DiamondTemp Ablation System Set-up**

ACT DiamondTemp Ablation System and Catheter should be prepped and deployed following the respective user manuals, IFUs and physician training. The recommended Generator and Irrigation Pump settings are listed in **Table 9**.

**Table 9. Recommended DiamondTemp RF Generator and Irrigation Pump Settings**

<b>RF Generator Settings</b>	
Operational Mode	Temperature Control
Maximum Temperature Set Point	60°Celcius
Maximum Power Setting	50 Watts
Ablation Duration	45 seconds
<b>Irrigation Pump Settings</b>	
High Irrigation Flow Rate (during ablation)	8 mL/min
Low Irrigation Flow Rate (minimum continuous flow rate)	2 mL/min

When using the DiamondTemp Catheter, the change in the high-resolution EGM can be used to guide the termination of the RF delivery. It is recommended that RF delivery be stopped five (5) seconds – ten (10) seconds after EGM amplitude attenuation is reached. The point of significant EGM attenuation is defined as the time when there are no more changes in the EGM amplitude and/or morphology of the low amplitude signal following the initial rapid EGM amplitude drop.

Investigators are recommended to not ablate for greater than 45 seconds without moving the tip of the investigational ablation catheter.

In the event of a generator cutoff (impedance, temperature) or if a steam pop is observed, the catheter must be withdrawn and the tip electrode observed for the presence of char or coagulum formation. The tip should be cleaned, if necessary, before RF current is reapplied. Purge the catheter prior to insertion into the subject.

### **Pulmonary Vein Electrical Mapping**

The electrical activity of the PVs must be mapped prior to ablation. The investigator may determine the order in which the PVs are mapped and if PV angiography is necessary to facilitate vein access.

To perform the electrical PV mapping, each vein should have a diagnostic catheter inserted to document the presence of PV potentials. Documentation of the PV electrical mapping (PV potentials or lack thereof) is required for each vein. If the mapping catheter is successfully positioned in the vein but no PV potentials are present, ablation of the PV is not recommended. Pre-ablation mapping determines which veins are clinically relevant for appropriate declaration of acute procedural success. If the investigator determines it is not clinically relevant to perform ablation of a PV, the rationale must be noted prior to starting the ablation.

### **Index Ablation Procedure**

The primary focus of the ablation procedure will be to create a series of point-by-point RF lesions encircling the left and right PVs to achieve PVI (electrical isolation of PVs from the LA).

Investigators may use their preferred approach to obtain PVI such as antral or WACA targeting PVs segmentally or PV pairs ipsilaterally. A circumferential approach applying RF application 1-2 cm outside of the PV ostium to prevent PV stenosis is recommended. Targeting non-PV foci and complex fractionated electrograms is not recommended in this investigation. If the investigator identifies additional focal or macroreentrant atrial sites to be clinically relevant to AF and requires ablation, the ablation location will be documented.

The order in which PVs are isolated is up to the investigator's discretion. While isolating the right superior PV, high-voltage pacing may be used before each RF application to check for phrenic nerve stimulation. Ablation should be avoided in areas of phrenic nerve capture as to not cause injury to the phrenic nerve. While ablating on the posterior wall in proximity to the esophagus it is highly recommended that Investigators use an esophageal temperature probe during RF ablation procedures to monitor esophageal temperature and help guide

energy delivery. Each ablation on the posterior LA wall needs to consider the duration, power and temperature (investigational catheter only) settings while in proximity to other structures that could potentially be injured, such as the esophagus. Moving a catheter after shorter durations of RF application, reducing the power (W) and/or temperature set point (investigational system only) is encouraged but is left to the discretion of the investigator.

PVI must be confirmed and documented by entrance block of potentials into the PV a minimum of 20 minutes following the last RF application in each PV or PV pair to monitor for PV reconnection. Adenosine (recommended) and/or isoproterenol may be administered 20 minutes following PVI to detect for the presence of dormant PV conduction.

Administration of isoproterenol for the sole purpose to identify non-PV triggers is allowed but not recommended. Exit block testing is not required, but if performed, exit block must be demonstrated for the PVI to be considered successful. If conduction resumes in any of the PVs, additional RF application can be applied until PVI is achieved. If additional ablation is performed following reconnection of PV, PVI must be reconfirmed at a minimum of 20 minutes following last ablation in the respective PV or PV pair.

Investigators may perform additional RF applications determined to be clinically relevant. The location and ablation parameters for ablation of non-PV foci must be documented. Empiric targeting of complex fractionated electrogram, rotors, ganglionated plexi or performing left atrial mitral isthmus or roof lines are not recommended. Ablation of the CTI is allowed if CTI-dependent (typical) flutter is induced during the procedure or if the subject has a known history of typical flutter. Cardioversions do not signify procedural failures and are not adverse events. A post-ablation EGM/12 lead ECG documenting the subject's rhythm at the end of the procedure will be collected.

All procedure logistical data, ablation parameters, procedural outcomes, adverse events, fluids administered from both catheter and non-catheter sources (i.e., steerable sheath, etc.) and medications administered will be recorded and reported throughout the procedure.

Prophylactic administration of intravenous diuretics during or after the procedure is allowed and will not be considered an adverse event. All ablation catheters must be removed from the subject and inspected for char and coagulum formation if there is a generator cutoff (impedance or temperature) as well as each time a steam pop is observed.

Ablation data collected during the procedure will include but may not be limited to:

- Catheter lot/serial number(s) used
- Temperature set point
- Power set point
- Total number of RF applications for PVI
- Total number of RF applications during the procedure
- Total RF time during the procedure
- ACT levels and times taken
- Location of additional ablations performed and number of RF applications per location
- Total fluid infused from the ablation catheter

- Presence of char or coagulum formation and incidence(s) of steam pops
- Procedure and fluoroscopy times
- EP recording system gain and filter settings for the ablation distal recording channel and manufacturer

If at any time during the ablation procedure the investigator is unable to continue the ablation with the investigational or control catheter (other than when ablating an RA flutter line), the investigator may consider the case a procedural failure and complete the case with a device determined best for the subject. The point at which failure was determined as well as the rationale must be documented.

After removal from the subject, the investigational or control catheter should be inspected, and if any abnormalities such as char or coagulum formation are noted on the catheter, it must be documented. All adverse experiences with the investigational device during the ablation procedure must be promptly reported to the Sponsor and documented on the CRF.

#### **Post-Procedure**

All sheaths will be removed immediately after ablation and hemostasis will be achieved either by direct pressure or the use of a commercially-available closure device.

Investigators may use protamine to reverse the intravenous heparin used during the procedure.

Subjects must be anticoagulated for a minimum of 60 days post index ablation procedure. It is up to the investigator's discretion which drug is best suited for the subject. If anticoagulation was discontinued prior to and during the ablation procedure, anticoagulation should be resumed within 24 hours post-procedure to achieve a therapeutic anticoagulation level. It is recommended that investigators follow the anticoagulation guidelines set forth in the 2017 ACC Expert Consensus Decision Pathway for Periprocedural Management of Anticoagulation in Patients with Nonvalvular Atrial Fibrillation<sup>[26]</sup>.

AADs may also be restarted after the procedure at the discretion of the investigator.

#### **11.6 Pre-Discharge Follow-Up Visit**

Prior to being discharged from the hospital, subjects will be complete a pre-discharge visit. The evaluation will include but is not limited to the following:

- Limited Physical Exam:
  - Weight, resting heart rate, and blood pressure
- Assess the subject for any adverse events following ablation procedure
- Perform a 12-lead ECG
  - Report presence or absence of atrial fibrillation or other supraventricular tachycardias
- NIH Stroke Scale Evaluation follow-up
- Provide subjects with cardiac event monitor and operating instructions

- Record medication changes since ablation procedure
  - Cardiac, AAD, diuretic, or anticoagulation

Subjects will be discharged from the hospital when stable, per the investigator's discretion.

### **11.7 Seven Day Follow-up Phone Call**

All subjects must be evaluated seven days ( $7 \pm 3$  days) post ablation procedure. The follow-up will be conducted over the phone and the following evaluation will be completed:

- Adverse Event Assessment
  - Ask the subject if there have experienced any new adverse events since discharge from the hospital and inquire about resolution of any previously reported event(s)
- Medication changes
  - Ask subject if there have been any changes in their regularly prescribed medications (cardiac, AAD, diuretic, or anticoagulation)
- Review event monitor data for recordings made due to symptomatic episodes of arrhythmias since the last follow-up

### **11.8 One Month Follow-Up Phone Call or Clinic Visit**

All subjects must be evaluated at one month ( $30 \pm 14$  days) after the index ablation procedure. During the follow up, the following will be performed:

- Assess the subject for any new adverse events and inquire about resolution of any previously reported events(s).
- Record any medication changes
- Review event monitor data for recordings made due to symptomatic episodes of arrhythmias since the last follow-up
  - If there has been an early recurrence of AF, investigator should schedule a visit so he/she can evaluate subject to determine if a repeat ablation procedure can be scheduled before the end of the 90-day blanking period.

### **11.9 Repeat Ablation Procedure (if applicable)**

It is expected that some subjects will have early recurrences of AF within the blanking period (90 days following the ablation procedure)<sup>18</sup>. Investigators may perform one repeat ablation procedure in subjects with early recurrence during the blanking period.

The repeat ablation procedure must be performed with the originally assigned investigational or control catheter. Prior to the repeat ablation procedure, subjects must meet the pre-ablation requirements described in Section 11.4 and repeat baseline NIH Stroke Scale and QOL survey. Investigators must follow all procedural requirements defined in Section 11.5 for the repeat ablation procedure. During the repeat procedure, the presence or absence of PV electrical reconnection will be recorded. In addition, the location of reconnection will be noted.

The blanking period and follow-up visit schedule will not restart following the repeat ablation procedure. Subjects that receive a repeat ablation procedure will undergo a repeat ablation pre-discharge visit.

### **11.10 Three Month Follow-Up Visit**

All subjects must be evaluated three-months ( $90 \pm 21$  days) following the index ablation procedure. During this follow-up visit, the following will be performed:

- Perform a limited physical exam (weight, resting heart rate, and blood pressure).
- Assess the subject for any new adverse events and inquire about resolution of any previously reported events(s).
- Perform a 12-lead ECG
  - Report the absence or presence of atrial fibrillation or other atrial tachyarrhythmia.
- Record any medication changes
- Review event monitor data for recordings made due to symptomatic episodes of arrhythmias since the last follow-up.

### **11.11 Six Month Follow-Up Visit**

All subjects must be evaluated six-months ( $180 \pm 28$  days) following the index ablation procedure. During this follow-up visit, the following will be performed:

- Perform a limited physical exam (weight, resting heart rate, and blood pressure).
- Assess the subject for any new adverse events and inquire about resolution of any previously reported events(s).
- Perform a 12-lead ECG
  - Report the absence or presence of atrial fibrillation or other atrial tachyarrhythmia.
- Record any medication changes
- Review event monitor data for recordings made due to symptomatic episodes of arrhythmias since the last follow-up.
- Subjects will be provided a 24-hour Holter monitor
  - Subjects will be given instructions for set-up and return to the core lab
- Administer a follow-up AFEQT Questionnaire (QOL)

### **11.12 Twelve Month Follow-Up Visit**

All subjects must be evaluated twelve-months ( $365 \pm 45$  days) following the index ablation procedure. During this follow-up visit, the following will be performed:

- Perform a limited physical exam (weight, resting heart rate, and blood pressure).
- Assess the subject for any new adverse events and inquire about resolution of any previously reported events(s).

- Perform a 12-lead ECG
  - Report the absence or presence of atrial fibrillation or other atrial tachyarrhythmia.
- Record any medication changes
- Review event monitor data for recordings made due to symptomatic episodes of arrhythmias since the last follow-up.
- Subjects will be provided a 24-hour Holter monitor
  - Subjects will be given instructions for set-up and return to the core lab
- Administer a follow-up QOL assessment (AFEQT Questionnaire)
- Administer a follow-up NIH Stroke Scale assessment

### **11.13 Unscheduled Visits**

Unscheduled visits may occur at any time during the study for the assessment of for example, possible adverse events and/or medication changes. Each unscheduled visit will be documented in a CRF.

### **11.14 Subject Lost to Follow-Up**

The investigator will attempt to contact a subject at least three times prior to designating them as lost-to-follow-up subjects; two of these attempts should include attempting to contact subject via registered mail. The investigator will document the date and type of attempted communication, and will complete the Study Completion Form when a subject is lost to follow-up.

### **11.15 Extended Follow-up Period (if applicable)**

Dependent on the safety and efficacy data collected in this study, it is possible that extended surveillance of subjects will be requested by a Regulatory Authority, including the FDA resulting in an extended follow-up period of up to three (3) years. If extended follow-up is requested, subjects would be re-consented and followed per standard of care for their Institution with continued adverse event collection and reporting. The information collected during these regular follow-up visits would be reported via the EDC system or equivalent and the decision to extend follow-up would be documented in a letter communicated at a minimum to the Investigators, IRB/EC and regulatory authorities as necessary. CEC review of clinical event information and DSMB oversight, if applicable would continue to occur as specified in the CEC/DSMB charter.

### **11.16 Study Completion**

It is the intent of the protocol that all subjects will be followed for a minimum of 12 months post procedure. Documentation of study completion will be required for all subjects, independent of the point at which they complete the study (including screening failure, early withdrawal or loss to follow-up as applicable).

## 12. STUDY CONDUCT

### 12.1. Statement of Compliance

This study will be conducted in accordance with the ethical principles stated in the latest Declaration of Helsinki, ISO 14155: 2011 and FDA 21 CFR parts 50, 54, 56, 812. The study will not begin until appropriate national and local approvals have been obtained, as appropriate. Any additional requirements imposed by the IRB/EC or regulatory authority will be followed where appropriate.

### 12.2. Regulatory Considerations

The clinical investigational plan, subject informed consent and associated documents will be reviewed by the relevant Ethics Committee (EC)/Institutional Review Board (IRB) and appropriate agencies prior to any subject enrollment. The study will not start without the written approval of the IRB/EC and, where needed, the FDA and/or Competent Authority (CA) approval, and after the completion of any other local regulation requirements.

### 12.3. Investigator Responsibilities

The Principal Investigator of an investigational center is responsible for ensuring that the study is conducted in accordance with all Clinical Study Agreements, the clinical investigational plan and applicable regulations in FDA 21 CFR part 812, as well as any prevailing local and/or country laws and/or regulations, whichever affords the greater protection of the subject's rights, safety and welfare. In addition, Investigators are responsible for:

- Ensuring that an IRB/EC reviews and approves Clinical Investigational Plan
- Maintaining adequate and accurate records related to:
  - Subject eligibility
  - Patient Informed Consent form
  - Study related subject source data as described in clinical investigational plan
  - Case report forms
  - Device accountability log
  - Staff delegation of authority and training logs
- Ensuring that conducting the study will not give rise to conflicts of interest
- Informing the Sponsor in writing of the reason(s) for any withdrawal of any IRB/EC approval.
- Ceasing the enrollment of subjects immediately in the event of the withdrawal of any IRB/EC approval.
- Ensuring that no subjects will be enrolled, without prior, written Approval to Enroll from the Sponsor.
- Agreeing to use their best efforts to satisfactorily complete the planned work and comply with accepted GCP.
- Ensuring that informed consent is obtained appropriately and that the conditions of informed consent are complied with.

- Ensuring the appropriate completion of all CRFs (paper and/or EDC) with the understanding that certain records and reports may be submitted to regulatory agencies by the Sponsor to support regulatory submissions.
- Supporting a monitor/auditor (as applicable) in their activities.
- Informing the Sponsor of all adverse events and adverse device effects in a timely manner and informing the IRB/EC of any serious adverse device effects as applicable.

#### **12.4. Confidentiality and Data Protection**

Health data will be recorded and forwarded to the sponsor of the study, and where needed, to participating IRB/EC and the FDA/CA for evaluation as required. Information obtained in this study that can be identified with the subject's identification will remain confidential. Any data that may be published in scientific journals will not reveal the identity of the study participants.

#### **12.5. Insurance**

As the Sponsor of this clinical investigation, ACT will provide proof and type of insurance coverage for subjects in the study, upon request or where required by local/country regulations.

#### **12.6. Protocol Amendments**

Changes to this study that affect the safety or welfare of the subject, scope of the investigation or scientific integrity of the data will require an amendment to the investigational plan. Amendments to the investigational plan may be initiated by ACT or at the request of an Investigator. A formal amendment cannot be initiated by an Investigator or clinical site staff without the approval of ACT.

Protocol amendments must be submitted and subsequently approved by the site IRB/EC and CA and FDA, if applicable.

ACT may make certain administrative changes to the protocol without prior approval of the IRB/EC. ACT will notify all investigative sites of such changes to ensure the study continues to be conducted consistently across all sites.

#### **12.7. Adverse Event Reporting**

All AEs observed by the Investigator or staff during a physical or laboratory examination, interventional procedure or mentioned by the subject, either spontaneously or upon questioning, will be recorded on an AE case report form. All AEs will be documented with the date of occurrence, relatedness to device or procedure, severity, action taken, resolution and any pertinent additional information. Additionally, the Investigator is responsible for providing appropriate treatment for the event and for adequately following the event until resolution.

All adverse events (AE) will be monitored from the time of signed ICF through the twelve-month follow-up visit. **Table 10** details AE classification, definitions and reporting timelines.

**Table 10. Adverse Event Classification, Definitions and Reporting Timelines**

Event Classification	Definition	Reporting Timeline
Adverse Event (AE)	Any untoward and unintended medical occurrence experienced by a clinical study subject. An AE can be any unfavorable and unintended sign (including an abnormal laboratory finding), symptom or disease temporally associated with the use of a Sponsor's investigational system or the control system, whether it is related to the product or not.	Study staff must complete an AE CRF for each AE that occurs per subject throughout the duration of the study. AE CRF will be completed in a timely manner.
Adverse Device Effect (ADE)	AE related to the use of an investigational medical device	Study staff must complete an AE and device deficiency CRF within <u>2 business days</u> after the event for each subject through the duration of the study.
Serious Adverse Event (SAE)	AE that: <ul style="list-style-type: none"> <li>• Led to death,</li> <li>• Led to serious deterioration in the health of the subject, that either resulted in: <ul style="list-style-type: none"> <li>○ a life-threatening illness or injury, or</li> <li>○ a permanent impairment of a body structure or a body function, or</li> <li>○ in-patient or prolonged hospitalization of existing hospitalization, or</li> <li>○ medical or surgical intervention to prevent life-threatening illness or injury or permanent impairment to a body structure or a body function</li> </ul> </li> <li>• Led to fetal distress, fetal death, or a congenital abnormality or birth defect.</li> </ul>	Study staff must complete an AE CRF within <u>2 business days</u> after becoming aware of an SAE for each subject through the duration of the study. Study staff must provide all relevant / supporting source information (de-identified) in a timely manner when documentation becomes available. SAE or SADE will be reported to IRB/EC or FDA/CA per local/regional regulations.
Serious Adverse Device Effect (SADE)	ADE that has resulted in any of the consequences characteristic of the above-mentioned SAE.	Study staff must complete an AE and device deficiency CRF within <u>2 business days</u> after becoming aware of an SAE for each subject through the duration of the study.
Unanticipated Adverse Device Effect (UADE)	Any SAE or any life-threatening problem or death caused by, or associated with, a device, if that effect, problem, or death was not previously identified in nature, severity, or degree of incidence in the investigational plan or risk analysis plan, or any other unanticipated serious problem associated with a device that relates to the rights, safety, or welfare of subjects.	Study staff must complete an AE and device deficiency CRF <u>within 1 business day</u> of becoming aware of the event and report to IRB/EC or FDA/CA per local/regional regulations.

Adverse events will be recorded, reported and followed for all subjects for the duration of their participation in the study regardless of whether they are in the investigational or control cohort. The Principal Investigator is responsible for informing the IRB/EC, and regulatory authorities of UADE(s) and SAE(s) as required by local/regional regulations.

Planned hospitalization for a pre-existing condition, or a procedure required by the clinical investigational plan, without serious deterioration in health, is not considered a SAE.

Additionally, underlying diseases/ pre-existing conditions will not be reported as an AE unless there has been a substantial increase in the severity or frequency of the problem which has not been attributed to natural history during the investigation. To this extent, hospitalizations due to recurrent AF / AFL or prolonged hospitalization following procedure to adjust anticoagulation regimen or to administer diuretic medication are not considered AEs for this study.

#### **Device-Related Adverse Event**

An AE is considered to be device-related (ADE) when, in the opinion of the Investigator, the clinical event has an association in time and/or proximity with the use of the investigational device such that it is reasonable and likely that the investigational device directly caused or contributed to the AE. A device-related adverse event that impacts or potentially impacts a primary and/or secondary safety endpoint will be reviewed and adjudicated by the independent CEC. ADEs include any AE resulting from insufficient or inadequate IFU, deployment, operation, or malfunction of the investigational medical device, as well as, from intentional misuse of the device.

#### **Procedure-Related Adverse Event**

An AE is considered to be procedure-related when, in the opinion of the Investigator, it is reasonable to believe that the event is associated with the ablation procedure and is not specific to the investigational device used and that other products, surgical techniques, or medications required specifically for the procedure are likely to have caused or contributed to the event. A procedure-related adverse event that impacts or potentially impacts a primary and/or secondary safety endpoint will be reviewed and adjudicated by the independent CEC.

#### **12.8. Device Deficiency Reporting**

A device deficiency is defined as any inadequacy of a medical device with respect to its identity, quality, durability, reliability, safety or performance. Device deficiencies include malfunctions, misuse or use errors and inadequate labeling.

Device deficiencies related to the investigational ablation systems may occur in the absence of any associated AE and must be completely documented on a CRF.

Device deficiencies related to the DiamondTemp Ablation System and associated accessories should be reported to the Sponsor within two (2) business days and returned to the sponsor for analysis as expeditiously as possible. Instructions for returning the clinical device(s) will be provided to investigational sites by the Sponsor. If it is not possible to return the device, the investigator should document why the device was not returned and the final disposition of the device. Device failures and malfunctions should also be documented in the subject's medical record. If a device deficiency is associated with an AE that specific event would be recorded as an AE.

Device deficiencies related to the control system will be handled per the hospital standard complaint handling procedure.

*Note: Any Device Deficiency that might have led to an SAE if a) suitable action had not been taken or b) intervention had not been made or c) if circumstances had been less fortunate is considered reportable and should be notified to ACT.*

### **12.9. Protocol Deviations**

The Investigator is not allowed to deviate from the protocol without prior approval by Sponsor and prior review and documented approval from the governing IRB/EC.

Under emergency circumstances, deviations from the clinical investigation plan to protect the rights, safety and well-being of human subjects may proceed without prior approval of the sponsor and the IRB/EC.

Reports of any deviation from the clinical investigational plan as per above emergency circumstances will be reported to the Sponsor and to the IRB/EC as soon as possible after detection, but no later than twenty-four (24) hours from the time of the deviation.

Deviations must be documented on the appropriate protocol deviation CRF.

Any report of withdrawal of IRB/EC approval will be submitted to the Sponsor within five (5) working days.

If a Clinical Monitor becomes aware that an Investigator is not complying with the signed Investigator's Agreement, the Investigational Plan, the requirements of ISO 14155 or other applicable regulations, or any conditions of approval imposed by the reviewing IRB/EC Committee, Sponsor will immediately either secure compliance or discontinue shipments of the device to the Investigator and terminate the Investigator's participation in the investigation. The Investigator will be required to return all investigational components to Sponsor, unless this action would jeopardize the rights, safety or welfare of a subject.

Protocol deviations will be analyzed by Sponsor for the impact to the overall integrity of the study. Input from the statistician and/or the Data Safety Monitoring Board (DSMB) may be obtained to determine if the deviation warrants disqualifying the Investigator.

Disqualification is warranted when an investigator has repeatedly or deliberately violated governing regulations or has repeatedly or deliberately submitted false information in any report. Where protocol deviations occur, which do not warrant disqualification from a study, Sponsor will implement appropriate corrective and preventive actions, including repeat training as deemed necessary.

### **12.10 Investigational Device Accountability**

No device supplies will be shipped to the Investigator until IRB/EC and regulatory authority (CA and/or FDA) approval has been achieved in writing and each Investigator has supplied Sponsor with copies of the IRB/EC approval document and the approved informed consent form to be used.

The investigational devices are to be used only in this clinical investigation and according to this protocol and the IFU. The devices for use in this study must be stored in a secure area. The secure area will have restricted access and the study devices will be kept separate from

other medical devices. The study devices will only be handled by trained personnel and will not be supplied to any individual not involved in the investigation. The study devices will be inventoried at regular intervals during the study and all unused or expired devices will be returned to the Sponsor when study enrollment is closed.

The Principal Investigator or his/her authorized representative is responsible to keep records documenting the receipt, use, return and disposal of the investigational devices. A form will be provided to the site that will log the device model, lot number or serial number and date received by the site. As the devices are used, the site will record the subject study identification number and date of procedure for each device. A space will be provided for recording returned product and the reason for the return.

### **12.11. Documentation**

Source documents may include a subject's medical record, hospital charts, clinic charts, the Investigator's study files, questionnaires and the results of diagnostic tests such as laboratory tests, electrocardiograms, CT angiograms, MR angiograms, echocardiograms and such. The Investigator's copy of the CRFs serves as part of the Investigator's record of a subject's study-related data.

The following information should be included in the subject's medical record:

- Name and contact information
- The study title (DIAMOND-AF Study), study number, and Sponsor name (Advanced Cardiac Therapeutics or ACT)
- Date the subject was informed about the study, that he/she had sufficient opportunity to ask questions and he/she was informed regarding alternative treatments
- The subject was allowed adequate time to consider participation prior to signing the consent form
- A statement that written informed consent was obtained
- Date of enrollment into the clinical study and the subject ID number
- Date of procedure, procedural type, and device lot number
- Visit dates
- Cardiac medications
- Occurrence of any adverse events
- Date subject exited the study, and a notation as to whether the subject completed the study or discontinued, with the corresponding reason.

The Investigator is responsible for ensuring that data are properly recorded in each subject's source data, CRFs and related documents and ensuring timely transfer of data to the CRF. The Investigator who signs the Protocol Signature Page should sign the CRFs requiring signatures to ensure that the observations and findings are recorded correctly and completely. Source data from baseline until 12-month follow-up, respectively, must be transferred to the CRF. All CRFs will be reviewed for completeness, accuracy and clarity. Queries for missing or unclear data will be made as necessary and must be answered within 10 business days.

### 12.12. Record Retention

The Investigator will maintain, at the investigative site, in original format, all essential study documents and source documents that support the data collected on the study subjects in compliance to ICH/GCP guidelines. Documents will be retained for at least two (2) years after the last approval of a marking application or until at least two (2) years have elapsed after the formal discontinuation of the clinical trial of the device. Documents may be retained longer by agreement with the Sponsor or in compliance with other local regulations. The Investigator will take measures to ensure that these essential documents are not accidentally damaged or destroyed. Sponsor requires to be notified in writing if the Investigator intends to leave the hospital so that both parties can be assured a new responsible person is appointed in the hospital responsible for maintaining these essential documents.

## 13. POTENTIAL RISKS AND BENEFITS

### 13.1. Anticipated Adverse Events

There are potential or anticipated risks associated with the use of the DiamondTemp Ablation System. The handling characteristics and principles of operation of the DiamondTemp System are like conventional RF ablation systems and it is anticipated that the rate of catheter/system related complications in this study will be similar to those reported from ablation procedures used with commercially approved ablation systems.

Specific risks are outlined in the system labeling, but in summary the possible risks for catheterization and RF ablation are, but are not limited to the following:

1. Access site complications, including:
  - a. Arteriovenous fistula
  - b. Ecchymosis
  - c. Hematoma
  - d. Hemorrhage or aneurysm
  - e. Infection
  - f. Pain
  - g. Surgical correction involving loss of limb
  - h. Thrombosis
2. Sequelae of fluoroscopic exposure, including:
  - a. Possible cancer risk
  - b. Risk of birth defect
  - c. Harm to fetus
  - d. Skin burns
3. Direct cardiac damage, including:
  - a. Cardiac tamponade / perforation resulting in pericardial effusion

- b. Catheter entrapment within heart or blood vessels, leading to damaged heart wall, valves, chordae tendineae or blood vessels, possibly requiring surgical correction or involving loss of function
  - c. Congestive heart failure
  - d. Damage to cardiac conduction system
  - e. Pulmonary vein stenosis
  - f. Endocarditis
  - g. Myocardial infarction
  - h. Pericarditis resulting in pericardial effusion
  - i. Persistence of an atrial septal defect (resulting from the transseptal puncture)
  - j. Stiff left atrial syndrome
  - k. Valve damage due to catheter entrapment
4. Other intrathoracic collateral effects, including:
  - a. Atrioesophageal fistula
  - b. Damage to trachea, bronchi or pulmonary tissue
  - c. Damage to great vessels
  - d. Esophageal injury
  - e. Phrenic nerve injury
  - f. Vagal nerve injury
5. Embolic phenomena including:
  - a. Coronary artery embolism with or without myocardial infarction
  - b. Gas embolism from procedural error or equipment malfunction with embolic phenomenon
  - c. Infarction of other tissues
  - d. Obstruction of vasculature leading to limbs causing the need for surgical interventions, loss of a limb, or loss of organ function
  - e. Pulmonary embolism
  - f. Paradoxical embolism through patent foramen ovale
  - g. Stroke or TIA
6. Arrhythmias including:
  - a. New arrhythmias occur
  - b. Worsening of existing arrhythmia
  - c. Creation of a partial or complete conduction block, with or without the implantation of a temporary or permanent pacemaker
7. The general sequelae of catheterization including:
  - a. Pulmonary edema
  - b. Skin burns
  - c. Hypotension
  - d. Sepsis

- e. Pneumothorax
- f. Myocardial infarction
- g. Cardiac arrest
- h. Death

8. Medication side effects, especially:

- a. Heparin administration: including bleeding, thrombosis, changes in circulating blood elements and skin necrosis
- b. Ionic and nonionic radiopaque contrast medium, major complications: life-threatening reactions including: cardiovascular collapse, severe respiratory difficulty, nervous system dysfunction, convulsions, coma and cardio-respiratory arrest
- c. Ionic and nonionic radiopaque contrast medium, minor complications: allergic reactions including: nausea, vomiting, facial flush, feeling of body warmth, dermal manifestations of urticaria with or without pruritus, erythema and maculopapular rash, dry mouth, allergic glossitis, sweating, conjunctival symptoms, facial, peripheral and angio-neurotic edema
- d. Anesthetic reactions: including respiratory difficulties, sedation induced apnea, pneumonia, low blood pressure, cardiac arrest (death) and nausea and/or vomiting.

### 13.2. Risk Minimization

A comprehensive functional risk analysis was performed to quantify the risks associated with the use of the DiamondTemp Ablation System. This functional risk analysis evaluated the potential interfaces of the DiamondTemp Ablation System with the subject and/or user and listed the potential harms and potential causes. The associated probability of each cause was estimated and risk control measures were considered and implemented to further reduce the potential for all risks.

The completed risk analyses of the DiamondTemp Ablation System identified all known potential risks to the subject and user. All risks were categorized in the negligible or marginal categories. Since all identified risks were low or moderate, the design is determined to be safe for human use. The risk analysis did not result in findings of any risk that would be considered intolerable. The potential risks associated with any ablation procedure include standard surgical risks for example: infection, electrical shock, perforation, tamponade, skin burns and complications associated with use of ancillary devices, drugs, and anesthetic. The DiamondTemp Ablation System does not create new risks nor does it increase procedural risks as compared with other ablation systems for electrophysiology procedures. The risks associated with the use of the DiamondTemp Ablation System have been identified and evaluated, controls have been put in place to adequately mitigate risks, and a system is implemented that monitors the effectiveness of the risk controls and provides a process to implement corrective and preventive actions.

The DiamondTemp Ablation System is similar in design to existing commercial ablation systems and intends to provide an equivalent functionality to existing irrigated electrophysiology ablation catheter/systems on the market. Additionally, technology integrated within the catheter allows to measure interface tissue temperature and the RF

generator can be set to automatically adjust the power to achieve a desired interface tissue temperature. The DiamondTemp Ablation System does not introduce any new or additional safety risks beyond those associated with similar cardiovascular and ablation procedures. Further, the system is also capable of assessing the extent of contact between the ablation electrode and the cardiac tissue ensuring good energy to transfer to the therapy location. This study is intended to evaluate the safety and performance effectiveness of the DiamondTemp Ablation System for the treatment of atrial arrhythmias.

Risks associated with the DIAMOND-AF Study can be minimized through appropriate training of Investigators and research staff, compliance to this protocol, adherence to inclusion / exclusion criteria and by promptly supplying Advanced Cardiac Therapeutics with data and information required by this protocol.

Additionally, extensive *in vitro* bench and *in vivo* animal studies have been successfully performed with the DiamondTemp Ablation System. Verification and lot release testing for all components of the system will be completed. The associated risks proposed in this study are similar to risks posed by other interventional, electrophysiological cardiac procedures.

Based upon the risk analysis conducted to assess the DiamondTemp Ablation System, ACT has determined that the benefits of the device can outweigh the risks if used in the appropriate patient population by a physician trained in the use of electrophysiology procedures. As a primary treatment for cardiac arrhythmias, the DiamondTemp Ablation System is determined to be safe for human use.

### **13.3. Benefits**

Participants in this research study may or may not receive benefits from participation in this study as compared to standard of care treatment of PAF.

Based on bench and clinical testing with the DiamondTemp Ablation System it is expected that the subjects enrolled in this study will experience similar benefits as those of the currently available commercial systems.

Subjects included in this research study may benefit from closer evaluation of their atrial fibrillation via more frequent office follow-ups, cardiac event monitoring and from having diagnostic non-invasive and invasive evaluation of their cardiac anatomy in the event of previously undiagnosed cardiac abnormalities. There is potential that subjects may have their AF eliminated or AF burden reduced resulting in a better quality of life and reduced need for medication.

Additionally, there may be a benefit to the subjects enrolled in this study through improved therapy delivery. The DiamondTemp system was designed to provide investigators with additional information to a) monitor real-time tissue interface temperatures b) automatically adjust output power to a temperature set point based on the composite temperature c) utilize a low irrigation flow rate for all power output up to 50 Watts.

## 14. MONITORING

Monitoring will be performed during the study to assess continued compliance with the protocol and applicable regulations. Monitoring will occur in line with the Study Monitoring Plan.

### 14.1 Study Monitor

Study Monitors assigned to the DIAMOND-AF study will be responsible for reviewing the device accountability documentation and subject data as collected on CRFs or via an EDC system. The monitor will ensure that the clinical protocol has been approved by the IRB/EC and will assure ongoing compliance with clinical protocol.

The Investigator/institution guarantees direct access to original source documents by Sponsor personnel, their designees, and appropriate regulatory authorities.

### 14.2. Monitoring Procedures

Monitoring visits to the clinical sites will be made periodically to ensure that Investigators and their staff understand and accept their defined responsibilities, assess compliance with current GCP guidelines, evaluate clinical trial progress, assess the continued acceptability of the clinical site facilities, assess compliance with the investigational plan, and verify the accuracy of data recorded on CRFs or via an EDC system to source documentation.

The Sponsor Monitor or its designated representative will be allowed to visit the clinical site and have direct access to all study records throughout the duration of the study. The Monitor will review all source data and compare them to the data documented in the case report forms, in addition to performing a review of the Regulatory Binder and conducting device accountability. Subject safety will be ensured by noting that consent was properly documented, the investigational plan was followed and that AEs were reported and followed-up as appropriate.

The Investigator and/or institution will provide direct access to source data/documents for trial-related monitoring, audits, IRB/EC review and regulatory inspection.

It is important that the Investigator and relevant study personnel are available during the monitoring visits and that sufficient time is devoted to the process.

Additionally, telephone and/or e-mail contact will be conducted on a regular basis with the Investigator and the site staff to ensure that the protocol is being followed and to address any issues that may occur during the trial.

If a deficiency is noted during the trial the Clinical Monitor is required to bring this to the attention of ACT Clinical Affairs Management to discuss the situation and (if required) to secure compliance.

The study Monitor will evaluate and summarize the results of each clinical site visit in written reports, identifying any repeated data problems with any Investigator and specifying recommendations for resolution of noted deficiencies.

As required by IDE regulations, the conduct and monitoring of the clinical investigation will be conducted in accordance with the Sponsor's approved monitoring plan.

#### **14.3. ECG Core Lab**

A designated CRO will provide centers and/or subjects with instructions and training on the use of an event monitors that serves as a hand-held event recorder for short duration recordings and can be worn as a 24 hr. Holter. Subjects will be provided with an event monitor prior to discharge from the hospital and instructed to collect 1-minute ECG recordings with their event monitor if they experience AF symptoms. The event monitors will be configured to automatically transmit recordings securely and wirelessly to the core lab. All events will be analyzed by the core lab to determine if symptoms are associated with arrhythmia recurrence. The core lab will be blinded to subject treatment assignment. The company will identify the subject's transmitted rhythm and send reports to the investigational center within 72 hours. If there is discordance between the core labs rhythm analysis in the report and the investigator, a third-party cardiologist will be used for final rhythm determination. All event monitors should be returned to the Core Lab after a subject completes the study.

At 6 and 12 months post-ablation procedure, the event monitor will be configured to take a 24-hr continuous reading (like a Holter monitor) supplied by the core lab.

#### **14.4 Data Safety Monitoring Board**

The purpose of the DSMB committee is to complete unbiased review of all safety data in comparison to the established criteria in order to determine if the rate of SAEs is acceptable, to evaluate interim data analysis results, to provide related advice on study management and progress, and to make any recommendations regarding the study protocol. Members of the DSMB will be comprised of three (3) voting individuals with relevant expertise for the study and a biostatistician, they will not be employees or shareholders of ACT and they will not be a participating DIAMOND-AF Investigator.

The DSMB will be responsible to communicate any safety, scientific concerns, or other perceived concerns to ACT or designee as soon as possible. The DSMB will provide, after each scheduled meeting, written recommendation regarding the continuation of the trial, early stopping, or any suggested changes for the conduct of the trial. ACT is responsible for informing the IRB/EC and regulatory authorities, as applicable, if the DSMB has advised them of any major safety concerns and has recommended the study be stopped or if they have made any recommendations to alter the study. DSMB decisions are final and non-negotiable by the sites.

#### **14.5. Clinical Events Committee**

The purpose of the CEC is to complete unbiased reviews and classification of serious adverse events and deaths reported by clinical study investigators. The CEC will consist of physicians who are not participating Investigators in the DIAMOND-AF Study and who do not have any significant investment in Sponsor's or any of their entities. The three (3) voting DSMB members will also serve on the CEC to provide an independent unbiased review and adjudication of clinical events throughout the trial. A complete description of CEC and DSMB responsibilities, qualifications, members and operating principles will be outlined in a combined charter.

#### 14.6. Steering Committee

The DIAMOND-AF Steering Committee is comprised of senior clinical, medical and regulatory members of ACT, as well as international physician investigator advisors and the study statistician. The role of the Steering Committee is to provide oversight of the clinical study regarding the design, submission and conduct of the study. Steering Committee members may participate in the review and approval of all requests for data analysis, abstract and manuscript preparation, and submission; however, ACT remains responsible for all decisions related to any such requests in line with approved study agreements.

### 15. SUSPENSION OR TERMINATION

#### 15.1. Premature Termination of the Study

ACT reserves the right to terminate the study at any stage but intends to exercise this right only for valid scientific or administrative reasons and reasons related to protection of subjects. Investigators, associated IRBs/ECs, and regulatory authorities, as applicable, will be notified in writing in the event of study termination.

Possible reasons for premature study termination include, but are not limited to, the following.

- The occurrence of UADEs that present a significant or unreasonable risk to subjects enrolled in the study;
- A decision on the part of Advanced Cardiac Therapeutics to suspend or discontinue development of the device.

#### 15.2. Termination of Participation

Any investigator or IRB/ EC involved in the DIAMOND-AF study may discontinue participation in the study or withdrawal approval of the study, respectively, with suitable written notice to Advanced Cardiac Therapeutics Investigators, associated IRBs/ECs, and regulatory authorities, as applicable.

#### Requirements for Documentation and Subject Follow-up

In the event of premature study termination by the Sponsor, a written statement as to why the premature termination has occurred will be provided to all participating centers by ACT. The IRB/EC and regulatory authorities, as applicable, will be notified. Detailed information on how enrolled subjects will be managed thereafter will be provided.

In the event an IRB or EC terminates participation in the study, participating investigators, associated IRBs/ECs, and regulatory authorities, as applicable, will be notified in writing. Detailed information on how enrolled subjects will be managed thereafter will be provided by ACT.

In the event an investigator terminates participation in the study, study responsibility will be transferred to a co-investigator when possible or another authorized clinical Investigator. In the event there are no opportunities to transfer investigator responsibility; detailed information on how enrolled subjects will be managed thereafter will be provided by ACT.

---

The investigator must return all documents and investigational product to ACT, unless this action would jeopardize the rights, safety, or welfare of the subjects.

**Criteria for Suspending/Terminating a Study Center**

ACT reserves the right to stop the inclusion of subjects at a study center at any time if no subjects have been enrolled for a period beyond 3 months after the site has been granted Approval to Enroll or if the center has multiple or severe protocol violations/noncompliance without justification and/or fails to follow remedial actions.

In the event of termination of investigator participation, all study-related devices and equipment, as applicable, will be returned to ACT unless this action would jeopardize the rights, safety or well-being of the subjects. The IRB/EC and regulatory authorities, as applicable, will be notified. All subjects enrolled in the study at the center will continue to be followed per protocol-defined follow-up. The Principal Investigator at the center must make provision for these follow-up visits unless ACT notifies the investigational center otherwise.

**16. PUBLICATION AND REPORTING POLICY**

Advanced Cardiac Therapeutics is committed to the publication and dissemination of clinical study results. Any publication or presentation relating to the DIAMOND-AF Study will require that ACT's role as a sponsor or financial supporter is included.

The final clinical study report of the conclusions of this study will be written within six (6) months of the closing of the database at the end of the study. The report will be signed by the global study principal investigators and provided to all study investigators. The study protocol will be registered at [www.clinicaltrials.gov](http://www.clinicaltrials.gov) before the inclusion of any study subjects.

**17. REIMBURSEMENT AND COMPENSATION FOR SUBJECTS**

Travel and other expenses incurred by subjects because of participation in the study may be reimbursed in accordance with pertinent country laws and regulations and per the study site's regulations.

## 18. ABBREVIATIONS AND DEFINITIONS

### 18.1. Table of Definitions

Term	Definition	
ACT	ACT is a test that is used to monitor the effectiveness of the administration of Heparin through measuring activated clotting time (ACT)	
Asymptomatic AF, AT or AFL	Also known as silent AF or silent atrial tachycardia (e.g. AT, AFL). Defined as an opportune diagnosis of AF, AT, and/or AFL with electrocardiographic data; specifically, subject's event monitor, 24 hr. Holter monitor or 12 lead ECG at clinic visit.	
Atrioesophageal fistula	Creation of direct communication between the left atrium and esophagus as documented by esophageal erosion combined with evidence of a fistulous connection to the atrium (e.g. air emboli, an embolic event or direct observation at the time of surgical repair). A CT or MRI scan is recommended to document event.	
Attempt Subject	Refers to a subject who has been enrolled and has treatment catheter introduced but does not receive an ablation with the treatment or control catheter per protocol.	
Blanking Period	The ~ 90-day period between ablation procedure and the 3-month follow-up visit. During the blanking period, a repeat ablation can be performed with the same treatment catheter subject originally randomized to and was treated with. Subjects can be prescribed antiarrhythmic drugs as determined necessary by the investigator during blanking period.	
Bleeding complication	Major bleed that requires a transfusion or results in a $\geq 20\%$ fall in hematocrit	
Cardiac tamponade / perforation	Significant pericardial effusion with hemodynamic compromise that requires elective or urgent pericardiocentesis or results in a 1-cm or more pericardial effusion as documented by echocardiography.	
CHA <sub>2</sub> DS <sub>2</sub> -VASc score	Clinical prediction rules for estimating stroke risk in patients with non-rheumatic AF. The rule gives a better risk stratification of low-risk patients than CHADS <sub>2</sub> score by inclusion of additional stroke risk modifier risk factors.	
	Condition	Points

	C	Congestive heart failure (or LV systolic dysfunction)	1
	H	Hypertension (consistently > 140/90mmHg or treated)	1
	A2	Age $\geq$ 75 years	2
	D	Diabetes Mellitus	1
	S2	Prior stroke or TIA or thromboembolism	2
	V	Vascular disease (e.g. peripheral artery disease, MI, aortic plaque)	1
	A	Age 65-74 years	1
	Sc	Sex category (i.e. female sex)	1
Char	The remains of solid biomass originating from intracavity blood or myocardium that has formed as proteins in the blood are denatured by excessive heating that present as friable material observed on the catheter after RF ablation.		
Congestive Heart Failure	Heart doesn't pump properly and fluid builds up in arms, legs, ankles, feet, lungs, or an organ.		
Coagulum	The remains of solid biomass originating from intracavity blood or myocardium that has formed as proteins in the blood are denatured by excessive heating that present as adherent material observed on the catheter after RF ablation.		
Death	Cardiovascular related death post ablation		
Effectiveness Evaluation Period	The period between subject's 3-month follow-up visit and 12-month follow-up visit during which the primary effectiveness endpoint will be assessed.		
Enrolled Subject	All subjects who sign ICF, meet eligibility criteria, are randomized into one of the two study groups and have the assigned treatment catheter inserted into the vasculature or any other RF ablation procedure attempted.		
Heart block	Damage to the heart's electrical system that controls heart rhythm.		

Hemoptysis	Coughing up blood
Femoral (groin) hematoma	Bleeding at the catheter insertion site that causes swelling or a pocket of blood. May need to be drained or require additional procedure.
Long Standing Persistent AF	Long-standing persistent AF is defined as continuous AF of greater than 12 months duration.
Myocardial infarction	MI as it relates to AF ablation resulting in the presence of any one of the following criteria: <ul style="list-style-type: none"> <li>• ECG changes indicative of new ischemia that persist for &gt; 1 hour</li> <li>• development of new pathological Q waves on an ECG</li> <li>• imaging evidence of new loss of viable myocardium or new regional wall motion abnormality</li> </ul>
Paroxysmal Atrial Fibrillation (PAF)	Recurrent atrial fibrillation that last $\geq$ 30 seconds and terminates spontaneously within 7 days.
Pericardial effusion	Accumulation of blood between heart and lining of the heart (pericardium). It is not uncommon to observe “trace” pericardial effusion following AF ablation. Trace effusion that does not need intervention is not considered a serious AE.
Persistent Atrial Fibrillation	Recurrent atrial fibrillation that lasts $\geq$ 7 days and does not terminate spontaneously
Self-Limiting Pericarditis	Pleuritic chest discomfort with or without pericardial rub and ECG changes and did not require additional hospitalization. Generally, not an SAE.
Serious Pericarditis	Pericarditis resulting in an effusion that leads to hemodynamic compromise, requires pericardiocentesis, prolongs hospitalization > 48 hours or persists for more than 30 days following procedure.
Source Data	Original records (or certified copies) of clinical findings, information, observations, or other activities in an investigations necessary for the reconstruction and evaluation of the clinical study.
Source Document	Printed or electronic document containing source data like hospital charts / records, lab notes, device accountability records, radiographs, signed procedural worksheets, records kept at the

	investigation site, and at the laboratories involved in the clinical study.
Phrenic nerve paralysis	Absence of phrenic nerve function assessed by a sniff test that persists > 7 days. A phrenic nerve paralysis is considered to be permanent when it is documented to be present $\geq$ 12 months following ablation.
Pulmonary edema	Pulmonary alveolar fluid accumulation accompanied by typical symptoms (dyspnea), physical findings (rales, hypoxemia), radiologic findings, and response to diuretic therapy and requiring hospitalization.
Screen Failure	A subject who has consented (signed ICF) but is found to not meet eligibility criteria through medical file review and/or screening procedures to confirm eligibility.
Steam pop	Excessive tissue temperatures over $\sim$ 100°C that may result in an audible pop. The pop is a sudden release or explosion due to the vaporization of interstitial fluid in myocardium. This may produce biotraumas and tissue disruption that is usually clinically benign but may cause rupture of thin-walled structures with subsequent pericardial tamponade, usually requiring emergency pericardiocentesis, and/or surgical repair.
Stroke post-ablation	Rapid onset of a focal or global neurological deficit with at least one of the following: change in level of consciousness, hemiplegia, hemiparesis, numbness or sensory loss affecting one side of the body, dysphasia or aphasia, hemianopia, amaurosis fugax that persists for $>24$ hours as determined by the consulting neurologist and subsequent neuroimaging procedure (MRI or CT scan or cerebral angiography).
Symptomatic AF, AT or AFL	Symptoms associated with AF, AT or AFL that were experienced by the subject, made them seek medical attention, and were concurrent with a documented episode by ECG, event monitor and/or Holter monitor. Symptoms may have included palpitations, irregular pulse (i.e. rapid, racing, pounding, fluttering, bradycardic), dizziness, weakness, chest discomfort, and breathlessness.
Thromboembolism	Occurrence of deep vein thrombosis or pulmonary embolism post ablation
Thrombus	An aggregation of blood factors, primarily platelets and fibrin with entrapment of cellular elements, frequently causing vascular obstruction at the point of its formation.

Transient ischemic attack (TIA) post-ablation	Rapid onset of new focal neurological deficit with immediate symptom resolution (usually 1 to 2 hours), always within 24 hours as determined by consulting neurologist and neuroimaging without tissue injury.
Vagal nerve injury	Esophageal dysmotility or gastroparesis requiring or prolonging hospitalization following an ablation procedure
Vascular access complications	Resulting in development of a hematoma, an AV fistula or a pseudoaneurysm that requires intervention, such as surgical repair or transfusion, prolongs the hospital stay, or requires hospital admission.
Vasospasm	Sudden narrowing of artery that usually relaxes with medication or by waiting a short period of time (minutes).
Wide Area Circumferential Ablation (WACA)	The location of PVI has moved more proximally, from the PV ostium to the antral insertion of the PV, several centimeters proximal to the PV ostium. This is called “wide area circumferential ablation” or WACA, and is also known as PV antral isolation. Technique has several advantages: 1) decreases risk of PV stenosis 2) eliminates proximal antral AF triggers 3) modification of nerve bundles that innervate the atria and contribute to AF maintenance may also be ablated.

## 18.2. Table of Abbreviations

Abbreviation	Definition
AAD	Anti-arrhythmic drugs
ACT	Activated Clotting Time
ACT	Advanced Cardiac Therapeutics
ADE	Adverse Device Effect
AE	Adverse Event
AF	Atrial Fibrillation
AFEQT	Atrial Fibrillation Quality of Life Survey
AFL	Atrial Flutter
AT	Atrial Tachycardia
BMI	Body Mass Index
CA	Competent Authority
CABG	Coronary artery bypass graft
CEC	Clinical Events Committee
CF	Contact Force
CFAE	Complex fractionated atrial electrogram
CS	Coronary Sinus
CT	Computed Tomography
CTI	Cavotricuspid Isthmus
DIP	Dispersive Indifferent Patch
DSMB	Data Safety Monitoring Board
EC	Ethics Committee (see IRB for US)
ECG	Electrocardiogram
EDC	Electronic Data Capture
EGM	Electrogram
EP	Electrophysiologist
EU	European Union
F	French size
FDA	US Food and Drug Administration
GCP	Good Clinical Practice
ICE	Intracardiac Echocardiography
ICF	Informed Consent Form
IFU	Instructions for Use
IRB	Institutional Review Board
IU	International Unit
IV	Intra-venous
LA	Left Atrium
LVEF	Left Ventricular Ejection Fraction
MACE	Major Adverse Cardiovascular Event
MRI	Magnetic Resonance Imaging
NYHA	New York Heart Association
PAF	Paroxysmal Atrial Fibrillation

PI	Principal Investigator
PV	Pulmonary Vein
PVI	Pulmonary Vein Isolation
QOL	Quality of Life
RF	Radiofrequency
RFCA	Radiofrequency catheter ablation
SADE	Serious Adverse Device Effect
SAE	Serious Adverse Event
SAP	Statistical Analysis Plan
TEE	Transesophageal echocardiography
TIA	Transient Ischemic Attack
TTE	Transthoracic echocardiography
TTM	Trans-telephonic Monitor
UADE	Unanticipated Adverse Device Effect
US	United States
W	Watts
WACA	Wide area circumferential ablation

## 19. BIBLIOGRAPHY

1. Feinberg, W.M., et al., *Prevalence, age distribution, and gender of patients with atrial fibrillation. Analysis and implications*. Arch Intern Med, 1995. **155**(5): p. 469-73.
2. Go, A.S., et al., *Prevalence of diagnosed atrial fibrillation in adults: national implications for rhythm management and stroke prevention: the Anticoagulation and Risk Factors in Atrial Fibrillation (ATRIA) Study*. JAMA, 2001. **285**(18): p. 2370-5.
3. Krahn, A.D., et al., *The natural history of atrial fibrillation: incidence, risk factors, and prognosis in the Manitoba Follow-Up Study*. Am J Med, 1995. **98**(5): p. 476-84.
4. Wann, L.S., et al., *2011 ACCF/AHA/HRS focused update on the management of patients with atrial fibrillation (update on Dabigatran): a report of the American College of Cardiology Foundation/American Heart Association Task Force on practice guidelines*. Circulation, 2011. **123**(10): p. 1144-50.
5. Friberg, J., et al., *Rising rates of hospital admissions for atrial fibrillation*. Epidemiology, 2003. **14**(6): p. 666-72.
6. Hamer, M.E., et al., *Quality-of-life assessment in patients with paroxysmal atrial fibrillation or paroxysmal supraventricular tachycardia*. Am J Cardiol, 1994. **74**(8): p. 826-9.
7. Dorian, P. and I. Mangat, *Quality of life variables in the selection of rate versus rhythm control in patients with atrial fibrillation: observations from the Canadian Trial of Atrial Fibrillation*. Card Electrophysiol Rev, 2003. **7**(3): p. 276-9.
8. Singh, S.N., et al., *Quality of life and exercise performance in patients in sinus rhythm versus persistent atrial fibrillation: a Veterans Affairs Cooperative Studies Program Substudy*. J Am Coll Cardiol, 2006. **48**(4): p. 721-30.
9. Fuster, V., et al., *2011 ACCF/AHA/HRS focused updates incorporated into the ACC/AHA/ESC 2006 guidelines for the management of patients with atrial fibrillation: a report of the American College of Cardiology Foundation/American Heart Association Task Force on practice guidelines*. Circulation, 2011. **123**(10): p. e269-367.
10. Nattel, S., *Cardiac Electrophysiology: From Cell to Bedside*. 2004: Saunders.
11. Allessie, M.A., et al., *Pathophysiology and prevention of atrial fibrillation*. Circulation, 2001. **103**(5): p. 769-77.
12. Haissaguerre, M., et al., *Spontaneous initiation of atrial fibrillation by ectopic beats originating in the pulmonary veins*. N Engl J Med, 1998. **339**(10): p. 659-66.
13. Fuster, V., et al., *ACC/AHA/ESC 2006 Guidelines for the Management of Patients with Atrial Fibrillation: a report of the American College of Cardiology/American Heart Association Task Force on Practice Guidelines and the European Society of Cardiology Committee for Practice Guidelines (Writing Committee to Revise the 2001 Guidelines for*

*the Management of Patients With Atrial Fibrillation): developed in collaboration with the European Heart Rhythm Association and the Heart Rhythm Society. Circulation, 2006. 114(7): p. e257-354.*

14. Calkins, H., et al., *2012 HRS/EHRA/ECAS Expert Consensus Statement on Catheter and Surgical Ablation of Atrial Fibrillation: recommendations for patient selection, procedural techniques, patient management and follow-up, definitions, endpoints, and research trial design*. Europace, 2012. 14(4): p. 528-606.
15. Neuzil, P., et al., *Electrical reconnection after pulmonary vein isolation is contingent on contact force during initial treatment: results from the EFFICAS I study*. Circ Arrhythm Electrophysiol, 2013. 6(2): p. 327-33.
16. Afzal, M.R., et al., *Use of Contact Force Sensing Technology During Radiofrequency Ablation Reduces Recurrence of Atrial Fibrillation: A Systematic Review and Meta-Analysis*. Heart Rhythm, 2015.
17. Packer, D.L., et al., *Cryoballoon ablation of pulmonary veins for paroxysmal atrial fibrillation: first results of the North American Arctic Front (STOP AF) pivotal trial*. J Am Coll Cardiol, 2013. 61(16): p. 1713-23.
18. Wilber, D.J., *Comparison of Antiarrhythmic Drug Therapy and Radiofrequency Catheter Ablation in Patients With Paroxysmal Atrial Fibrillation A Randomized Controlled Trial*. Journal American Medical Association, 2010. 303(4): p. 333-340.
19. Yokoyama, K., et al., *Novel contact force sensor incorporated in irrigated radiofrequency ablation catheter predicts lesion size and incidence of steam pop and thrombus*. Circ Arrhythm Electrophysiol, 2008. 1(5): p. 354-62.
20. Kuck, K.H., et al., *A novel radiofrequency ablation catheter using contact force sensing: Toccata study*. Heart Rhythm, 2012. 9(1): p. 18-23.
21. Ikeda, A., et al., *Relationship between catheter contact force and radiofrequency lesion size and incidence of steam pop in the beating canine heart: electrogram amplitude, impedance, and electrode temperature are poor predictors of electrode-tissue contact force and lesion size*. Circ Arrhythm Electrophysiol, 2014. 7(6): p. 1174-80.
22. Nakagawa, H., et al., *Locations of high contact force during left atrial mapping in atrial fibrillation patients: electrogram amplitude and impedance are poor predictors of electrode-tissue contact force for ablation of atrial fibrillation*. Circ Arrhythm Electrophysiol, 2013. 6(4): p. 746-53.
23. Nakagawa, H. and W.M. Jackman, *The Role Of Contact Force In Atrial Fibrillation Ablation*. J Atr Fibrillation, 2014. 7(1): p. 1027.
24. Natale, A., et al., *Paroxysmal AF catheter ablation with a contact force sensing catheter: results of the prospective, multicenter SMART-AF trial*. J Am Coll Cardiol, 2014. 64(7): p. 647-56.

25. Reddy, V.Y., et al., *Randomized, Controlled Trial of the Safety and Effectiveness of a Contact Force-Sensing Irrigated Catheter for Ablation of Paroxysmal Atrial Fibrillation: Results of the TactiCath Contact Force Ablation Catheter Study for Atrial Fibrillation (TOCCASTAR) Study*. *Circulation*, 2015. **132**(10): p. 907-15.
26. Calkins, H., et al., *2017 HRS/EHRA/ECAS/APHRS/SOLAECE Expert Consensus Statement on Catheter and Surgical Ablation of Atrial Fibrillation*. *Heart Rhythm*, 2017.
27. Doherty, J.U., et al., *2017 ACC Expert Consensus Decision Pathway for Periprocedural Management of Anticoagulation in Patients With Nonvalvular Atrial Fibrillation: A Report of the American College of Cardiology Clinical Expert Consensus Document Task Force*. *J Am Coll Cardiol*, 2017. **69**(7): p. 871-898.