

## Study Protocol

# **CLINICAL INVESTIGATION OF THE TECNIS® NEXT-GENERATION INTRAOCULAR LENSES**

NCT Number: NCT03372434

Document date: 14 Dec 2017

**CONFIDENTIAL**

The following contains confidential, proprietary information that is the property of Johnson & Johnson Vision

**Clinical Investigation of the  
TECNIS® Next-Generation Intraocular Lenses**

**PROTOCOL NUMBER: SUR-CAT-652-1001**

**SPONSOR:** Abbott Medical Optics Inc./Johnson & Johnson Vision  
1700 E. St. Andrew Place  
Santa Ana, CA 92705  
714-247-8200

**Investigator Agreement**

**As an Investigator, I agree to:**

- Implement and conduct this study diligently and in strict compliance with this agreement; the protocol; Good Clinical Practices; 21CFR812, ISO 14155:2011 and all other applicable FDA regulations; conditions of approval imposed by the reviewing Institutional Review Board (IRB), FDA or other regulatory authorities; and all other applicable laws and regulations.
- Supervise all testing of the device where human subjects are involved.
- Ensure that the requirements for obtaining informed consent are met.
- Obtain authorization for use/disclosure of health information (e.g., HIPAA authorization or equivalent).
- Maintain all information supplied by Johnson & Johnson Vision in confidence and, when this information is submitted to an independent IRB or any other group, it will be submitted with a designation that the material is confidential.

**I have read this protocol in its entirety and I agree to all aspects.**

_____	_____	_____
Investigator Printed Name	Signature	Date
_____	_____	_____
Sub-Investigator Printed Name	Signature	Date
_____	_____	_____
Sub-Investigator Printed Name	Signature	Date
_____	_____	_____
Sub-Investigator Printed Name	Signature	Date
_____	_____	_____
Sub-Investigator Printed Name	Signature	Date

## TABLE OF CONTENTS

<u>TITLE</u>	<u>PAGE</u>
Table of Contents .....	ii
Personnel and Facilities.....	iv
<b>1. Synopsis.....</b>	<b>1</b>
<b>2. Background/Introduction .....</b>	<b>5</b>
<b>3. Clinical Hypothesis.....</b>	<b>6</b>
<b>4. Study Design.....</b>	<b>6</b>
<b>5. Acronyms .....</b>	<b>6</b>
<b>6. Study Objectives and Endpoints .....</b>	<b>7</b>
6.1 Primary Effectiveness Endpoints .....	7
6.2 Primary Safety Endpoints .....	7
6.3 Other Endpoints.....	7
<b>7. Study Products .....</b>	<b>8</b>
7.1 Intraocular Lenses .....	8
7.2 IOL Implantation Systems.....	14
<b>8. Study Population .....</b>	<b>14</b>
8.1 Inclusion Criteria.....	14
8.2 Exclusion Criteria.....	15
<b>9. Investigator Selection.....</b>	<b>16</b>
9.1 Investigator Qualifications.....	16
9.2 Investigator Obligations .....	16
9.3 Investigator Approval.....	17
<b>10. Experimental Plan.....</b>	<b>18</b>
10.1 Overview .....	18
10.2 Visit Schedule.....	19
10.3 Preoperative Procedures .....	20
10.4 Randomization and Masking.....	22
10.5 Study Lens Supply.....	23
10.6 Operative Procedures.....	23
10.7 Postoperative Procedures .....	25
10.8 Exit of Subjects.....	31
10.9 Unscheduled Visits .....	32
10.10 Protocol Deviations.....	33
<b>11. Adverse Events and Product Complaints .....</b>	<b>33</b>
11.1 Adverse Event Definitions.....	33
11.2 Product Complaint/Device Deficiency Definition .....	35
11.3 Adverse Event and Complaint Reporting Requirements .....	35
11.4 Causal Relationship.....	36
11.5 Adverse Event Follow-up.....	37
<b>12. Protocol Changes/Amendments.....</b>	<b>37</b>

<b>13. Ethics Review and Patient Welfare</b> .....	<b>38</b>
13.1 Institutional Review Board (IRB) .....	38
13.2 Informed Consent.....	38
<b>14. Documentation</b> .....	<b>38</b>
14.1 Source Documents .....	38
14.2 Subject Confidentiality .....	39
14.3 Case Report Form Completion .....	39
14.4 Study Summary .....	40
<b>15. Monitoring</b> .....	<b>40</b>
15.1 Data Monitoring .....	40
15.2 Administrative Monitoring .....	40
15.3 Safety Monitoring.....	42
<b>16. Publications</b> .....	<b>42</b>
<b>17. Risk Analysis</b> .....	<b>42</b>
<b>18. Records Retention</b> .....	<b>43</b>
<b>19. Termination of the Investigation</b> .....	<b>44</b>
<b>20. Statistical Methods</b> .....	<b>44</b>
20.1 Analysis Population .....	44
20.2 Primary Study Endpoints .....	45
20.3 Additional Endpoints.....	47
20.4 Visual Acuity conventions and General Statistics.....	48
20.5 Interim Reports.....	49
20.6 Sample Size Calculations .....	49
<b>Appendix A Summary of Procedures Required at Each Visit</b> .....	<b>50</b>
<b>Appendix B Equipment List</b> .....	<b>51</b>
<b>Appendix C Maximum Plus Manifest Refraction Technique with Cylinder Refinement</b> .....	<b>52</b>
<b>Appendix D Refraction Adjustments</b> .....	<b>53</b>
<b>Appendix E Instructions for Using the M&amp;S System</b> .....	<b>54</b>
<b>Appendix F Instructions for Distance Visual Acuity Testing</b> .....	<b>56</b>
<b>Appendix G Instructions for Intermediate Visual Acuity testing</b> .....	<b>58</b>
<b>Appendix H Instructions For Near Visual Acuity Testing</b> .....	<b>59</b>
<b>Appendix I Instructions for Depth of Focus Testing</b> .....	<b>61</b>
<b>Appendix J Instructions for Pupil Size Measurements</b> .....	<b>62</b>
<b>Appendix K Instructions for Contrast Sensitivity Testing</b> .....	<b>63</b>
<b>Appendix L Slit-Lamp Exam Ratings</b> .....	<b>65</b>

**PERSONNEL AND FACILITIES**

**SPONSOR:** Abbott Medical Optics Inc./  
Johnson & Johnson Vision (“JJV”)  
1700 E. Saint Andrew Place  
Santa Ana, CA 92705

**SPONSOR PERSONNEL:**

**Medical Monitor:** [REDACTED]  
Global Medical Director - Cataract  
Johnson & Johnson Vision  
1700 East St. Andrew Place  
Santa Ana, CA 92705  
[REDACTED]

**Director, Clinical Research:** [REDACTED]  
Director, Clinical Research – Cataract  
[REDACTED]

**Study Manager:** [REDACTED]  
Principal Clinical Research Associate  
[REDACTED]

**Director, Clinical Operations:** [REDACTED]  
Director, Clinical Operations  
[REDACTED]

**Biostatisticians:** [REDACTED]  
Research Fellow,  
Biostatistics and Data Management  
[REDACTED]

[REDACTED]  
Principal Research Statistician  
[REDACTED]

**EMERGENCY TELEPHONE NUMBERS:**

[REDACTED]  
[REDACTED]  
[REDACTED]  
[REDACTED]

## Protocol Change History

Version	Section(s)	Page(s)	Description of Change(s)	Rationale for Change(s)
1.0	N/A	N/A	Original	N/A

## 1. SYNOPSIS

**PROTOCOL:** Clinical Investigation of the TECNIS® Next-Generation Intraocular Lenses  
Protocol Number: SUR-CAT-652-1001

**STUDY TREATMENTS:**

Investigational Lens 1:

- TECNIS® Next-Generation IOL, Model ZFR00

Investigational Lens 2:

- TECNIS® Next-Generation IOL, Model ZYR00

Control Lens:

- TECNIS® Multifocal IOL, Model ZLB00 (Johnson & Johnson Vision, Santa Ana, CA), commercially available

**STUDY OBJECTIVE:** The purpose of this clinical trial is to evaluate the safety and effectiveness of the next-generation TECNIS® IOLs.

**CLINICAL HYPOTHESIS:** The next generation of TECNIS IOLs, Models ZFR00 and ZYR00, will provide improved intermediate (at 66 cm) visual acuity compared to the TECNIS Multifocal Model ZLB00 control IOL.  
Complication and adverse event rates associated with the next generation IOLs will be within the rates for posterior chamber IOLs given in ISO 11979-7:2006/ Amd 1:2012(E).

**OVERALL STUDY DESIGN:**

**Structure:** Prospective, multicenter, randomized, bilateral subject/evaluator-masked clinical trial

**Number of sites:** Up to 14 sites in the United States

**Duration:** 6 months

**Administration:** Surgeons will perform routine, small-incision, cataract surgery and implant the study lenses using a sponsor-recommended implantation system. The target for refractive outcomes will be emmetropia for both eyes.

**Visit Schedule:** Subjects will be bilaterally implanted with the same lens type; the second eye is to be implanted within 1 month of the first-eye surgery.

All subjects will undergo a minimum of 9 visits: Preoperative for both eyes; Operative, 1-day and 1-week visits for each eye; and 1-month and 6-month visits for both eyes together.

### **STUDY POPULATION CHARACTERISTICS:**

**Condition:** Bilateral cataracts with otherwise healthy eyes

**Number of Subjects:** Up to 260 subjects will be enrolled to achieve approximately 220 randomized and bilaterally-implanted subjects, resulting in approximately 195 evaluable subjects (65 in each test group and 65 in the control group) at 1 and 6 months.

Each site should enroll approximately 15 subjects, and no site may enroll more than 25% of the enrollment total.

#### **Inclusion Criteria (all criteria apply to each study eye):**

- Minimum 22 years of age
- Bilateral cataracts for which posterior chamber IOL implantation has been planned
- Preoperative best corrected distance visual acuity (BCDVA) of 20/40 Snellen or worse with a glare source or 20/40 Snellen or worse without a glare source
- Potential for postoperative BCDVA of 20/30 Snellen or better
- Corneal astigmatism:
  - Normal corneal topography
  - Preoperative corneal astigmatism of 1.00 D or less in both eyes
- Clear intraocular media other than cataract in each eye
- Availability, willingness and sufficient cognitive awareness to comply with examination procedures
- Signed informed consent and HIPAA authorization or equivalent documentation necessary to comply with applicable privacy laws pertaining to medical treatment in the governing countries
- Ability to understand and respond to a questionnaire in English

#### **Exclusion Criteria (all criteria apply to each study eye):**

- Requiring an intraocular lens power outside the available range of +14.0 D to +26.0 D
- Any clinically-significant pupil abnormalities (non-reactive, fixed pupils, or abnormally-shaped pupils)



- Irregular corneal astigmatism
- Inability to focus or fixate for prolonged periods of time (e.g., due to strabismus, nystagmus, etc.)
- Prior corneal refractive (LASIK, LASEK, RK, PRK, etc.) or intraocular surgery.  
Note: Prophylactic peripheral iridotomies and peripheral laser retinal repairs that, in the opinion of the investigator will not confound study outcome or increase risk to the subject, are acceptable.
- Corneal abnormalities such as stromal, epithelial or endothelial dystrophies that are predicted to cause visual acuity losses to a level worse than 20/30 Snellen during the study
- Inability to achieve keratometric stability for contact lens wearers (per procedure outlined in Section 10.3)
- Recent ocular trauma or ocular surgery that is not resolved/stable or may affect visual outcomes or increase risk to the subject
- Subjects with diagnosed degenerative visual disorders (e.g., macular degeneration or other retinal disorders) that are predicted to cause visual acuity losses to a level worse than 20/30 Snellen during the study
- Subjects with conditions associated with increased risk of zonular rupture, including capsular or zonular abnormalities that may lead to IOL decentration or tilt, such as pseudoexfoliation, trauma, or posterior capsule defects
- Use of systemic or ocular medications that may affect vision
- Prior, current, or anticipated use during the course of the 6-month study of tamsulosin or silodosin (e.g., Flomax, Flomaxtra, Rapaflo) that may, in the opinion of the investigator, confound the outcome or increase the risk to the subject (e.g., poor dilation or a lack of adequate iris structure to perform standard cataract surgery)
- Poorly-controlled diabetes
- Acute, chronic, or uncontrolled systemic or ocular disease or illness that, in the opinion of the investigator, would increase the operative risk or confound the outcome(s) of the study (e.g., immunocompromised, connective tissue disease, suspected glaucoma, glaucomatous changes in the fundus or visual field, ocular inflammation, etc.). Note: controlled ocular hypertension without glaucomatous changes (optic nerve cupping and visual field loss) is acceptable.
- Known ocular disease or pathology that, in the opinion of the investigator,
  - may affect visual acuity
  - may require surgical intervention during the course of the study (macular degeneration, cystoid macular edema, diabetic retinopathy, uncontrolled glaucoma, etc.)
  - may be expected to require retinal laser treatment or other surgical intervention during the course of the study (macular degeneration, cystoid macular edema, diabetic retinopathy, etc.)
- Patient is pregnant, plans to become pregnant, is lactating or has another condition associated with the fluctuation of hormones that could lead to refractive changes
- Concurrent participation or participation within 60 days prior to preoperative visit in any other clinical trial
- Desire for monovision correction

**EVALUATION CRITERIA:**

The purpose of this clinical study is to evaluate the safety and effectiveness of the next-generation TECNIS IOLs. The primary effectiveness endpoint is mean monocular distance corrected intermediate visual acuity under photopic conditions at 66 cm. Other effectiveness endpoints include mean monocular and binocular diopters of defocus, monocular and binocular uncorrected and best corrected distance, uncorrected intermediate, uncorrected near and distance corrected near, monocular and binocular 10% low-contrast distance corrected visual acuities, and questionnaire responses.

The primary safety endpoint is adverse event rates versus ISO 11979-7:2006/ Amd.1:2012(E) Safety and Performance Endpoint (SPE) rates. Additional safety endpoints include the proportion of first-implanted eyes achieving 20/40 or better monocular photopic best corrected distance visual acuity vs. the ISO SPE rate, optical/visual symptoms, medical/lens findings, binocular best corrected distance contrast sensitivity and visual symptoms via PRO instrument.

**DATA ANALYSIS:**

The investigational TECNIS Model ZFR00 and Model ZYR00 IOLs will each be compared separately to the TECNIS Multifocal Model ZLB00 control IOL. For the primary effectiveness endpoints of monocular distance corrected intermediate visual acuity, comparisons between the Model ZFR00 group vs. the Model ZLB00 control group, and comparisons between the Model ZYR00 group vs. the Model ZLB00 control group, will be performed using one-sided, two-sample t-tests with an alpha of 0.025. For the primary safety endpoints, adverse event rates, the adverse event rate of the Model ZFR00 IOL will be compared to the ISO grid value using one-sided exact tests with an alpha of 0.05 and the adverse event rate of the Model ZYR00 IOL will be compared to the ISO grid value using one-sided exact tests with an alpha of 0.05.

The safety population with available data will be used for all analyses. The key study timeframe for all endpoints will be the 1-month postoperative visit, although data will be reviewed at other time points as well. Descriptive statistics including means, standard deviations, minimum and maximum values will be reported for visual acuity, refractive data and contrast sensitivity. The frequency and proportion will be reported for subjects with adverse events, medical findings, lens findings, ocular visual symptoms and questionnaires data.

**STUDY VISITS AND PROCEDURES:**

Inclusion and exclusion qualifications will be assessed at the preoperative visit according to the inclusion/exclusion criteria. The Informed Consent Form and Authorization for Use/Disclosure of Health Information form (HIPAA authorization) must be signed by any patients who agree to participate in the study prior to undergoing any study-specific

procedures. Those subjects who meet the inclusion/exclusion criteria and agree to participate will be randomized to receive lenses from the same lens group in both eyes, either Model ZFR00, Model ZYR00 or control, Model ZLB00. The eye implanted first will be considered the primary study eye. All subjects are intended to have bilateral cataract surgery with the second-eye surgery occurring after the 1-week exam for the first eye but no more than 30 days after the first-eye surgery. Subjects and study personnel performing the postoperative vision testing and refractions will be masked for the duration of the study.

Key preoperative data include ocular health and history, visual acuities, manifest refraction, keratometry, topography, biomicroscopic slit-lamp findings, ocular symptoms and biometry. The operative visit will include standard procedures for cataract surgery and IOL implantation. Key postoperative data collection includes monocular and binocular uncorrected and distance corrected visual acuities, contrast sensitivity, defocus curve, slit-lamp findings, non-directed visual symptoms, questionnaires and adverse events.

## **2. BACKGROUND/INTRODUCTION**

Presbyopia, defined as the age-related loss of accommodative amplitude, affects essentially all human beings beyond the age of 45 and impacts the ability of the eye to focus at near distances<sup>1,2</sup>. Current intraocular lens options for cataract patients who desire improved vision across a range of distances include a choice of monovision or multifocality. Patients implanted with standard monofocal lenses often need spectacles for reading or performing other near tasks, even if a monovision option is selected. Patients implanted with multifocal lenses, while being able to read and perform other near tasks without spectacles, sometimes experience dysphotopsias (e.g., halos), particularly at night, and may have limited intermediate ability (e.g., may need spectacles to work on a computer). Some accommodating lenses are also available on the market, although their effect depends upon fit within the capsular bag or capsular bag elasticity.

On July 15, 2016, another option was made available to cataract patients when the TECNIS Symphony Extended Range of Vision IOL, Model ZXR00, became commercially available in the United States. Utilizing a diffractive technology to elongate the depth of focus, the Symphony IOLs provide cataract patients with good distance vision, and improved intermediate and near vision compared to standard monofocal IOLs.

The investigational IOL devices in this protocol, Models ZFR00 and ZYR00, are enhanced versions of the commercially-available Symphony and Multifocal IOLs. The diffractive technology on the posterior optic surface of the TECNIS Symphony IOL was modified for both investigational IOLs, with the goal of providing improved intermediate vision as compared to the Multifocal Model ZLB00 control IOL.

### 3. CLINICAL HYPOTHESIS

This study will demonstrate that the TECNIS Model ZFR00 and Model ZYR00 IOLs will provide improved intermediate (at 66 cm) visual acuity compared to the TECNIS Multifocal Model ZLB00 control IOL. Complication and adverse event rates associated with the next generation IOLs will be within the rates for posterior chamber IOLs given in ISO 11979-7:2006/ Amd 1:2012(E).

### 4. STUDY DESIGN

This study is a 6-month, prospective, multicenter, subject/evaluator-masked, bilateral, randomized clinical investigation of the TECNIS Next-Generation Model ZFR00 and Model ZYR00 IOLs versus the TECNIS Multifocal Model ZLB00 control IOL.

The study will be conducted at up to 14 sites in the U.S.A and will enroll up to 260 subjects to achieve approximately 220 randomized and bilaterally-implanted subjects, resulting in approximately 195 evaluable subjects (65 in each test group and 65 in the control group) at 1 and 6 months. Subjects are to be implanted with the same IOL in both eyes, the ZFR00 IOL, the ZYR00 IOL or the ZLB00 control IOL. The eye implanted first will be considered the primary study eye.

#### JUSTIFICATION OF STUDY DESIGN

This study is being conducted to capture preliminary safety and effectiveness information on two design candidates, with the goal of selecting a final lens design. The prospective, multicenter, subject/evaluator-masked, bilateral, randomized study design was chosen to optimize comparison of visual outcomes between the Models ZFR00 and ZYR00 investigational IOLs and the Model ZLB00 control IOL, while minimizing the number of subjects by utilizing the same control group for statistical comparisons.

### 5. ACRONYMS

The following acronyms are used throughout the document:

- UCDVA: uncorrected distance visual acuity
- BCDVA: best corrected distance visual acuity
- UCIVA: uncorrected intermediate visual acuity
- DCIVA: distance corrected intermediate visual acuity
- UCNVA: uncorrected near visual acuity
- DCNVA: distance corrected near visual acuity
- D: diopters

## 6. STUDY OBJECTIVES AND ENDPOINTS

The purpose of this study is to evaluate the safety and effectiveness of the next-generation TECNIS Model ZFR00 and Model ZYR00 IOLs. The key study timeframe for all endpoints will be the 1-month postoperative visit, although data will be reviewed at other time points as well.

### 6.1 PRIMARY EFFECTIVENESS ENDPOINTS

#### FOR MODEL ZFR00: MONOCULAR, PHOTOPIC DCIVA AT 66 CM

Success criteria: Statistically significant improvement in mean distance corrected intermediate visual acuity for the investigational Model ZFR00 eyes vs. control eyes.

#### FOR MODEL ZYR00: MONOCULAR, PHOTOPIC DCIVA AT 66 CM

Success criteria: Statistically significant improvement in mean distance corrected intermediate visual acuity for the investigational Model ZYR00 eyes vs. control eyes.

### 6.2 PRIMARY SAFETY ENDPOINTS

For Model ZFR00: Rates of adverse events vs. ISO SPE rates

For Model ZYR00: Rates of adverse events vs. ISO SPE rates

### 6.3 OTHER ENDPOINTS

- Monocular and binocular, best corrected distance depth of focus
- Monocular BCDVA percent 20/40 or better vs. ISO SPE rate
- Binocular UCDVA, BCDVA, UCIVA, DCIVA, UCNVA and DCNVA
- Monocular UCDVA, UCIVA, UCNVA and DCNVA
- Monocular and binocular low-contrast BCDVA (10%)
- Monocular and binocular best corrected distance contrast sensitivity vs control (mesopic with and without glare at 1.5, 3, 6, and 12 cpd, photopic without glare at 3, 6, 12, and 18 cpd)
- Visual symptoms via PRO instrument
- Ocular/visual symptoms (non-directed responses as obtained from the open-ended question "Are you having any difficulties with your eyes or vision?")
- Subject spectacle independence and satisfaction questionnaire responses
- Medical findings/complications
- Lens findings/complications

## 7. STUDY PRODUCTS

### 7.1 INTRAOCULAR LENSES

The three lens models used in this study include the investigational TECNIS Next-Generation IOLs, Model ZFR00 and ZYR00, and the TECNIS Multifocal Model ZLB00 control IOL. The investigational IOLs are modifications of the Symphony and Multifocal IOLs, single-piece, SENSAR acrylic IOLs with a modified prolate (aspheric) design on the anterior optic surface to reduce spherical aberration and a diffractive posterior optic design.

#### **Investigational TECNIS Next-Generation IOLs, Models ZFR00 and ZYR00**


The TECNIS Next-Generation IOLs, Models ZFR00 and ZYR00, are posterior chamber, 1-piece, aspheric, diffractive, acrylic, foldable IOLs designed for placement in the capsular bag (**Figures 1 and 2**). The lenses are made of the same hydrophobic SENSAR acrylic material as the material/mechanical 1-piece parent, the JJV SENSAR 1 Piece IOL, Model AAB00, and one of the optical parents, the TECNIS Symphony IOL, Model ZXR00 (**Figure 3**). The lenses have the same overall geometry/dimensions (13 mm overall length and 6 mm optic diameter) as the material/mechanical 1-piece parent IOL, the JJV SENSAR IOL, Model AAB00, and both optical parents, the TECNIS Symphony IOL, Model ZXR00, and the TECNIS Multifocal IOL, Model ZM900. The investigational lenses also have the same TECNIS modified prolate (aspheric) design on the anterior optic surface as the optical parents, the Symphony and Multifocal IOLs, to reduce spherical aberration.

The Model ZLB00 control IOL (**Figure 5**) is derived from the same predecessor lenses as those for the subject devices. Model ZLB00 shares the same lens material, general dimensions, lens geometry, and one-piece soft acrylic lens platform as the SENSAR 1-Piece IOL, Model AAB00, which is the material/mechanical parent of the subject devices. Model ZLB00 also incorporates the same aspheric anterior optic feature and similar diffractive profile on its posterior optic as the TECNIS Multifocal IOL, Model ZM900, and the TECNIS Symphony IOL, Model ZXR00, which are both optical parents of the subject devices. Therefore, the ZLB00 control IOL can be considered a multifocal analog of the subject devices.


The posterior optic designs of the investigational lenses have been modified compared to the optical parent IOLs. The Model ZFR00 has a diffractive profile consisting of 14 concentric rings compared to the 9 concentric rings (10 zones) of the parent Symphony IOL and 32 concentric rings of the parent Multifocal IOL, Model ZM900 (**Figure 4**). The Model ZYR00 has a diffractive profile consisting of 22 concentric rings. The modifications to the posterior diffractive optics of both investigational IOLs are designed

to further extend the depth of focus compared to the Symphony IOL and provide improved intermediate visual acuity compared to the TECNIS Multifocal IOL.


**Figure 1: Drawing and Photograph of a TECNIS Model ZFR00 IOL**

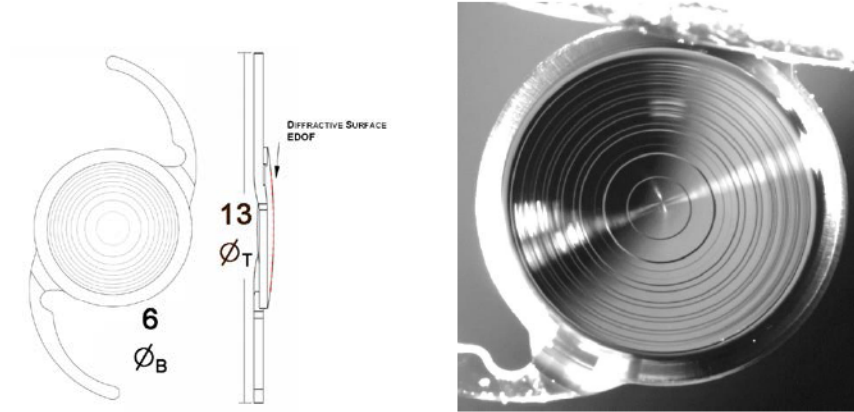


**Figure 2: Drawing and Photograph of a TECNIS Model ZYR00 IOL**

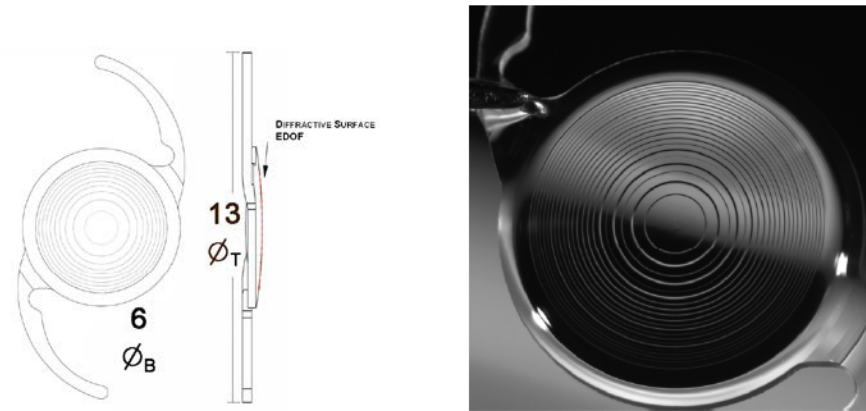


**Figure 3: Drawing and Photograph of a TECNIS Symphony IOL**

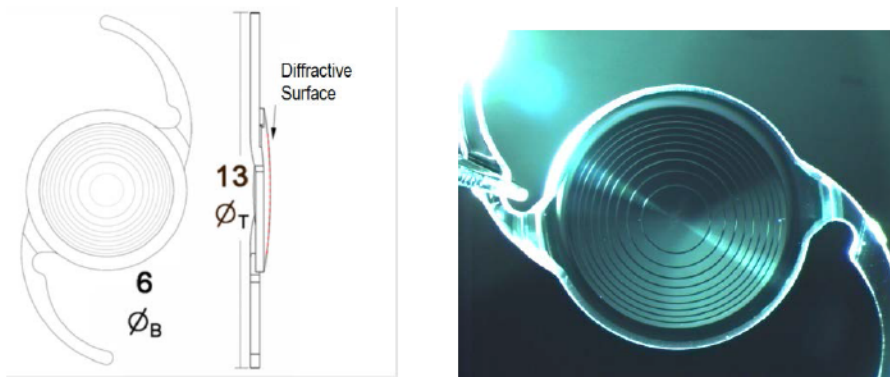

**Figure 4: Drawing and Photograph of a TECNIS Multifocal IOL, Model ZM900**

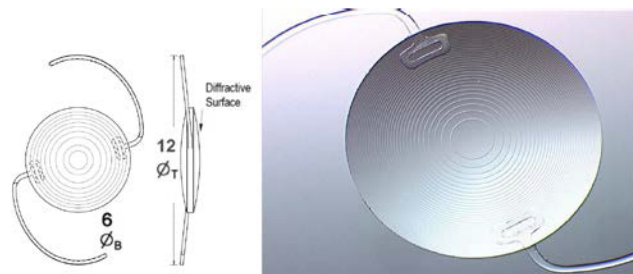

**Figure 5: Drawing and Photograph of a TECNIS Multifocal IOL, Model ZLB00**

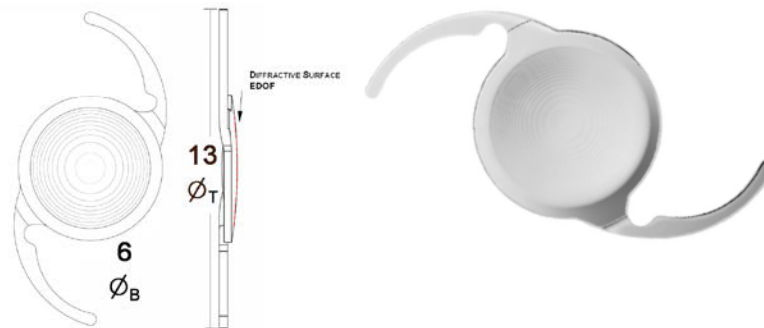

Like all of JJV's 1-piece soft acrylic IOLs, Models ZFR00, ZYR00, Model ZXR00, and the Model ZLB00 control, have a surface treatment of Polyethylene Glycol (PEG) to reduce tackiness of the lens surface and include a ProTEC 360° barrier edge, the stability of Tri-Fix 3-point design, and a frosted-edge treatment.

#### INDICATIONS FOR INVESTIGATIONAL IOLS

The Model ZFR00 is currently indicated for primary implantation for the visual correction of aphakia, in adult patients with less than 1 diopter of preexisting corneal astigmatism, in whom a cataractous lens has been removed. The lens mitigates the effects of presbyopia; compared to a standard multifocal IOL, the lens is intended to provide improved intermediate visual acuity, while maintaining comparable near and distance visual acuity. The Model ZFR00 IOL is intended for placement in the capsular bag only.

The Model ZYR00 is currently indicated for primary implantation for the visual correction of aphakia, in adult patients with less than 1 diopter of preexisting corneal astigmatism,



in whom a cataractous lens has been removed. The lens mitigates the effects of presbyopia; compared to a standard multifocal IOL, the lens is intended to provide improved intermediate visual acuity, while maintaining comparable near and distance visual acuity. The Model ZYR00 IOL is intended for placement in the capsular bag only.

#### INDICATIONS FOR CONTROL IOL

The TECNIS Multifocal IOL, Model ZLB00, is indicated for primary implantation for the visual correction of aphakia, in adult patients with or without presbyopia in whom a cataractous lens has been removed by phacoemulsification and who desire near, intermediate, and distance vision with increased spectacle independence. The Model ZLB00 IOL is intended for capsular bag placement only.

#### STORAGE AND DISTRIBUTION

Consignments of all three study lenses will be supplied to the sites. All study lenses should be stored in the original packaging and kept in a dry place. Lenses should not be stored in direct sunlight or at temperatures greater than 45° C (113°F). Each lens is packaged in a lens tray and sealed in a peel-pouch. The lens is sterile as long as the package has not been opened or damaged and the shelf-life expiration date has not been exceeded. The Principal Investigator is responsible for ensuring that the investigational lenses are used only for subjects enrolled in this study.

#### COMPARISON CHART

**Table 1** describes the dimensional and optical similarities between the study lenses and other associated JJV lenses.

Table 1: Comparison of Design Features

	<b>SENSAR 1-PIECE IOL, MODEL AAB00 (MECHANICAL / MATERIAL PARENT)</b>	<b>TECNIS 1-PIECE IOL, MODEL ZCB00 (MONOFOCAL ANALOG)</b>	<b>TECNIS MULTIFOCAL IOL, MODEL ZM900 (OPTICAL PARENT)</b>	<b>TECNIS SYMPHONY EXTENDED RANGE OF VISION IOL, MODEL ZXR00 (OPTICAL PARENT)</b>	<b>MODEL ZFR00 (SUBJECT DEVICE)</b>	<b>MODEL ZYR00 (SUBJECT DEVICE)</b>
<b>LENS DESIGN</b>	1-piece acrylic monofocal with spherical anterior surface	1-piece acrylic monofocal with aspheric anterior surface	3-piece silicone multifocal with aspheric anterior surface	1-piece acrylic extended range of vision IOL with aspheric anterior surface	1-piece acrylic diffractive hybrid IOL with aspheric anterior surface	
<b>LENS MATERIAL</b>	Surface-treated SENSAR® soft acrylic material	Same as AAB00	Polysiloxane	Same as AAB00		
<b>DIMENSIONAL FEATURES</b>						
<b>OVERALL DIAMETER</b>	13.0 mm	Same as AAB00	12.0 mm	Same as AAB00		
<b>OPTICAL CENTER THICKNESS</b>	0.74 mm (20 D lens)	0.72 mm (20 D lens)	1.13 mm (20D lens)	0.66 mm (20 D lens)		
<b>HAPTIC ANGLE</b>	No angulation, but offset from optic body	Same as AAB00	5°	Same as AAB00		
<b>OPTIC BODY DIAMETER</b>	6.0 mm	Same as AAB00	Same as AAB00	Same as AAB00		
<b>HAPTIC MATERIAL</b>	Same as optic	Same as AAB00	Polyvinylidene fluoride (PVDF)	Same as AAB00		
<b>HAPTIC WIDTH</b>	0.39 mm	Same as AAB00	0.18 mm	Same as AAB00		
<b>HAPTIC THICKNESS</b>	0.46 mm	Same as AAB00	0.18 mm	Same as AAB00		
<b>HAPTIC STYLE</b>	C-Loop	Same as AAB00	Cap C	Same as AAB00		
<b>OPTICAL FEATURES</b>						
<b>OPTIC SHAPE</b>	Biconvex	Same as AAB00	Same as AAB00	Same as AAB00		
<b>ANTERIOR OPTIC PROFILE</b>	Spherical	Aspheric	Same as ZCB00	Same as ZCB00		
<b>POSTERIOR OPTIC</b>	Spherical monofocal	Same as AAB00	Spherical diffractive	Spherical diffractive	Modified spherical diffractive	

	<b>SENSAR 1-PIECE IOL, MODEL AAB00 (MECHANICAL / MATERIAL PARENT)</b>	<b>TECNIS 1-PIECE IOL, MODEL ZCB00 (MONOFOCAL ANALOG)</b>	<b>TECNIS MULTIFOCAL IOL, MODEL ZM900 (OPTICAL PARENT)</b>	<b>TECNIS SYMFONY EXTENDED RANGE OF VISION IOL, MODEL ZXR00 (OPTICAL PARENT)</b>	<b>MODEL ZFR00 (SUBJECT DEVICE)</b>	<b>MODEL ZYR00 (SUBJECT DEVICE)</b>
<b>PROFILE</b>						
<b>OPTIC EDGE DESIGN</b>	PROTEC squared edge	Same as AAB00	Squared edge	Same as AAB00		
<b>DIOPTER POWER RANGE</b>	+6.0 to +30.0D in 0.5D increments	+5.0 to +34.0D in 0.5D increments	Same as ZCB00	Same as ZCB00	Same as ZCB00 <sup>1</sup>	+10.0 to +34.0D in 0.5D increments <sup>1</sup>
<b>REFRACTIVE INDEX</b>	1.470 (35° C)	Same as AAB00	1.46 (37° C)	Same as AAB00		
<b>ADD POWER</b>	N/A	N/A	+4 D	N/A <sup>2</sup>	N/A <sup>3</sup>	
<b>RANGE OF VISION</b>	N/A	N/A	N/A	Through 2.0 D <sup>2</sup>	Through 3.0 D <sup>3</sup>	

<sup>1</sup> Only IOLs from +14.0 D to +26.0 D will be used in the clinical study.

<sup>2</sup> There is no distinct add power. Clinically, the range of the defocus with binocular visual acuity above 0.2 LogMAR is approximately 2.0 D in the near direction.

<sup>3</sup> There is no distinct add power.

## 7.2 IOL IMPLANTATION SYSTEMS

The investigational TECNIS Models ZFR00 and ZYR00 and the control TECNIS Model ZLB00 lenses are to be implanted using the UNFOLDER Platinum 1 Series Implantation System (DK7796 handpiece with the UNFOLDER Platinum 1 Series cartridge, Model 1MTEC30) or the ONE SERIES Ultra Implantation System (DK7786 or DK7791 handpiece with the One Series Ultra cartridge, Model 1VIPR30).

## 8. STUDY POPULATION

All study subjects will be enrolled from the normal surgical cataract population at up to 14 sites in the U.S.A. Approximately 260 subjects will be enrolled (signed informed consent document) to achieve approximately 220 randomized and bilaterally-implanted subjects, resulting in approximately 195 evaluable subjects (65 in each test group and 65 in the control group) at 1 and 6 months. This allows a screen failure rate of approximately 15% and a drop-out rate of approximately 10% for implanted subjects. Each site should implant approximately 15 subjects, and no site may implant more than 25% of the enrollment total.

This study will include only subjects undergoing bilateral primary cataract extraction and IOL implantation and who meet all of the study inclusion and exclusion criteria in both eyes. All subjects who meet the eligibility criteria will be offered enrollment in the study. Eligibility criteria may not be waived by the investigator. Any questions regarding patient eligibility are to be discussed with JJV prior to subject enrollment. Those subjects who meet the eligibility criteria and agree to participate will be randomized to receive lenses from the same lens group in both eyes, either Model ZFR00, Model ZYR00 or Model ZLB00 control. Subjects will be enrolled at each site sequentially until the overall study recruitment goals are met or the site limit is reached.

### 8.1 INCLUSION CRITERIA

Note: All criteria apply to each eye

- Minimum 22 years of age
- Bilateral cataracts for which posterior chamber IOL implantation has been planned
- Preoperative best corrected distance visual acuity (BCDVA) of 20/40 Snellen with a glare source or 20/40 Snellen or worse without a glare source
- Potential for postoperative BCDVA of 20/30 Snellen or better
- Corneal astigmatism:
  - Normal corneal topography
  - Preoperative corneal astigmatism of 1.00 D or less in both eyes
- Clear intraocular media other than cataract in each eye
- Availability, willingness and sufficient cognitive awareness to comply with examination procedures

- Signed informed consent and HIPAA authorization or equivalent documentation necessary to comply with applicable privacy laws pertaining to medical treatment in the governing countries
- Ability to understand and respond to a questionnaire in English

## 8.2 EXCLUSION CRITERIA

Note: All criteria apply to each eye

- Requiring an intraocular lens power outside the available range of +14.0 D to +26.0 D
- Any clinically-significant pupil abnormalities (non-reactive, fixed pupils, or abnormally-shaped pupils)
- Irregular corneal astigmatism
- Inability to focus or fixate for prolonged periods of time (e.g., due to strabismus, nystagmus, etc.)
- Prior corneal refractive (LASIK, LASEK, RK, PRK, etc.) or intraocular surgery. Note: Prophylactic peripheral iridotomies and peripheral laser retinal repairs that, in the opinion of the investigator will not confound study outcome or increase risk to the subject, are acceptable.
- Corneal abnormalities such as stromal, epithelial or endothelial dystrophies that are predicted to cause visual acuity losses to a level worse than 20/30 Snellen during the study
- Inability to achieve keratometric stability for contact lens wearers (per procedure outlined in Section 10.3)
- Recent ocular trauma or ocular surgery that is not resolved/stable or may affect visual outcomes or increase risk to the subject
- Subjects with diagnosed degenerative visual disorders (e.g., macular degeneration or other retinal disorders) that are predicted to cause visual acuity losses to a level worse than 20/30 Snellen during the study
- Subjects with conditions associated with increased risk of zonular rupture, including capsular or zonular abnormalities that may lead to IOL decentration or tilt, such as pseudoexfoliation, trauma, or posterior capsule defects
- Use of systemic or ocular medications that may affect vision
- Prior, current, or anticipated use during the course of the 6-month study of tamsulosin or silodosin (e.g., Flomax, Flomaxtra, Rapaflo) that may, in the opinion of the investigator, confound the outcome or increase the risk to the subject (e.g., poor dilation or a lack of adequate iris structure to perform standard cataract surgery)
- Poorly-controlled diabetes
- Acute, chronic, or uncontrolled systemic or ocular disease or illness that, in the opinion of the investigator, would increase the operative risk or confound the outcome(s) of the study (e.g., immunocompromised, connective tissue disease, suspected glaucoma, glaucomatous changes in the fundus or visual field, ocular inflammation, etc.). Note: controlled ocular hypertension without glaucomatous changes (optic nerve cupping and visual field loss) is acceptable.
- Known ocular disease or pathology that, in the opinion of the investigator,
  - may affect visual acuity
  - may require surgical intervention during the course of the study (macular degeneration, cystoid macular edema, diabetic retinopathy, uncontrolled glaucoma, etc.)

- may be expected to require retinal laser treatment or other surgical intervention during the course of the study (macular degeneration, cystoid macular edema, diabetic retinopathy, etc.)
- Patient is pregnant, plans to become pregnant, is lactating or has another condition associated with the fluctuation of hormones that could lead to refractive changes
- Concurrent participation or participation within 60 days prior to preoperative visit in any other clinical trial
- Desire for monovision correction

## **9. INVESTIGATOR SELECTION**

### **9.1 INVESTIGATOR QUALIFICATIONS**

JJV will select ophthalmic surgeons who have completed a residency in ophthalmology (or its documented equivalent) and are licensed to practice medicine and perform surgery at his/her investigative site. Each site will have one designated principal investigator; some sites may have additional implanting sub-investigators/surgeons.

Investigators will be selected from surgeons who are experienced in small-incision, surgery and have implanted TECNIS Multifocal ZLB00 IOLs in cataract patients. Investigators should have established their personalized A-constant for the TECNIS Multifocal ZLB00 IOL. All sites are required to have adequate staff support for reporting and subject follow-up, as well as the necessary instrumentation to conduct study testing.

### **9.2 INVESTIGATOR OBLIGATIONS**

Investigators are required to fulfill the following obligations:

- Conduct the study in accordance with the relevant and current protocol. Investigator will make changes to a protocol only after notifying and obtaining approval from JJV, the FDA and the Investigational Review Board (IRB), except when necessary to protect the safety, rights or welfare of subjects
- Personally conduct and supervise the study
- Maintain a list of appropriately qualified persons to whom the investigator has delegated significant trial-related duties
- Be responsible for protecting the rights, safety and welfare of subjects under the investigator's care and be responsible for the control and documentation of the devices under investigation
- Inform patients that the device(s) are being used for investigational purposes and that requirements relating to obtaining informed consent and IRB approval are met according to 21CFR50, 21CFR56, 21CFR812 and all other applicable laws and regulations
- Maintain confidentiality as required by HIPAA or similar laws and regulations
- Shall not obtain written informed consent from any subject to participate or allow any subject to participate before obtaining FDA and IRB approval

- Document in each subject's case history that informed consent was obtained prior to participation in the study as required by 21CFR812
- Report to JJV and the reviewing IRB any adverse experiences that occur during the course of the study in accordance with applicable laws and regulations
- Maintain adequate and accurate records in accordance with applicable laws and regulations and make available all study documents and subject medical records for inspection by either JJV, duly authorized regulatory agencies (e.g., FDA, PMDA, Health Canada, MOH, etc.) and/or the IRB
- Submit progress reports on the investigation to JJV and the reviewing IRB at regular intervals, but no less often than yearly as required by 21CFR812.150
- Ensure the IRB that is responsible for initial and continuing review of the study complies with applicable laws and regulations
- Report all changes in research activity and all unanticipated problems involving risks to patients to the IRB and JJV
- Supervise and permit investigational device use and disposition in accordance with applicable regulations and protocol requirements. Upon completion of enrollment or termination of the study or the investigator's part of the study, or at JJV's request, return to JJV any remaining supply of the investigational device
- Provide sufficient accurate financial information to JJV to allow JJV to submit complete and accurate certification or disclosure statements as required by 21CFR54. Promptly update this information if any relevant changes occur during the course of the investigation or for up to one year following completion of the study
- Comply with all other obligations of clinical investigators and requirements according to all applicable FDA regulations (e.g., 21CFR812), all other applicable laws and regulations, and all conditions of approval imposed by the reviewing IRB and the FDA
- Ensure that all associates, colleagues and employees assisting in the conduct of the study are adequately informed about the protocol, the investigational device, their study-related duties and functions and agree to fulfill their obligations in meeting the above commitments.

Investigators shall provide adequate time and resources to conduct and report on the study. The Investigator, or delegate, shall notify JJV of any change in the conduct of the study including changes in study personnel assigned to the study project, location of the investigational device(s), or maintenance of study records, etc.

### **9.3 INVESTIGATOR APPROVAL**

It is the responsibility of the investigator to obtain prospective approval of the study protocol, protocol amendments or changes, informed consent forms and other relevant documents (e.g., advertisements) from the IRB. All correspondence with the IRB should be retained in the Investigator Study Files/Notebook. Copies of IRB submissions and approvals should be forwarded to JJV. Study sites will obtain IRB approvals and fulfill any other site-specific regulatory requirements. The investigator is required to report to

JJV within five working days any withdrawal of approval by the reviewing IRB for his/her participation in the investigation.

Prior to the start of subject enrollment, the following documents must be signed and returned to JJV:

- Confidentiality Agreement
- Clinical Trial Agreement
- Investigator Agreement/Protocol Signature page
- Clinical Investigator Brochure Signature page
- Financial Disclosure form
- Signed and dated copy of investigator's current curriculum vitae
- Copy of the investigator's current medical license
- Hospital/Ambulatory Surgery Center Clinical Study Acknowledgement, if required

By signing the study documents, the investigator agrees to conduct this study according to the obligations above and all other applicable regulatory and legal requirements.

## **10. EXPERIMENTAL PLAN**

### **10.1 OVERVIEW**

This study will be conducted in accordance with U.S. Code of Federal Regulations, the Declaration of Helsinki, ISO 14155:2011 and all other applicable laws and regulations. The study will not begin until regulatory and IRB approvals have been obtained.

This study will be a prospective, multicenter, bilateral, randomized, comparative subject/evaluator-masked clinical investigation conducted at up to 14 sites. Up to 260 subjects will be enrolled to achieve approximately 220 randomized and bilaterally implanted subjects, resulting in approximately 195 evaluable subjects (65 in each test group and 65 in the control group) at 1 and 6 months. After informed consent is obtained and confirmation that all eligibility criteria are met, the eye(s) may be treated.

After signing the informed consent form, subjects meeting all eligibility criteria will be randomized to receive lenses from the same lens group in both eyes, either the investigational Model ZFR00 or Model ZYR00 IOLs, or the Model ZLB00 control IOL. For each subject, the investigator will choose which eye to operate on first at his/her discretion based on his/her standard clinical practice (e.g., the eye with the worse cataract, poorer best corrected distance vision and/or more severe optical/visual complaints). All subjects are intended to have bilateral cataract surgery with the second-eye surgery occurring after the 1-week postoperative exam for the first eye, but no more than 30 days after the first-eye surgery. All subjects will be examined through 6 months postoperatively according to the visit schedule described in Section 10.2, Visit Schedule.



Although the investigators implanting the lenses cannot be masked, subjects and study evaluators responsible for conducting all vision testing will remain masked to which lenses were implanted through the 6-month study visit. Because differences between the investigative and control lenses may be discernible upon slit-lamp examination, special care must be taken to maintain masking of study technicians. As such, it is recommended that only the investigator, sub-investigator or other designated and trained clinician perform all biomicroscopic slit-lamp exams. To maintain consistency, as well as masking, it is recommended that a single individual (study technician or coordinator designated by the investigator) conduct all postoperative study-related vision testing, although a back-up person should also be designated and trained.

Key preoperative data include ocular health and history, visual acuities, manifest refraction, keratometry, topography, biomicroscopic slit-lamp findings, ocular symptoms and biometry. The operative visit will include standard procedures for cataract surgery and IOL implantation. Key postoperative data collection includes monocular and binocular uncorrected and distance corrected visual acuities, contrast sensitivity, defocus curve, slit-lamp findings, non-directed visual symptoms, questionnaires and adverse events. A chart summary of all examination procedures required at each study visit is provided in **Appendix A**. If needed, specific equipment necessary to perform the required procedures will be supplied for the duration of the study (**Appendix B**).

## 10.2 VISIT SCHEDULE

The study visit schedule for all study subjects is outlined in **Table 2**.

All subjects are intended to have bilateral cataract surgery with the second-eye surgery occurring after the 1-week exam for the first eye but no more than 30 days after the first-eye surgery. After each surgery, each eye will be examined 1 day postoperatively (1-2 days) and again at 1 week (7-14 days). Following the second-eye surgery, both eyes will be evaluated at 1 month (30-60 days) and 6 months (120-180 days). Unscheduled visits may be conducted as necessary at the discretion of the investigator for medically-indicated follow-up.

TABLE 2: Visit Schedule

VISIT	EYES EVALUATED	EXAM	VISIT WINDOW
1	Both Eyes	Preoperative Exam	Within 60 days prior to 1 <sup>st</sup> surgery
2	First Eye	Operative	0-60 days after preoperative exam
3	First Eye	1 day	1-2 days postoperative
4	First Eye	1 week <sup>a</sup>	7-14 days postoperative
5	Second Eye	Operative <sup>a</sup>	No more than 30 days after 1 <sup>st</sup> eye surgery
6	Second Eye	1 day	1-2 days postoperative
7	Second Eye	1 week	7-14 days postoperative
8	Both Eyes	1 month <sup>b</sup>	30-60 days postoperative from 2 <sup>nd</sup> implant
9	Both Eyes	6 months <sup>c</sup>	120-180 days postoperative from 2 <sup>nd</sup> implant

<sup>a</sup> The 1-week exam for the first eye is to be completed prior to surgery on the second eye.

<sup>b</sup> If for any reason the second eye does not get implanted, the first eye should be seen for the 1-month study visit 37 - 90 days following the first-eye implant.

<sup>c</sup> If for any reason the second eye does not get implanted, the first eye should be seen for the 6-month study visit 127 - 210 days following the first-eye implant.

### 10.3 PREOPERATIVE PROCEDURES

All subjects treated in the study must sign the current IRB-approved informed consent form and meet the eligibility criteria. The informed consent form must be signed before any study-specific examinations are performed, and this must be documented in the source documents. An Authorization for Use/Disclosure of Health Information Form (HIPAA authorization) or similar medical treatment privacy law documentation must also be signed.

All preoperative testing for the study must be completed within 60 days prior to the first surgery. Data from routine (non-study-specific) preoperative cataract examinations performed prior to the informed consent process may be included, provided these tests are conducted no more than 60 days prior to the first-eye surgery and the test date(s) are documented on the preoperative Case Report Form (CRF). If a test/exam is required by the protocol, but is not part of the routine testing the investigator performs for the cataract evaluation, that test/exam is considered to be study-specific and is not to be done until after the informed consent form has been signed by the subject. Following the informed consent process, completion of the preoperative study exam and determination that the subject meets all of the required entrance criteria (including lens power determination), the subject may be randomized and scheduled for surgery.

As the Informed Consent Form is signed at the beginning of the preoperative study exam, some subjects may not qualify after study-specific testing is performed. Subjects will be considered screen-failures if they do not qualify, or if they qualify but decide not to

participate further in the study, or if they decide not to proceed with surgery. These subjects will be exited from the study.

Preoperative testing to be performed for each eye includes the following:

#### POTENTIAL DISTANCE VISUAL ACUITY

The subject must be capable of achieving Snellen 20/30 or better best corrected distance vision in each eye after cataract extraction and IOL implantation. The surgeon may use his/her judgment, the Potential Acuity Meter (PAM), or other methods (e.g., pinhole, laser interferometer, etc.) to estimate the subject's potential postoperative acuity.

#### UNCORRECTED DISTANCE VISUAL ACUITY

Monocular uncorrected distance visual acuity (UCDVA) is to be measured using a standard Snellen chart or equivalent.

#### BEST CORRECTED DISTANCE VISUAL ACUITY AND MANIFEST REFRACTION

Preoperative manifest refraction is required. Monocular, best corrected distance visual acuity (BCDVA) is to be measured using a standard Snellen chart or equivalent and must be Snellen 20/40 or worse, with or without a glare source.

#### KERATOMETRY AND TOPOGRAPHY

Preoperative corneal astigmatism, as measured by keratometry or topography, should be 1.00 D or less. No irregular astigmatism should be present preoperatively, and topography should be normal.

#### CONTACT LENS WEAR AND CORNEAL STABILITY

For contact lens wearers, keratometric corneal stability following cessation of contact lens wear must be verified before surgery. PMMA contact lenses are not to be worn for at least 6 months; rigid gas-permeable contact lenses are not to be worn for at least 1 month; and extended-wear or daily-wear soft contact lenses are not to be worn for at least 1 week prior to the preoperative visit. Corneal stability must be verified for any subject who has worn PMMA lenses within 5 years or any other type of contact lenses within 6 months prior to the preoperative visit. To verify stability, repeat the keratometric measurements at least 1 week after the initial preoperative baseline keratometric measurement. Corneal curvature is considered to be stable if the difference in keratometric cylinder (vertical vs. horizontal keratometric readings) between the two time points does not exceed 0.50 D. Additionally, the difference between the two horizontal readings as well as the difference between the two vertical readings must be no more than 0.50 D. Changes in keratometric axis must be no more than  $\pm 15^\circ$ . If a change exceeding these criteria is noted, surgery is to be postponed until keratometric stability is

demonstrated. Final biometry measurements and surgery should not take place until keratometric stability is achieved. Note: if this method of determining corneal stability is not a standard procedure in your practice, the subject must sign the informed consent form prior to starting the stability procedure.

#### IOL POWER AND TARGETED REFRACTION

Axial length and anterior chamber depth (ACD) must be measured to determine the appropriate lens power to implant using an A-Constant. IOLMaster, Lenstar or immersion biometry methods are preferred; however, surgeons should use the biometry method with which they have the most experience and which was used in the determination of the personalized A-Constant for the TECNIS Multifocal Model ZLB00 lens. The investigator's personalized A-Constant for the TECNIS Multifocal Model ZLB00 lens will also be used for the investigational TECNIS Models ZFR00 and ZYR00 lenses. The lens power should be calculated to achieve emmetropia at distance. Intentional over- or under-correction (outside  $\pm 0.50$  D) should NOT be planned for either eye; however, surgeons may adjust the targeted refraction as necessary to achieve emmetropia based on surgeon factors, study subject experience and/or subject first-eye outcomes.

#### ADDITIONAL PREOPERATIVE INFORMATION TO BE COLLECTED:

- Informed consent documentation
- Subject demographic information
- Planned surgery dates for each eye
- Ocular history, including presence of ocular pathology for each eye
- Intraocular pressure for each eye
- Cataract type and density for each eye
- Dilated fundus exam results for each eye
- Medical findings from a biomicroscopic slit-lamp exam for each eye
- Ocular symptoms for each eye
- Ocular and systemic medications
- Questionnaire to collect preoperative patient expectations

#### **10.4 RANDOMIZATION AND MASKING**

A randomization list will be created by the JJV biostatistician for each investigative site and the randomization code will be uploaded into the electronic data capture system (EDC). Subjects will be randomized to the investigational Model ZFR00 IOL, the investigational Model ZYR00 IOL or the Model ZLB00 control IOL. Unmasked study personnel at the site will be trained to the randomization process through the EDC system and will randomize subjects after the subject has signed the informed consent form, has met all eligibility criteria and the investigator has documented which eye will be the first implanted.

As part of the informed consent process, the investigator or delegate will explain to the subject the requirements of a randomized study and the differences expected between the three lens models: the Models ZFR00 and ZYR00 investigational lenses and the Model ZLB00 control lens. The surgeon and the operative staff will know which lens type is implanted. There may also be site coordinators and other site study staff, such as those performing slit-lamp exams, who will be unmasked. Unmasked study site staff will be instructed not to disclose the lens type the subject received or to talk about the lens to any masked evaluators or to the study subjects.

The subjects and the study technicians performing the postoperative vision tests are to be masked through study completion. To maintain subject/technician-masking through the 6-month study exams, a masking plan will be tailored for each site to detail how lens assignment information will be concealed from masked technicians. Recommended steps to maintain masking include ensuring that all items pertaining to lens group assignment and lens implantation records are kept separately from all other study documents and subject medical records until after completion of the final study visit. For example, lens stickers (indicating the lens model implanted) may be kept in the operating room study notebook until completion of the final study visit, at which time they may be placed in the subject medical charts. In the meantime, temporary lens stickers (without lens model designations) may be used in the subject's medical chart.

To maintain subject masking, a temporary IOL implant identification card will be issued to the subject at the time of surgery. Following completion of the final study exam, each subject will be given the permanent IOL implant identification card.

#### **10.5 STUDY LENS SUPPLY**

The investigational Model ZFR00 or ZYR00 lenses and the Model ZLB00 control lenses will be obtained from site consignments, supplied by JJV following IRB approval. Two lenses should be available for each case, a primary lens and a back-up lens. Unused back-up lenses are to be returned to the site consignment. At the completion of study enrollment, any remaining consignment lenses will be shipped back to JJV following reconciliation of investigational lens inventory by an JJV CRA. Any remaining control lenses will also be returned to JJV. At all times, the storage, access and use of all investigational lenses must be controlled and complete lens accountability maintained (See Section 15.2.1 Lens Accountability).

#### **10.6 OPERATIVE PROCEDURES**

The investigator should use his or her standard, small-incision, cataract extraction surgical technique. Lenses should be folded for implantation and inserted into the capsular bag using one of the JJV-validated insertion systems described in Section 7.2.

Investigators should manage surgical outcomes to ensure that the total postoperative refractive astigmatism is as minimal as possible. The total postoperative astigmatism, including surgically-induced astigmatism, should be targeted to be no greater than 1.0 D. Astigmatism may be managed by incision type and placement only. **No additional refractive procedures are to be performed during the operative procedure or throughout the postoperative study period (e.g., LRI, OCCI, CRI, AK, PRK, LASIK or LASEK).**

Operative case report forms will include the following information:

#### INCISION TYPE AND SIZE

Lenses should be inserted through an incision ranging in size from approximately 2.2-3.0 mm, per the investigator's standard technique when using the UNFOLDER Platinum 1 Series Implantation System or the ONE SERIES Ultra Implantation System. The incision may be clear corneal, limbal or scleral tunnel at the discretion of the investigator.

#### CAPSULORHEXIS SIZE AND METHOD

The anterior capsulotomy should be a continuous, curvilinear capsulorhexis approximately 5.0 to 5.5 mm in diameter to allow slight overlap of the lens optic edge. The anterior capsulotomy method may be manual (rhexis) or laser-assisted.

#### LENS REMOVAL

Lens removal may occur using laser fragmentation combined with phacoemulsification/aspiration or using only phacoemulsification/aspiration.

#### VISCOELASTIC

Viscoelastic materials should be used as is customary for each investigator and recorded on the case report form (CRF).

#### IMPLANT INSTRUMENTATION USED

Lenses should be folded for implantation and inserted into the capsular bag using either the UNFOLDER Platinum 1 Series Implantation System (DK7796 handpiece with the Platinum 1 Series cartridge, Model 1MTEC30) or the ONE SERIES Ultra Implantation System (DK7786 [plunger] or the DK7791 [twist] handpieces with the ONE SERIES Ultra cartridge, Model 1VIPR30).

#### SURGICAL COMPLICATIONS

Should a surgical complication occur, implantation of a study lens will be at the investigator's discretion. In the event of capsular bag or zonular rupture, the lens should not be implanted if the complication may result in lens instability. Additionally, the lens is

not to be implanted in the sulcus. In this case, the investigator may implant his/her choice of a back-up, non-investigational IOL. The subject should be exited from the study if a non-study lens is implanted as a result of a surgical complication during the first-eye implantation; however, the eye will be followed until resolution of the complication prior to exiting the subject. Should a surgical complication occur during the second-eye surgery and result in implantation of a non-study lens, the subject will not be exited from the study; the first eye will continue to be followed per-protocol, although data may be analyzed separately, and the second eye will be followed for safety until resolution of the complication.

### MEDICATIONS

Preoperative, operative and intraoperative medications should be used as is customary for each investigator and will be recorded on the CRF.

### TYPE OF CLOSURE

Wound closure is left to the surgeon's discretion and will be recorded on the CRF.

### ADDITIONAL OPERATIVE INFORMATION COLLECTED INCLUDES:

- Date of surgery
- Operative eye
- Lens power and serial number
- Lens placement
- Other surgical procedures
- Surgical technique according to protocol
- Product complaints
- Serious and/or device-related adverse events

## **10.7 POSTOPERATIVE PROCEDURES**

Postoperatively, subjects will be examined according to the schedule in Section 10.2, Visit Schedule. Only the most recently operated eye will be evaluated at the 1-day and 1-week visits. Both eyes will be evaluated at the 1-month and 6-month visits.

Study technicians responsible for conducting all vision testing will be masked. Therefore, it is recommended that only the investigator/sub-investigator or other designated and trained clinician perform the biomicroscopic slit-lamp exams. To maintain consistency and masking throughout the study, it is recommended that a single individual (study technician or coordinator designated by the investigator) conduct all postoperative study-related vision testing, although a back-up person should also be designated and trained.

Note: Subjects are not to wear contact lenses postoperatively until after completion of this study. Wearing contact lenses may potentially cause corneal edema or topography changes that may influence the visual acuity results. During the study, if correction is required, spectacles should be prescribed.

A postoperative CRF will collect the following information, although not all data are required at every visit (see **Appendix A**):

#### MANIFEST REFRACTION AND REFRACTION ADJUSTMENTS (MASKED PROCEDURE)

Postoperative study manifest refractions are to be performed using the M&S System at a distance of 4.0 meters. Manifest refraction (MR) is to be performed using the Maximum Plus refraction method as detailed in **Appendix C**.

Because 4.0 meters is not optical infinity, refraction adjustments are necessary to ensure proper vision testing taking into account test distance and refraction distance.

**Appendix D** lists the refraction adjustments required for the various vision tests using the BCDVA refraction.

#### DISTANCE VISUAL ACUITY TESTING (MASKED PROCEDURE)

Distance visual acuity will be measured postoperatively under photopic lighting conditions (85 cd/m<sup>2</sup>, 80–110 cd/m<sup>2</sup> acceptable) using the M&S System at a test distance of 4.0 meters. For eyes unable to achieve a postoperative BCDVA of Snellen 20/40 (i.e., LogMAR 0.3, number of letters correct 70), a reason must be specified. Instructions for using the M&S System are detailed in **Appendix E**, and for distance visual acuity in **Appendix F**.

#### LOW CONTRAST DISTANCE VISUAL ACUITY (10%) (MASKED PROCEDURE)

Low contrast (10% contrast) distance visual acuity will be measured under photopic conditions (85 cd/m<sup>2</sup>, 80-110 cd/m<sup>2</sup> acceptable) using the M&S System at a test distance of 4.0 m. Instructions for low contrast distance testing are detailed in **Appendix F**.



The following distance visual acuity measurements are to be performed per the visit schedule in **Appendix A**:

Test	Test Distance	Illumination	Type of Testing	Refraction Adjustment
UCDVA	4 m	Photopic (85 cd/m <sup>2</sup> )	Monocular Binocular	+0.25 D adjustment only
BCDVA	4 m	Photopic (85 cd/m <sup>2</sup> )	Monocular Binocular	No adjustment; ETDRS Rx only
BCDVA Low Contrast	4 m	Photopic (85 cd/m <sup>2</sup> )	Monocular Binocular	No adjustment; ETDRS Rx only

#### INTERMEDIATE VISUAL ACUITY (MASKED PROCEDURE)

Intermediate visual acuity will be measured under photopic conditions (85 cd/m<sup>2</sup>, 80-110 cd/m<sup>2</sup> acceptable) using the M&S System at a test distance of 66 cm. Instructions for using the M&S System are detailed in **Appendix E** and for intermediate testing in **Appendix G**.

The following intermediate visual acuity measurements are to be performed per the visit schedule in **Appendix A**:

Test	Test Distance	Illumination	Type of Testing	Refraction Adjustment
UCIVA	66 cm	Photopic (85 cd/m <sup>2</sup> )	Monocular Binocular	No adjustment
DCIVA	66 cm	Photopic (85 cd/m <sup>2</sup> )	Monocular Binocular	-0.25 D added to ETDRS sphere Rx

#### NEAR VISUAL ACUITY (MASKED PROCEDURE)

Near visual acuity will be measured under photopic conditions (85 cd/m<sup>2</sup>, 80-110 cd/m<sup>2</sup> acceptable) using the Good-Lite self-calibrating, retro-illuminated box with 100% contrast ETDRS near charts at a test distance of 40 cm.

Instructions for using the ETDRS near chart, including setting appropriate lighting conditions, and the visual acuity conversion chart between the number of ETDRS letters read and Snellen equivalents are provided in **Appendix H**.

The following near visual acuity measurements are to be performed per the visit schedule in **Appendix A**:

Test	Test Distance	Illumination	Type of Testing	Refraction Adjustment
UCNVA	40 cm	Photopic (85 cd/m <sup>2</sup> )	Monocular Binocular	No adjustment
DCNVA	40 cm	Photopic (85 cd/m <sup>2</sup> )	Monocular Binocular	-0.25 D added to ETDRS sphere Rx

#### DEPTH OF FOCUS TESTING (MASKED PROCEDURE)

Monocular, best corrected distance depth of focus testing will be performed at the 1-month visit on the first eye only for all subjects, and binocular best corrected distance depth of focus testing will be performed at the 6-month visit on all subjects.

Depth of focus testing will be performed under photopic conditions (85 cd/m<sup>2</sup>, 80-110 cd/m<sup>2</sup> acceptable) using the M&S System at 4.0 meters with the ETDRS refraction in place (no adjustment necessary for test distance). The subject is to be defocused in -0.50 D increments with spherical minus lenses; at each defocus increment, a LogMAR measurement is obtained. Testing is to be conducted from +2.00 D through -4.00 D of defocus. Further instructions for defocus testing are detailed in **Appendix I**.

The following defocus curve measurements are to be performed per the visit schedule in **Appendix A**:

Test	Test Distance	Illumination	Type of Testing	Refraction Adjustment
Monocular Depth of Focus	4 m	Photopic (85 cd/m <sup>2</sup> )	Monocular	No adjustment; ETDRS Rx only
Binocular Depth of Focus	4 m	Photopic (85 cd/m <sup>2</sup> )	Binocular	No adjustment; ETDRS Rx only

#### PUPIL SIZE

Photopic (without glare), and mesopic with and without glare pupil sizes will be measured postoperatively during the study. For consistency, the same method of measurement should be used throughout the study.

Photopic pupil size measurements are to be performed under the same lighting conditions at which photopic distance visual acuity is tested. Pupil sizes under the other lighting conditions will be measured during the contrast sensitivity testing procedures. Instructions for measuring pupil size are detailed in **Appendix J**.

DISTANCE CONTRAST SENSITIVITY TESTING (MASKED PROCEDURE)

Best corrected distance contrast sensitivity will be tested under mesopic with and without glare and photopic without glare conditions using the M&S System for sine-wave gratings at 1.5, 3.0, 6.0, 12.0 cycles per degree (cpd) (mesopic and mesopic with glare) and 3.0, 6.0, 12.0 and 18.0 cpd (photopic without glare). **The test distance is 8 feet (2.5 meters).** Best corrected distance contrast sensitivity is to be performed with a +0.12 D refractive adjustment to the sphere of the manifest refraction. Detailed instructions for contrast sensitivity testing are provided in **Appendix K**.

The following contrast sensitivity measurements are to be performed per the visit schedule in **Appendix A**:

<b>Contrast Sensitivity Test</b>	<b>Test Distance</b>	<b>Spatial Frequency</b>	<b>Type of Testing</b>	<b>Refraction Adjustment</b>
Photopic (85 cd/m <sup>2</sup> ) without glare	2.5 m	3, 6, 12 and 18 cpd	Monocular Binocular	+0.12 D added to ETDRS sphere Rx
Mesopic (3 cd/m <sup>2</sup> ) without glare	2.5 m	1.5, 3, 6 and 12 cpd	Monocular Binocular	+0.12 D added to ETDRS sphere Rx
Mesopic (3 cd/m <sup>2</sup> ) with glare	2.5 m	1.5, 3, 6 and 12 cpd	Monocular Binocular	+0.12 D added to ETDRS sphere Rx

BIOMICROSCOPIC SLIT-LAMP EXAM

A biomicroscopic slit-lamp exam must be performed at each postoperative visit to determine the presence or absence of any medical or lens findings, complications or adverse events. IOL decentration and tilt are to be determined subjectively. The center of the lens relative to the pupil can be used to determine IOL decentration, with the diffractive rings used as a guide to locate the center of the IOL. Note that the pupil center may not always be aligned with the visual axis of the eye; therefore, the investigator should consider deviations in pupil center from visual axis when reporting IOL decentration.

Findings of aqueous cells and flare, corneal edema, posterior capsule striae (wrinkles), posterior capsular opacification and IOL glistenings are to be rated using standardized grading scales of 0 to +4 (0 = none, +4 = severe) during the slit-lamp biomicroscopy. The specific grading scales are provided in **Appendix L**.

ND:YAG CAPSULOTOMY

If an Nd:YAG capsulotomy is necessary, it is recommended that the procedure be performed at least 1 week prior to a study exam; this is particularly important for the

6-month study visit, as this is the key study exam for evaluation of safety and effectiveness.

#### DILATED FUNDUS EXAM

A dilated fundus exam is to be performed at the 6-month visit to evaluate retinal status and fundus visualization.

#### INTRAOCULAR PRESSURE

Intraocular pressure (IOP) is to be measured using the investigator's usual method. It is recommended that the same method be used for all study subjects at the site for the duration of the study.

#### OCULAR SYMPTOMS (NON-DIRECTED; SPONTANEOUS)

Subjective ocular symptoms are to be assessed at each postoperative visit by asking "Are you having any difficulties with your eyes/vision?" Subjects should not be prompted for specific responses; however, if a subject reports halos, night glare or starbursts, the level of severity should be determined (mild, moderate or severe).

#### MEDICATIONS

Postoperative ocular medications should be used as is customary for each investigator and recorded in the source document for each subject. Medications will be recorded on a medication log CRF as applicable.

#### ADVERSE EVENTS

Subjects should be assessed at each visit for occurrence of and/or change in status of any adverse events, particularly serious and/or device-related adverse events. See Section 11.0, Adverse Events, for further information.

#### QUESTIONNAIRES

Questionnaires will be administered at the 1-month and 6-month visits to collect information regarding spectacle usage, visual symptoms, visual quality and subject satisfaction. In order to minimize any effect the doctor-patient relationship may have on a subject's responses on the questionnaire, the study questionnaires will be self-administered by the subjects. The questionnaires are to be administered at the start of the 1-month and 6-month study visits, prior to any visual acuity testing.

In addition, if a subject is seen after the 1-month postoperative visit for an unscheduled visit due to an optical/visual symptom complaint, the PRO Visual Symptoms Questionnaire (PRVSQ) will be administered at that visit, as well as prior to any secondary surgical intervention for an optical/visual symptom complaint. If additional unscheduled visits and/or a secondary surgical intervention due to the same

optical/visual symptom complaint occur within 2 weeks of each other, it is not necessary to complete the PRO Visual Symptoms Questionnaire a second time.

The optical visual symptom complaints that trigger the PRO Visual Symptoms Questionnaire include any of the seven symptoms from the PRVSQ: halos, glare, starbursts, sensitivity to light, streaks of light, occlusions, or poor light vision.

If the subject indicates in the PRO Visual Symptoms Questionnaire that s/he has visual symptoms or other problems with their vision that are bothersome enough to want the lenses removed and replaced, the investigator will document a determination for whether or not, in their opinion, the problem is related to the optical properties of the lens.

## **10.8 EXIT OF SUBJECTS**

An Exit CRF will be completed for all subjects, either when they complete the study or if they exit early.

It is the responsibility of the investigator to provide complete follow-up data to JJV for each subject, and every attempt should be made to gather that complete follow-up data for all subjects enrolled, as missing data can have a negative effect on the study results. Patients who would be traveling, relocating or otherwise unavailable for postoperative follow-up visits should not be enrolled in this clinical study.

A subject will be considered a "screen failure" if he/she does not meet the eligibility criteria or if consent is withdrawn prior to randomization.

A subject will be considered "discontinued prior to treatment" if the subject is randomized but does not undergo surgery or receive a study lens for various reasons including: the planned implant being aborted due to surgical complications, the subject withdrawing consent prior to treatment or the subject died prior to treatment.

Subjects will be "discontinued" from the study if one study lens (if implanted unilaterally) or both study lenses (if implanted bilaterally) are removed or if the subject dies.

If a subject receives at least one study lens, he/she is to be followed according to the schedule in Table 2 (Section 10.2) for visit windows.

Subjects will be considered "lost-to-follow-up" from the study only if irretrievably lost for unavoidable reasons such as: subject moved/unable to locate, subject ill/unable to travel, subject uncooperative/refuses further study participation. In the event of subject relocation, effort must be made by the investigator to secure follow-up information (i.e., slit-lamp findings and general visual acuity, etc.) from the subject's new physician.

If a subject is exited early from the study, the investigator must indicate the reason for study exit on the CRF. In the event of a lens removal or other serious adverse event, the subject may be exited from the study; however, effort must be made by the investigator to follow the subject until resolution of the adverse event before exiting the subject from the study.

Following study completion or early exit, subjects will be informed about which lens model they received. Additionally, all study subjects are to be instructed to undergo regular eye examinations at least yearly and also to return to their doctor if any eye complications are experienced.

### **10.9 UNSCHEDULED VISITS**

During the study period, if a non-protocol-required visit is done for the purpose of medically-indicated follow-up for a study eye, data from this visit should be reported using the Unscheduled Visit CRF. The need for unscheduled visits is at the investigator's discretion. Specific examinations to be performed at unscheduled visits are also at the discretion of the investigator (based on the reason for the unscheduled visit) and data are to be recorded in the appropriate section of the CRF.

Data to be collected may include:

- Snellen manifest refraction
- Uncorrected and best corrected distance visual acuity using a Snellen chart
- Intraocular pressure
- Slit-lamp examination for medical and/or lens findings
- Dilated fundus exam
- Ocular symptoms
- Adverse events
- Medications

If, prior to the second-eye surgery, the fellow eye is re-examined (e.g., at a first-eye, 1-day visit) and there are clinically significant changes from the preoperative exam, data is to reported using the Unscheduled Visit CRF. If there are no changes or non-clinically significant changes from the original preoperative exam, an Unscheduled Visit CRF is not required.

If the first eye is examined at a second-eye visit (e.g., 1 day or 1 week) and there are medical and/or lens findings, and/or a subject has an optical/visual symptom complaint, data are to be reported using the Unscheduled Visit CRF.

Conditions found postoperatively, but previously documented at the preoperative visit, do not trigger an unscheduled visit report. However, if the severity of the condition increases from the preoperative visit, an Unscheduled Visit CRF is needed.

In addition, if a subject is seen after the 1-month postoperative visit for an unscheduled visit due to an optical/visual symptom complaint, the PRO Visual Symptoms Questionnaire must be administered at that visit, as well as prior to any secondary surgical intervention for an optical/visual symptom complaint. If additional unscheduled visits and/or a secondary surgical intervention due to the same optical/visual symptom complaint occur within 2 weeks of each other, it is not necessary to complete the PRO Visual Symptoms Questionnaire a second time.

The optical visual symptom complaints that trigger the PRO Visual Symptoms Questionnaire include any of the seven symptoms from the PRVSQ: halos, glare, starbursts, sensitivity to light, streaks of light, occlusions, or poor light vision.

## 10.10 PROTOCOL DEVIATIONS

Any departure from the protocol procedures represents a protocol deviation. Protocol deviations may be subject-based (e.g., inclusion/exclusion criteria, informed consent deviation, etc.) or procedural-based (e.g., out-of-interval visits, non-compliance with testing procedures, etc.). All protocol deviations will be documented using the protocol deviation CRF. Any deviation made to protect the life or physical well-being of a subject in an emergency as well as any use of the investigational device without obtaining informed consent must be reported to JJV within 5 working days. Protocol deviations will be monitored by JJV, and if the non-compliance is persistent or egregious, JJV may take action, including but not limited to termination of the investigator's participation in the study. The investigator is also responsible for informing the reviewing IRB of instances of protocol non-compliance in accordance with the IRB requirements.

## 11. ADVERSE EVENTS AND PRODUCT COMPLAINTS

### 11.1 ADVERSE EVENT DEFINITIONS

#### Adverse Event (AE)

An adverse event is defined (following ISO 14155) as any untoward medical occurrence, unintended disease or injury, or untoward clinical signs (including abnormal laboratory findings) in subjects, users or other persons, whether or not related to the study device.

#### Serious Adverse Event (SAE)

An adverse event is considered serious (following ISO 14155) if it is an untoward occurrence which may or may not be related to use of the study device that

- is sight- or life-threatening,
- results in death,
- requires inpatient hospitalization or prolongation of hospitalization (a planned hospitalization for a pre-existing condition without a serious deterioration in health is not considered a serious adverse event),

- results in permanent impairment of a body structure or body function,
- necessitates medical or surgical intervention to prevent permanent impairment to a body structure or function, or
- results in fetal distress, fetal death or a congenital abnormality or birth defect

### **Device-Related Adverse Event/Adverse Device Effect (ADE)**

A device-related adverse event is defined as any adverse event that is believed to be definitely, probably or possibly related to the study device (following the guidelines in Section 11.4, Causal Relationship). A device-related event is also considered an adverse device effect (ADE; following ISO 14155) resulting from the use of the study device that may result from user error, insufficiencies or inadequacies in the instructions for use, deployment, implantation, installation, operation of any malfunction of the device.

### **Study-Specific Serious Anticipated Adverse Events**

The following is a list including, but not limited to, ocular serious adverse events (SAE) that are anticipated and must be reported to JJV for this study. Any events that are unlikely but anticipated (i.e., endophthalmitis) will be reported to the FDA and other appropriate regulatory agencies.

- Endophthalmitis/Intraocular infection
- Hypopyon
- Hyphema
- IOL dislocation
- Cystoid macular edema
- Pupillary block
- Retinal detachment/tear
- Persistent corneal edema
- Persistent iritis
- Persistent uveitis
- Persistent raised IOP requiring treatment
- Toxic anterior segment syndrome
- Visual symptoms requiring secondary surgical intervention (e.g., lens removal)
- Tilt and decentration requiring secondary surgical intervention (e.g., repositioning)
- Residual refractive error resulting in a secondary surgical intervention
- Retained lens material resulting in secondary surgical intervention

**NOTE 1:** Wound burps during the first week postoperatively, suture removal, planned blepharoplasty and Nd:YAG capsulotomy (for PCO) are not considered adverse events for this study.



**NOTE 2:** Raised IOP requiring treatment, corneal edema, and iritis will only be considered serious if persistent at the final study visit (120-180 days postoperative) or sight-threatening at the time of occurrence. Treatment merely to hasten the resolution of such conditions (and not intended to prevent permanent damage to the eye) will not be reported as serious adverse events.

### **Unanticipated Adverse Device Effect (UADE)/Unanticipated Serious Adverse Device Effect (USADE)**

Any UADE (USA 21CFR 812.3(s)) or USADE (ISO 14155) is defined as any serious adverse effect on health or safety or any life-threatening problem or death caused by, or associated with, a device, if that effect, problem, or death was not previously identified in nature, severity, or degree of incidence in the investigational plan (i.e., this protocol), application (including a supplementary plan or application), or risk assessment, or any other unanticipated serious problem associated with a device that relates to the rights, safety, or welfare of subjects.

### **11.2 PRODUCT COMPLAINT/DEVICE DEFICIENCY DEFINITION**

A product complaint/device deficiency is defined (21 CFR 820.3(b) and ISO 14155) as any alleged deficiency related to the identity, quality, durability, reliability, safety, effectiveness, or performance of a device. This may include malfunctions, use error and inadequacies in labeling. Product complaints can pertain to any marketed JJV device being used in the study as well as the investigational device. The investigator is to assess whether the deficiency could have led to a serious adverse event without suitable action or intervention or under less fortunate circumstances.

### **11.3 ADVERSE EVENT AND COMPLAINT REPORTING REQUIREMENTS**

All adverse events and any complaint encountered using any JJV product, regardless of severity and whether or not attributed to the study device(s), are to be reported to JJV and recorded on the case report form corresponding to the visit during which awareness of the event occurred. Adverse events are also to be reported to the reviewing IRB as per the IRB's reporting requirements. If required, adverse events will be reported to the appropriate regulatory agencies (e.g., FDA) according to all applicable laws and regulations.

Reporting of adverse events shall follow the USA Code of Federal Regulations (21CFR812) for sites in the USA. General guidelines are provided below:

#### **Adverse Event Reporting**

An adverse event that is not serious or device-related is to be reported to JJV in a timely manner. Notification of non-serious and non-device related adverse events will occur by

recording events on the CRF when noted. Such adverse events are also to be reported to the reviewing IRB per their reporting requirements.

### **Complaints/Device Deficiency Reporting**

A general product complaint or device deficiency is to be reported to JJV in a timely manner. Notification of complaints/device deficiencies will occur by recording complaints on the CRF at the visit the complaint occurs (e.g., operative visit) and/or by a phone call to JJV.

Any device deficiency that could have led to a serious adverse event without suitable action or intervention, or under less fortunate circumstances, must be reported to the sponsor immediately (no later than 24 hours after detection). Device deficiencies that could have led to a serious adverse event should also be reported to the investigator's IRB per their reporting requirements.

### **Serious and/or Device-Related Adverse Event Reporting**

SAEs and/or ADEs are to be documented using the Serious Adverse Event/Adverse Device Effect (SAE/ADE) CRF. In the event of an SAE, JJV must be notified immediately (no later than 24 hours after detection). Any SAE/ADE is to be reported to JJV by phone, email and/or by submitting the completed SAE/ADE CRF. Any SAE or device-related AE should also be reported to the investigator's IRB per their reporting requirements.

### **Unanticipated Adverse Device Effect (UADE)/Unanticipated Serious Adverse Device Effect (USADE) Reporting**

If during the study, a serious adverse event occurs that may reasonably be regarded as device-related and was not previously expected in nature, severity, or degree of incidence, the investigator is to report the UADE/USADE to JJV within 24 hours, and to the investigator's IRB as soon as possible (and no later than 10 working days after learning of the event for sites in the USA as required by 21CFR812).

## **11.4 CAUSAL RELATIONSHIP**

The investigator should always be alert to adverse events that may be related to the study device or the use of the study device (i.e., the procedure specific to the initial application of the device). An attempt should be made in every case to determine the causality of the event. The following definitions are to be used as guidelines in determining the relationship between the event and the study device and/or use of the device.

Definitely related: If the event is associated with the device and/or the use of the device beyond a reasonable doubt, a causal relationship exists

- between the adverse event and the device and/or the use of the study device.
- Probably related: There is a reasonable possibility of a causal relationship between the adverse event and the device and/or the use of the study device and/or the adverse event cannot be reasonably explained by another cause.
- Possibly related: The adverse event has not been determined to be related to the device or the use of the device, but no other cause has been identified and the device and/or the use of the study device cannot be ruled out as a possible cause.
- Unlikely to be related: The possibility of a potential causal relationship between adverse event and the device and/or the use of the device could exist, but the adverse event can be reasonably explained by another cause.
- Not related: There is no possibility of a causal relationship between the adverse event and the device and/or the use of the study device and/or the adverse event can be attributed to another cause.

If an adverse event is believed to be definitely, probably or possibly related to the study device and/or the use of the device, the event will be considered related to the study device and/or the use of the device.

### **11.5 ADVERSE EVENT FOLLOW-UP**

For every adverse event, appropriate measures should be undertaken to treat and/or monitor the subject until resolution occurs. The subject's files are to include all pertinent medical data relating to the event including the subject's medical records, medical reports and/or judgments from colleagues or outside specialists who assisted in the treatment and follow-up of the subject. The investigator should keep JJV closely informed as to the outcome of serious and/or device-related adverse events, thereby allowing JJV to comply with the appropriate regulatory reporting requirements. An SAE/ADE CRF should be completed each time the subject returns to the investigator or other specialist(s) for follow-up of a serious and/or device-related adverse event until resolution of the event. Any subject who is to be exited from the study due to a serious and/or device-related adverse event should be followed until the outcome is determined prior to being exited from the study.

## **12. PROTOCOL CHANGES/AMENDMENTS**

If the investigator wishes to modify any procedure and/or the design of the study, he or she must contact and obtain consent from JJV regarding the proposed changes prior to implementation. Any modifications (including additional data collection) require approval

by the FDA and all other appropriate regulatory agencies, as well as approval of the governing IRBs prior to implementation.

### **13. ETHICS REVIEW AND PATIENT WELFARE**

#### **13.1 INSTITUTIONAL REVIEW BOARD (IRB)**

It is the responsibility of the investigator to obtain prospective approval of the study protocol, protocol amendments or changes, informed consent forms and other relevant documents (e.g., advertisements) from the IRB. All correspondence with the IRB should be retained in the Investigator Notebook. Copies of IRB submissions and approvals should be forwarded to JJV.

The investigator is responsible for notifying the IRB of reportable adverse events as well as any other circumstance in which additional procedures outside the protocol were conducted to eliminate apparent hazards to subjects.

#### **13.2 INFORMED CONSENT**

The current version of the IRB-approved study informed consent form must be signed by each study subject prior to any study-specific examinations being performed. The IRB-approved informed consent form is to be signed and dated by the subject as well as by the person who conducted the informed consent discussion. The signed informed consent form will be maintained by the investigator as a permanent part of the subject's medical records. A copy of the signed and dated form is to be provided to the subject. The investigator will provide JJV written acknowledgement on the preoperative case report form that a signed agreement of informed consent has been obtained and is in the investigator's possession for each subject. As required by 21CFR812 Part G, the site shall document in the source documents that informed consent was obtained prior to participation in the study for each subject enrolled.

NOTE: The informed consent process also includes obtaining the subject's signature on an Authorization for Use/Disclosure of Health Information for Research Form or equivalent documentation necessary to comply with applicable privacy laws pertaining to medical treatment in the governing countries.

NOTE: The sponsor will secure appropriate insurance for study subjects prior to study start.

### **14. DOCUMENTATION**

#### **14.1 SOURCE DOCUMENTS**

Source documents must be kept for all study subjects. Source documents may include a subject's medical records, hospital charts, clinic charts, the investigator's subject study

files, as well as results of any diagnostic tests or procedures such as topographies or laboratory tests with photographs or instrument printouts.

Each site is expected to adhere to the clinic's own standard documentation requirements for medical charts/clinic notes. For the purposes of this clinical study, the medical charts/clinic notes must also include, at a minimum, the following data that will be considered source data and will be reviewed by JJV:

- Subject's name and study identification number
- Subject's contact information
- Study protocol number and the Sponsor name (JJV)
- A statement that informed consent was obtained prior to participation in the study (including the date)
- Evidence of subject eligibility
- Dates of all subject visits and surgeries throughout the duration of the study
- Implant serial number identification (NOTE: This is masked information, and may only be reviewed by unmasked study staff)
- Concurrent medications
- Corrected and uncorrected distance visual acuity (NOTE: M&S electronic data and near visual acuity score sheets are considered source documentation and are to be retained by the site. A paper copy of the M&S results will be printed and validated by the site)
- Manifest refraction
- Occurrence and status of any operative complications, postoperative medical or lens findings and adverse events
- Occurrence and status of any subject complaints, e.g., ocular/visual symptoms
- The date the subject exited the study, and a notation as to whether the subject completed the study or reason for early exit.

#### **14.2 SUBJECT CONFIDENTIALITY**

Subjects will be assigned a site/subject number to maintain subject confidentiality. Subject names may possibly be disclosed to JJV or regulatory agencies during inspection of medical records related to the study, but reasonable precautions will be taken to maintain confidentiality of personal information to the extent permitted by applicable laws and regulations.

#### **14.3 CASE REPORT FORM COMPLETION**

This study will use an electronic data capture system. All study staff responsible for entering data into the system must complete certification prior to using the system. The investigator is responsible for ensuring that data are properly recorded on each subject's case report forms and related documents. Prior to database lock, the investigator will verify completeness and accuracy of data submitted to JJV.

#### **14.4 STUDY SUMMARY**

A final investigator's summary (study close-out) will be provided to JJV and the reviewing IRB after termination or the completion of the study or the investigator's part of the investigation, as directed by JJV.

### **15. MONITORING**

JJV will perform three types of monitoring to ensure compliance with regulations: data monitoring, administrative monitoring, and safety monitoring.

#### **15.1 DATA MONITORING**

In order to ensure a well-controlled clinical trial, JJV will follow specific data monitoring procedures, routinely generate reports and periodically review safety and effectiveness data. To avoid bias, any analyses generated prior to site closures will not be disseminated to any of the investigative sites.

An electronic data capture system (EDC) will be used to transmit case report forms from the investigative site to JJV. Requests for data clarification will be handled through this same system.

To minimize data omissions and inconsistencies on clinical reports and to ensure that data are accurately transcribed to computer data files, JJV will follow internal data processing procedures that include automated and manual quality control checks to identify any data discrepancies. Any such items will be resolved and documented as needed in EDC.

#### **Prevention of Missing Data**

Methods used to safeguard against missing data that can have deleterious effects on the study integrity and reliability of its outcomes will include training study staff with WebEx, centralized and/or on-site programs. In addition, subjects will be encouraged at the time of informed consent to avoid missing study visits, as missing data may affect the study reliability and diminish the scientific value of their contribution to the study.

#### **15.2 ADMINISTRATIVE MONITORING**

Administrative monitoring procedures will ensure that study devices, subjects, and forms can be traced and will allow monitoring of investigator progress and compliance. Accountability and traceability of study devices will be monitored by trained JJV personnel.

#### **Device Accountability**

Complete lens accountability will be maintained at the investigative site by maintaining records of all investigational lenses (Models ZFR00 and ZYR00 lenses) received from

and returned to JJV. A site log will be used to track all lenses for date of receipt, eye implanted, serial number, lens power, use and disposition/return to JJV. This site log and any other investigational lens information will be maintained in the operative room study binder. During periodic investigative site monitoring visits, JJV personnel will review investigative site lens inventory records and logs to ensure IOL accountability compliance and complete investigational lens traceability.

### **Site Monitoring Plan**

Prior to performing any study implants, the requirements of the study and reporting mechanisms will be explained to each investigator either personally at the investigative site or at a formal study investigator meeting. When necessary, a pre-study site qualification visit may be performed to assess the adequacy of the site to perform the study for sites that have not previously worked with JJV or have undergone significant changes, or have not been visited in the past year. A study initiation visit will be conducted for all sites prior to the first implant.

Throughout the duration of the study, site visits to monitor compliance to this protocol will be made at each investigative site. During interim site monitoring visits, JJV will review informed consent documents and subject eligibility, and the data on study case report forms will be verified against subject charts and other source documents to ensure complete and accurate reporting. The subject files will also be reviewed to assure that all adverse events and any issues encountered with JJV products have been reported in a timely fashion.

JJV will also review source documents to verify that all required items have been documented in the subject medical charts. Refer to Section 14.1, Source Documents, for a list of items that are required for source documentation. In addition to subject files, study logs will be checked and conformance to lighting levels for visual acuity tests will be verified.

Training on study-specific procedures may also be conducted during monitoring visits. For this study in particular, a training/monitoring visit is likely to occur just prior to or during the first of the 1-month and 6-month visits, wherein the most extensive vision testing occurs.

Upon study completion, a final close-out site visit to each site will be made to monitor the last of the subject data records and finalize any outstanding study issues.

A separate Study Monitoring Plan will be established prior to study start that will define the type and frequency of monitoring visits and frequency of record monitoring.

### 15.3 SAFETY MONITORING

The medical monitor will review results throughout the clinical trial as necessary to ensure the continued safety of the device and to ensure that no subjects are exposed to unreasonable risk. The medical monitor will be available to answer all questions from investigators. The medical monitor will review and assess any reports of serious and/or device-related adverse events as well as device deficiencies that could have led to a serious adverse event, and discuss these with the reporting investigator(s) as necessary. The medical monitor, as well as any other qualified personnel designated by JJV, shall also review any interim progress reports, as applicable.

### 16. PUBLICATIONS

Refer to the Clinical Trial Agreement for information regarding JJV publication policies.

### 17. RISK ANALYSIS

#### POTENTIAL RISKS AND RISK MANAGEMENT

##### *RISKS OF THE TECNIS NEXT-GENERATION IOLS, MODELS ZFR00 AND ZYR00*

The TECNIS Models ZFR00 and ZYR00 IOLs are designed to provide far, intermediate and near vision; however, glasses may still be needed to improve distance vision and/or to have useful vision for intermediate or near tasks. Visual symptoms, particularly dysphotopsias such as halos, night glare, starbursts, etc., are expected to be comparable to or less than with a standard multifocal IOL. Dysphotopsias may become less noticeable over time; however, the IOL may be removed if necessary. There may be a reduction in contrast sensitivity under certain conditions compared to a monofocal lens although contrast sensitivity is expected to be in between that of the TECNIS Symphony IOL and TECNIS Multifocal IOLs. Due to the diffractive optic design, the ability to perform some eye treatments (e.g., retinal photocoagulation) may be affected, and caution should be used when interpreting results of autorefractors or wavefront aberrometers that utilize infrared light, or when performing a duochrome test. These risks are not unlike other diffractive technology IOLs.

##### *GENERAL RISKS OF CATARACT SURGERY AND IOL IMPLANTATION*

There are risks and complications associated with cataract surgery and IOL implantation in general. These can include worsening of vision, hemorrhage, loss of corneal clarity, inflammation, infections, retinal detachment, pupil changes, glaucoma, etc. Complications can result in poor vision, loss of vision or loss of the eye.

##### *RISK MANAGEMENT*

Subjects will be closely monitored throughout the trial duration. The occurrence of adverse events and complaints will be assessed at each study visit and reported to JJV



according to Section 11.0, Adverse Events and Product Complaints. Additionally, JJV will monitor incoming data following the procedures outlined in Section 15.0, Monitoring. The Medical Monitor will ensure subjects are not exposed to additional risks by monitoring serious adverse events, device-related adverse events, and device-deficiencies that could have led to serious adverse events (Section 15.3, Safety Monitoring).

### POTENTIAL BENEFITS

The general clinical performance of the TECNIS Next-Generation IOLs, Models ZFR00 and ZYR00, are expected to be similar to the TECNIS Model ZLB00 control IOL regarding distance and near visual acuities and safety outcomes. Improved intermediate visual acuity and functionality may be achieved with the TECNIS Next-Generation IOLs, Models ZFR00 and ZYR00 with comparable or less levels of dysphotopsia as compared to the control IOL.

### CONCLUSION

The hazards/risks associated with the TECNIS Next-Generation IOLs, Models ZFR00 and ZYR00, are acceptable and within those of JJV's other advanced optic IOLs. The potential clinical benefits of the TECNIS Next-Generation IOLs, Models ZFR00 and ZYR00, outweigh the residual risks when the device is used as intended.

## **18. RECORDS RETENTION**

All study-related correspondence, subject records, consent forms, Authorization for Use/Disclosure of Health Information Forms or similar medical treatment privacy law documentation, records of the distribution and use of all study products, and original case report forms should be maintained by the investigator.

The investigator must maintain and have access to the following essential documents until notified by the Sponsor. Note: This may be for a minimum of 25 years after completion of the study. JJV requires notification if the investigator wishes to relinquish ownership of the data so that mutually agreed-upon arrangements can be made for transfer of ownership to a suitably-qualified, responsible person.

- All case report forms
- All adverse event information (i.e., medical records, medical reports and/or judgments from colleagues or outside specialists who assisted in the treatment and follow-up of the subject)
- Investigational supply records/inventory
- IRB approval documentation
- Study correspondence
- Study agreements

- Site visit documentation
- Protocol(s)
- Subject log(s)
- Clinical Investigator's Brochure
- Completed subject informed consent forms and medical privacy forms (e.g., Authorization for Use/Disclosure of Health information)
- Subject medical chart/clinic notes (Not applicable for transfer of ownership to JJV)

## **19. TERMINATION OF THE INVESTIGATION**

The clinical investigation will be suspended in the event of high levels of complications and/or adverse events that are unexpected in nature and/or severity and evaluated as to causality relative to the study device. The clinical investigation may be suspended if the Medical Monitor or the IRB, upon review and evaluation of the clinical data, finds unacceptable clinical performance or the level of single or total complications and/or adverse events unacceptable for continuation of the investigation.

If causality is shown not to be related to the study device, the study may be resumed in accordance with the IRB and regulations of the FDA. The study will be terminated if causality is shown to be related to the study device.

Additionally, the investigator or JJV may stop a subject's participation at any time. JJV may also stop the study at any time for reasons it determines appropriate. However, no suspension of the study would be made to disadvantage the study subjects. Following suspension of the study for any reason, all study subjects who have already received treatment would continue to be followed through completion of the study visit schedule.

## **20. STATISTICAL METHODS**

This section highlights the analyses to be performed for key study endpoints. The key study timeframe for all endpoints will be the 1-month postoperative visit, although data will be reviewed at other time points as well. TECNIS Models ZFR00 and ZYR00 will both be compared to the TECNIS Model ZLB00 control separately for all analyses. All data will be reported by IOL group.

### **20.1 ANALYSIS POPULATION**

The safety population (SP) of all subjects implanted who have available data will be used for all analysis. No data imputation will be performed for missing data. For the monocular endpoints, the safety population will consist of first eyes implanted with a study IOL; for binocular endpoints, the safety population will consist of subjects implanted with the same IOL in both eyes. The primary analysis population will be the

safety population (SP) for all endpoints. Second eye data will only be reported for monocular safety endpoints as supportive data.

## 20.2 PRIMARY STUDY ENDPOINTS

### Primary Effectiveness Endpoints

#### MODEL ZFR00: MONOCULAR DISTANCE CORRECTED INTERMEDIATE VISUAL ACUITY (DCIVA) AT 66 CM

The primary effectiveness endpoint for the Model ZFR00 IOL is mean (LogMAR), photopic, monocular, first-eye, distance corrected intermediate visual acuity (66 cm) at 1 month postoperative. The mean, SD, median, minimum, maximum and 95% C.I. will be reported by IOL group. Results will be reported by lens group for first eyes using one-sided, two-sample t-tests with an alpha level of 0.025. Note that a lower LogMAR value is a better acuity and a higher LogMAR value is a poorer acuity. The null hypothesis is that the mean monocular DCIVA LogMAR value for the Model ZFR00 eyes is worse than or equal to that for control eyes. The alternate hypothesis is that the mean monocular DCIVA LogMAR value for Model ZFR00 eyes is better than that for control eyes.

$$H_0: \mu_c - \mu_t \leq 0 \text{ (Model ZFR00 lens is worse than (higher LogMAR) or equal to control)}$$

$$H_1: \mu_c - \mu_t > 0 \text{ (Model ZFR00 lens is better (lower LogMAR) than control)}$$

where

$\mu_t$  = mean LogMAR DCIVA for the Model ZFR00 lens

$\mu_c$  = mean LogMAR DCIVA for control lens

Reject the null hypothesis if one-sided p-value  $\leq 0.025$ .

The success criterion is a statistically significantly lower mean LogMAR value for the Model ZFR00 investigational lens compared to the control lens ( $p \leq 0.025$ ).

#### MODEL ZYR00: MONOCULAR DISTANCE CORRECTED INTERMEDIATE VISUAL ACUITY (DCIVA) AT 66 CM

The primary effectiveness endpoint for the Model ZYR00 IOL is mean (LogMAR), photopic, monocular, first-eye, distance corrected intermediate visual acuity (66 cm) at 1 month postoperative. Analysis for the Model ZYR00 will be similar to the Model ZHR00 described above. Results will be reported by lens group for first eyes using one-sided, two-sample t-tests with an alpha level of 0.025. Note that a lower LogMAR value is a better acuity and a higher LogMAR value is a poorer acuity. The null hypothesis is that the mean monocular DCIVA LogMAR value for the Model ZYR00 eyes is worse than or equal to that for control eyes. The alternate hypothesis is that the mean monocular DCIVA LogMAR value for Model ZYR00 eyes is better than that for control eyes.

$H_0: \mu_c - \mu_t \leq 0$  (Model ZYR00 lens is worse than (higher LogMAR) or equal to control)  
 $H_1: \mu_c - \mu_t > 0$  (Model ZYR00 lens is better (lower LogMAR) than control)

where

$\mu_t$  = mean LogMAR DCIVA for the Model ZYR00 lens

$\mu_c$  = mean LogMAR DCIVA for control lens

Reject the null hypothesis if one-sided p-value  $\leq 0.025$ .

The success criterion is a statistically significantly lower mean LogMAR value for the Model ZYR00 compared to the control lens ( $p \leq 0.025$ ).

### **Primary Safety Endpoints**

#### **MODEL ZFR00: RATES OF ADVERSE EVENTS VS. ISO SPE RATES**

The primary Model ZFR00 safety endpoint for this study is the rate of adverse events vs. ISO SPE rates at 1 month postoperative. The frequency and proportion of first eyes and second eyes with these events will be reported over time by IOL group. Statistical comparisons to ISO SPE rates will be based on first-eye data; adverse event rates for the Model ZFR00 investigational lens first eyes will be compared to the ISO SPE rates using a one-sided, exact test based on the binomial distribution. The null hypothesis is that the AE rate for the Model ZFR00 investigational lens eyes is lower than or equal to the ISO SPE values, and the alternative hypothesis is that the AE rate for study eyes is higher than the ISO SPE values.

$H_0: p_t \leq p_i$

$H_1: p_t > p_i$

where

$p_t$  = proportion of Model ZFR00 investigational lens eyes with the AE

$p_i$  = proportion of eyes reported in ISO SPE rates with the AE

Reject the null hypothesis if one-sided p-value  $< 0.05$ .

#### **MODEL ZYR00: RATES OF ADVERSE EVENTS VS. ISO SPE RATES**

The primary Model ZYR00 safety endpoint for this study is the rate of adverse events vs. ISO SPE rates at 1 month postoperative. The frequency and proportion of first and second eyes with these events will be reported over time by IOL group. Statistical comparisons to ISO SPE rates will be based on first-eye data; adverse event rates for Model ZYR00 investigational lens first eyes will be compared to the ISO SPE rates using a one-sided, exact test based on the binomial distribution. The null hypothesis is that the AE rate for Model ZYR00 investigational lens eyes is lower than or equal to the ISO SPE values, and the alternative hypothesis is that the AE rate for study eyes is higher than the ISO SPE values.

$$H_0: p_t \leq p_i$$

$$H_1: p_t > p_i$$

where

$p_t$  = proportion of Model ZYR00 investigational lens eyes with the AE

$p_i$  = proportion of eyes reported in ISO SPE rates with the AE

Reject the null hypothesis if one-sided p-value < 0.05.

### 20.3 ADDITIONAL ENDPOINTS

#### Intermediate Visual Acuity endpoints

Other intermediate endpoints include binocular UCIVA and DCIVA, and monocular UCIVA. For binocular UCIVA and DCIVA and monocular UCIVA, superiority approach similar to DCIVA described above will be used.

In addition, the frequency and proportion achieving each line for all other intermediate endpoints will be reported over time by IOL group.

#### Near and Distance Visual Acuity endpoints

For monocular photopic BCDVA, the frequency and proportion of eyes achieving each acuity line will be reported over time by IOL group. The proportion of investigational lens eyes achieving 20/40 or better at 1 month will be compared to the ISO SPE rate for posterior chamber IOLs (all first eyes) using a one-sided, exact test based on binomial distribution. The null hypothesis (based on the ISO guidance document) is that the proportion of investigational lens eyes achieving 20/40 or better BCDVA is greater than or equal to the ISO SPE values, and the alternative hypothesis is that the proportion of investigational lens eyes achieving 20/40 or better BCDVA is less than the ISO SPE values.

In addition, the mean logMAR photopic BCDVA will be compared between lens groups for first eyes using a non-inferiority method. The null hypothesis is that the mean difference (control minus investigational lens) between the control and investigational IOLs is  $\leq -0.1$  LogMAR (1 line) with the alternative hypothesis that the mean difference is  $> -0.1$  LogMAR. A 90% confidence interval (CI) of a two-sample, two-sided, t-test will be used for evaluation. The success criteria is achieved if the lower limit of the 90% CI of the difference is greater than  $-0.1$  LogMAR.

For monocular and binocular UCDVA, BCDVA with low contrast (10%) and binocular photopic BCDVA, similar statistics using a non-inferior method will be used. Frequency and proportion of eyes achieving each line will also be reported over time by IOL group.

For all near endpoints, a non-inferior approach similar to photopic BCDVA described above will be used. In addition, the frequency and proportion of eyes achieving each line will be reported over time by IOL group.

### **Defocus Endpoints**

For defocus results, the defocus curve will be produced by IOL group. The diopters of defocus where the mean visual acuity 20/32 or better is achieved will be derived by visual inspection of the defocus curve.

### **Manifest refraction endpoint**

Descriptive analysis of refractive sphere, cylinder and spherical equivalent (MRSE) will be reported by IOL groups for both eyes. Since refraction was performed at 4M, 0.25D will be subtracted from the sphere value. Refractive data will then be converted to plus cylinder notation.

MRSE is then calculated by the following formula:  $MRSE = \text{sphere} + \frac{1}{2} \text{cylinder}$ .

### **Questionnaire Endpoints**

For questionnaire data, including visual symptoms, the frequency and proportion of subjects with a given response will be reported by IOL group. For comparisons between IOL groups, Wilcoxon Rank-Sum test will be used for ordinal data, and Fisher's exact test will be used for categorical data. The null hypothesis is that there is no difference between responses, and the alternative hypothesis is that there is a difference between responses. Two-sided testing and alpha of 0.05 will be used to evaluate questionnaire data.

### **Safety endpoints**

For contrast sensitivity data, descriptive analyses including mean, standard deviation, median, minimum, maximum and 90% confidence intervals will be presented by IOL group.

The frequency and percentage of medical findings, lens findings and non-directed ocular/visual symptoms will be reported over time by IOL group for both eyes.

## **20.4 VISUAL ACUITY CONVENTIONS AND GENERAL STATISTICS**

Visual acuity data will be converted to LogMAR values prior to analysis and adjusted for the test distance used if it is not the standard distance for the chart. Descriptive statistics will typically include sample size (N), mean, standard deviation (SD), median, minimum (Min) and maximum (Max) as appropriate for continuous variables. For continuous variables, statistical tests (e.g., t-test) assuming normality will generally be used. For categorical data, the frequency and proportion will be reported and Fisher's

exact test or Chi-square test will generally be applied. For ordinal categorical data, the frequency and proportion will be reported with the Wilcoxon Rank-Sum test generally used.

## **20.5 INTERIM REPORTS**

Although interim study progress reports will be conducted for this study, all masking of study subjects and masked study technicians will be maintained and interim reports will not be disseminated to investigators/site personnel.

## **20.6 SAMPLE SIZE CALCULATIONS**

For the primary endpoint of distance corrected intermediate visual acuity, there is 90% power to detect a 1-line or greater difference in mean visual acuity between the investigational lens groups and the control group (assume one-sided testing with an alpha of 0.025 and standard deviation of 1.6 lines) with 65 subjects in each lens group.

For contrast sensitivity there is 80% power to detect a non-inferiority margin of 0.15 log units between the investigational lens groups and the control group (assume one-sided alpha=0.05 and standard deviation of 0.34) with 65 subjects in each lens group.

If the dropout rate is assumed at 10%, approximately 73 subjects will be implanted in each lens group to achieve a minimum of 65 subjects in each lens group at 1 and 6 months.

## APPENDIX A SUMMARY OF PROCEDURES REQUIRED AT EACH VISIT

Shaded lines indicate masked testing

Examination	Preop Both eyes	Op 1 <sup>st</sup> eye and 2 <sup>nd</sup> eye	1 day 1 <sup>st</sup> eye and 2 <sup>nd</sup> eye	1 week 1 <sup>st</sup> eye and 2 <sup>nd</sup> eye	1 month Both eyes	6 months Both eyes
Informed consent, ocular history, inclusion/exclusion criteria <sup>a</sup> , potential visual acuity, targeted refraction, IOL power calculations, biometry and randomization if required	X					
Lens power/serial number (masked)/operative procedures		X				
Manifest refraction (Snellen preop; ETDRS postop)	X			X	X	X
UCDVA - photopic, monocular (Snellen preop; ETDRS postop) <sup>c</sup>	X			X	X	X
UCDVA - photopic, binocular (ETDRS)					X	X
BCDVA - photopic, monocular (Snellen preop; ETDRS postop) <sup>c</sup>	X			X	X	X
BCDVA - photopic, binocular (ETDRS)					X	X
UCIVA and DCIVA - photopic, monocular at 66 cm (ETDRS) <sup>c</sup>					X	X
UCIVA and DCIVA - photopic, binocular at 66 cm (ETDRS)					X	X
UCNVA and DCNVA - photopic, monocular at 40 cm (ETDRS) <sup>c</sup>					X	X
UCNVA and DCNVA - photopic, binocular at 40 cm (ETDRS)					X	X
BCDVA, monocular <sup>c</sup> (M) and binocular (B), low contrast acuity (10%)					M	B
Defocus testing, monocular <sup>c</sup> (M) and binocular (B)					M	B
Contrast Sensitivity testing, monocular <sup>c</sup> (M) and binocular (B)					M	B
Pupil size (photopic and under contrast sensitivity conditions)					X	X
Keratometry	X <sup>b</sup>					
Topography	X					
Intraocular pressure	X		X	X	X	X
Biomicroscopic slit-lamp exam <sup>b</sup>	X		X	X	X	X
Dilated fundus exam with fundus visualization	X					X
Adverse events		X	X	X	X	X
Ocular medications	X	X	X	X	X	X
Ocular/visual symptoms (non-directed)	X		X	X	X	X
Subject questionnaires	X				X	X

<sup>a</sup> With corneal stability check for contact lens wearers

<sup>b</sup> Includes determination of medical and lens findings/complications

<sup>c</sup> Monocular testing required for first-eye only



## APPENDIX B EQUIPMENT LIST

The following equipment will be supplied to an investigative site for the duration of the study provided that the site does not already have such equipment available for use. This equipment loan will be documented in the Clinical Trial Agreement, which indicates that the equipment is to be returned to JJV at the completion of the study.

- M&S Technologies CTS-1000 Smart System<sup>®</sup> Computerized Vision Testing System, including laptop computer, tablet, and glare bracket (“M&S System”)
- Good-Lite EVS-1500 retro-illuminated visual acuity light box and stand
- Four Good-Lite ETDRS near visual acuity charts (100% contrast) on two cards, for a test distance of 40 cm
- Neutral density trial frame lenses for mesopic testing
- +0.12 D trial frame lenses
- Gossen Light Meter
- Tape measure (meters)
- Colvard Pupillometer (if site does not use a NeurOptics pupillometer)
- JJV insertion systems:
  - ONE SERIES Ultra Implantation System with cartridges, or
  - UNFOLDER Platinum 1 Series Implantation System with cartridges

## APPENDIX C MAXIMUM PLUS MANIFEST REFRACTION TECHNIQUE WITH CYLINDER REFINEMENT

Manifest refraction testing will be performed using the M&S System at 4.0 meters with the room lighting set to that required for photopic distance visual acuity testing (85 cd/m<sup>2</sup>). NOTE: Objective refraction by either retinoscopy or autorefractometry can be used as a starting point for the Manifest Refraction. Always ensure that the endpoint of refraction is maximum plus (or minimum minus) power that yields maximum visual acuity.

- 1) Occlude the fellow eye.
- 2) SPHERE: Starting with the objective refraction, refine the sphere to yield best visual acuity. **Important:** Add plus power (or reduce minus) until subject demonstrates at least a 1-line loss from best visual acuity (fogging). Then step down to the most plus (or least minus) sphere power until visual acuity and clarity show no improvement.
- 3) CYLINDER AXIS: Refine cylinder with a cross-cylinder and the objective cylinder refraction as the starting point. Refine axis first and power second, since the correct axis can be found with an incorrect power, but the correct power cannot be found with an incorrect axis.
  - a. Direct the subject's attention to 1 line above (larger letters) the best visual acuity. With the trial cylinder (axis and power) in the phoropter, introduce cross-cylinder for axis refinement. When asking the subject which cross-cylinder axis position is better, "one or two?", remind the subject to look at different letters on the line and report preference based on the overall clarity of the letters.
  - b. Refine the axis based on the subject's responses, using small steps (less than five degrees), until the subject reports no difference in the two choices.
  - c. Cylinder axis may be further confirmed by bracketing: Slowly rotate the trial cylinder in one direction until the subject reports blurring and note the axis. Rotate the trial cylinder in the opposite direction past the presumed axis until the subject reports blurring, again noting the axis. The average of the two noted axes can be taken as the final astigmatism axis.
- 4) CYLINDER POWER: Set the cross cylinder to refine cylinder power and present choices to the subject, reminding the subject to look at different letters on the line and report preference based on overall clarity of the letters. Reduce or increase trial cylinder power accordingly.
  - a. Maintain the spherical equivalent throughout cylinder power refinement by adjusting the sphere once for every two clicks of cylinder power change.
- 5) SPHERE CHECK: Introduce plus sphere in 0.25 D increments until the subject reports and demonstrates a reduction in visual acuity. Then reduce sphere power in 0.25 D steps until visual acuity and clarity show no improvement.

## APPENDIX D REFRACTION ADJUSTMENTS

Postoperative study manifest refractions are to be performed using the M&S System at a distance of 4.0 meters. Because 4.0 meters is not optical infinity, refraction adjustments are necessary to ensure proper vision testing taking into account test distance and refraction distance. The adjustment required (in diopters) is  $1/\text{test distance}$  (in meters). To adjust a 4.0-meter refraction to optical infinity,  $-0.25$  D is to be added to the sphere of the refraction to obtain a true distance (infinity) correction. On the other hand, to adjust optical infinity to a 4.0-meter test distance,  $+0.25$  D is to be given. In the case where the refraction distance (4.0 meters) and the vision test distance (4.0 meters) are the same, no adjustment is necessary. The following table lists the refraction adjustments required for the various vision tests in this study:

**Refraction Adjustments for Vision Testing**

<u>Vision Test</u>	<u>Test Distance</u>	<u>Correction/Adjustment</u>
Uncorrected distance visual acuity (UCDVA)	4.0 m	+0.25 D adjustment only
Best corrected distance visual acuity (BCDVA)	4.0 m	No adjustment; ETDRS Rx only
Best corrected distance visual acuity (BCDVA), 10% contrast	4.0 m	No adjustment; ETDRS Rx only
Best corrected distance defocus curve testing	4.0 m	No adjustment; ETDRS Rx only
Uncorrected intermediate visual acuity (UCIVA)	66 cm	No adjustment
Distance corrected intermediate visual acuity (DCIVA)	66 cm	-0.25 D added to ETDRS sphere Rx
Uncorrected near visual acuity (UCNVA)	40 cm	No adjustment
Distance corrected near visual acuity (DCNVA)	40 cm	-0.25 D added to ETDRS sphere Rx
Best corrected distance contrast sensitivity	2.5 m	+0.12 D added to ETDRS sphere Rx

## APPENDIX E INSTRUCTIONS FOR USING THE M&S SYSTEM

Distance and intermediate visual acuity, low-contrast distance visual acuity, defocus, and contrast sensitivity testing will be performed using the M&S System. This system provides descending LogMAR charts with proportionally spaced SLOAN letters at 100% contrast for high contrast visual acuity and defocus testing, 10% contrast for low-contrast distance visual acuity and appropriate contrast levels for contrast sensitivity testing. Each presentation is randomized and is consistent and repeatable. The system is calibrated for both distance to subject and pixels/inch so that optotypes precisely follow ANSI Z80.21-2010 and ISO 8596:2000 in regard to size, spacing between optotypes and spacing between lines.

Figure 4: Example of LogMAR 4.0 meter chart screen

V K O Z S	32
● R Z N D O	25
H O Z S D	20
S V N Z C	16
C D V S O	12.5
O N Z D K	10

The M&S System background luminance is automatically set to 85 cd/m<sup>2</sup> (range of 80-110 cd/m<sup>2</sup> is acceptable) for photopic testing and, with a neutral density filter placed in front of the laptop, lighting is reduced to 3 ± 0.5 cd/m<sup>2</sup> for mesopic testing. Room lighting is to be set to a level lower than the illumination from the laptop screen. Ambient lighting should be dim to dark (less than 50 lux) to maximize pupil size. No surface (including reflective surfaces) within the subject's field of vision should be brighter than the chart background in luminance. The room lighting and screen luminance will be verified each time the computer is turned on using the JJV-provided, auto-adjusting, monitor-calibration system to ensure light levels are appropriate.

The M&S System will be set up to perform required visual tests in a specific order, with prompts on the screen to allow the technician to set up the subject for monocular or binocular testing, refraction adjustments as needed and uncorrected or best corrected testing. Letters on all charts will appear randomly, with the technician controlling movement through charts based on subject responses.

As a subject completes a visual acuity line, the technician will select the total number of letters correctly read for that line on the handheld controller, press "Enter" and then

confirm the number of letters correct at the next prompt. The M&S System will then advance to the next line of testing and the process will repeat. The system will end the test when the subject no longer has any correct responses. The number of letters correctly read will be displayed on the laptop screen, along with the LogMAR value and Snellen acuity. Record the total number of letters read. A similar process will be done for contrast sensitivity grating responses. Once a test is completed, follow the prompts on the computer screen to start the next test.

Test results are stored in the M&S computer and a hard copy will be printed and validated as a back-up.

## APPENDIX F INSTRUCTIONS FOR DISTANCE VISUAL ACUITY TESTING

For distance visual acuities, the M&S System laptop should be placed at a test distance of 4.0 meters from the subject for testing distance visual acuities. A laptop setting may be used to reverse charts for rooms that require “folding” via a mirror to reach a distance of 4.0 meters. Whether standard or “folded”, measure and record the test distance accurately. If the room set-up does not allow the computer to be placed at precisely 4.0 meters, the M&S System can be adjusted to account for the actual test distance used.

The M&S System will be set up to perform the required distance visual acuity tests in a specific order, with prompts on the screen to allow the technician to set up the subject for monocular or binocular testing, refraction adjustment as needed and uncorrected or best corrected testing.

Subjects should be reminded prior to testing that squinting is not allowed. The technician is to observe the subject to ensure the subject is not squinting during visual acuity testing. If squinting is observed, the subject is to be reminded by the testing technician not to squint.

Distance visual acuity measurements are to be performed per the visit schedule in **Appendix A**. Monocular testing is required on the first eye implanted only; to test subjects monocularly, occlude the second eye in the phoropter or with an occluder if trial lenses are used.

Visual acuity measurements are based on the total number of correctly read letters. Subjects should be persuaded to read the smallest letters possible even if they have to guess. Follow the testing process listed in **Appendix E**. At the end of the test, the number of letters correctly read will be displayed on the laptop screen, along with the LogMAR value and Snellen acuity. Record the total number of letters read in the EDC system.

**BEST CORRECTED DISTANCE VISUAL ACUITY (BCDVA) LOW CONTRAST (10%)**  
Monocular testing is required on the first eye implanted only; to test subjects monocularly, occlude the second eye in the phoropter or with an occluder if trial lenses are used.

Visual acuity measurements are based on the total number of correctly read letters. Subjects should be persuaded to read the smallest letters possible even if they have to guess. Follow the testing process listed in **Appendix E**. At the end of the test, the number of letters correctly read will be displayed on the laptop screen, along with the

LogMAR value and Snellen acuity. Record the total number of letters read in the EDC system.

## APPENDIX G INSTRUCTIONS FOR INTERMEDIATE VISUAL ACUITY TESTING

Intermediate visual acuity will be measured using the M&S System at a test distance of 66 cm. Subjects should be reminded prior to testing that squinting is not allowed and the testing technician should carefully observe to ensure the subject is not squinting. If squinting is observed, the subject is to be reminded by the testing technician not to squint.

The M&S System will be set up to perform the required intermediate visual acuity tests in a specific order, with prompts on the screen to allow the technician to set up the subject for monocular or binocular testing, refraction adjustment as needed, and uncorrected or distance corrected testing.

Intermediate visual acuity measurements are to be performed per the visit schedule in **Appendix A**. Monocular testing is required on the first eye implanted only; to test subjects monocularly, occlude the second eye in the phoropter or with an occluder if trial lenses are used.

Visual acuity measurements are based on the total number of correctly read letters. Subjects should be persuaded to read the smallest letters possible even if they have to guess. Follow the testing process listed in **Appendix E**. At the end of the test, the number of letters correctly read will be displayed on the laptop screen, along with the LogMAR value and Snellen acuity. Record the total number of letters read in the EDC system.



## APPENDIX H INSTRUCTIONS FOR NEAR VISUAL ACUITY TESTING

Near visual acuity will be measured using a using Good-Lite 100% ETDRS near charts designed for 40 cm and the Good-Lite self-illuminated and self-calibrated illumination box. The Good-Lite illumination box is self-illuminated and self-calibrates to a light level of approximately 85 cd/m<sup>2</sup> (range of 80–110 cd/m<sup>2</sup> is acceptable). Room lighting is to be set at a level lower than the illumination from the light box, per manufacturer instructions. Ambient luminance should be from dim to dark to maximize pupil size. No surface (including reflective surfaces) within the subject's field of vision should exceed the chart background in luminance.

The light box should be placed at a test distance of 40 cm from the subject for testing near visual acuities. Subjects should be reminded prior to testing that squinting is not allowed and the testing technician should carefully observe. If squinting is observed, the subject is to be reminded by the testing technician not to squint.

To avoid chart memorization, charts will be changed between every visual acuity measurement. Monocular testing will be required on the first eye implanted only, with the second eye occluded. Monocular and binocular uncorrected testing will be completed before monocular and binocular distance corrected testing are done.

Near visual acuity testing is to be performed per **Appendix A**. Visual acuity measurements are based on the total number of correctly read letters. Subjects should be persuaded to read the smallest letters possible even if they have to guess. Record the total number of letters read correctly for each near test on the case report form. Near score grids are to be used and must be retained as source documentation. A reference chart for the conversion of the number of correctly-read ETDRS letters to a Snellen line equivalent is provided later in this section.

**PROCEDURE:** Begin with monocular uncorrected near visual acuity testing for the first eye implanted with the second eye occluded, and instruct subjects to read each line from left to right until they cannot read any additional letters. Subjects should be persuaded to read the smallest letters possible even if they have to guess. Alternate the near chart per the score sheet and perform binocular uncorrected near visual testing. Change the near chart per the score sheet and ensure the refractive adjustment of -0.25 D has been added for corrected near acuities. Begin testing with monocular distance corrected visual acuity (in the first eye) followed by binocular distance corrected visual acuity. Record the total number of letters read for each test condition on the score grid and in the EDC system.

**Conversion Reference Chart for GOOD-LITE Near (40 cm) Chart (ETDRS)**

Standard Snellen Line Equivalent	Number of ETDRS Letters Read at 40 cm	Standard Snellen Line Equivalent	Number of ETDRS Letters Read at 40 cm
20/10	85	20/50	49
	84		48
	83	20/60	47
20/13	82		46
	81		45
	80		44
	79		43
	78	20/80	42
20/16	77		41
	76		40
	75		39
	74		38
	73	20/100	37
20/20	72		36
	71		35
	70		34
	69		33
	68	20/126	32
20/25	67		31
	66		30
	65		29
	64		28
	63	20/160	27
20/32	62		26
	61		25
	60		24
	59		23
	58	20/200	22
20/40	57		21
	56		20
	55		19
	54		18
	53	>20/200	17
20/50	52		16
	51		15
	50		

## APPENDIX I INSTRUCTIONS FOR DEPTH OF FOCUS TESTING

All depth of focus testing is to be performed under photopic conditions using the M&S System at a test distance of 4.0 meters. Subjects should be reminded prior to testing that squinting is not allowed and the testing technician should carefully observe to ensure the subject is not squinting. If squinting is observed, the subject is to be reminded by the testing technician not to squint.

This test is to be done monocularly at the 1-month visit for all subjects and binocularly at the 6-month visit for all subjects. Only the first eye implanted will be tested at the 1-month visit.

Monocular Depth of Focus Testing (1-month visit): With the subject's distance correction in place for the first eye and the second eye occluded, defocus the image by +2.00 D over the manifest distance correction in the first eye. Start the test by instructing the subject to read as many letters as possible on the M&S system, even if they have to guess. The technician will control movement through charts based on subject responses and the system will end the testing when a threshold is reached. The number of letters correctly read and the LogMAR score will be displayed on the laptop screen; record the total number of letters correct in EDC. Continue to change the defocus in -0.50 D increments, repeating the test and recording the total number of letters correct at each level of defocus. Continue to change the defocus to -4.00 D over the subject's distance correction.

Binocular Depth of Focus Testing (6-month visit): Begin binocular testing by defocusing the image by +2.00 D over the manifest distance correction in both eyes. Start the test by instructing the subject to read as many letters as they can on the M&S system, even if they have to guess. The technician will control movement through charts based on subject responses and the system will end the testing when a threshold is reached. The number of letters correctly read and the LogMAR score will be displayed on the laptop screen; record the total number of letters correct in EDC. Continue to change the defocus in -0.50 D increments in both eyes, repeating the test and recording the total number of letters correct at each level of defocus. Continue to change the defocus to -4.00 D over the subject's distance correction.

## APPENDIX J INSTRUCTIONS FOR PUPIL SIZE MEASUREMENTS

Pupil size should be measured by a Colvard pupillometer (Oasis Medical) or a NeurOptics pupillometer (NeurOptics, Inc.). For consistency, the same method should be used throughout the study. Pupil size should be recorded to the nearest one-half millimeter (one-tenth millimeter for NeurOptics).

### PHOTOPIC PUPIL SIZE:

Photopic pupil size for each eye should be measured under the same lighting conditions as the photopic distance visual acuity testing. To measure photopic pupil size, have the subject look at a spot in the distance (without glasses) and allow one eye to be exposed to the ambient room lighting while measuring the pupil of the other eye. Repeat the measurement on the second eye, and record the photopic pupil size for both eyes.

### MESOPIC PUPIL SIZE:

Mesopic pupil size for each eye should be measured under mesopic conditions. Room lights should be off and the 1.5 ND filter placed in front of the M&S System to reduce the lighting to 3 cd/m<sup>2</sup>. Place a 1.5 ND filter lens for each eye in the trial frames/phoropter. After 10 minutes of dark adaptation, have the subject (without glasses and/or trial frames) look at a spot on the mesopic contrast sensitivity chart and allow one eye to continuously be exposed to the lighting condition while measuring the pupil of the other eye. Repeat the measurement on the second eye, and record the mesopic pupil size for both eyes.

### MESOPIC WITH GLARE PUPIL SIZE:

Mesopic with glare pupil size for each eye should be measured under mesopic with glare contrast sensitivity conditions. Room lights should be off, the 1.5 ND filter placed in front of the M&S System to reduce the lighting to 3 cd/m<sup>2</sup>, and the glare lights from the M&S System on. Have the subject (without glasses and/or trial frames) look at a spot on the mesopic with glare contrast sensitivity chart and allow one eye to continuously be exposed to the lighting condition while measuring the pupil of the other eye. Repeat the measurement on the second eye, and record the mesopic with glare pupil size for both eyes.

## APPENDIX K INSTRUCTIONS FOR CONTRAST SENSITIVITY TESTING

Contrast sensitivity testing will be measured using the M&S system for sine-wave gratings (1.5, 3, 6, 12 and/or 18 cycles per degree). Testing will be done under mesopic and mesopic with glare and photopic lighting conditions. **The test distance for the M&S system is 8 feet (2.5 meters).** Mesopic testing without glare will be performed before contrast sensitivity with glare testing.

This test is to be done monocularly at the 1-month and binocularly at the 6-month visit for all subjects. Only the first eye implanted will be tested at the 1-month visit. All subjects will be tested with best corrected manifest refraction in place, and a refraction adjustment of +0.12 D over manifest refraction in place. Subjects should be shown the contrast sensitivity target samples before dark adaptation for mesopic testing is started.

Contrast sensitivity measurements are based on subject identification of the orientation of a low contrast grating (vertical, horizontal, tilted left or tilted right). For each grating presented, the subject will have to identify or guess the orientation of the grating. After an automated protocol, contrast sensitivity values will be displayed on the laptop screen for 1.5, 3, 6, 12 and/or 18 cpd.

Monocular Testing (1-month visit): The test will begin with the photopic lighting condition and then proceed to the mesopic without glare lighting condition. Dim to dark room lighting will be used along with a 1.5 ND filter in front of the M&S system laptop computer screen. Dark adapt the subject for 10 minutes and measure mesopic pupil size per **Appendix J** prior to beginning the test. Place the subject's distance correction with the +0.12 D refraction adjustment in place for the first eye implanted and occlude the second eye implanted. Ensure the 1.5 ND filter lenses have been removed from the trial frames/phoropter before testing begins. The 1.5 ND filter is only to be in front of the M&S system laptop computer screen. Begin testing and instruct the subject to report the orientation of the contrast grating out loud as they view the grating, documenting the subject responses on the M&S tablet. Encourage the subject to continue through all gratings, even if they have to guess. The M&S System will advance to the next set of gratings based on the technician input of the subject's responses. Record the contrast sensitivity percentages displayed on the laptop computer for all the spatial frequencies in EDC.

Binocular Testing (6-month visit): The test will begin with the photopic lighting condition. Proceed to mesopic without glare lighting condition. Dim to dark room lighting will be used along with a 1.5 ND filter in front of the M&S system laptop computer screen. Dark adapt the subject for 10 minutes and measure mesopic pupil size per **Appendix J** prior to beginning the test. Place the subject's distance correction with the +0.12 D refraction adjustment in place for both eyes. Ensure the 1.5 ND filter lenses have been removed

from the trial frames/phoropter before testing begins. The 1.5 ND filter is only to be in front of the M&S system laptop computer screen. Begin testing and instruct the subjects to report the orientation of the contrast grating out loud as they view the grating, documenting the subject responses on the M&S tablet. Encourage the subject to continue through all gratings, even if they have to guess. The M&S System will advance to the next set of gratings based on the technician input of the subject's responses. Record the contrast sensitivity percentages displayed on the laptop computer for all the spatial frequencies in EDC.

## APPENDIX L SLIT-LAMP EXAM RATINGS

### A. Ratings of Aqueous Cells and Flare

For consistency across study sites, the SUN (Standardization of Uveitis Nomenclature) Working Group Grading Scheme is to be used for grading of anterior chamber cells and flare as reported in: Standardization of uveitis nomenclature for reporting clinical data. Results of The First International Workshop; The standardization of uveitis nomenclature (SUN) working group. Am J Ophthalmol 2005;140:509-516.

#### CELLS

Grade	Cells in Field (Field is a 1x1 mm slit beam)
0	<1
0.5+	1 - 5
1+	6 - 15
2+	16 - 25
3+	26 - 50
4+	>50

#### FLARE

Grade	Description
0	None
1+	Faint
2+	Moderate (iris and lens details clear)
3+	Marked (iris and lens details hazy)
4+	Intense (fibrin or plastic aqueous)

### B. Ratings of Corneal Edema

Corneal edema should be classified according to the haziness of the epithelium, the number of microcysts observed, and the clouding of the stroma.

Amount	Grade	Description
None	0	Normal transparency: a. No epithelial or sub-epithelial haziness b. No microcysts c. No stromal cloudiness
Trace	+1	a. Barely discernible localized epithelial or sub-epithelial haziness, and/or b. 1 to 20 microcysts, and/or c. Barely discernible localized stromal cloudiness
Mild	+2	a. Faint but definite localized or generalized epithelial, sub-epithelial or stromal haziness/cloudiness, and/or b. 21-50 microcysts
Moderate	+3	a. Significant localized or generalized epithelial, sub-epithelial or stromal haziness/cloudiness and/or b. 51-100 microcysts
Severe	+4	a. Definite widespread epithelial or stromal cloudiness, giving dull glass appearance to cornea or numerous coalescent bullae (please note the number and location of bullae), and/or b. >100 microcysts or bullae, and/or c. Numerous striae (please note the number and location of striae or folds)

### C. Posterior Capsule Striae Grading Scale

The following five-point grading scale is to be used for rating striae in the posterior capsule:

Amount	Grade	Description
None	0	None
Trace	+1	One detectable, barely noticeable striae
Mild	+2	One or two prominent striae
Moderate	+3	Three or more prominent striae, but visibility of retina is not impacted
Severe	+4	Three or more prominent striae affecting visualization of retina

### D. Posterior Capsule Opacification Grading Scale

Below is the five-point grading scale to be used for PCO determination:

Amount	Grade	Description
None	0	Normal posterior capsule with no area of opacity. Red reflex bright.
Trace	+1	Some loss of transparency involving the posterior capsule. Red reflex fairly bright
Mild	+2	Mild loss of transparency with cloudiness extending through most of the posterior capsule. There may be a few Elschnig's pearls in the posterior capsule. Red reflex mildly diminished.
Moderate	+3	Moderate loss of transparency with difficulty visualizing the retina. There may be multiple Elschnig's pearls in the posterior capsule. Red reflex markedly diminished.
Severe	+4	Posterior capsule very opaque with inability to view the retina. The posterior capsule may have confluent Elschnig's pearls and fibrous scarring. Red reflex barely visible.

### E. IOL Glistenings

Use the following scale to grade IOL glistenings, using a slit beam 2.0 mm wide and 10.0 mm long:

Amount	Grade	Description
None	0	No glistenings visible
Rare	+0.5	<10 glistenings visible
Trace	+1	10-19 glistenings visible
Mild	+2	20-29 glistenings visible
Moderate	+3	30-39 glistenings visible
Severe	+4	≥40 glistenings visible