

Johnson & Johnson Vision Care, Inc.

Clinical Study Protocol

Clinical Evaluation of a Reusable Multifocal Optical Design in a Presbyopic Population
Phase II

Protocol CR-6267

Version: 2.0 Amendment 1

Date: 22 June 2018

Investigational Products: JJV Investigational senofilcon A Multifocal Contact Lens and
1-Day Acuvue® Moist Brand Multifocal Contact Lens

Key Words: Presbyopia, Multifocal, etafilcon A, senofilcon A, Daily Wear, Daily
Disposable, Reusable, Dispensing, Randomized

Statement of Compliance to protocol, GCP and applicable regulatory guidelines:

This trial will be conducted in compliance with the protocol, ISO 14155,¹ the International Conference on Harmonization Good Clinical Practice E6 (ICH-GCP),² the Declaration of Helsinki,³ and all applicable regulatory requirements.

Confidentiality Statement:

This document contains confidential information, which should not be copied, referred to, released or published without written approval from Johnson & Johnson Vision Care, Inc. The information may not be disclosed to others except to the extent necessary to obtain Institutional Review Board/Independent Ethics Committee approval and informed consent, or as required by International, Federal and State Laws, as applicable. Persons to whom this information is disclosed must be informed that this information is privileged and confidential and that it should not be further disclosed without the written permission of Johnson & Johnson Vision Care, Inc. Any supplemental information that may be added to this document is also confidential and proprietary to Johnson & Johnson Vision Care, Inc. and must be kept in confidence in the same manner as the contents of this document.

TABLE OF CONTENTS

PROTOCOL TITLE, NUMBER, VERSION.....	6
SPONSOR NAME AND ADDRESS.....	6
MEDICAL MONITOR.....	6
AUTHORIZED SIGNATURES.....	7
CHANGE HISTORY.....	8
SYNOPSIS.....	9
COMMONLY USED ABBREVIATIONS AND DEFINITIONS OF TERMS	14
1. INTRODUCTION AND BACKGROUND	16
1.1. Name and Descriptions of Investigational Products	16
1.2. Intended Use of Investigational Products.....	16
1.3. Summary of Findings from Nonclinical Studies.....	16
1.4. Summary of Known Risks and Benefits to Human Subjects.....	16
1.5. Relevant Literature References and Prior Clinical Data Relevant to Proposed Clinical Study.....	17
2. STUDY OBJECTIVES, ENDPOINTS AND HYPOTHESES	18
2.1. Objectives.....	18
2.2. Endpoints.....	18
2.3. Hypotheses	18
3. TARGETED STUDY POPULATION	19
3.1. General Characteristics	19
3.2. Inclusion Criteria.....	19
3.3. Exclusion Criteria.....	19
3.4. Enrollment Strategy.....	20
4. STUDY DESIGN AND RATIONALE	20
4.1. Description of Study Design	20
4.2. Study Design Rationale.....	20
4.3. Enrollment Target and Study Duration	21
5. TEST ARTICLE ALLOCATION AND MASKING	21
5.1. Test Article Allocation	21
5.2. Masking.....	21
5.3. Procedures for Maintaining and Breaking the Masking.....	22
6. STUDY INTERVENTION.....	22

6.1.	Identity of Test Articles.....	22
6.2	Ancillary Supplies/Products.....	23
6.3.	Administration of Test Articles.....	23
6.4.	Packaging and Labeling	23
6.5.	Storage Conditions	24
6.6.	Collection and Storage of Samples	24
6.7.	Accountability of Test Articles	24
7.	STUDY EVALUATIONS	25
7.1.	Time and Event Schedule.....	25
7.2.	Detailed Study Procedures	29
	VISIT 1	29
	VISIT 2	35
	VISIT 3	39
	VISIT 4	44
	VISIT 5	50
	VISIT 6	55
	VISIT 7	59
	FINAL EVALUATION.....	62
7.3.	Unscheduled Visits.....	62
7.4.	Laboratory Procedures	64
8.	SUBJECTS COMPLETION/WITHDRAWAL.....	64
8.1.	Completion Criteria.....	64
8.2.	Withdrawal/Discontinuation from the Study	64
9.	PRE-STUDY AND CONCOMITANT INTERVENTION/MEDICATION	65
10.	DEVIATIONS FROM THE PROTOCOL	65
11.	STUDY TERMINATION	65
12.	PROCEDURE FOR HANDLING PRODUCT QUALITY COMPLAINTS	66
13.	ADVERSE EVENTS.....	67
13.1.	Definitions and Classifications	67
13.2.	Assessing Adverse Events	70
	13.2.1. Causality Assessment.....	70
	13.2.2. Severity Assessment.....	70
13.3.	Documentation and Follow-Up of Adverse Events.....	71
13.4.	Reporting Adverse Events	72

13.4.1.	Reporting Adverse Events to Sponsor	72
13.4.2.	Reporting Adverse Events to the Responsible IEC/IRB and Health Authorities.....	73
13.4.3.	Event of Special Interest	73
13.5.	Reporting of Pregnancy	73
14.	STATISTICAL METHODS.....	74
14.1.	General Considerations.....	74
14.2.	Sample Size Justification.....	74
14.3.	Analysis Populations	74
14.4.	Level of Statistical Significance	75
14.5.	Primary Analysis	75
14.6.	Secondary Analysis	75
14.7.	Other Exploratory Analyses	75
14.8.	Interim Analysis	76
14.9.	Procedure for Handling Missing Data and Drop-Outs	76
14.10.	Procedure for Reporting Deviations from Statistical Plan	76
15.	DATA HANDLING AND RECORD KEEPING/ARCHIVING.....	76
15.1.	Electronic Case Report Form/Data Collection	76
15.2.	Subject Record.....	77
16.	DATA MANAGEMENT.....	77
16.1.	Access to Source Data/Document	77
16.2.	Confidentiality of Information.....	77
16.3.	Data Quality Assurance	78
17.	MONITORING.....	78
18.	ETHICAL AND REGULATORY ASPECTS	78
18.1.	Study-Specific Design Considerations	78
18.2.	Investigator Responsibility	79
18.3.	Independent Ethics Committee or Institutional Review Board (IEC/IRB)	79
18.4.	Informed Consent	80
18.5.	Privacy of Personal Data	81
19.	STUDY RECORD RETENTION.....	81
20.	FINANCIAL CONSIDERATIONS	82
21.	PUBLICATION.....	82
22.	REFERENCES	83
	APPENDIX A: PATIENT REPORTED OUTCOMES (STUDY QUESTIONNAIRES)	84

APPENDIX B : PATIENT INSTRUCTION GUIDE	116
APPENDIX C: PACKAGE INSERT (APPROVED PRODUCT).....	117
APPENDIX D: BINOCULAR OVER REFRACTION	148
APPENDIX E: PRESBYOPIC SYMPTOMS QUESTIONNAIRE.....	149
APPENDIX F: OCULAR DOMINANCE.....	150
APPENDIX G: Test LENS FITTING GUIDE	151
APPENDIX H: CONTROL LENS FITTING GUIDE.....	153
APPENDIX I: CLINICAL TECHNICAL PROCEDURES (CTP).....	155
██████████ LIMBAL AND CONJUNCTIVAL (BULBAR) REDNESS.....	156
██████████ EXPANDED SODIUM FLUORESCEIN CORNEAL STAINING.....	164
██████████ DETERMINATION OF NEAR ADDITION	169
██████████ NEAR LOGMAR VISUAL ACUITY MEASUREMENT PROCEDURE.....	177
██████████ LENS FITTING CHARACTERISTICS	180
██████████ SUBJECT REPORTED OCULAR SYMPTOMS/PROBLEMS.....	187
██████████ DETERMINATION OF DISTANCE SPHEROCYLINDRICAL REFRACTIONS	189
██████████ BIOMICROSCOPY SCALE	196
██████████ KERATOMETRY PROCEDURE.....	202
██████████ DISTANCE AND NEAR VISUAL ACUITY EVALUATION.....	204
██████████ DISTANCE LOGMAR VISUAL ACUITY MEASUREMENT PROCEDURE	209
██████████ Visual Acuity Chart Luminance and Room Illumination Testing	213
PROTOCOL COMPLIANCE INVESTIGATOR(S) SIGNATURE PAGE	218

TABLE OF CONTENTS

Figure 1: Study Flowchart	13
---------------------------------	----

TABLE OF CONTENTS

Table 1: Test Articles.....	22
Table 2: Ancillary Supplies	23
Table 3: Time and Events	25

PROTOCOL TITLE, NUMBER, VERSION

Title: Clinical Evaluation of a Reusable Multifocal Optical Design in a Presbyopic Population Phase II

Protocol Number: CR-6267

Version: 2.0 Amendment 1

Date: 22 June 2018

SPONSOR NAME AND ADDRESS

Johnson & Johnson Vision (JJV)
7500 Centurion Parkway
Jacksonville, FL 32256

MEDICAL MONITOR

Name: Thomas R. Karkkainen, OD, MS, FAAO

Title: Sr. Principal Research Optometrist

Address: 7500 Centurion Parkway, Jacksonville, Florida 32256








Email: TKarkkai@its.jnj.com

The Medical Monitor must be notified by the clinical institution/site by e-mail, fax, or telephone within 24 hours of learning of a Serious Adverse Event. The Medical Monitor may be contacted during business hours for adverse event questions. General study related questions should be directed towards your assigned clinical research associate.

The Medical Monitoring Plan is maintained as a separate document and included in the Trial Master File.

AUTHORIZED SIGNATURES

The signature below constitutes the approval of this protocol and the attachments, and provides the necessary assurances that this trial will be conducted according to all stipulations of the protocol, including all statements regarding confidentiality, and according to local legal and regulatory requirements and applicable U.S. federal regulations,⁴ ICH guidelines,² ISO 14155,¹ and the Declaration of Helsinki.³

Author	<u>See Electronic Signature Report</u> Thomas R. Karkkainen, OD, MS, FAAO Sr. Principal Research Optometrist	_____ DATE
Clinical Operations Manager	 <u>See Electronic Signature Report</u> 	_____ DATE
Biostatistician	 <u>See Electronic Signature Report</u> 	_____ DATE
Data Management	<u>See Electronic Signature Report</u> 	_____ DATE
Reviewer	<u>See Electronic Signature Report</u> 	_____ DATE
Approver	<u>See Electronic Signature Report</u> 	_____ DATE

CHANGE HISTORY

Version	Originator	Description of Change(s) and Section Number(s) Affected	Date
1.0	Tom Karkkainen	Original Protocol	30-Apr-2018
2.0 Amendment 1	Tom Karkkainen	-Revised Section 6.1 Test Article the Investigational Multifocal Lens Codes -Updated Version and Date throughout the Document.	22-Jun-2018

SYNOPSIS


Protocol Title	Clinical Evaluation of a Reusable Multifocal Optical Design in a Presbyopic Population Phase II
Sponsor	JJV, 7500 Centurion Parkway, Jacksonville, FL 32256
Clinical Phase	Development phase, Phase 2
Trial Registration	This study will be registered on ClinicalTrials.gov.
Test Article(s)	Investigational Product: JJV Investigational Multifocal Contact Lens manufactured in senofilcon A material. Marketed Product: 1-Day Acuvue® Moist Brand Multifocal Contact Lens.
Wear and Replacement Schedules	Wear Schedule: The Test and Control lenses are used as daily wear (note: the Test lens will be reusable and the Control lens daily disposable). Replacement Schedule: The Test lens will be replaced at the optimization visit. The Control lens will be replaced after each day of wear as well as the optimization visit and the visit after the first week of wear in the optimized pair. The Test and Control lenses will also be replaced when lost or damaged.
Objectives	This study is an evaluation of the visual performance, subjective response, lens fit and ocular physiological response of the JJV Investigational senofilcon A Multifocal Contact Lens. The Test lens will be compared to the 1-Day Acuvue® Moist Brand Multifocal Contact Lens manufactured in etafilcon A material for CLUE subjective vision.
Study Endpoints	Primary endpoints: CLUE vision scores Other observations: logMAR visual acuity scores, lens fit, summary of number of lenses needed to fit (optimize) the subject, CLUE comfort/handling scores, corneal staining, and ocular redness.
Study Design	This is a single-masked, randomized-controlled, dispensing clinical trial. A total of approximately 60 eligible hyperopic subjects will be targeted to complete the study. The subjects will be fit in each study lens and wear the lens for 2-4 days then undergo optimization, if applicable, and wear the optimized pair for approximately 2 weeks with a follow-up at 1 week. The primary endpoints will be CLUE vision scores.
Sample Size	A total of approximately 60 subjects will be targeted to complete.
Study Duration	The study will last approximately 2-4 months.

Anticipated Study Population	Healthy male and female volunteers with presbyopia will be invited to participate in the study. Subjects will be adapted soft contact lens wearers in both eyes. Additional information regarding the eligibility of the population can be found in the inclusion/exclusion criteria outlined below.
Eligibility Criteria	<p>Potential subjects must satisfy all the following criteria to be enrolled in the study</p> <ol style="list-style-type: none"> 1. The subject must read, understand, and sign the STATEMENT OF INFORMED CONSENT and receive a fully executed copy of the form. 2. The subject must appear able and willing to adhere to the instructions set forth in this clinical protocol. 3. The subject must be between 40 and 70 years of age (inclusive). 4. The subject's distance spherical equivalent refraction must be in the range of +1.25 D to +3.75 D in each eye. 5. The subject's refractive cylinder must be ≤ 0.75 D in each eye. 6. The subject's ADD power must be in the range of +0.75 D to +2.50 D. 7. The subject must have best corrected visual acuity of 20/20⁻³ or better in each eye. 8. Subjects must own a wearable pair of spectacles if required for their distance vision. 9. The subject must be an adapted soft contact lens wearer in both eyes (i.e. worn lenses a minimum of 2 days per week for at least 8 hours per wear day, for 1 month of more duration). 10. The subject must either already be wearing a presbyopic contact lens correction (e.g., reading spectacles over contact lenses, multifocal or monovision contact lenses, etc.) or if not respond positively to at least one symptom on the "Presbyopic Symptoms Questionnaire". <p>Potential subjects who meet any of the following criteria will be excluded from participating in the study:</p> <ol style="list-style-type: none"> 1. Currently pregnant or lactating. 2. Any active or ongoing ocular or systemic allergies that may interfere with contact lens wear. 3. Any active or ongoing systemic disease, autoimmune disease, or use of medication, which may interfere with contact lens wear. This may include, but not be limited to, diabetes, hyperthyroidism, Sjögren's syndrome, xerophthalmia, acne rosacea, Stevens-Johnson



	<p>syndrome, and immunosuppressive diseases or any infectious diseases (e.g. hepatitis, tuberculosis).</p> <ol style="list-style-type: none"> 4. Clinically significant (Grade 3 or 4) corneal edema, corneal vascularization, corneal staining, tarsal abnormalities or bulbar injection, or any other corneal or ocular abnormalities which would contraindicate contact lens wear. 5. Entropion, ectropion, extrusions, chalazia, recurrent styes, dry eye, glaucoma, history of recurrent corneal erosions. 6. Any previous, or planned, ocular or intraocular surgery (e.g. radial keratotomy, PRK, LASIK, lid procedures, cataract surgery, retinal surgery, etc.). 7. A history of amblyopia, strabismus or binocular vision abnormality. 8. Any current ocular infection or inflammation. 9. Any current ocular abnormality that may interfere with contact lens wear. 10. Use of any of the following oral medications within 1 week prior to enrollment: oral retinoid isotretinoin (e.g. Accutane), oral tetracyclines, topical scopolamine, oral antihistamines (e.g., Chlor-Trimeton, and Benadryl), systemic steroids. 11. Use of any ocular medication, with the exception of rewetting drops. 12. History of herpetic keratitis. 13. Participation in any contact lens or lens care product clinical trial within 30 days prior to study enrollment. 14. Employee or immediate family member of an employee of clinical site (e.g., Investigator, Coordinator, Technician). 15. Any known hypersensitivity or allergic reaction to Optifree® Replenish® multi-purpose care solution or Eye-Cept® rewetting drop solution.
Disallowed Medications/Interventions	Use of any prescription or over-the-counter (OTC) medications that may affect contact lens wear.
Measurements and Procedures	See Section 7.2 for the detailed procedures.
Microbiology or Other Laboratory Testing	None

Study Termination	The occurrence of one or more Unanticipated Adverse Device Effect (UADE), or any SAE where relationship to study agent cannot be ruled out, will result in stopping further dispensing investigational product. In the event of a UADE or SAE, the Sponsor Medical Monitor may unmask the treatment regimen of subject(s) and may discuss this with the Principal Investigator before any further subjects are enrolled.
Ancillary Supplies/ Study-Specific Materials	Eye-Cept Rewetting drops, lens cases, glass vials, saline, ETDRS light cabinet, logMAR charts, and Near logMAR charts. Optifree® Replenish® Contact Solution.
Principal Investigator(s) and Study Institution(s)/Site(s)	A full list of Principal Investigators, clinical sites, and institutions is kept separately from the Study Protocol and is included in the study Trial Master File.

Figure 1: Study Flowchart

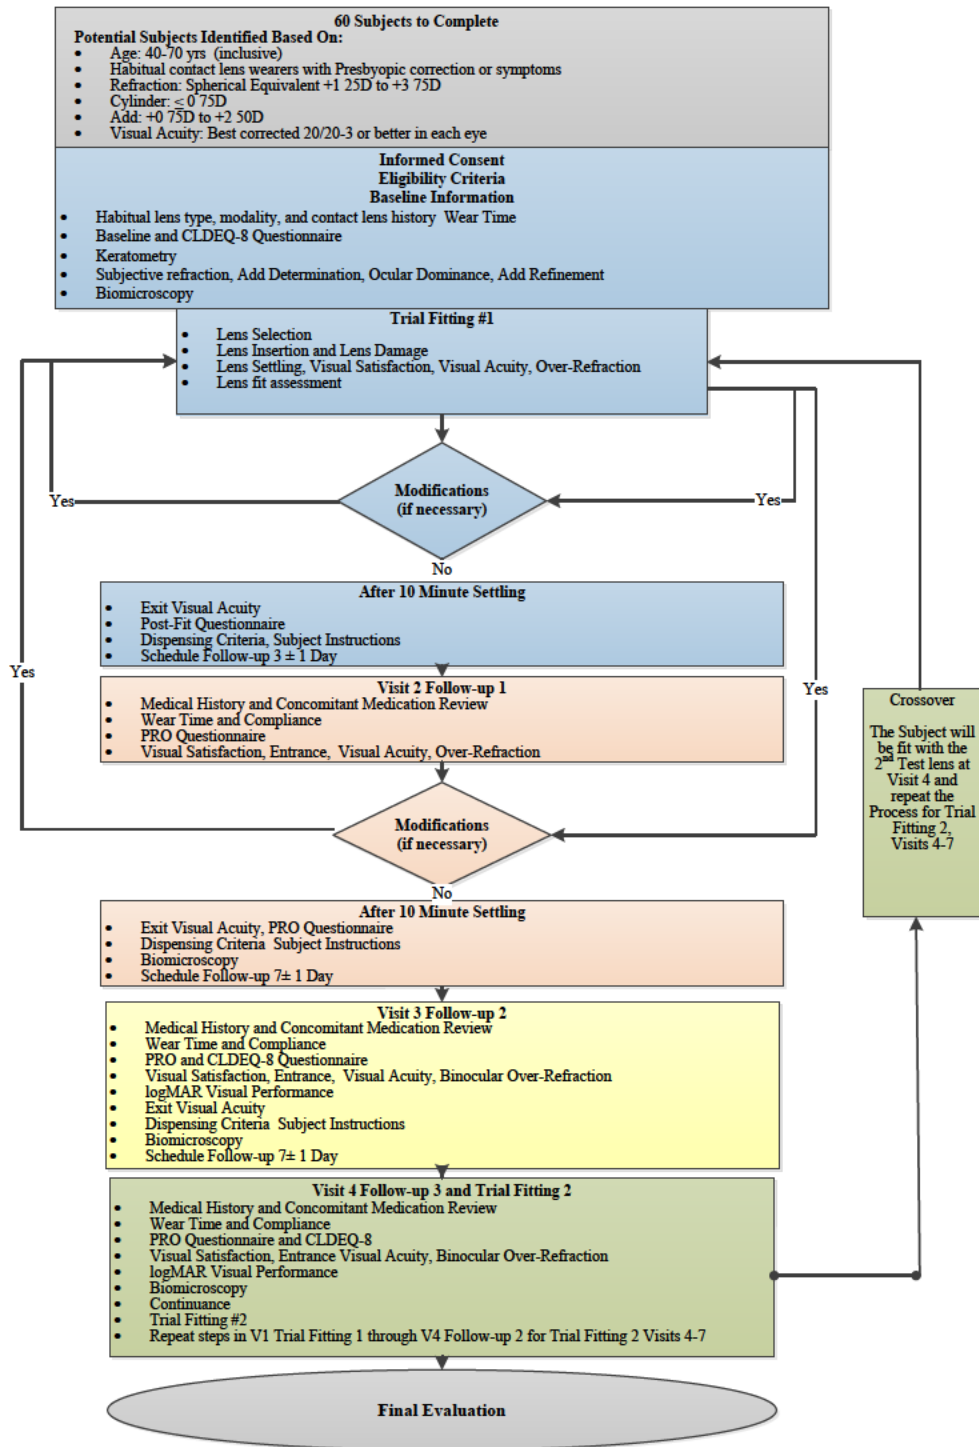

COMMONLY USED ABBREVIATIONS AND DEFINITIONS OF TERMS

ADD	Plus Power Required For Near Use
ADE	Adverse Device Effect
AE	Adverse Event/Adverse Experience
BCC	Binocular Crossed Cylinder
BCVA	Best Corrected Visual Acuity
BSCVA	Best Spectacle Corrected Visual Acuity
CFR	Code of Federal Regulations
CLDEQ-8	Contact Lens Dry Eye Questionnaire-8
CLUE	Contact Lens User Experience
COAS	Complete Ophthalmic Analysis System
COM	Clinical Operations Manager
CRA	Clinical Research Associate
CRF	Case Report Form
CRO	Contract Research Organization
CT	Center Thickness
	
D	Diopter
DMC	Data Monitoring Committee
eCRF	Electronic Case Report Form
EDC	Electronic Data Capture
ETDRS	Early Treatment Diabetic Retinopathy Study
FDA	Food and Drug Administration
GCP	Good Clinical Practice
HIPAA	Health Insurance Portability and Accountability Act
HIV	Human Immunodeficiency Virus
IB	Investigator's Brochure
ICF	Informed Consent Form
ICH	International Council for Harmonization
IDE	Investigational Device Exemption
IEC	Independent Ethics Committee
IRB	Institutional Review Board
ISO	International Organization for Standardization
ITT	Intent-to-Treat
JJVC	Johnson & Johnson Vision, Inc.
LC	Limbus Center
LogMAR	Logarithm of Minimal Angle of Resolution
LSM	Least Square Means
MedDRA [®]	Medical Dictionary for Regulatory Activities
MOP	Manual of Procedures
NIH	National Institutes of Health
OD	Right Eye
OHRP	Office for Human Research Protections
OHSR	Office for Human Subjects Research
OS	Left Eye
OU	Both Eyes

PD	Protocol Deviation
PHI	Protected Health Information
PI	Principal Investigator
PIG	Patient Instruction Guide
PQC	Product Quality Complaint
PRO	Patient Reported Outcome
QA	Quality Assurance
QC	Quality Control
SAE	Serious Adverse Event/Serious Adverse Experience
SAP	Statistical Analysis Plan
SAS	Statistical Analysis System
SD	Standard Deviation
SOP	Standard Operating Procedure
UADE	Unanticipated Adverse Device Effect
USADE	Unanticipated Serious Adverse Device Effect
VA	Visual Acuity

1. INTRODUCTION AND BACKGROUND

Johnson & Johnson Vision recently launched a multifocal contact lens, 1-DAY ACUVUE® Moist Multifocal. The lens is the only marketed soft multifocal lens to have its optical design optimized for the changes that occur in pupil size with refractive error. The modality for the lens is daily disposable. There is a desire to evaluate the same optical design in a reusable modality. The purpose of this study is to evaluate a multifocal optical design manufactured from senofilcon-A material and compare the visual performance to the 1-DAY ACUVUE® Moist Multifocal.

1.1. Name and Descriptions of Investigational Products

Test Lens: JJV Investigational senofilcon-A Multifocal Contact Lens-The lens has the same optical design, diameter, base curve and aspheric back surface design as the 1-Day Acuvue® Moist Brand Multifocal. The lens is manufactured in senofilcon-A.

Control Lens: Marketed 1-Day Acuvue® Moist Brand Multifocal Contact Lenses

1.2. Intended Use of Investigational Products

Both lenses are intended to correct spherical refractive error and presbyopia. The Test lenses are intended to be used as a 2-week, reusable, daily wear lens. The lenses require use of a care system to clean and disinfect the lenses. The control lenses are daily wear lenses that are disposed of at the end of each wear cycle. No care system is required for the control lenses.

1.3. Summary of Findings from Nonclinical Studies

All previous pre-clinical findings were deemed satisfactory prior to proceeding with clinical trials on humans. For the most comprehensive nonclinical information regarding JJV investigational senofilcon-A multifocal refer to the latest version of the Investigator Brochure.

1.4. Summary of Known Risks and Benefits to Human Subjects

The Investigational multifocal contact lenses are designed as a continuous asphere providing for the correction of refractive spherical ametropia and presbyopia. The material is a silicone hydrogel material, senofilcon-A.

The 1-Day Acuvue® Moist Brand Multifocal Contact Lens is a currently marketed product that is made of the etafilcon-A material. The contact lenses are available as continuous aspheres providing for the correction of a subjects refractive spherical ametropia and presbyopia.

The intent of the Test lens is daily wear, reusable lens that the subject wears while awake. This lens is not intended for extended wear. Anticipated risks and adverse reactions with this lens are similar to other soft daily wear contact lenses used to correct presbyopia. A listing of examples of adverse reactions is found in the Section 13 of this protocol. The investigator should follow normal clinical guidelines regarding examination and care of subjects who participate in this trial. For the most comprehensive clinical information regarding the JJV

2. STUDY OBJECTIVES, ENDPOINTS AND HYPOTHESES

2.1. Objectives

This study is an evaluation of the visual performance, subjective response, lens fit and ocular physiological response of the JJV Investigational senofilcon A Multifocal Contact Lens. The Test lenses will be compared to the 1-Day Acuvue® Moist Brand Multifocal Contact Lens manufactured in etafilcon A material for CLUE subjective vision.

Primary Objective

This study is an evaluation of how the subjective response of the JJV Investigational senofilcon A Multifocal Contact Lens compares to the 1-Day Acuvue® Moist Brand Multifocal Contact Lens manufactured in etafilcon A material.

2.2. Endpoints

The study endpoints will be the subjective CLUE Vision scores. Additional endpoints will be logMAR visual acuity at distance, intermediate and near a summary of lenses needed to fit (optimize) the subject, CLUE comfort/handling scores, the lens fit and ocular physiological responses.

Primary Endpoints

- CLUE vision scores

Other Observation(s)

- LogMAR visual acuity scores
- Lens fit
- Corneal staining
- Ocular redness (bulbar and limbal)
- Summary of lenses needed to fit (optimize) the subject
- CLUE comfort/handling scores
- PRO individual questions

2.3. Hypotheses

The following primary hypothesis will be tested throughout this investigation.

Primary Hypothesis:

1. After 14 to 20 days of wear, the PRO CLUE vision score for the Test lenses will be statistically better than 32 points. This will be recorded by the subject using the CLUE Follow-up Questionnaire.

If the primary hypothesis is met, the following secondary hypothesis will be tested.

Secondary Hypothesis:

1. After 14 to 20 days of wear, the PRO CLUE vision score for the Test lenses will be non-inferior to the control lens. A non-inferiority margin of 5 CLUE points will be used. This will be recorded by the subject using the CLUE Follow-up Questionnaire.

3. TARGETED STUDY POPULATION

3.1. General Characteristics

Healthy male and female subjects who are habitual soft contact lens wearers will be recruited. Subjects will be at least 40 years of age and not older than 70 years of age. They will be hyperopic and have presbyopia.

3.2. Inclusion Criteria

Potential subjects must satisfy all the following criteria to be enrolled in the study:

1. The subject must read, understand, and sign the STATEMENT OF INFORMED CONSENT and receive a fully executed copy of the form.
2. The subject must appear able and willing to adhere to the instructions set forth in this clinical protocol.
3. The subject must be between 40 and 70 years of age (inclusive).
4. The subject's distance spherical equivalent refraction must be in the range of +1.25 D to +3.75 D in each eye.
5. The subject's refractive cylinder must be ≤ 0.75 D in each eye.
6. The subject's ADD power must be in the range of +0.75 D to +2.50 D.
7. The subject must have distance best corrected visual acuity of 20/20⁻³ or better in each eye.
8. Subjects must own a wearable pair of spectacles if required for their distance vision.
9. The subject must be an adapted soft contact lens wearer in both eyes (i.e. worn lenses a minimum of 2 days per week for at least 8 hours per wear day, for 1 month of more duration).
10. The subject must either already be wearing a presbyopic contact lens correction (e.g., reading spectacles over contact lenses, multifocal or monovision contact lenses, etc.) or if not respond positively to at least one symptom on the "Presbyopic Symptoms Questionnaire".

3.3. Exclusion Criteria

Potential subjects who meet any of the following criteria will be excluded from participating in the study:

1. Currently pregnant or lactating.
2. Any active or ongoing ocular or systemic allergies that may interfere with contact lens wear.
3. Any active or ongoing systemic disease, autoimmune disease, or use of medication, which may interfere with contact lens wear. This may include, but not be limited to, diabetes, hyperthyroidism, Sjögren's syndrome, xerophthalmia, acne rosacea,

- Stevens-Johnson syndrome, and immunosuppressive diseases or any infectious diseases (e.g. hepatitis, tuberculosis).
4. Clinically significant (Grade 3 or 4) corneal edema, corneal vascularization, corneal staining, tarsal abnormalities or bulbar injection, or any other corneal or ocular abnormalities which would contraindicate contact lens wear.
 5. Entropion, ectropion, extrusions, chalazia, recurrent styes, dry eye, glaucoma, history of recurrent corneal erosions.
 6. Any previous, or planned, ocular or intraocular surgery (e.g. radial keratotomy, PRK, LASIK, lid procedures, cataract surgery, retinal surgery, etc.).
 7. A history of amblyopia, strabismus or binocular vision abnormality.
 8. Any current ocular infection or inflammation.
 9. Any current ocular abnormality that may interfere with contact lens wear.
 10. Use of any of the following oral medications within 1 week prior to enrollment: oral retinoid isotretinoin (e.g. Accutane), oral tetracyclines, topical scopolamine, oral antihistamines (e.g., Chlor-Trimeton, and Benadryl), systemic steroids.
 11. Use of any ocular medication, with the exception of rewetting drops.
 12. History of herpetic keratitis.
 13. Participation in any contact lens or lens care product clinical trial within 30 days prior to study enrollment.
 14. Employee or immediate family member of an employee of clinical site (e.g., Investigator, Coordinator, Technician).
 15. Any known hypersensitivity or allergic reaction to Optifree® Replenish® multi-purpose care solution or Eye-Cept® rewetting drop solution.

3.4. Enrollment Strategy

Study subjects will be recruited from the Institution/clinical site's subject database and/or utilizing Independent Ethics Committee (IEC) or Institutional Review Board (IRB) approved materials.

4. STUDY DESIGN AND RATIONALE

4.1. Description of Study Design

The clinical study is a randomized-controlled, single-masked, cross-over clinical trial. There are two study treatments. A total of approximately 60 eligible hyperopic subjects will be targeted to complete the study. Each Test article will be dispensed for 3±1 days and an optimization visit will occur. The final lens pair will be dispensed for 7±1 days and the first follow-up on the final lens pair will occur. The lenses will be dispensed for an additional 7±1 days and the final lens measurements will be made. The second study lenses will then be fit and the above sequence repeated.

4.2. Study Design Rationale

The study is intended to compare two study lens types and the initial performance, in terms of the subjective response after a period of lens dispensing. The lenses are dispensed to determine the subjective responses and the comparison is made after a total of 14-20 days of wear.

The cross-over study design was chosen to control for variables that may impact the lens performance between subjects. It was determined that a washout was not required as previous studies on similar populations with similar multifocal designs did not show a significant carry over effect on the primary/secondary endpoints measured in the study.

4.3. Enrollment Target and Study Duration

A total of approximately 70 eligible subjects will be enrolled with 60 targeted to complete the study.

5. TEST ARTICLE ALLOCATION AND MASKING

5.1. Test Article Allocation

The study lenses will be worn in a bilateral and random fashion using a 2×2 crossover design with 2 lens types and 2 periods. Using a computer-generated randomization scheme provided by the study biostatistician, each subject will randomly be assigned to one of two unique sequences (Test/Control or Control/Test). Randomization will be stratified by site.

Permuted block randomization will be used to avoid bias in the assignment of subjects to treatment, and to enhance the validity of statistical comparisons across treatment groups. Each block will contain two different lens trial sequences.

The order of lens wear will be based on the randomization scheme assigned to the study site. The study site will follow the randomization scheme provided and will complete enrollment according to the randomization list and will not pre-select or assign subjects.

5.2. Masking

This is a single-masked study with the subjects being masked. Subjects will be unaware of the identity of the investigational product. Investigators and clinical site personnel involved in the data collection will not be masked as to the identity of the investigational product.

Under normal circumstances, the mask should not be broken until all subjects have completed the study and the database is finalized. Otherwise, the mask should be broken only if specific emergency treatment/course of action would be dictated by knowing the treatment status of the subject. In such cases, the Investigator may, in an emergency, contact the medical monitor. In the event the mask is broken, the Sponsor must be informed as soon as possible. The date, time, and reason for the unmasking must be documented in the subject record. The Investigator is also advised not to reveal the study treatment assignment to the clinical site or Sponsor personnel.

Subjects who have had their treatment assignment unmasked are expected to return for all remaining scheduled evaluations. Subjects who are discontinued may be replaced.

5.3. Procedures for Maintaining and Breaking the Masking

The test articles mask shall not be broken unless information concerning the lens type is necessary for the urgent medical treatment of a subject. The Sponsor must be notified before the mask is broken.

When dispensing test articles, the following steps should be followed to maintain randomization codes:



1. Investigator or designee (documented on the Delegation Log) will consult the lens fitting schedule/randomization scheme to obtain the test article assignment for that subject prior to dispensing
2. Investigator or designee will record the subject's number on the appropriate line of the randomization scheme if applicable
3. Investigator or designee will pull the appropriate test articles from the study supply. All test articles that are opened, whether dispensed (placed/fit on eye or dispensed outside the clinical site) or not, must be recorded on the Test Article Accountability Log in the "Dispensed" section

6. STUDY INTERVENTION

6.1. Identity of Test Articles

The following contact lenses will be used in this study:

Table 1: Test Articles

	Test		Control	
Name	JJV Investigational Multifocal Contact Lens	ACUVUE OASYS® 2-WEEK with HYDRACLEAR® PLUS	1-Day Acuvue® Moist Brand Multifocal Contact Lens	1-Day Acuvue® Moist Brand Contact Lens
Manufacturer	Johnson & Johnson® Vision, Inc.	Johnson & Johnson® Vision, Inc.	Johnson & Johnson® Vision, Inc.	Johnson & Johnson® Vision, Inc.
		Over labeled	Over labeled	Over labeled
Lens Material	senofilcon A	senofilcon A	etafilcon A	etafilcon A
Nominal Base Curve @ 22 °C	8.35 mm	8.4	8.4 mm	8.5
Nominal Diameter @ 22 °C	14.3 mm	14.0	14.3mm	14.2
Nominal Distance Powers (D)	+1.00 D to +4.00 D in 0.25 D steps	+1.00 D to +4.00 D in 0.25 D steps	+1.00 D to +4.00 D in 0.25 D steps	+1.00 D to +4.00 D in 0.25 D steps

	Test		Control	
Nominal Cylinder Powers (D) and Axes	None	None	None	None
Nominal ADD Powers (D)	Low, Mid, High	None	Low, Mid, High	None
Water Content	38%	38%	58%	58%
Center Thickness	0.070 mm (-3.00 D)	0.070 mm (-3.00 D)	0.084 mm (-3.00 D)	0.084 mm (-3.00 D)
Oxygen Permeability (Dk)	122.0	122.0	28.0	28.0
Wear Schedule in Current Study	Daily Wear Reusable	Daily Wear Reusable	Daily Wear	Daily Wear
Replacement Frequency	Two Weeks	Two Weeks	Daily Disposable	Daily Disposable
Packaging Form (vial, blister, etc.)	Blister	Blister	Blister	Blister

6.2 Ancillary Supplies/Products

The following solutions will be used in this study:

Table 2: Ancillary Supplies


	Solution	
Solution Name/Description	Eye-Cept® Rewetting Drops	OPTI-FREE® Replenish® Multipurpose Disinfecting Solution
Manufacturer	Optics Laboratory	Alcon Laboratories
Preservative	Non-Preserved	Myristamidopropyl dimethylamine 0.0005% polyquaternium-1 0.001%

6.3. Administration of Test Articles

Test articles will be dispensed to subject meeting all eligibility requirements, including any dispensing requirements set forth in this clinical protocol. Subjects will be dispensed an adequate supply of test articles to complete the study. Lost or damaged test articles may be replaced at the discretion of the Investigator and/or the Sponsor.

6.4. Packaging and Labeling

The test articles will be packaged in blisters, as the primary packaging. The test article will be over-labeled to mask the subject to the identity of the lens. The test articles will be in investigational cartons sealed with a tamper evident seal, commercial cartons, or in plastic bags as the secondary packaging form. The sample study label is shown below:

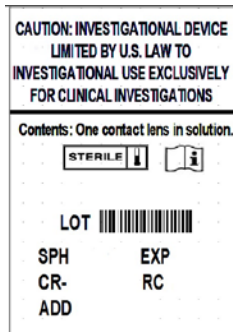

6.5. Storage Conditions

Test articles will be maintained at ambient temperatures at the clinical site. Test articles must be kept under secure conditions.

6.6. Collection and Storage of Samples

When possible, any lens or test article associated with an Adverse Events and/or a Product Quality Complaint must be retained and stored in a glass vial with moderate solution pending directions from the sponsor for potential return to JJV.

6.7. Accountability of Test Articles

JJV will provide the Investigator with sufficient quantities of study article and supplies to complete the investigation. The Investigator is asked to retain all lens shipment documentation for the test article accountability records.

Test article must be kept in a locked storage cabinet, accessible only to those assigned by the Investigator for dispensing. The Investigator may delegate this activity to authorized study site personnel listed on the Site Delegation Log. All test articles must be accounted. This includes:

1. What was dispensed for the subject for trial fitting, to wear out of the office, or issued for the subject to replace appropriately between visits
2. What was returned to the Investigator unused
3. The number and reason for unplanned replacements

The Investigator will collect all unused test articles from the subjects at the end of the subject's participation. Subject returned unused test articles must be separated from the clinical study inventory of un-dispensed test articles, and must be labeled with the subject number and date of return. Following final reconciliation of test articles by the monitor, the Investigator or monitor will return all unused test articles to the Sponsor.

If there is a discrepancy between the shipment documents and the contents, contact the study monitor immediately.

[REDACTED] Site Instructions for Test Article Receipt and Test Article Accountability for additional information

7. STUDY EVALUATIONS

7.1. Time and Event Schedule

Table 3: Time and Events

Visit Information	Visit 1 Screening, Baseline, Treatment 1	Visit 2 Treatment 1 Follow-up 1 Optimization	Visit 3 Treatment 1 Follow-up 2	Visit 4 Treatment 1 Follow-up 3 Treatment 2 Fitting	Visit 5 Treatment 2 Follow-up 1 Optimization	Visit 6 Treatment 2 Follow-up 2	Visit 7 Treatment 2 Follow-up 3
Time Point	Day 0	Day 3±1 from V1	Day 7±1 from V2	Day 7±1 from V3 Fitting Day 0	Day 3±1 from V4	Day 7±1 from V5	Day 7±1 from V6
Estimated Visit Duration	2.5 hours	1.0 hours	1.5 hours	2.5 hours	1.0 hours	1.5 hours	1.5 hours
Statement of Informed Consent	x						
Demographics	x						
Medical History/Concomitant Medications	x						
Adverse Events and Concomitant Medications Review		x	x	x	x	x	x
Compliance		x	x	x	x	x	x
Habitual Contact Lens Information	x						
Contact Lens History	x						

Visit Information	Visit 1 Screening, Baseline, Treatment 1	Visit 2 Treatment 1 Follow-up 1 Optimization	Visit 3 Treatment 1 Follow-up 2	Visit 4 Treatment 1 Follow-up 3 Treatment 2 Fitting	Visit 5 Treatment 2 Follow-up 1 Optimization	Visit 6 Treatment 2 Follow-up 2	Visit 7 Treatment 2 Follow-up 3
Time Point	Day 0	Day 3±1 from V1	Day 7±1 from V2	Day 7±1 from V3 Fitting Day 0	Day 3±1 from V4	Day 7±1 from V5	Day 7±1 from V6
Estimated Visit Duration	2.5 hours	1.0 hours	1.5 hours	2.5 hours	1.0 hours	1.5 hours	1.5 hours
Wear Time and Comfortable Wear Time with lenses	x	x	x	x	x	x	x
Screening Inclusion/Exclusion Criteria	x						
Subject Reported Ocular Symptoms	x	x	x	x	x	x	x
Baseline Questionnaire	x						
CLDEQ-8 Questionnaire	x		x	x		x	x
Distance and Near Entrance Visual Acuity	x	x	x	x	x	x	x
Lens Removal	x	x	x	x	x	x	x
Keratometry	x						
Subjective Refraction and Distance Visual Acuity	x						

Visit Information	Visit 1 Screening, Baseline, Treatment 1	Visit 2 Treatment 1 Follow-up 1 Optimization	Visit 3 Treatment 1 Follow-up 2	Visit 4 Treatment 1 Follow-up 3 Treatment 2 Fitting	Visit 5 Treatment 2 Follow-up 1 Optimization	Visit 6 Treatment 2 Follow-up 2	Visit 7 Treatment 2 Follow-up 3
Time Point	Day 0	Day 3±1 from V1	Day 7±1 from V2	Day 7±1 from V3 Fitting Day 0	Day 3±1 from V4	Day 7±1 from V5	Day 7±1 from V6
Estimated Visit Duration	2.5 hours	1.0 hours	1.5 hours	2.5 hours	1.0 hours	1.5 hours	1.5 hours
Near ADD Determination	x						
Ocular Dominance	x						
ADD Refinement	x						
Near Visual Acuity	x						
Biomicroscopy	x	x	x	x	x	x	x
Baseline Inclusion/Exclusion Criteria	x						
Continuance				x			
Lens Selection	x			x			
Lens Insertion	x	x	x	x	x	x	
10 Minute Settling	x	x		x	x		
Visual Satisfaction / Subjective Acceptance	x	x	x	x	x	x	x
Study Lens Distance and Near Visual Acuity	x	x	x	x	x	x	x
Distance Over	x	x		x	x		

Visit Information	Visit 1 Screening, Baseline, Treatment 1	Visit 2 Treatment 1 Follow-up 1 Optimization	Visit 3 Treatment 1 Follow-up 2	Visit 4 Treatment 1 Follow-up 3 Treatment 2 Fitting	Visit 5 Treatment 2 Follow-up 1 Optimization	Visit 6 Treatment 2 Follow-up 2	Visit 7 Treatment 2 Follow-up 3
Time Point	Day 0	Day 3±1 from V1	Day 7±1 from V2	Day 7±1 from V3 Fitting Day 0	Day 3±1 from V4	Day 7±1 from V5	Day 7±1 from V6
Estimated Visit Duration	2.5 hours	1.0 hours	1.5 hours	2.5 hours	1.0 hours	1.5 hours	1.5 hours
Refraction and Visual Acuity							
Subjective Lens Fit Assessment	x	x	x	x	x	x	x
Binocular Over Refraction			x	x		x	x
Visual Performance			x	x		x	x
Modifications	x	x		x	x		
Post-Fit Questionnaire	x	x		x	x		
Worn Lens Collection		x		x	x		x
PRO Questionnaire	x	x	x	x	x	x	x
Distance and Near Exit Visual Acuity	x	x	x	x	x	x	x
Dispensing Criteria	x	x	x	x	x	x	
Instructions	x	x	x	x	x	x	
Schedule Follow-up	x	x	x	x	x	x	
Final Evaluation							x

7.2. Detailed Study Procedures

VISIT 1

Subjects must report to the visit wearing their habitual contact lenses to accurately assess baseline CLUE performance. If the subject is not wearing their lenses they must be rescheduled.

Visit 1: Screening			
Step	Procedure	Details	
1.1	Statement of Informed Consent	Each subject must read, understand, and sign the Statement of Informed Consent before being enrolled into the study. The Principal Investigator or his/her designee conducting the informed consent discussion must also sign the consent form. Note: The subject must be provided a signed copy of this document.	
1.2	Demographics	Record the subject's age, gender, race and ethnicity.	
1.3	Medical History and Concomitant Medications	Questions regarding the subjects' medical history and concomitant medications.	
1.4	Habitual Lenses	Questions regarding the subject's habitual lens type and parameters.	
1.5	Contact Lens History	Record the subject's correction type (i.e. monovision, multifocal, sphere with readers, etc.).	
1.6	Wear time and Comfortable Wear time with Habitual lenses	Record the subjects wear time and comfortable wear time with their habitual contact lenses.	
1.7	Eligibility after Screening	All responses to Screening Inclusion Criteria questions must be answered "yes" and all responses to Exclusion Criteria must be answered "no" for the subject to be considered eligible.	

Visit 1: Baseline			
Step	Procedure	Details	
1.8	Baseline and CLDEQ-8 Questionnaires	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of their habitual lenses using the PRO questions.	

1.9	Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.	
1.10	Entrance Visual Acuity	Distance and near Snellen visual acuity will be measured for each eye with the subject's habitual contact lenses in place. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.	
1.11	Lens Removal	Have the subject remove their habitual lenses and store in an approved storage solution.	
1.12	Keratometry	Keratometry will be performed OD and OS and the steep and flat dioptric power and corresponding meridians recorded.	
1.13	Subjective Refraction and Distance Visual Acuity	An optimal, binocular balanced distance sphero-cylindrical refraction will be performed. Record the refraction and distance visual acuity to the nearest letter. <i>Note: Best distance visual acuity with sphero-cylindrical refraction must be at least 20/20³ in each eye for the subject to be eligible in the study.</i>	
1.14	Near ADD Determination	The near reading addition will be determined using the binocular crossed cylinder technique (BCC) at 40 cm followed by optimization in a trial frame in step 1.16 below.	
1.15	Ocular Dominance	Determine the distance ocular dominance with the best distance correction in place using a +1.00-blur test. If the results are equivocal use the sighting dominance test to determine the dominant eye used for the study.	Appendix F
1.16	ADD Refinement	Place the BCC result in the trial frame and refine the near prescription with trial lenses (or flippers) under binocular conditions.	
1.17	Near Visual Acuity	Using the ETDRS 2000 Series Chart 1 or 2 near card placed at 40 cm. Record the near visual acuity OD, OS and OU at 40 cm.	
1.18	Biomicroscopy	FDA Slit Lamp Classification Scale will be used to grade the findings and determine eligibility. For the conjunctival redness [REDACTED] 0.5 unit increments will be used in the grading. Corneal Staining Assessment [REDACTED] will be graded in 1.0 increments.	

		<p>If any of these slit lamp findings are Grade 3 or higher, the subject will be discontinued. If discontinued a final examination must be completed.</p> <p>If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.</p>	
1.19	Eligibility after Baseline	<p>All responses to Inclusion Criteria questions must be answered “yes” and all responses to Exclusion Criteria questions must be answered “no” for the subject to be considered eligible. If so, proceed to lens fitting. If not, complete the final evaluation and discharge the subject.</p>	

Visit 1: Treatment 1 Lens Fitting			
Step	Procedure	Details	
1.20	Randomization and Lens Wear Schedule	Record the randomization ID and lens wear schedule (daily disposable, daily reusable wear).	
1.21	Lens Selection	Select the lens pair and power based on the Randomization and fitting guide for each eye. Record the test lens parameters (power and lot number).	Appendix G and H (Fitting Guides)
1.22	Lens Insertion	<p>Subjects will insert the lenses themselves. If the lens is uncomfortable, inspect for damage and remove, reinsert or replace as necessary.</p> <p>Damaged lenses will be stored in labeled vial with sterile saline, and clearly differentiated from the other worn lenses that will be shipped back to the Sponsor. Complete the Quality Product Complaint form.</p>	
1.23	Lens Settling	Allow the study lenses to settle for a minimum of 10 minutes.	
1.24	Determine Visual Satisfaction	Determine if the subject’s vision is acceptable with the lenses. Allow the subject to look down a hallway or out of a window for distance vision assessments, and for them to read a book, magazine or similar for near vision.	
1.25	Study Lens Distance and Near Visual Acuity	<p>Measure the distance and near visual acuity OD, OS and OU. Record the results.</p> <p>Note: Use the ETDRS 2000 Series Chart 1 or</p>	

		2 near card placed at 40 cm to measure the Near visual acuity	
1.26	Distance Over-Refracton and Distance Visual Acuity	Perform a distance over-refraction OD and OS using loose lenses outside of the phoropter under ambient room illumination. The distance over-refraction may also be refined under binocular conditions. Record the results. The results of the distance over-refraction may also be checked for the impact on near vision under monocular and/or binocular conditions.	
1.27	Subjective Lens Fit Assessment	<p>Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test).</p> <ul style="list-style-type: none"> • The subject should not proceed to wear the lenses if any of the following is observed: • presence of limbal exposure (appearance of clear cornea) in any gaze • presence of edge lift • presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, upgaze, and push-up). <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp evaluation, and complete the Final Evaluation form.</i></p>	
1.28	Modifications	<p>If the subject reports unsatisfactory vision, or is unable to obtain 20/30 distance visual acuity OU with the lenses then a modification must be attempted. If the subject reports satisfactory vision with the lenses a modification is not required, however at the Investigator's discretion and based upon their findings on the measured visual acuity and/or over- refraction the investigator may make a modification. Up to two attempts at modification are permitted if necessary, in order to achieve an acceptable distance and near binocular performance for the subject, and to enable them to wear that particular lens type. Follow the fitting guide allowing for at least 10 minutes of settling time between each lens modification attempted.</p>	Appendix G and H (Fitting Guides)

		If modifications are required steps 1.21-1.27 will be repeated for each modification.	
1.29	Post-Fit Questionnaire	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
1.30	Distance and Near Exit Visual Acuity	Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU. Note: The distance visual acuity must be at least 20/30 OU for the lenses to be dispensed.	
1.31	Dispensing Criteria	The lenses will be dispensed for 2-4 days. <ul style="list-style-type: none"> Distance Snellen acuity equal to or better than 20/30 OU Subject must indicate that the vision is acceptable. Subject must indicate that the comfort of the lenses is acceptable. Lenses must have an acceptable general lens fit. 	
1.32	Patient Instructions for Daily Disposable Lenses	Instruct the Subject the following: <ul style="list-style-type: none"> The lenses will be worn on a daily wear basis. Only enough lenses will be dispensed to the subject to wear for the required number of days until their follow-up visit. No additional lenses will be dispensed. A new lens will be opened and worn each day. Instruct the subject to bring back all unworn study lenses. No cleaning or disinfecting solutions will be used. If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. 	

		<ul style="list-style-type: none"> • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. • A patient instruction booklet will be provided. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
1.33	Patient Instructions for Daily Reusable Wear Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • OPTI-FREE® Replenish® solution will be used in a rub regime to disinfect and store the lenses each night in the lens case provided. • If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. • A patient instruction booklet will be provided. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint</i></p>	

		<i>Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i>	
1.34	Schedule Follow-up	<p>The subject will be scheduled to return for their follow-up appointment in 3±1 day.</p> <p>Note: To count the follow-up visit as a day of wear the Subject must have worn the study lenses for 6 hours prior to the visit.</p>	

VISIT 2

The subjects must present to Visit 2 wearing the study lenses. To be counted as a day of wear the lenses need to have been worn for at least six (6) hours prior to the visit.

Visit 2: Treatment 1 Follow-up 1			
Step	Procedure	Details	
2.1	Adverse Events and Concomitant Medications Review	<p>Review the subject's concomitant medications and record any changes from the previous study visit.</p> <p>Record any adverse events or medical history changes from the previous study visit.</p>	
2.2	Wear Time	Record the hours the subject has worn the study lenses and the comfortable wear time on the day of follow-up.	
2.3	Compliance	<p>Record the subject's compliance with wearing the study lenses.</p> <p>Note: Subjects must have worn lenses for at least 6 hours per day To be counted as a day of wear at this visit the Subject must have worn the study lenses for 6 hours prior to the visit.</p>	
2.4	PRO Questionnaire	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
2.5	Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.	
2.6	Subjective Acceptance	Record whether the subjects distance and near vision with the lenses is acceptable.	
2.7	Distance and Near Entrance Visual Acuity	<p>Measure the distance and near visual acuity OD, OS and OU. Record the results.</p> <p>Note: Use the ETDRS 2000 Series Chart 1 or</p>	

		2 near card placed at 40 cm to measure the Near visual acuity	
2.8	Distance Over-Refracton and Distance Visual Acuity	Perform a distance over-refraction OD and OS using loose lenses outside of the phoropter under ambient room illumination. The distance over-refraction may also be refined under binocular conditions. Record the results and distance visual acuity OD and OS. The results of the distance over-refraction may also be checked for the impact on near vision under monocular and/or binocular conditions.	
2.9	Determination of Lens Optimization	<p>If the subject reports unsatisfactory vision, or is unable to obtain 20/30 distance visual acuity OU with the lenses then a modification must be attempted.</p> <p>If the subject reports satisfactory vision with the lenses a modification is not required, however at the Investigator's discretion and based upon their findings on the measured visual acuity and/or over- refraction the investigator may make a modification.</p> <p>Up to two attempts at modification are permitted if necessary, in order to achieve an acceptable distance and near binocular performance for the subject, and to enable them to wear that particular lens type.</p> <p>Follow the fitting guide allowing for at least 10 minutes of settling time between each lens modification attempted.</p>	Appendix G and H (Fitting Guides)
2.10	Lens Fit Assessment:	<p>Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test).</p> <ul style="list-style-type: none"> • The subject should not proceed to wear the lenses if any of the following is observed: • presence of limbal exposure (appearance of clear cornea) in any gaze • presence of edge lift • presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, upgaze, and push-up). <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp</i></p>	

		<i>evaluation, and complete the Final Evaluation form.</i>	
2.11	Collection of unworn lenses (if applicable)	<p>Collect unworn lenses returned by the subject when lens power has been optimized</p> <p>Note: If lens power was not changed allow the subject to use the unworn lenses dispensed at Visit 1 and dispense enough lenses of the same power to last the subject until their next visit.</p>	
2.12	Lens Removal	The study lenses will be removed and discarded.	
2.13	Biomicroscopy	<p>Perform biomicroscopy OD and OS. Slit Lamp Classification Scales will be used to grade the findings.</p> <p>For the conjunctival redness [REDACTED] 0.5 unit increments will be used in the grading. Corneal Staining Assessment (CTP-2003) will be graded in 1.0 increments.</p> <p>If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.</p>	[REDACTED]
2.14	Insertion of Study Lenses	Dispense the subject a new pair of lenses that match the distance and ADD power of the lenses that were removed in Step 2.12 above.	
2.15	PRO Questionnaire	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
2.16	Distance and Near Exit Visual Acuity	<p>Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place.</p> <p>For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.</p> <p>Note: The distance visual acuity must be at least 20/30 OU for the lenses to be dispensed.</p>	[REDACTED]
2.17	Dispensing Criteria	<p>The lenses will be dispensed for 7±1 day.</p> <ul style="list-style-type: none"> Distance Snellen acuity equal to or better than 20/30 OU Subject must indicate that the vision is acceptable. 	

		<ul style="list-style-type: none"> • Subject must indicate that the comfort of the lenses is acceptable. • Lenses must have an acceptable general lens fit. 	
2.18	Patient Instructions for Daily Disposable Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • Only enough lenses will be dispensed to the subject to wear for the required number of days until their follow-up visit. No additional lenses will be dispensed. • A new lens will be opened and worn each day. • Instruct the subject to bring back all unworn study lenses. • No cleaning or disinfecting solutions will be used. If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. • A patient instruction booklet will be provided. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
2.19	Patient Instructions for Daily Reusable Wear Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • OPTI-FREE® Replenish® solution will be 	

		<p>used in a rub regime to disinfect and store the lenses each night in the lens case provided.</p> <ul style="list-style-type: none"> • If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
2.20	Schedule Follow-up	<p>The subject will be scheduled to return for their follow-up appointment in 7±1 days.</p> <p><i>Note: To count the follow-up visit as a day of wear the Subject must have worn the study lenses for 6 hours prior to the visit.</i></p>	

VISIT 3

The subjects must present to Visit 3 wearing the study lenses. To be counted as a day of wear the lenses need to have been worn for at least six (6) hours prior to the visit.

Visit 3: Treatment 1 Follow-up 2			
Step	Procedure	Details	
3.1	Adverse Events and Concomitant Medications Review	<p>Review the subject's concomitant medications and record any changes from the previous study visit.</p> <p>Record any adverse events or medical history changes from the previous study visit.</p>	
3.2	Wear Time	Record the hours the subject has worn the	

		study lenses and the comfortable wear time on the day of follow-up.	
3.3	Compliance	Record the subject's compliance with wearing the study lenses. <i>Note: Subjects must have worn lenses for at least 6 hours per day To be counted as a day of wear at this visit the Subject must have worn the study lenses for 6 hours prior to the visit.</i>	
3.4	PRO and CLDEQ-8 Questionnaires	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
3.5	Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire	
3.6	Subjective Acceptance	Record whether the subjects distance and near vision with the lenses is acceptable.	
3.7	Distance and Near Entrance Visual Acuity	Measure the distance and near visual acuity OD, OS and OU. Record the results. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.	
3.8	Visual Performance Distance (3M) Intermediate (64 cm) Near (40 cm)	Visual performance will be recorded OU for the following: Distance, Bright Illuminance <i>ETDRS Charts 3M-HC#3 and LC#3</i> Near, Bright Illuminance <i>Reduced Guillon-Poling Charts Intermediate (64 cm) High Contrast (1 Chart) and Low Contrast (1 Chart). Near (40 cm) High Contrast (1 Chart) and Low Contrast (1 Chart).</i> Distance, Dim Illuminance (with <u>Distance</u> goggles) <i>ETDRS Charts 3M-HC#6</i> Near, Dim Illuminance (with <u>Near</u> goggles) <i>Reduced Guillon-Poling charts High Contrast (1 Chart at each distance) Intermediate (64 cm) and Near (40 cm).</i> Note:	

		<ul style="list-style-type: none"> • The room illuminance must be between 7.3 and 7.9 EV. • Distance, HC-1 Chart luminance Acceptable EV Range 10.5-10.7. • Guillon-Poling, Near Chart Luminance Acceptable EV Range 10.8-11.1. • Do not use the Mesopic filter for Dim luminance (Dim luminance will be simulated by using the goggles) 	
3.9	Binocular Distance Over-refraction and Distance Visual Acuity	<p>Perform a binocular over-refraction and record the OD and OS results and distance visual acuity.</p> <p>Note: No lens changes are allowed based on the over-refraction.</p>	Appendix D
3.10	Lens Fit Assessment:	<p>Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test).</p> <ul style="list-style-type: none"> • The subject should not proceed to wear the lenses if any of the following is observed: • presence of limbal exposure (appearance of clear cornea) in any gaze • presence of edge lift • presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, upgaze, and push-up). <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp evaluation, and complete the Final Evaluation form.</i></p>	
3.11	Lens Removal	<p>Have the subject wearing the daily disposable lenses remove and discard the lenses.</p> <p>Subjects that are wearing the daily wear lens will remove and temporarily store in a lens case in OPTI-FREE® Replenish® to be reinserted after biomicroscopy.</p>	
3.12	Biomicroscopy	<p>Perform biomicroscopy OD and OS. Slit Lamp Classification Scales will be used to grade the findings.</p> <p>For the conjunctival redness [REDACTED] 0.5</p>	

		<p>unit increments will be used in the grading. Corneal Staining Assessment [REDACTED] will be graded in 1.0 increments.</p> <p>If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.</p>	
3.13	Insertion of Study Lenses	<p>Dispense the subject new lenses if wearing the daily disposable lenses that match the Distance and ADD power of the lenses that were removed in Step 3.11 above.</p> <p>Subjects that are wearing the daily reusable wear lenses will reinsert the lenses that were temporarily stored.</p>	
3.14	Distance and Near Exit Visual Acuity	<p>Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place.</p> <p>For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.</p> <p>Note: The distance visual acuity must be at least 20/30 OU for the lenses to be dispensed.</p>	[REDACTED]
3.15	Dispensing Criteria	<p>The lenses will be dispensed for 7±1 day.</p> <ul style="list-style-type: none"> Distance Snellen acuity equal to or better than 20/30 OU Subject must indicate that the vision is acceptable. Subject must indicate that the comfort of the lenses is acceptable. Lenses must have an acceptable general lens fit. 	
3.16	Patient Instructions for Daily Disposable Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> The lenses will be worn on a daily wear basis. Only enough lenses will be dispensed to the subject to wear for the required number of days until their follow-up visit. No additional lenses will be dispensed. A new lens will be opened and worn each day. 	

		<ul style="list-style-type: none"> • Instruct the subject to bring back all unworn study lenses. • No cleaning or disinfecting solutions will be used. If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
3.17	Patient Instructions for Daily Reusable Wear Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • OPTI-FREE® Replenish® solution will be used in a rub regime to disinfect and store the lenses each night in the lens case provided. • If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site</i></p>	

		<i>for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i>	
3.18	Schedule Follow-up	<p>The subject will be scheduled to return for their follow-up appointment in 7±1 days.</p> <p>Note: To count the follow-up visit as a day of wear the Subject must have worn the study lenses for 6 hours prior to the visit.</p>	

VISIT 4

The subjects must present to Visit 4 wearing the study lenses. To be counted as a day of wear the lenses need to have been worn for at least six (6) hours prior to the visit.

Visit 4: Treatment 1 Follow-up 3			
Step	Procedure	Details	
4.1	Adverse Events and Concomitant Medications Review	<p>Review the subject's concomitant medications and record any changes from the previous study visit.</p> <p>Record any adverse events or medical history changes from the previous study visit.</p>	
4.2	Wear Time	Record the hours the subject has worn the study lenses and the comfortable wear time on the day of follow-up.	
4.3	Compliance	<p>Record the subject's compliance with wearing the study lenses.</p> <p>Note: Subjects must have worn lenses for at least 6 hours per day To be counted as a day of wear at this visit the Subject must have worn the study lenses for 6 hours prior to the visit.</p>	
4.4	PRO and CLDEQ-8 Questionnaires	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
4.5	Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.	
4.6	Distance and Near Entrance Visual	Distance and near Snellen visual acuity will be measured for each eye with the study contact	

	Acuity	lenses in place. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.	
4.7	Visual Performance Distance (3M) Intermediate (64 cm) Near (40 cm)	<p>Visual performance will be recorded OD, OS, and OU for the following:</p> <p>Distance, Bright Illuminance <i>ETDRS Charts 3M-HC#1, HC#2, HC#3 and LC#1, LC#2 and LC#3</i></p> <p>Near, Bright Illuminance <i>Reduced Guillon-Poling Charts High Contrast and Low Contrast Intermediate (64 cm) and Near (40 cm).</i></p> <p>Distance, Dim Illuminance (with <u>Distance</u> goggles) <i>ETDRS Charts 3M-HC#4, HC#5, HC#6</i></p> <p>Near, Dim Illuminance (with <u>Near</u> goggles) <i>Reduced Guillon-Poling charts</i> High Contrast Intermediate (64 cm) and Near (40 cm).</p> <p>Note:</p> <ul style="list-style-type: none"> • The room illuminance must be between 7.3 and 7.9 EV. • Distance, HC-1 Chart luminance Acceptable EV Range 10.5-10.7. • Guillon-Poling, Near Chart Luminance Acceptable EV Range 10.8-11.1. • Do not use the Mesopic filter for Dim luminance (Dim luminance will be simulated by using the goggles). 	
4.8	Binocular Distance Over-refraction and Distance Visual Acuity	Perform a binocular over-refraction and record the OD and OS results and distance visual acuity. Note: No lens changes are allowed based on the over-refraction.	Appendix D
4.9	Lens Fit Assessment:	<p>Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test).</p> <p>The subject should not proceed to wear the lenses if any of the following is observed:</p> <ul style="list-style-type: none"> • presence of limbal exposure (appearance of clear cornea) in any gaze 	

		<ul style="list-style-type: none"> • presence of edge lift • presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, upgaze, and push-up). <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp evaluation, and complete the Final Evaluation form.</i></p>	
4.10	Lens Removal	Have the subject remove the study lenses and store in saline in a labeled glass vial. Note: Lenses do not need to be stored in a refrigerator.	
4.11	Biomicroscopy	<p>FDA Slit Lamp Classification Scale will be used to grade the findings and determine eligibility.</p> <p>For the conjunctival redness [REDACTED] 0.5 unit increments will be used in the grading. Corneal Staining Assessment [REDACTED]) will be graded in 1.0 increments.</p> <p>If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.</p>	[REDACTED]
4.12	Continuance	Determine whether the subject is eligible to continue in the study based on the examination findings.	

Visit 4: Treatment 2 Lens Fitting			
Step	Procedure	Details	
4.13	Lens Wear Schedule	Record the lens wear schedule (daily disposable, daily reusable wear).	
4.14	Lens Selection	Select the lens pair and power based on the Randomization and fitting guide for each eye. Record the Test lens parameters (power and lot number).	Appendix G and H (Fitting Guides)
4.15	Lens Insertion	<p>Subjects will insert the lenses themselves. If the lens is uncomfortable, inspect for damage and remove, reinsert or replace as necessary.</p> <p>Damaged lenses will be stored in labeled vial with sterile saline, and clearly differentiated</p>	

		from the other worn lenses that will be shipped back to the Sponsor. Complete the Quality Product Complaint form.	
4.16	Lens Settling	Allow the study lenses to settle for a minimum of 10 minutes.	
4.17	Determine Visual Satisfaction	Determine if the subject's vision is acceptable with the lenses. Allow the subject to look down a hallway or out of a window for distance vision assessments, and for them to read a book, magazine or similar for near vision.	
4.18	Study Lens Distance and Near Visual Acuity	Measure the distance and near visual acuity OD, OS and OU. Record the results. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.	
4.19	Distance Over-Refracton and Distance Visual Acuity	Perform a distance over-refraction OD and OS using loose lenses outside of the phoropter under ambient room illumination. The distance over-refraction may also be refined under binocular conditions. Record the results. The results of the distance over-refraction may also be checked for the impact on near vision under monocular and/or binocular conditions.	
4.20	Subjective Lens Fit Assessment	<p>Evaluate overall lens fit acceptance (acceptable or unacceptable) based on centration, movement and other fitting characteristics.</p> <p>An unacceptable fit is deemed by one of the following criteria:</p> <ul style="list-style-type: none"> • limbal exposure at primary gaze or with extreme eye movement; • edge lift; • excessive movement in primary and up gaze; or • insufficient movement in all three of the following conditions: primary gaze, up gaze, and Josephson push up. <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp evaluation, and complete the Final Evaluation form.</i></p>	
4.21	Modifications	If the subject reports unsatisfactory vision, or is unable to obtain 20/30 distance visual acuity	Appendix G (Fitting

		<p>OU with the lenses then a modification must be attempted.</p> <p>If the subject reports satisfactory vision with the lenses a modification is not required, however at the Investigator's discretion and based upon their findings on the measured visual acuity and/or over-refraction the investigator may make a modification.</p> <p>Up to two attempts at modification are permitted if necessary, in order to achieve an acceptable distance and near binocular performance for the subject, and to enable them to wear that particular lens type. Follow the fitting guide allowing for at least 10 minutes of settling time between each lens modification attempted.</p> <p>If modifications are required steps 4.14-4.20 will be repeated for each modification</p>	Guide)
4.22	Post-Fit Questionnaire	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
4.23	Distance and Near Exit Visual Acuity	<p>Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place.</p> <p>For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.</p> <p>Note: The distance visual acuity must be at least 20/30 OU for the lenses to be dispensed.</p>	
4.24	Dispensing Criteria	<p>The lenses will be dispensed for 2-4 days.</p> <ul style="list-style-type: none"> Distance Snellen acuity equal to or better than 20/30 OU Subject must indicate that the vision is acceptable. Subject must indicate that the comfort of the lenses is acceptable. Lenses must have an acceptable general lens fit. 	
4.25	Patient Instructions for Daily Disposable Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> The lenses will be worn on a daily wear basis. 	

		<ul style="list-style-type: none"> • Only enough lenses will be dispensed to the subject to wear for the required number of days until their follow-up visit. No additional lenses will be dispensed. • A new lens will be opened and worn each day. • Instruct the subject to bring back all unworn study lenses. • No cleaning or disinfecting solutions will be used. If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. • A patient instruction booklet will be provided. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
4.26	Patient Instructions for Daily Reusable Wear Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • OPTI-FREE® Replenish® solution will be used in a rub regime to disinfect and store the lenses each night in the lens case provided. • If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses 	

		<p>for a minimum of 6 hours a day, every day during the study.</p> <ul style="list-style-type: none"> • Subjects will be instructed to wear their glasses when not wearing the study lenses. • A patient instruction booklet will be provided. <p>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</p>	
4.27	Schedule Follow-up	<p>The subject will be scheduled to return for their follow-up appointment in 3±1 day.</p> <p>Note: To count the follow-up visit as a day of wear the Subject must have worn the study lenses for 6 hours prior to the visit.</p>	

VISIT 5

The subjects must present to Visit 5 wearing the study lenses. To be counted as a day of wear the lenses need to have been worn for at least six (6) hours prior to the visit.

Visit 5: Treatment 2 Follow-up 1			
Step	Procedure	Details	
5.1	Adverse Events and Concomitant Medications Review	<p>Review the subject's concomitant medications and record any changes from the previous study visit.</p> <p>Record any adverse events or medical history changes from the previous study visit.</p>	
5.2	Wear Time	Record the hours the subject has worn the study lenses and the comfortable wear time on the day of follow-up.	
5.3	Compliance	<p>Record the subject's compliance with wearing the study lenses.</p> <p>Note: Subjects must have worn lenses for at least 6 hours per day To be counted as a day of wear at this visit the Subject must have worn the study lenses for 6 hours prior to the visit.</p>	
5.4	PRO Questionnaire	The subject will evaluate the vision	

		characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
5.5	Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire	
5.6	Subjective Acceptance	Record whether the subjects distance and near vision with the lenses is acceptable.	
5.7	Distance and Near Entrance Visual Acuity	Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.	
5.8	Distance Over-Refracton and Distance Visual Acuity	Perform a distance over-refraction OD and OS using loose lenses outside of the phoropter under ambient room illumination. The distance over-refraction may also be refined under binocular conditions. Record the results and distance visual acuity OD and OS. The results of the distance over-refraction may also be checked for the impact on near vision under monocular and/or binocular conditions.	
5.9	Determination of Lens Optimization	If the subject reports unsatisfactory vision, or is unable to obtain 20/30 distance visual acuity OU with the lenses then a modification must be attempted. If the subject reports satisfactory vision with the lenses a modification is not required, however at the Investigator's discretion and based upon their findings on the measured visual acuity and/or over- refraction the investigator may make a modification. Up to two attempts at modification are permitted if necessary, in order to achieve an acceptable distance and near binocular performance for the subject, and to enable them to wear that particular lens type. Follow the fitting guide allowing for at least 10 minutes of settling time between each lens modification attempted.	Appendix G and H (Fitting Guides)
5.10	Lens Fit Assessment:	Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test). The subject should not proceed to wear the	

		<p>lenses if any of the following is observed:</p> <ul style="list-style-type: none"> • presence of limbal exposure (appearance of clear cornea) in any gaze • presence of edge lift • presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, upgaze, and push-up). <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp evaluation, and complete the Final Evaluation form.</i></p>	
5.11	Collection of unworn lenses (if applicable)	<p>Collect unworn lenses returned by the subject when lens power has been optimized</p> <p>Note: If lens power was not changed allow the subject to use the unworn lenses dispensed at Visit 4 and dispense enough lenses of the same power to last the subject until their next visit.</p>	
5.12	Lens Removal	The study lenses will be removed and discarded.	
5.13	Biomicroscopy	<p>Perform biomicroscopy OD and OS. Slit Lamp Classification Scales will be used to grade the findings.</p> <p>For the conjunctival redness [REDACTED] 0.5 unit increments will be used in the grading.</p> <p>Corneal Staining Assessment [REDACTED] will be graded in 1.0 increments.</p> <p>If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.</p>	[REDACTED]
5.14	Insertion of Study Lenses	Dispense the subject new lenses that match the distance and ADD power of the lenses that were removed in Step 5.12 above.	
5.15	PRO Questionnaire	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
5.16	Distance and Near Exit Visual Acuity	Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place.	[REDACTED]

		<p>For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.</p> <p>Note: The distance visual acuity must be at least 20/30 OU for the lenses to be dispensed.</p>	
5.17	Dispensing Criteria	<p>The lenses will be dispensed for 7±1 day.</p> <ul style="list-style-type: none"> • Distance Snellen acuity equal to or better than 20/30 OU • Subject must indicate that the vision is acceptable. • Subject must indicate that the comfort of the lenses is acceptable. • Lenses must have an acceptable general lens fit. 	
5.18	Patient Instructions for Daily Disposable Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • Only enough lenses will be dispensed to the subject to wear for the required number of days until their follow-up visit. No additional lenses will be dispensed. • A new lens will be opened and worn each day. • Instruct the subject to bring back all unworn study lenses. • No cleaning or disinfecting solutions will be used. If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably</i></p>	

		<p><i>possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
5.19	Patient Instructions for Daily Reusable Wear Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • OPTI-FREE® Replenish® solution will be used in a rub regime to disinfect and store the lenses each night in the lens case provided. • If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
5.20	Schedule Follow-up	<p>The subject will be scheduled to return for their follow-up appointment in 7±1 days.</p> <p><i>Note: To count the follow-up visit as a day of wear the Subject must have worn the study lenses for 6 hours prior to the visit.</i></p>	

VISIT 6

The subjects must present to Visit 6 wearing the study lenses. To be counted as a day of wear the lenses need to have been worn for at least six (6) hours prior to the visit.

Visit 6: Treatment 2 Follow-up 2			
Step	Procedure	Details	
6.1	Adverse Events and Concomitant Medications Review	Review the subject's concomitant medications and record any changes from the previous study visit. Record any adverse events or medical history changes from the previous study visit.	
6.2	Wear Time	Record the hours the subject has worn the study lenses and the comfortable wear time on the day of follow-up.	
6.3	Compliance	Record the subject's compliance with wearing the study lenses. <i>Note: Subjects must have worn lenses for at least 6 hours per day To be counted as a day of wear at this visit the Subject must have worn the study lenses for 6 hours prior to the visit.</i>	
6.4	PRO Questionnaires and CLDEQ-8	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
6.5	Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire	
6.6	Subjective Acceptance	Record whether the subjects distance and near vision with the lenses is acceptable.	
6.7	Distance and Near Entrance Visual Acuity	Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.	
6.8	Visual Performance Distance (3M) Intermediate (64 cm) Near (40 cm)	Visual performance will be recorded OU for the following: Distance, Bright Illuminance <i>ETDRS Charts 3M-HC#3 and LC#3</i> Near, Bright Illuminance <i>Reduced Guillon-Poling Charts Intermediate (64 cm) High Contrast (1 Chart) and Low</i>	

		<p>Contrast (1 Chart). Near (40 cm) High Contrast (1 Chart) and Low Contrast (1 Chart).</p> <p>Distance, Dim Illuminance (with <u>Distance</u> goggles) <i>ETDRS Charts 3M-HC#6</i></p> <p>Near, Dim Illuminance (with <u>Near</u> goggles) <i>Reduced Guillon-Poling charts</i></p> <p>High Contrast (1 Chart at each distance) Intermediate (64 cm) and Near (40 cm).</p> <p>Note:</p> <ul style="list-style-type: none"> • The room illuminance must be between 7.3 and 7.9 EV. • Distance, HC-1 Chart luminance Acceptable EV Range 10.5-10.7. • Guillon-Poling, Near Chart Luminance Acceptable EV Range 10.8-11.1. • Do not use the Mesopic filter for Dim luminance (Dim luminance will be simulated by using the goggles) 	
6.9	Binocular Distance Over-refraction and Distance Visual Acuity	<p>Perform a binocular over-refraction and record the OD and OS results and distance visual acuity. Note: No lens changes are allowed based on the over-refraction.</p>	Appendix D
6.10	Lens Fit Assessment:	<p>Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test).</p> <p>The subject should not proceed to wear the lenses if any of the following is observed:</p> <ul style="list-style-type: none"> • presence of limbal exposure (appearance of clear cornea) in any gaze • presence of edge lift • presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, upgaze, and push-up). <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp</i></p>	

		<i>evaluation, and complete the Final Evaluation form.</i>	
6.11	Lens Removal	<p>Have the subject wearing the daily disposable lenses remove and discard the lenses.</p> <p>Subjects that are wearing the daily reusable wear lens will remove and temporarily store in a lens case in OPTI-FREE® Replenish® to be reinserted after biomicroscopy.</p>	
6.12	Biomicroscopy	<p>Perform biomicroscopy OD and OS. Slit Lamp Classification Scales will be used to grade the findings.</p> <p>For the conjunctival redness [REDACTED] 0.5 unit increments will be used in the grading.</p> <p>Corneal Staining Assessment [REDACTED] will be graded in 1.0 increments.</p> <p>If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.</p>	[REDACTED]
6.13	Insertion of Study Lenses	<p>Dispense the subject new lenses if wearing the daily disposable lenses that match the Distance and ADD power of the lenses that were removed in Step 6.11 above.</p> <p>Subjects that are wearing the daily wear lenses will reinsert the lenses that were temporarily stored.</p>	
6.14	Distance and Near Exit Visual Acuity	<p>Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place.</p> <p>For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.</p> <p>Note: The distance visual acuity must be at least 20/30 OU for the lenses to be dispensed.</p>	[REDACTED]
6.15	Dispensing Criteria	<p>The lenses will be dispensed for 7±1 day.</p> <ul style="list-style-type: none"> Distance Snellen acuity equal to or better than 20/30 OU Subject must indicate that the vision is acceptable. Subject must indicate that the comfort of the lenses is acceptable. 	

		<ul style="list-style-type: none"> • Lenses must have an acceptable general lens fit. 	
6.16	Patient Instructions for Daily Disposable Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • Only enough lenses will be dispensed to the subject to wear for the required number of days until their follow-up visit. No additional lenses will be dispensed. • A new lens will be opened and worn each day. • Instruct the subject to bring back all unworn study lenses. • No cleaning or disinfecting solutions will be used. If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
6.17	Patient Instructions for Daily Reusable Wear Lenses	<p>Instruct the Subject the following:</p> <ul style="list-style-type: none"> • The lenses will be worn on a daily wear basis. • OPTI-FREE® Replenish® solution will be used in a rub regime to disinfect and store the lenses each night in the lens case provided. 	

		<ul style="list-style-type: none"> • If determined necessary by the Investigator sterile non-preserved rewetting drops may be dispensed to be used as needed for dryness. • Subjects will be instructed to wear lenses for a minimum of 6 hours a day, every day during the study. • Subjects will be instructed to wear their glasses when not wearing the study lenses. <p><i>Note: In the event a lens is lost or damaged, the subject will return to the investigator site for replacement. As much as reasonably possible, a damaged lens should be returned to the investigational site and then returned to the Sponsor. If lens damage is present, complete the Product Quality Complaint Form. The lens will be stored in labeled vial with sterile saline, and returned to the Sponsor.</i></p>	
6.18	Schedule Follow-up	<p>The subject will be scheduled to return for their follow-up appointment in 7±1 days.</p> <p><i>Note: To count the follow-up visit as a day of wear the Subject must have worn the study lenses for 6 hours prior to the visit.</i></p>	

VISIT 7

The subjects must present to Visit 7 wearing the study lenses. To be counted as a day of wear the lenses need to have been worn for at least six (6) hours prior to the visit.

Visit 7: Treatment 2 Follow-up 3			
Step	Procedure	Details	
7.1	Adverse Events and Concomitant Medications Review	<p>Review the subject's concomitant medications and record any changes from the previous study visit.</p> <p>Record any adverse events or medical history changes from the previous study visit.</p>	
7.2	Wear Time	Record the hours the subject has worn the study lenses and the comfortable wear time on the day of follow-up.	
7.3	Compliance	Record the subject's compliance with wearing the study lenses.	

		<p><i>Note: Subjects must have worn lenses for at least 6 hours per day To be counted as a day of wear at this visit the Subject must have worn the study lenses for 6 hours prior to the visit.</i></p>	
7.4	PRO and CLDEQ-8 Questionnaires	The subject will evaluate the vision characteristics, comfort characteristics, handling characteristics, and visual symptoms of the study lenses using the PRO questionnaire.	
7.5	Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.	
7.6	Distance and Near Entrance Visual Acuity	<p>Distance and near Snellen visual acuity will be measured for each eye with the study contact lenses in place.</p> <p>For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.</p>	
7.7	Visual Performance Distance (3 M) Intermediate (64 cm) Near (40 cm)	<p>Visual performance will be recorded OD, OS, and OU for the following:</p> <p>Distance, Bright Illuminance <i>ETDRS Charts 3M-HC#1, HC#2, HC#3 and LC#1, LC#2 and LC#3</i></p> <p>Near, Bright Illuminance <i>Reduced Guillon-Poling Charts High Contrast and Low Contrast Intermediate (64 cm) and Near (40 cm).</i></p> <p>Distance, Dim Illuminance (with <u>Distance</u> goggles) <i>ETDRS Charts 3M-HC#4, HC#5, HC#6</i></p> <p>Near, Dim Illuminance (with <u>Near</u> goggles) <i>Reduced Guillon-Poling charts</i> High Contrast Intermediate (64 cm) and Near (40 cm).</p> <p>Note:</p> <ul style="list-style-type: none"> • The room illuminance must be between 7.3 and 7.9 EV. • Distance, HC-1 Chart luminance Acceptable EV Range 10.5-10.7. • Guillon-Poling, Near Chart Luminance Acceptable EV Range 10.8-11.1 	

		<ul style="list-style-type: none"> Do not use the Mesopic filter for Dim luminance (Dim luminance will be simulated by using the goggles) 	
7.8	Binocular Distance Over-refraction and Distance Visual Acuity	<p>Perform a binocular over-refraction and record the OD and OS results and distance visual acuity.</p> <p>Note: No lens changes are allowed based on the over-refraction.</p>	Appendix D
7.9	Lens Fit Assessment:	<p>Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test).</p> <p>The subject should not proceed to wear the lenses if any of the following is observed:</p> <ul style="list-style-type: none"> presence of limbal exposure (appearance of clear cornea) in any gaze presence of edge lift presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, upgaze, and push-up). <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp evaluation, and complete the Final Evaluation form.</i></p>	
7.10	Lens Removal	<p>Have the subject remove the study lenses and store in saline in a labeled glass vial.</p> <p>Note: The lenses do not need to be stored in a refrigerator.</p>	
7.11	Biomicroscopy	<p>FDA Slit Lamp Classification Scale will be used to grade the findings and determine eligibility.</p> <p>For the conjunctival redness [REDACTED] 0.5 unit increments will be used in the grading. Corneal Staining Assessment [REDACTED] will be graded in 1.0 increments.</p> <p>If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.</p>	

FINAL EVALUATION

The final evaluation will ordinarily take place immediately following the last scheduled follow-up visit per the study protocol. It may also take place at any point the subject discontinues the study or is terminated from the study.

Final Evaluation			
Step	Procedure	Details	
F.1	Distance Subjective Sphero-cylindrical Refraction and Distance Exit Visual Acuity	An optimal, binocular balanced distance sphero-cylindrical refraction will be performed. Record the refraction and distance visual acuity to the nearest letter.	
F.2	Subject Disposition	Indicate if the subject completed the study successfully. If subject discontinued from the study indicate the reason.	

7.3. Unscheduled Visits

If, during the investigation, a subject requires an unscheduled visit to the clinical site, the following information will be collected at a minimum:

- Chief complaint prompting the visit. If the reason is an adverse event, the applicable eCRF for the adverse event must be completed and subject record completed as appropriate
- Date and time of the visit and all procedures completed at the unscheduled visit
- Review of adverse event and concomitant medications
- Documentation of any test article dispensed or collected from the subject, if applicable
- Slit lamp findings (using the Slit Lamp Classification Scale)

If the Investigator withdraws a subject from the study, the final study visit case report forms must be completed indicating the reason(s) why the subject was withdrawn. The subject record must be completed documenting the date and primary reason for withdrawal and the study CRA notified.

Any ocular and non-ocular Adverse Events that are ongoing at the time of the study visit will be followed by the Investigator, within licensure, until they have resolved, returned to pre-treatment status, stabilized, or been satisfactorily explained. If further treatment i.e., beyond licensure is required, the subject will be referred to the appropriate health care provider.

The following information will be collected during an unscheduled visit.

Unscheduled Visit			
Step	Procedure	Details	
U.1	Chief Complaints	Record the subject's chief complaints for reasons for the unscheduled visit	

Unscheduled Visit			
U.2	Adverse Events and Concomitant Medications Review	Review the subject's concomitant medications and record any changes from the previous study visit.	
U.3	Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.	
U.4	Entrance VA	Record the entrance distance and near visual acuity (OD, OS and OU) to the nearest letter. For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.	
U.5	Subjective Sphero-cylindrical Refraction	An optimal, binocular balanced distance sphero-cylindrical refraction will be performed. Record the refraction and distance visual acuity to the nearest letter.	
U.6	Biomicroscopy	FDA Slit Lamp Classification Scale will be used to grade the findings and determine eligibility. For the conjunctival redness [REDACTED] 0.5 unit increments will be used in the grading. Corneal Staining Assessment [REDACTED] will be graded in 1.0 increments. If the clearance of the fluorescein needs to be expedited, preservative-free rewetting drops or saline may be instilled.	
U.7	Lens Dispensing	Additional study lenses may be dispensed when required.	
U.8	Lens Fit Assessment:	Evaluate and grade lens centration, primary gaze movement, upgaze movement and tightness (push-up test). The subject should not proceed to wear the lenses if any of the following is observed: <ul style="list-style-type: none"> • presence of limbal exposure (appearance of clear cornea) in any gaze • presence of edge lift • presence of unacceptable movement (excessive or insufficient) in <u>all three</u> movement categories (primary gaze, 	

Unscheduled Visit			
		<p>upgaze, and push-up).</p> <p><i>If either lens is deemed unacceptable, the subject will be discontinued from the study. Remove the lenses, perform a slit-lamp evaluation, and complete the Final Evaluation form.</i></p>	
U.9	Exit Visual Acuity	<p>Record the subject's exit distance and near visual acuity (OD, OS and OU) to the nearest letter.</p> <p>For near measures use the ETDRS 2000 Series Chart 1 or 2. The acuity will be recorded to the nearest letter OD, OS and OU.</p>	

7.4. Laboratory Procedures

Not Applicable

8. SUBJECTS COMPLETION/WITHDRAWAL

8.1. Completion Criteria

Subjects are considered to have completed the study if they:

- provided informed consent
- they are eligible
- completed all study visits

8.2. Withdrawal/Discontinuation from the Study

A subject will be withdrawn from the study for any of the following reasons:

- Subject death during the study period
- Subject withdrawal of consent
- Subject not compliant to protocol
- Subject lost to follow-up
- Subject no longer meets eligibility criteria (e.g. the subject becomes pregnant)
- Subject develops significant or serious adverse events causing discontinuation of study lens wear
- Subjects who have experienced a Corneal Infiltrative Event (CIE)
- Investigator's clinical judgment regarding the subject safety reasons (that it is in the best interest of the subject to stop treatment)
- Subject missed two consecutive study visits
- Subject not compliant with study lens wear schedule
- Subject not successfully dispensed due to lack of efficacy and safety including poor vision, poor comfort or unacceptable fit

For discontinued subjects, the Investigator will:

- Complete the current visit (scheduled or unscheduled)
- Complete the Final Evaluation, indicating the reason that the subject was discontinued from the study
- Record the spherocylindrical refraction with best corrected distance visual acuity
- Collect used test article(s) (worn or brought to the visit) from the subject and discard them, unless otherwise stated in Section 7.2
- Collect all unused test article(s) from the subject

An additional subject may be enrolled if a subject discontinues from the study prematurely.

In cases where a subject is lost to follow-up, every possible effort must be made to contact the subject and determine the reason for discontinuation/withdrawal. The measures taken to follow up must be documented including two written attempts and a certified letter (or equivalent) as the final attempt.

9. PRE-STUDY AND CONCOMITANT INTERVENTION/MEDICATION

Concomitant medications will be documented during screening and updated during the study. Disallowed medications and therapies are medications or therapies that contraindicate contact lens wear. See the Exclusion criteria for specific details.

10. DEVIATIONS FROM THE PROTOCOL

Investigator will notify study sponsor upon identification of a protocol deviation. Major protocol deviations must be reported to the sponsor within 24 hours after discovery of the protocol deviation. The Investigator will report deviations per IRB/IEC requirements. All deviations will be tracked and corrective actions implemented as appropriate.

If it becomes necessary for the Investigator to implement a deviation in order to eliminate an immediate hazard to the trial subject, the Investigator may implement the deviation immediately without notification to the sponsor. Within 24 hours after the implemented deviation, the Investigator must notify and provide the rationale to the Sponsor and, as required, the IEC/IRB.

11. STUDY TERMINATION

If more than 2 subjects in the investigational soft contact lens group develop serious expected (e.g., definite or probable MK) or unexpected device related adverse events, the study will be suspended. Upon review and consultation with IRB, DMC, and JJV safety review committee, the study may be terminated. This potential stopping rule is established based on our trial involving approximately 200 subjects wearing the investigational soft contact lens for up to 3 years with an assumed MK rate that is below 0.2% per patient-year. The rate of 0.2% per patient year is the established rate for extended wear lenses in adults, which was requested by the FDA as a criterion for evaluating a contact lens for pediatric use in an FDA response to a

pre-IDE submission. To be conservative, 200 independent patient years were used in the calculation. The probability of observing 2 cases or more incidents of MK is 0.061, and 3 cases or more incidents of MK is 0.007 (given an MK rate of 0.2% per patient year).

The occurrence of one or more Unanticipated Serious Adverse Device Effect (USADE), or any SAE where the relationship to study agent cannot be ruled out, may result in stopping further dispensing of test article. In the event of a USADE or SAE, the Sponsor may unmask the treatment regimen for the subject(s) and will discuss this with the Investigator before any further subjects are enrolled.

The Sponsor will determine when a study will be stopped. The Principal Investigator always has the discretion to initiate stopping the study based on patient safety or if information indicates the study's results are compromised.

JJV reserves the right to terminate the study at any time for any reason. Additionally, the IEC/IRB reserves the right to terminate the study if an unreasonable risk is determined. The study can be terminated by the Principal Investigator at the individual clinical site due to specific clinical observations, if in their opinion, after a discussion with JJV, it is determined that it would be unwise to continue at the clinical site.

JJV (and the IEC/IRB and DMC, if applicable) will evaluate all adverse events. If it is determined that an adverse event presents an unreasonable risk, the investigation, or that part of the investigation presenting the risk, will be terminated, as soon as possible.

Should the study be terminated (either prematurely or as scheduled), the Investigator will notify the IEC/IRB and Regulatory Authority as required by local regulatory requirements.

12. PROCEDURE FOR HANDLING PRODUCT QUALITY COMPLAINTS

A Product Quality Complaint (PQC) refers to any written, electronic, or oral communication that alleges deficiencies related to the identity, quality, durability, reliability, safety, effectiveness or performance of test articles after they have been released for clinical trial use.

Potential complaints may come from a variety of sources including but not limited to subjects, clinical research associates (CRA), clinical operations managers (COM), medical monitors, and site personnel, etc. The following are not considered product quality complaints:

- Subject satisfaction inquiries reported via “Subjective Questionnaires” and “Patient Reported Outcomes (PRO)”
- Clinical test articles that are stored improperly or damaged after receipt at the investigational site
- Lens replacements that occur due to drops/fall-outs
- Damage deemed by clinicians or clinical staff to be caused by handling by the user, and not indicative of a quality deficiency (i.e. tears, rips, etc.), only in situations where there is no deficiency alleged by the subject

Within 24 hours of site personnel becoming aware that a PQC has occurred, the PQC must be recorded in the EDC system, which will trigger an automatic email notification to the appropriate COM/CRA and Clinical QA representative. In cases where the EDC system in use is not configured to send automatic notifications or when an EDC system is not used, the COM/CRA is responsible for notifying Clinical QA upon discovery that a PQC has occurred.

Upon receipt of the EDC notification, the COM/CRA will contact the study site to collect additional information which will include:

- Date the complaint was received/recorded in the EDC System (Date of Sponsor Awareness)
- Who received the complaint
- Study number
- Clinical site information (contact name, site ID, telephone number)
- Lot number(s)
- Unique Subject Identifier(s)
- Indication of who first observed complaint (site personnel or subject)
- OD/OS indication, along with whether the lens was inserted
- Any related AE number if applicable
- Detailed complaint description (scheduled/unscheduled visit, wear time, symptoms, resolution of symptoms, etc.)
- Eye Care Provider objective (slit lamp) findings if applicable
- Confirmation of product availability for return (and tracking information, if available), or rationale if product is not available for return [REDACTED]

Once a complaint is received, it will be assessed by the COM, CRA, or trained site personnel to determine if it is an Adverse Event/Serious Adverse Event (AE/SAE). If the complaint results in an AE/SAE, the COM/CRA, or trained site personnel will follow Section 13 of this protocol. If the AE/SAE was potentially the result of a product quality related deficiency, these procedures also apply and will be executed in parallel.

In some cases, a PQC form may be generated in EDC by the site in error. In this event, the PQC forms will be marked “Intentionally Left Blank” or “ILB”. Justification for ILB must be documented.

13. ADVERSE EVENTS

13.1. Definitions and Classifications

Adverse Event (AE) – An AE is “any untoward medical occurrence, unintended disease or injury, or untoward clinical signs (including abnormal laboratory findings) in subjects, users or other persons, whether or not related to the investigational medical device.

Note 1 to entry: This definition includes events related to the investigational medical device or the comparator.

Note 2 to entry: This definition includes events related to the procedures involved.

Note 3 to entry: For users or other persons, this definition is restricted to events related to investigational medical devices.”¹

An AE includes any condition (including a pre-existing condition) that:

1. Was not present prior to the study, but appeared or reappeared following initiation of the study
2. Was present prior to the study, but worsened during the study. This would include any condition resulting from concomitant illnesses, reactions to concomitant medications, or progression of disease states
3. Pregnancy must be documented as an adverse event and must be reported to the clinical monitor and to the Sponsor immediately upon learning of the event

Serious Adverse Event (SAE) – An SAE is any untoward medical occurrence that:

- Results in death
- Is life threatening
- Requires in-patient hospitalization or prolongation of existing hospitalization
- Results in persistent or significant disability/incapacity (e.g., a sight threatening event, a significant persistent or permanent change, impairment, damage, or disruption to the subject’s body)
- Is a congenital anomaly/birth defect
- Requires intervention to prevent permanent damage (the use of the test article resulting in a condition which requires medical or surgical intervention to preclude permanent impairment of the body structure or a body function). Important medical events that may not result in death, be life-threatening, or require hospitalization may be considered an SAE when, based upon appropriate medical judgment, they may jeopardize the patient or subject and may require medical or surgical intervention to prevent one of the outcomes listed in the above definition

Diagnoses and conditions that are considered Ocular Serious Adverse Events include, but not limited to:

- Microbial Keratitis (MK)
- Iritis (including cells in the anterior chamber)
- Permanent decrease in best spectacle corrected visual acuity equivalent to 2 acuity lines or greater
- Central Corneal Opacity
- Central Corneal Neovascularization
- Uveitis
- Endophthalmitis
- Hypopyon
- Hyphemia
- Penetration of Bowman’s Membrane
- Persistent Epithelial Defect
- Limbal cell Damage leading to Conjunctivalization

Significant Adverse Events – Those events that are usually symptomatic and warrant discontinuation (temporary or permanent) of the test article (excluding Serious Adverse Events).

Diagnoses and conditions that are considered Ocular Significant Adverse Events include, but not limited to the following:

- Contact Lens Induced Peripheral Ulcer (CLPU)
- Significant Infiltrative Events (SIE)
- Superior Epithelial Arcuate Lesions (SEALs)
- Any Temporary Loss of > 2 Lines of BSCVA
- Other Grade 3 or higher corneal findings, such as abrasions or edema
- Non-contact lens related corneal events - e.g. Epidemic Keratoconjunctivitis (EKC)
- Asymptomatic Corneal Scar
- Any corneal event which necessitates temporary lens discontinuation > 2 weeks

Non-Significant Adverse Events – Those conditions that are usually asymptomatic and usually do not warrant discontinuation (temporary or permanent) of the test article. However, the Investigator may choose to treat as a precautionary measure.

Diagnoses and conditions that are considered Ocular Non-Significant Adverse Events include, but not limited to the following:

- Non-significant Infiltrative Event (NSIE)
- Contact Lens Papillary Conjunctivitis (CLPC)
- Superficial Punctate Keratitis (SPK)
- Conjunctivitis: Bacterial, Viral, Allergic
- Blepharitis
- Meibomianitis
- Contact Dermatitis
- Localized Allergic Reactions
- Any corneal event not explicitly defined as serious or significant adverse event, which necessitates temporary lens discontinuation < 2 weeks

Adverse Device Effect (ADE) – An ADE is an “adverse event related to the use of an investigational medical device.

Note 1 to entry: This definition includes adverse events resulting from insufficient or inadequate instructions for use, deployment, implantation, installation, or operation, or any malfunction of the investigational medical device.

Note 2 to entry: This definition includes any event resulting from use error or from intentional misuse of the investigational medical device.”¹

Unanticipated Adverse Device Effect (UADE) – Any serious adverse effect on health or safety or any life-threatening problem or death caused by, or associated with, the test article, if that effect, problem, or death was not previously identified in nature, severity, or degree of incidence in the investigational plan, Investigator’s Brochure or protocol, or any other

unanticipated serious problem associated with the test article that relates to the rights, safety and welfare of subjects.

13.2. Assessing Adverse Events

In conjunction with the medical monitor, the Investigator will evaluate adverse events to ensure the events are categorized correctly. Elements of categorization will include:

- Seriousness/Classifications (see definition in Section 13.1)
- Causality or Relatedness – i.e. the relationship between the test article, study treatment or study procedures and the adverse event (not related; unlikely related; possibly related; related - see definition in Section 13.2.1)
- Adverse Event Severity – Adverse event severity is used to assess the degree of intensity of the adverse event (mild; moderate; severe for all events - see definition in Section 0)
- Outcome – not recovered or not resolved; recovering or resolving; recovered or resolved with sequelae; recovered or resolved; death related to adverse event; unknown
- Actions Taken – none; temporarily discontinued; permanently discontinued; other

13.2.1. Causality Assessment

Causality Assessment – A determination of the relationship between an adverse event and the test article. The test article relationship for each adverse event should be determined by the investigator using these explanations:

- Not Related- An adverse event that is not related to the use of the test article, study treatment or study procedures
- Unlikely Related – An adverse event for which an alternative explanation is more likely, e.g. concomitant treatment, concomitant disease(s), or the relationship of time suggests that a causal relationship is not likely
- Possibly Related – An adverse event that might be due to the use of the test article, or to the study treatment or study procedures. An alternative explanation, e.g. concomitant treatment, concomitant disease(s), is inconclusive. The relationship in time is reasonable. Therefore, the causal relationship cannot be excluded
- Related – An adverse event that is listed as a possible adverse effect (device) or adverse reaction (drug) and cannot be reasonably explained by an alternative explanation, e.g. concomitant treatment of concomitant disease(s). The relationship in time is very suggestive, e.g. it is confirmed by de-challenge and re-challenge

13.2.2. Severity Assessment

Severity Assessment – A qualitative assessment of the degree of intensity of an adverse event as determined by the Investigator or reported to him/her by the subject. The assessment of severity is made irrespective of test article, study treatment or study procedure relationship or seriousness of the event and should be evaluated according to the following scale:

- Mild – Event is noticeable to the subject, but is easily tolerated and does not interfere with the subject's daily activities

- Moderate – Event is bothersome, possibly requiring additional therapy, and may interfere with the subject's daily activities
- Severe – Event is intolerable, necessitates additional therapy or alteration of therapy and interferes with the subject's daily activities

13.3. Documentation and Follow-Up of Adverse Events

The recording and documenting of adverse events (ocular and non-ocular) begins when the subjects are exposed to the test article, study treatment or study procedure. Adverse events reported before the use of test article, start of study treatment, or study procedures will be recorded as medical history. However, if the condition deteriorates at any time during the study it will be recorded and reported as an AE. Unrelated medical events reported after the subject's exit from the study will be recorded as adverse events at the discretion of the Investigator.

Upon finding an adverse event, the Principal Investigator will document the condition in the subject record and in the eCRFs. He/she will complete the Adverse Event /eCRF.

Complete descriptions of all adverse events must be available in the subject record. All Adverse Events including local and systemic reactions not meeting the criteria for "serious adverse events" shall be captured on the appropriate case report form or electronic data system. All adverse events occurring while the subject is enrolled in the study must be documented appropriately regardless of relationship.

It is the Investigator's responsibility to maintain documentation of each reported adverse event. All adverse events will be followed in accordance with applicable licensing requirements. Such documentation will include the following:

- Adverse event (diagnosis not symptom)
- Drawings or photographs (where appropriate) that detail the finding (e.g., size, location, and depth, etc.)
- Date the clinical site was notified
- Date and time of onset
- Date and time of resolution
- Adverse event classification, severity, and relationship to test articles, as applicable
- Treatment regimen instituted, including concomitant medications prescribed, in accordance with applicable licensing requirements
- Any referral to another health care provider if needed
- Outcome, ocular damage (if any)
- Likely etiology
- Best corrected visual acuity at the discovery of the event and upon conclusion of the event

In addition, if an infiltrate(s) is present, he/she will complete the Corneal Infiltrate Assessment eCRF. Where necessary, a culture of the corneal lesion will be collected to determine if the infection is microbial in nature. If cultures are collected, the date of culture collection and laboratory utilized will be recorded.

Changes in the severity of an AE shall be documented to allow an assessment of the duration of the event at each level of intensity to be performed. Adverse events characterized as intermittent require documentation of the onset and duration of each episode. Changes in the assessment of relationship to the test article shall also be clearly documented.

Subjects who present with an adverse event shall be followed by the Investigator, within licensure, until all signs and symptoms have returned to pre-treatment status, stabilized, or been satisfactorily resolved. If further treatment beyond licensure is required, the patient will be referred to the appropriate health care provider. The Investigator will use his/her clinical judgment as to whether a subject reporting with an adverse event will continue in the study. If a subject is discontinued from the study, it will be the responsibility of the Investigator to record the reason for discontinuation. The Investigator will also document the adverse event appropriately and complete the Adverse Event eCRF. Any subjects with ongoing adverse events related to the test article, study treatment or study procedures, as of the final study visit date, should be followed to resolution of the adverse event or until referral to an appropriate health care provider, as recommended by the Investigator. Non-ocular adverse events that are not related to the test article, study treatment, or study procedures may be recorded as “ongoing” without further follow-up.

13.4. Reporting Adverse Events

The Investigator will notify the Sponsor of an adverse event by e-mail, facsimile, or telephone as soon as possible and no later than 24 hours from discovery for any serious /significant adverse events, and 2 days from discovery for any non-significant adverse event. In addition, a written report will be submitted by the Principal Investigator to the IEC/IRB according to their requirements (Section 13.4.2). The report will comment whether the adverse event was considered to be related to the test article, study treatment or study procedures.

13.4.1. Reporting Adverse Events to Sponsor

Serious/Significant Adverse Events

The Investigator will inform the sponsor of all serious/significant adverse events occurring during the study period as soon as possible by e-mail, fax, or telephone, but no later than 24 hours following discovery of the event. The Investigator is obligated to pursue and obtain information requested by the Sponsor in addition to that information reported on the eCRF. All subjects experiencing a serious/significant adverse event must be followed up and all outcomes must be reported.

When medically necessary, the Investigator may break the randomization code to determine the identity of the treatment that the subject received. The Sponsor and study monitor should be notified prior to unmasking the test articles.

In the event of a serious/significant adverse event, the Investigator must:

- Notify the Sponsor immediately

- Obtain and maintain in the subject's records all pertinent medical information and medical judgment for colleagues who assisted in the treatment and follow-up of the subject
- Provide the Sponsor with a complete case history which includes a statement as to whether the event was or was not related to the use of the test article
- Notify the IEC/IRB as required by the IEC/IRB reporting procedure according to national regulations

Unanticipated (Serious) Adverse Device Effect (UADE)

In the event of an Unanticipated (Serious) Adverse Device Effect (UADE), the Investigator will submit a report of the UADE to the Sponsor and IEC/IRB as soon as possible, but no later than 24 hours after the Investigator first learns of the effect. This report is in addition to the immediate notification mentioned above.

The Sponsor must conduct an evaluation of the UADE and must report the results of the evaluation to FDA, the IEC/IRB and participating Investigators within 10 working days after the Sponsor first receives notification of the effect.

Non-Serious Adverse Events

All non-serious adverse events, including non-serious adverse device effects, will be reported to the sponsor by the Investigator no later than 2 days from discovery.

13.4.2. Reporting Adverse Events to the Responsible IEC/IRB and Health Authorities

Adverse events that meet the IEC/IRB requirements for reporting must be reported within the IEC/IRB's written guidelines. Each clinical site will refer to and follow any guidelines set forth by their Approving IEC/IRB. Each clinical site will refer to and follow any guidelines set forth by their local governing Health Authorities.

The Sponsor will report applicable Adverse Events to the local health authorities according the written guidelines, including reporting timelines.

13.4.3. Event of Special Interest

None

13.5. Reporting of Pregnancy

Subjects reporting pregnancy (by self-report) during the study will be discontinued after the event is recorded as an Adverse Event. Once discontinued, pregnant participants and their fetuses will not be monitored for study related purposes. At the Investigator's discretion, the study participant may be followed by the Investigator through delivery. However, this data will not be collected as part of the clinical study database. Pregnant participants are not discontinued from contact lens or solution related studies for safety concerns, but due to general concerns relating to pregnancy and contact lens use. Specifically, pregnant women are discontinued due to fluctuations in refractive error and/or visual acuity that occur secondary to systemic hormonal changes, and not due to unforeseen health risks to the mother or fetus.

14. STATISTICAL METHODS

14.1. General Considerations

All data summaries and statistical analyses will be performed using the Statistical Analysis System (SAS) software Version 9.4 (SAS Institute, Cary, NC). Throughout the analysis of data, the results for each subject/eye will be used when available for summarization and statistical analysis. Unscheduled visits will be summarized separately and will be excluded from the statistical analysis.

Summary tables (Descriptive statistics and/or frequency tables) will be provided for all baseline variables, efficacy variables and safety variables as appropriate. Continuous variables will be summarized with descriptive statistics (n, mean, standard deviation [SD], median, minimum and maximum). Frequency count and percentage of subjects or eyes within each category will be provided for categorical data.

Summaries will be presented by study lens type and will be performed separately by completion status (Safety Population or Per-Protocol Population). All analyses will be conducted on per-protocol population (see Section 14.3).

14.2. Sample Size Justification

Using the POWER procedure in SAS 9.4, it required at least 59 hyperopic subjects to complete the study to satisfy both primary and secondary hypotheses with overall type I error 0.05 and power no less than 90%. At the end of this section, a summary table of the sample sizes required for each individual hypothesis is provided.

Primary Hypothesis:	Criteria	# of subjects needed	Power
CLUE Vision	>32	19	0.9
Secondary Hypothesis	Criteria	# of subjects needed	Power
CLUE Vision	Test-Control \geq -5	59	0.9

14.3. Analysis Populations

Safety Population:

All subjects who were administered any test article excluding subjects who drop out prior to administering any test article. At least one observation should be recorded.

Per-Protocol Population:

All subjects who have successfully completed all visits and did not substantially deviate from the protocol as determined by the trial cohort review committee prior to database hard lock (Per-Protocol Population). Justification of excluding subjects with protocol deviations in the Per-Protocol Population set will be documented in a memo to file.

Intent-to-Treat (ITT) Population:

All subjects regardless of actual treatment and subsequent withdrawal from study or deviation from protocol. At least one observation should be recorded.

14.4. Level of Statistical Significance

All planned analysis for this study will be conducted with an overall type I error rate of 5%.

14.5. Primary Analysis

Primary efficacy analysis:

CLUE Vision:

Overall quality of vision scores will be analyzed using a linear mixed model adjusting for baseline values as fixed covariates. The model will include the experimental design factors: sequence of lens wear, period, lens type, time point and interaction between lens and time point as fixed effects. The covariance between residual errors from the same subject across lens wearing periods/time point will be selected based on the finite-sample corrected Akaike's Information Criterion (Keselman et al. 1998)⁶. Covariance structures considered may include: Homogenous compound symmetry (CS) and Unstructured covariance structure (UN). The structure that returns the lowest Akaike Information Criteria Corrected (AICC) will be selected as the structure that best fit the data.

Primary Hypothesis:

Comparisons will be carried out using 95% confidence intervals constructed of least-square means (LSM) from the linear mixed models of CLUE vision scores for each study population. Statistically superiority will be concluded if the lower limit of the confidence intervals of the test lens are greater than 32 points.

Secondary Hypothesis:

Comparisons between the test lens and control lens at each time point (1 week and 2 weeks) will be carried out using 95% confidence intervals constructed of least-square means (LSM) differences (Test minus Control) from the linear mixed model. The non-inferiority of the test lens relative to the control will be concluded if the lower confidence limit of LSM difference is above the non-inferiority margin -5. The superiority will be established if the lower confidence limit is above 0.

In all models, the Kenward and Roger method (Kenward and Roger, 1997)⁷ will be used for the calculation of the denominator of degrees of freedom.

14.6. Secondary Analysis

See section 14.5.

14.7. Other Exploratory Analyses

Not Applicable

14.8. Interim Analysis

Not Applicable

14.9. Procedure for Handling Missing Data and Drop-Outs

Missing or spurious values will not be imputed. The count of missing values will be included in the summary tables and listings.

Subject dropout is expected to be one of the main reasons of missing data in this clinical trial. Past clinical trials don't provide the evidence that subject dropout is systematic or not-at-random. To evaluate the impact of missing data, sensitivity analysis will be conducted using multiple imputation methods if the proportion of subject dropout is greater than the 15%. The SAS/STAT procedures PROC MI and PROC MIANALYZE will be utilized with a parametric regression method used to make at least 5 imputations.

14.10. Procedure for Reporting Deviations from Statistical Plan

The analysis will be conducted according to that specified in above sections. There are no known reasons for which it is planned to deviate from these analysis methods. If for any reason a change is made, the change will be documented in the study report along with a justification for the change.

15. DATA HANDLING AND RECORD KEEPING/ARCHIVING

15.1. Electronic Case Report Form/Data Collection

The data for this study will be captured on electronic case report forms (eCRFs) using an EDC system (Bioclinica). An authorized data originator will enter study data into the eCRFs using the EDC system. Data collected on equipment that is not captured in EDC will be formatted to the specification of the JJV database manager and sent to JJV for analysis.

External Data Sources for this study include:

Not Applicable

The clinical data will be recorded on dedicated eCRFs specifically designed to match the study procedures for each visit. Once completed, the eCRFs will be reviewed for accuracy and completeness and signed by the Investigator. The sponsor or sponsor's representatives will be authorized to gain access to the subject recordation for the purposes of monitoring and auditing the study.

Edit checks, electronic queries, and audit trails are built into the system to ensure accurate and complete data collection. Data will be transmitted from the clinical site to a secure central database as forms are completed or updated, ensuring information accuracy, security, and confidentiality. After the final database lock, the Investigator will be provided with Individual Patient Profiles (IPP) including the full audit trail on electronic media in PDF format for all of the study data. The IPP must be retained in the study files as a certified copy of the source data for the study.

The content and structure of the eCRFs are compliant with ISO14155:2011.¹

15.2. Subject Record

At a minimum, subject record should be available for the following:

- subject identification
- eligibility
- study identification
- study discussion
- provision of and date of informed consent
- visit dates
- results of safety and efficacy parameters as required by the protocol
- a record of all adverse events
- follow-up of adverse events
- medical history and concomitant medication
- test article receipt/dispensing/return records
- date of study completion
- reason for early discontinuation of test article or withdrawal from the study, if applicable

The subject record is the eCRF or an external record. The author of an entry in the subject record must be identifiable. The first point of entry is considered to be the source record.

Adverse event notes must be reviewed and initialed by the Investigator.

16. DATA MANAGEMENT

16.1. Access to Source Data/Document

The Investigator/Institution will permit trial-related monitoring, audits, IEC/IRB review and regulatory inspection(s) by providing direct access to source data/documents. Should the clinical site be contacted for an audit by an IEC/IRB or regulatory authority, JJV must be contacted and notified in writing within 24 hours.

16.2. Confidentiality of Information

Information concerning the investigational product and patent application processes, scientific data or other pertinent information is confidential and remains the property of JJV. The Investigator may use this information for the purposes of the study only. It is understood by the Investigator that JJV will use information developed in this clinical study in connection with the development of the investigational product and therefore may disclose it as required to other clinical investigators and to regulatory agencies. In order to allow the use of the information derived from this clinical study, the Investigator understands that he/she has an obligation to provide complete test results and all data developed during this study to the Sponsor.

16.3. Data Quality Assurance

Steps will be taken to ensure the accuracy and reliability of data, include the selection of qualified investigators and appropriate clinical sites and review of protocol procedures with the Principal Investigator. The Principal Investigator, in turn, must ensure that all Sub-Investigators and clinical site personnel are familiar with the protocol and all study-specific procedures and have appropriate knowledge of the study article.

Training on case report form completion will be provided to clinical site personnel before the start of the study. The Sponsor will review case report forms for accuracy and completeness remotely during the conduct of the study, during monitoring visits, and after transmission to data management. Any data discrepancies will be resolved with the Investigator or designee, as appropriate.

Quality Assurance representatives from JJV may visit clinical sites to review data produced during the study and to access compliance with applicable regulations pertaining to the conduct of clinical trials. The clinical sites will provide direct access to study-related source data/documents and reports for the purpose of monitoring and auditing by JJV and for inspection by local and regulatory authorities.

17. MONITORING

The study monitors will maintain close contact with the Principal Investigator and the Investigator's designated clinical site personnel. The monitor's responsibilities will include:

- Ensuring that the investigation is being conducted according to the protocol, any subsequent amendments, and regulatory requirements are maintained
- Ensuring the rights and wellbeing of subjects are protected
- Ensuring adequate resources, including facilities, laboratories, equipment, and qualified clinical site personnel
- Ensuring that protocol deviations are documented with corrective action plans, as applicable
- Ensuring that the clinical site has sufficient test article and supplies
- Clarifying questions regarding the study
- Resolving study issues or problems that may arise
- Reviewing of study records and source documentation verification in accordance with the monitoring plan

18. ETHICAL AND REGULATORY ASPECTS

18.1. Study-Specific Design Considerations

Potential subjects will be fully informed of the risks and requirements of the study and, during the study, subjects will be given any new information that may affect their decision to continue participation. Subjects will be told that their consent to participate in the study is voluntary and may be withdrawn at any time with no reason given and without penalty or loss of benefits to which they would otherwise be entitled. Only subjects who are fully able

to understand the risks, benefits, and potential adverse events of the study, and provide their consent voluntarily will be enrolled.

18.2. Investigator Responsibility

The Principal Investigator is responsible for ensuring that the clinical study is performed in accordance with the signed agreement, the investigational plan, Section 4 of the ICH E6 guidelines on Good Clinical Practice (GCP),² and applicable regulatory requirements. GCP is an international ethical and scientific quality standard for designing, conducting, recording, and reporting studies that involve the participation of human subjects. Compliance with this standard provides public assurance that the rights, safety, and well-being of study subjects are protected, consistent with the principles of the Declaration of Helsinki 64th WMA General Assembly 2013³ and that the clinical study data are credible. The Investigator must maintain clinical study files in accordance with Section 8 of the ICH E6 guidelines on Good Clinical Practice (GCP),² and applicable regulatory requirements.

18.3. Independent Ethics Committee or Institutional Review Board (IEC/IRB)

Before the start of the study, the Investigator (or Sponsor when applicable) will provide the IEC/IRB with current and complete copies of the following documents (where applicable):

- Final protocol and, if applicable, amendments
- Sponsor-approved informed consent form (and any other written materials to be provided to the subjects)
- Investigator's Brochure (or equivalent information) and amendments
- Sponsor-approved subject recruitment materials
- Information on compensation for study-related injuries or payment to subjects for participation in the study
- Investigator's curriculum vitae, clinical licenses, or equivalent information (unless not required, as documented by IEC/IRB)
- Information regarding funding, name of the Sponsor, institutional affiliations, other potential conflicts of interest, and incentives for subjects
- Any other documents that the IEC/IRB requests to fulfill its obligation

This study will be undertaken only after IEC/IRB has given full approval of the final protocol, amendments (if any), the informed consent form, applicable recruiting materials, and subject compensation programs, and the Sponsor has received a copy of this approval. This approval letter must be dated and must clearly identify the documents being approved.

During the study, the Investigator (or Sponsor when applicable) will send the following documents to the IEC/IRB for their review and approval, where appropriate:

- Protocol amendments
- Revision(s) to informed consent form and any other written materials to be provided to subjects
- If applicable, new or revised subject recruitment materials approved by the Sponsor
- Revisions to compensation for study-related injuries or payment to subjects for participation in the study
- Investigator's Brochure amendments or new edition(s)

- Summaries of the status of the study (at least annually or at intervals stipulated in guidelines of the IEC/IRB)
- Reports of adverse events that are serious, unanticipated, and associated with the test articles, according to the IRB's requirements
- New information that may adversely affect the safety of the subjects or the conduct of the study
- Major protocol deviations as required by the IEC/IRB
- Report of deaths of subjects under the Investigator's care
- Notification if a new Investigator is responsible for the study at the clinical site
- Any other requirements of the IEC/IRB

For protocol amendments that increase subject risk, the amendment and applicable informed consent form revisions must be submitted promptly to the IEC/IRB for review and approval before implementation of the change(s).

At least once a year, the IEC/IRB will review and reapprove this clinical study. This request should be documented in writing.

At the end of the study, the Investigator (or Sponsor where required) will notify the IEC/IRB about the study completion. Documentation of this notification must be retained at the clinical site and a copy provided to the CRO or Sponsor as applicable.

18.4. Informed Consent

Each subject must give written consent according to local requirements after the nature of the study has been fully explained. The consent form must be signed before performance of any study-related activity. The consent form that is used must be approved by both the Sponsor and by the reviewing IEC/IRB. The informed consent is in accordance with principles that originated in the Declaration of Helsinki,³ current ICH² and ISO 14155¹ guidelines, applicable regulatory requirements, and Sponsor Policy.

Before entry into the study, the Investigator or an authorized member of the clinical site personnel must explain to potential subject the aims, methods, reasonably anticipated benefits, and potential hazards of the study, and any discomfort it may entail. Subjects will be informed that their participation is voluntary and that they may withdraw consent to participate at any time.

The subject will be given sufficient time to read the informed consent form and the opportunity to ask questions. After this explanation and before entry into the study, consent should be appropriately recorded by means of the subject's dated signature. After having obtained the consent, a copy of the informed consent form must be given to the subject.

The collection, processing and disclosure of personal data and medical information related to the Study Subject, and personal data related to Principal Investigator and any clinical site personnel (e.g., name, clinic address and phone number, curriculum vitae) is subject to compliance with the Health Information Portability and Accountability Act (HIPAA) in the United States⁵ and other applicable personal data protection and security laws and

regulations. Appropriate measures will be employed to safeguard these data, to maintain the confidentiality of the person's related health and medical information, to properly inform the concerned persons about the collection and processing of their personal data, to grant them reasonable access to their personal data and to prevent access by unauthorized persons.

All information obtained during the course of the investigation will be regarded as confidential. All personal data gathered in this trial will be treated in strictest confidence by Investigators, monitors, Sponsor's personnel and IEC/IRB. No data will be disclosed to any third party without the express permission of the subject concerned, with the exception of Sponsor personnel (monitor, auditor), IEC/IRB and regulatory organizations in the context of their investigation related activities that, as part of the investigation will have access to the CRFs and subject records.

18.5. Privacy of Personal Data

The collection and processing of personal data from subjects enrolled in this study will be limited to those data that are necessary to investigate the efficacy, safety, quality, and utility of the investigational product(s) used in this study.

These data must be collected and processed with adequate precautions to ensure confidentiality and compliance with applicable data privacy protection laws and regulations.

The Sponsor ensures that the personal data will be:

- processed fairly and lawfully
- collected for specified, explicit, and legitimate purposes and not further processed in a way incompatible with these purposes
- adequate, relevant, and not excessive in relation to said purposes
- accurate and, where necessary, kept current

Explicit consent for the processing of personal data will be obtained from the participating subject before collection of data. Such consent should also address the transfer of the data to other entities and to other countries.

The subject has the right to request through the Investigator access to his personal data and the right to request rectification of any data that are not correct or complete. Reasonable steps should be taken to respond to such a request, taking into consideration the nature of the request, the conditions of the study, and the applicable laws and regulations.

Appropriate technical and organizational measures to protect the personal data against unauthorized disclosures or access, accidental or unlawful destruction, or accidental loss or alteration must be put in place. Sponsor personnel whose responsibilities require access to personal data agree to keep the identity of study subjects confidential.

19. STUDY RECORD RETENTION

In compliance with the ICH/GCP guidelines,² the Investigator/Institution will maintain all CRFs and all subject records that support the data collected from each subject, as well as all study documents as specified in ICH/GCP² and all study documents as specified by the

applicable regulatory requirement(s). The Investigator/Institution will take measures to prevent accidental or premature destruction of these documents.

Essential documents must be retained until at least two (2) years after the last approval of a marketing application in an ICH region and until there are no pending or contemplated marketing applications in an ICH region or until at least two (2) years have elapsed since the formal discontinuation of clinical development of the investigational product. These documents will be retained for a longer period if required by the applicable regulatory requirements or instructed by the Sponsor. It is the responsibility of the Sponsor to inform the Investigator/Institution as to when these documents no longer need to be retained.

If the responsible Investigator retires, relocates, or for other reasons withdraws from the responsibility of keeping the study records, custody must be transferred to a person who will accept the responsibility. The Sponsor must be notified in writing of the name and address of the new custodian. Under no circumstance shall the Investigator relocate or dispose of any study documents before having obtained written approval from the Sponsor.

If it becomes necessary for the Sponsor or the appropriate regulatory authority to review any documentation relating to this study, the Investigator must permit access to such reports. If the Investigator has a question regarding retention of study records, he/she should contact JJV.

20. FINANCIAL CONSIDERATIONS

Remuneration for study services and expenses will be set forth in detail in the Clinical Research Agreement. The Research Agreement will be signed by the Principal Investigator and a JJV management representative prior to study initiation.

JJV reserves the right to withhold remuneration for costs associated with protocol violations such as:

- Continuing an ineligible subject in the study
- Scheduling a study visit outside the subject's acceptable visit range

JJV reserves the right to withhold final remuneration until all study related activities have been completed, such as:

- Query resolution
- Case Report Form signature
- Completion of any follow-up action items


21. PUBLICATION


This study will be registered on ClinicalTrials.gov by the Sponsor.


22. REFERENCES


1. ISO 14155:2011: Clinical Investigation of Medical Devices for Human Subjects — Good Clinical Practice. Available at: <https://www.iso.org/standard/45557.html>
2. International Conference on Harmonization Good Clinical Practice E6 (ICH-GCP). Available at: <http://www.ich.org/products/guidelines/efficacy/article/efficacy-guidelines.html>
3. Declaration of Helsinki - Ethical principles for Medical Research Involving Human Subjects. Available at: <https://www.wma.net/policies-post/wma-declaration-of-helsinki-ethical-principles-for-medical-research-involving-human-subjects/>
4. United States (US) Code of Federal Regulations (CFR). Available at: <https://www.gpo.gov/fdsys/browse/collectionCfr.action?collectionCode=CFR>
5. Health Information Portability and Accountability Act (HIPAA). Available at: <https://www.hhs.gov/hipaa/for-professionals/privacy/index.html>
6. Keselman HJ, Algina J, Kowalchuk RK, Wolfinger RD. A Comparison of Two Approaches for Selecting Covariance Structures in the Analysis of Repeated Measures. *Communications in Statistics—Simulation and Computation*. 1998;27:591-604.
7. Kenward MG, Roger JH. Small Sample Inference for Fixed Effects from Restricted Maximum Likelihood. *Biometrics*. 1997;53:983–997.


APPENDIX A: PATIENT REPORTED OUTCOMES (STUDY QUESTIONNAIRES)

























































































APPENDIX B : PATIENT INSTRUCTION GUIDE

Patient Instruction Guide will be provided separately.

APPENDIX C: PACKAGE INSERT (APPROVED PRODUCT)

ACUVUE OASYS®

1-DAY ACUVUE® MOIST MULTIFOCAL

1-DAY ACUVUE® MOIST

If vision is acceptable, perform a full lamp examination to assess adequate fit (centration and movement). If it is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (post dispensing and follow-up information in PATIENT MANAGEMENT).

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

TORIC FITTING GUIDELINES

Although most aspects of the fitting procedure are identical for all types of soft contact lenses, including torics, there are some additional steps and/or rules to follow to ensure the proper fit of toric lenses.

The only new steps you must follow in prescribing ACUVUE OASYS® for ASTIGMATIC contact lenses are that you must determine the contact lens astigmatism and drift angle of the lens so that you can prescribe the correct lens size for your patient.

A. How to Determine Lens Cylinder and Axis Orientation

1. **Locate the Orientation Marks**
To help determine the proper orientation of the toric lens, you'll find two primary marks about 1 mm from the lens edge representing the vertical position on opposite sides of the lens at 6 and 12 o'clock (Fig. 1). Because of the lens' balancing system, optical mark can represent the vertical position - there is no "top" and "bottom" as in a prism-balanced lens. You don't need to view both marks to assess orientation; simply look for the 6 o'clock mark as you would with a prism-balanced lens.

Figure 1
You'll need a biomicroscope and a 1 mm or 2 mm parallelopiped beam to register the marks when the lens is fitted to the eye. There are a number of techniques you can use to improve the visibility of the 6 o'clock mark. Using a parallelopiped beam and medium magnification (10x or 16x), slowly can down the lens, looking just below the direct illumination of the retilluminated area. Backgrounding the mark this way should make it more visible. Sometimes manipulating the lens will help you see the necessary to uncover the mark.

2. **Choose Lens Rotation and Stability**
Observe the position and stability of the "bottom" mark. It usually stabilizes at the 6 o'clock position. If it does, calculation of the lens power will be straightforward. The 6 o'clock position is not a "pivot", however, the astigmatism requirement is that the axis position be stable and repeatable.

Allow the lenses to settle for about 20 minutes with the correct power lenses in place. Walk across the room and have the patient look at eye. Assess the patient's reaction to distance vision under those circumstances. Then have the patient look at familiar near objects such as a watch face or fragments. Again assess the reaction. As the patient continues to look around the room at both near and distance objects, observe the rotations. Only after these vision tests are completed should the patient be asked to read print. Evaluate the patient's reaction to large print (e.g., newspaper copy) at first and then gradually to newspaper and truly smaller type sizes.

After the patient's performance under the above conditions is completed, tests of visual acuity and reading ability under conditions of moderately dim illumination should be attempted.

An initial unblinded response in the office, while indicative of a guarded prognosis, should not immediately rule out a more extensive trial under the usual conditions in which a patient functions.

4. **Adaptation**
Visually demanding situations should be avoided during the initial wearing period. A patient may at first experience some mild blurring, vision, head-aches, and a feeling of slight imbalance. You should explain the adaptation symptoms to the patient. These symptoms may last for a brief interval or for several weeks. The longer these symptoms persist, the poorer the prognosis for successful adaptation.

To help in the adaptation process, the patient can be advised to first use the lenses in a comfortable familiar environment such as in the home.

Some patients find that automatic driving performance may not be optimal during the adaptation process. This is particularly true when driving at night. Before driving a motor vehicle, it may be recommended that the patient use a passenger but to make sure that their vision is satisfactory for operating an automobile. During the first several weeks of wear (when adaptation is occurring), it may be advisable for the patient to only drive during adaptation driving conditions. After adaptation and success with these activities, the patient should be able to drive under other conditions with caution.

D. Other Suggestions

The success of the monovision technique may be further improved by having the patient follow the suggestions below:

- Have a third contact lens (distance power) to use when critical distance viewing is needed.
- Have a third contact lens (near power) to use when critical near viewing is needed.
- Having supplemental spectacles to wear over the monovision contact lenses

The mark may stabilize somewhat left or right (drift) of the vertical meridian and still enable you to fit a toric lens for that eye, as long as the lens always returns to the patient's "start" position after settling. The deviation can be compensated for in the first prescription. Your objective is to ensure that whatever position the initial lens assumes near 6 o'clock, the position must be stable and repeatable. With full eye movement or heavy blinks, you may see the marks swing away, but they must return quickly to the original stable position. If the lens does not return quickly, you may need to select a different lens.

Assessing Rotation

Imagine the eye as a clock dial and every hour represents a 30° interval. If the orientation mark of the initial lens stabilizes somewhat left or right of the vertical position, the trial lens will start on the eye with the same deviation. You can use an axis rotate in the trial lamp or use a second lens in a specialized trial frame to measure or estimate the "trial angle" of the cylinder axis.

To compensate for this "trial" measure or estimate the "trial" turn and/or axis from the refractive axis to determine the correct cylinder axis. Use the LASER (Left Add, Right Subtract) method to determine which direction to compensate.

B. How to Determine the Final Lens Power

When the diagnostic lens has been aligned in the same meridian as the patient's refractive axis, a spherocylindrical over-refraction may be performed and visual acuity determined. However, in the case of crossed axes, such as when the diagnostic lens axis is different from the patient's refractive axis, it is not advisable to over-refract because of the difficulty in computing the resultant power. In fitting contact lenses, it is customary to prescribe the full power in the sphere, in the cylinder, however, any rotation is visually disturbing to the patient, so it is more practical to prescribe as weak a cylinder as possible. So, here is how to determine the final lens power.

For the Sphero:

If sphere axis or combined sphere and cylinder Rx is +4.00D, compensate for vertex distance. If sphere axis or combined sphere and cylinder Rx is +4.00D, sphere compensation is not necessary.

For the Cylinder:

Adjust the axis by the drift angle using LASER. Choose a cylinder that is ±0.50D from the refractive cylinder.

Case Examples:

Example 1
Manifest Spectacle refraction:
O.D. -2.50 -1.25 x 180 20/20
O.S. -2.00 -1.00 x 180 20/20

Choose a diagnostic lens for each eye with an axis as close to 180° as possible. Place the lens on each eye and allow a minimum of 3 minutes for

for specific visual tasks may improve the success of monovision correction. The particularly applicable to those patients who cannot pass static distance requirements with monovision correction.

Make use of proper illumination when carrying out visual tests.

Monovision fitting success can be improved by the following suggestions:

- Repeat the distance and near eyes if a patient is having trouble adapting.
- Refine the lens power if there is trouble with adaptation. Accurate near vision is critical for presbyopic patients.
- Emphasize the benefits of clear near vision and straight ahead and upward gaze with monovision.

The decision to fit a patient with a monovision correction is most appropriately left to the Eye Care Professional in conjunction with the patient after carefully considering the patient's needs.

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

PATIENT MANAGEMENT

Dispensing Visit

- PROVIDE THE PATIENT WITH A COPY OF THE PATIENT INSTRUCTION GUIDE FOR THESE LENSES. REVIEW THESE INSTRUCTIONS WITH THE PATIENT SO THAT HE OR SHE FULLY UNDERSTANDS THE PRESCRIBED WEARING AND REPLACEMENT SCHEDULE (DISPOSABLE OR FREQUENT REPLACEMENT).
- Recommend an appropriate cleaning and disinfecting system and provide the patient with instructions regarding proper lens care. Chemical or hydrogen peroxide disinfection is recommended.
- Schedule a follow-up examination.

Follow-up Examinations

- Follow-up care (necessary to ensure continued successful contact lens wear) should include routine periodic progress examinations, management of specific problems (if any) and a review with the patient of the wear schedule, lens replacement schedule, and proper lens care and handling procedures.
- Recommended Follow-up Examination Schedule (combinations and specific problems should be managed on an individual patient basis):
 1. One week from the initial lens dispensing to patient
 2. One month post-dispensing
 3. Every three to six months thereafter

It to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, reschedule until stable.

Check the orientation of the axis mark. If the bottom axis mark is in the 6 o'clock position on both eyes, choose the appropriate cylinder as listed previously. If the lens has not yet stabilized, reschedule until stable.

Example 2

Manifest Spectacle refraction:
O.D. -3.00 -1.25 x 180
O.S. -2.00 -0.75 x 180

Choose diagnostic lenses of -3.00 -0.75 x 90 for the right eye and -4.00 -1.75 x 90 for the left eye, the nearest lenses available to the spherical power and axis needed. Place the lens on each eye and allow a minimum of 3 minutes for the patient to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, reschedule until stable. The orientation mark on the right lens rotates left from the 6 o'clock position by 10°.

The Tiling Indicates the Following:

Right Eye:
Compensate the 10° axis drift by adding it to the manifest refraction axis. Here is the Rx prescribed:

O.D. -3.00 -0.75 x 100

Left Eye

The lens on the left eye shows good centration, movement and a constant tendency for the mark to drift right by 10° from the 6 o'clock position following a forced blink. Since the manifest refraction called for a power of -4.75D, adjust for the vertex distance and reduce the sphere to 0.50D and prescribe the -1.75D cylinder. Compensate for the 10° axis drift by subtracting 10° from the manifest refraction.

Here is the Rx Prescribed:

O.S. -4.50 -1.75 x 10

If vision is acceptable, perform a full lamp examination to assess adequate fit (centration and movement). If it is acceptable, dispense the lenses in-

structing the patient to return in one week for reassessment (post dispensing and follow-up information in PATIENT MANAGEMENT).

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

NOTE: More frequent or additional follow-up visits may be recommended for patients on an extended wear schedule.

- Potentially, at the follow-up visits, lenses should be worn for at least six hours.

If the lenses are being worn for continuous wear, the acclimation should be performed as early as possible on the morning following overnight wear.

- Recommended Procedures for Follow-Up Visits:
 1. Solicit and record patient's symptoms, if any.
 2. Measure visual acuity monocularly and binocularly at distance and near with the contact lenses.
 3. Perform an over-refraction at distance and near to check for residual refractive error.
 4. With the biomicroscope, judge the lens fitting characteristics (as described in the GENERAL FITTING GUIDELINES) and evaluate the lens surface for deposits and damage.
 5. Following lens removal, examine the cornea and conjunctiva with the biomicroscope and biomicroscope (lenses contraindicated).
 6. The presence of vertical corneal astigmatism in the posterior corneal curvatures or corneal neovascularization is indicative of acceptable corneal edema.
 7. The presence of corneal staining and/or latent conjunctival hyperemia can be indicative of an unknown lens, a reaction to solution preservatives, excessive lens wear, and/or a poorly fitting lens.
 8. Prolonged conjunctival changes may be indicative of an undetected anterior drainage lens.
 9. Particularly perform lamination and specific rotations. The values should be recorded and compared to the baseline measurements.

If any observations are abnormal, use professional judgment to alleviate the problem and return the eye to optimal conditions. If the criteria for successful fit are not satisfied during any follow-up examinations, repeat the patient's trial fitting procedure and refit the patient.

WEARING SCHEDULE

The wearing and replacement schedule should be determined by the Eye Care Professional. Regular checkups, as determined by the Eye Care Professional, are also extremely important.

For Daily Wear:

Patients tend to overwear the lenses initially. The Eye Care Professional should emphasize the importance of adhering to the initial maximum wearing schedule. Maximum wearing time should be determined by the Eye Care Professional based upon the patient's physiological eye condition, because individual response to contact lenses varies.

MULTIFOCAL FITTING GUIDELINES

A. Presbyopic Needs Assessment & Patient Education

Multifocal contact lenses may produce compromises to vision under certain circumstances and the patient should understand that they may not find their vision acceptable in specific situations (e.g., reading a menu in a dim restaurant, driving at night in rainy/dry conditions, etc.). Therefore, caution should be exercised when the patient is wearing the correction for the first time until they are comfortable with the vision provided in visually challenging environments. Occupational and environmental visual demands should be discussed. If the patient requires critical visual acuity and stereopsis, it should be determined by the Eye Care Professional if function adequately with the ACUVUE OASYS® for PRESBYOPIA contact lenses. Wear may not be optimal for activities such as:

- 1. Visually demanding situations such as operating potentially dangerous machinery or performing other potentially hazardous activities, and
- 2. driving automobiles (e.g., driving at night, driving where cannot pass that state driver's license requirements with those demands should be advised to not drive with this correction, OR may require that additional over-the-counter be provided).

These lenses are not recommended for patients who have +0.00 or greater of refractive cylinder as this level of uncorrected cylinder may lead to additional visual compromise.

These lenses are available in the following ACD powers:

- Lens "LOW", "near" near ACD lens (Max +1.25 ACD)
- Lens "MID", "midrange" near ACD lens (Max +1.75 ACD)
- Lens "HIGH", "high" near ACD lens (Max +2.00 ACD)

B. Fitting Instructions

1. **Determine the following:**
 - Eye dominance (the methods described in MONOVISION FITTING GUIDELINES may be used)
 - Spherical equivalent distance prescription (vertex corrected if necessary and rounded to less minus if between powers)
 - Near ACD
2. **Select the initial trial lens as follows:**
 - For each eye select the trial lens distance power that is closest to the patient's distance spherical equivalent.

The maximum suggested wearing time for these lenses is:

DAY	HOURS
1	6-8
2	8-10
3	10-12
4	12-14
5 and after	all wearing hours

For Extended Wear:

It is recommended that the contact lens wear time be evaluated on a daily wear schedule. If successful, then a gradual introduction of extended wear can be followed as determined by the Eye Care Professional.

These lenses have been approved for extended wear for up to 7 nights/7 days of continuous wear. Not all patients can achieve the maximum wear time.

For Therapeutic Lens wear, close supervision by the Eye Care Professional is necessary. These lenses can be worn for extended wear for up to 7 nights/7 days of continuous wear. The Eye Care Professional should determine the appropriate wearing time and provide specific instructions to the patient regarding lens care, insertion, and removal.

REPLACEMENT SCHEDULE

For Lenses Prescribed for Frequent Replacement:

When prescribed for daily wear (frequent replacement), it is recommended that the lenses be discarded and replaced with a new lens every 2 weeks. However, the Eye Care Professional is encouraged to determine an appropriate replacement schedule based upon the response of the patient.

For Lenses Prescribed for Disposable Wear:

When prescribed for disposable wear, the replacement schedule should be determined by the Eye Care Professional based upon the patient's history and their ocular condition, as well as the practitioner's experience and clinical judgment.

Once removed, it is recommended that the lens remain out of the eye for a period of one day/overnight or longer and be discarded in accordance with the prescribed wearing schedule. The Eye Care Professional should examine the patient during the early stages of extended wear.

- Select the near power of the lens based on the patient's ACD range as follows:

ACD: +0.75 to +1.25 use a "LOW" near ACD lens on each eye

ACD: +1.50 to +1.75 use a "MID" near ACD lens on each eye

ACD: +2.00 to +2.50 use a "HIGH" near ACD lens on each eye

Allow the lens to settle for a minimum 10 minutes.

3. Assess the distance and near vision binocularly and monocularly.

- Demonstrate the vision under various lighting conditions (normal and dimmed illumination) and at distance, intermediate and near.
- Make adjustments in power as necessary (use Multifocal Troubleshooting below). The use of hand-held test lenses is recommended.

If distance and near vision is acceptable, perform a full lamp examination to assess adequate fit (centration and movement). If it is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (post dispensing and follow-up information in PATIENT MANAGEMENT).

C. Multifocal Troubleshooting

Unacceptable Near Vision:
Determine the amount of additional plus, or less minus, over one or both eyes that is acceptable while checking the effect on distance and near vision. If vision is still not acceptable, change the non-dominant eye to the "next highest ACD power."

Unacceptable Distance Vision:
Determine the amount of additional minus, or less plus, over one or both eyes that is acceptable while checking the effect on distance and near vision. If vision is still not acceptable, change the dominant eye to the next lowest ACD power. If the patient is wearing two low ACD lenses, change the dominant eye to a slightly less with a power equal to the spherical equivalent distance prescription.

Unacceptable Distance and Near Vision:

Determine the amount of additional plus/minus over one or both eyes that is acceptable while checking the effect on distance and near vision. If additional plus/minus is not required, change the lens power in the dominant eye to the next lowest ACD power and the lens power in the non-dominant eye to the next highest ACD power, if applicable.

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

LENS CARE DIRECTIONS

When lenses are dispensed, the Eye Care Professional should provide the patient with appropriate and adequate warnings and instructions in accordance with the individual patient's lens type and wearing schedule. The Eye Care Professional should recommend an appropriate care system tailored to the patient's individual requirements.

For complete information concerning contact lens handling, care, cleaning, disinfecting and storage, refer to the Patient Instruction Guide for these lenses. Copies are available for download at www.acuvue.com.

For Lenses Prescribed for Frequent Replacement Wear:

The Eye Care Professional should review with the patient, lens care directions for cleaning, disinfecting and storing, including both basic lens care information and specific instructions on the lens care regimen recommended for the patient.

For Lenses Prescribed for Disposable Wear:

The Eye Care Professional should review with patients that no cleaning or disinfection is needed with disposable lenses. Patients should always dispose of lenses when they are removed and have replacement lenses or spectacles available. Lenses should only be cleaned, rinsed, and disinfected on an emergency basis when replacement lenses or spectacles are not available.

Care for a Direct Out (Dry/Night) Lens

If the haptic design (edge movement), the patient should be instructed to apply a lens and wait until the lens begins to move freely on the eye before removing it. If from movement of the lens continues after a few minutes, the patient should immediately contact the Eye Care Professional.

Care for Blocking (Non-Moving) Lenses

If the lens shows edge movement, the patient should be instructed to apply a lens and wait until the lens begins to move freely on the eye before removing it. If from movement of the lens continues after a few minutes, the patient should immediately contact the Eye Care Professional.

EMERGENCIES

The patient should be informed that if chemicals of any kind (household products, gardening solutions, laboratory chemicals, etc.) are splashed into the eyes, the patient should FLUSH EYES IMMEDIATELY WITH 100 WATER AND IMMEDIATELY CONTACT THE EYE CARE PROFESSIONAL OR VISIT A HOSPITAL EMERGENCY ROOM WITHOUT DELAY.

MONOVISION FITTING GUIDELINES

A. Patient Selection

Monovision Needs Assessment
For a good prognosis, the patient should have adequately corrected distance and near visual acuity in each eye. The anisometropic patient or the patient with significant astigmatism (greater than 1.00D in one eye) may not be a good candidate for monovision correction with these lenses.

Occupational and environmental visual demands should be considered. If the patient requires critical visual acuity and stereopsis, it should be determined by the Eye Care Professional if function adequately with monovision correction. Monovision contact lenses wear may not be optimal for activities such as:

- 1. Visually demanding situations such as operating potentially dangerous machinery or performing other potentially hazardous activities, and
- 2. driving automobiles (e.g., driving at night, driving where cannot pass that state driver's license requirements with those demands should be advised to not drive with this correction, OR may require that additional over-the-counter be provided).

Patient Education

All patients do not function equally well with monovision correction. Patients may not perform as well for certain tasks with this correction as they have with spectacles (driving, school, travel, vacation, progressed). Each patient should understand that monovision, as well as other presbyopic alternatives, can create a vision compromise that may reduce visual acuity and depth perception for distance and near tasks. Therefore, caution should be exercised when the patient is wearing the correction for the first time until they are familiar with the vision provided in visually challenging environments (e.g., reading a menu in a dim restaurant, driving at night in rainy/dry conditions, etc.).

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

B. Eye Selection

Generally, the non-dominant eye is corrected for near vision. The following two methods for eye dominance can be used.

1. Occlude Preference Determination Methods

Method 1: Determine which eye is the "righting eye." Have the patient point at an object at the far end of the room. Cover one eye. If the patient is still pointing directly at the object, the eye being used is the dominant (righting) eye.

Method 2: Determine which eye will accept the added power with the least reduction in vision. Place a hand-held trial lens equal to the spectacle near ADD in front of one eye and then the other while the distance refractive error correction is in place for both eyes. Determine whether the patient functions best with the near ADD lens over the right or left eye.

Other methods include the refractive error method and the visual demands method.

2. Refractive Error Method
For anisometropic correction, it is generally best to fit the more hyperopic (less myopic) eye for distance and the more myopic (less hyperopic) eye for near.

3. Visual Demands Method
Consider the patient's occupation during the eye selection process to determine the critical vision requirements. If a patient's gaze for near tasks is usually in one direction, correct the eye on that side for near.

Example: A secondary who places copy to the left side of the desk will function best with the near lens on the left eye.

C. Specific Fitting Characteristics

1. Unilateral Lens Correction
There are circumstances where only one contact lens is required. As an example, an anisometropic patient would only require a near lens with a bilateral myopia may only require a distance lens.

Example: A presbyopic anisometropic patient who requires a +1.75D ADD would have a +1.75D lens on the near eye and the other eye left without a lens. A presbyopic patient requiring a +1.50D ADD who is -2.50D in the right eye and -1.50D myopia in the left eye may have the right eye corrected for distance and the left uncorrected for near.

2. Near ADD Determination
Always prescribe the lens power for the near eye that provides optimal near acuity at the midpoint of the patient's natural reading distance. However, when more than one power provides optimal reading performance, prescribe the least plus (most minus) of the powers.

3. Trial Lens Fitting
After the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

Method 2: Determine which eye will accept the added power with the least reduction in vision. Place a hand-held trial lens equal to the spectacle near ADD in front of one eye and then the other while the distance refractive error correction is in place for both eyes. Determine whether the patient functions best with the near ADD lens over the right or left eye.

Other methods include the refractive error method and the visual demands method.

2. Refractive Error Method
For anisometropic correction, it is generally best to fit the more hyperopic (less myopic) eye for distance and the more myopic (less hyperopic) eye for near.

3. Visual Demands Method
Consider the patient's occupation during the eye selection process to determine the critical vision requirements. If a patient's gaze for near tasks is usually in one direction, correct the eye on that side for near.

Example: A secondary who places copy to the left side of the desk will function best with the near lens on the left eye.

C. Specific Fitting Characteristics

1. Unilateral Lens Correction
There are circumstances where only one contact lens is required. As an example, an anisometropic patient would only require a near lens with a bilateral myopia may only require a distance lens.

Example: A presbyopic anisometropic patient who requires a +1.7

IMPORTANT: Please read carefully and keep this information for future use.

This Package Insert and Fitting Instruction Guide is intended for the Eye Care Professional, but should be made available to patients upon request.

The Eye Care Professional should provide the patient with the appropriate instructions that pertain to the patient's prescribed lenses. Copies are available for download at www.acuvue.com.

1-DAY **ACUVUE®**
MOIST
BRAND CONTACT LENSES

1-DAY ACUVUE® MOIST Brand Contact Lenses

1-DAY ACUVUE® MOIST Brand Contact Lenses for ASTIGMATISM

1-DAY ACUVUE® MOIST Brand MULTIFOCAL Contact Lenses













etafilcon A Soft (hydrophilic) Contact Lenses
Visibility Tinted with UV Blocker
for Daily Disposable Wear



CAUTION: U.S. Federal law restricts this device to sale by or on the order of a licensed practitioner.

SYMBOLS KEY

The following symbols may appear on the label or packaging:

SYMBOL	DEFINITION
	Consult Instructions for Use
	Manufacturer
	Date of Manufacture
	Use By Date (expiration date)
	Batch Code
	Sterilized Using Steam Heat
	Do Not Re-Use (Single Use)
	Lens Orientation Correct
	Lens Orientation Incorrect (Lens Inside Out)
	Quality System Certification Symbol
	Fee Paid for Waste Management
	Authorized Representative in the European Community

Visit www.acuvue.com/guides for additional information about symbols.

DESCRIPTION

1-DAY ACUVUE® MOIST Brand Contact Lenses, 1-DAY ACUVUE® MOIST Brand Contact Lenses for ASTIGMATISM, and 1-DAY ACUVUE® MOIST Brand MULTIFOCAL Contact Lenses are soft (hydrophilic) contact lenses available as spherical, toric, or multifocal lenses, and include LACREON® Technology.

The lens material (etafilcon A) is a copolymer of 2-hydroxyethyl methacrylate and methacrylic acid cross-linked with 1, 1, 1-trimethylol propane trimethacrylate and ethylene glycol dimethacrylate.

The lenses are tinted blue using Reactive Blue Dye #4 to make the lenses more visible for handling. A benzotriazole UV absorbing monomer is used to block UV radiation.

Lens Properties:

The physical/optical properties of the lens are:

- Specific Gravity (calculated): 0.98 – 1.12
- Refractive Index: 1.40
- Light Transmittance: 85% minimum
- Surface Character: Hydrophilic
- Water Content: 58%
- Oxygen Permeability (D/k):

VALUE

21.4 x 10⁻¹¹ (cm²/sec)
(ml O₂/ml x mm Hg) @ 35°C
28.0 x 10⁻¹¹ (cm²/sec)
(ml O₂/ml x mm Hg) @ 35°C

METHOD

Fatt (boundary corrected, edge corrected)
Fatt (boundary corrected, non-edge corrected)

Lens Parameters Ranges:

- Diameter (DIA): 12.0 mm to 15.0 mm
- Center Thickness: Varies with power
- Base Curve (BC): 7.85 mm to 10.00 mm
- Spherical Power (D): -20.00D to +20.00D
- Cylinder Power (CYL): -0.25D to -10.00D
- Axis (AXIS): 2.5° to 180°
- ADD Powers: +0.25D to +4.00D

AVAILABLE LENS PARAMETERS

1-DAY ACUVUE® MOIST Brand Contact Lenses are hemispherical shells of the following dimensions:

- Diameter (DIA):** 14.2 mm
Center Thickness: 0.084 mm to 0.230 mm (varies with power)

Base Curve (BC): 8.5 mm, 9.0 mm
Powers (D): -0.50D to -6.00D (in 0.25D increments)
-6.50D to -12.00D (in 0.50D increments)
+0.50D to +6.00D (in 0.25D increments)

1-DAY ACUVUE® MOIST Brand Contact Lenses for ASTIGMATISM are hemitoric shells of the following dimensions:


Diameter (DIA): 14.5 mm
Center Thickness: 0.090 mm to 0.189 mm (varies with power)
Base Curve (BC): 8.5 mm
Powers (D): +0.00 to -6.00D (in 0.25D increments)
Cylinders (CYL): -0.75D, -1.25D, -1.75D, -2.25D*
Axis (AXIS): 10° to 180° in 10° increments
*-2.25D cylinder is available in 10°, 20°, 70°, 80°, 90°, 100°, 110°, 160°, 170°, 180° axes only
-6.50D to -9.00D (in 0.50D increments)
Cylinders (CYL): -0.75D, -1.25D, -1.75D, -2.25D*
Axis (AXIS): 10°, 20°, 60°, 70°, 80°, 90°, 100°, 110°, 120°, 160°, 170°, 180°
*-2.25D cylinder is available in 20°, 90°, 160°, 180° axes only
+0.25D to +4.00D (in 0.25D increments)
Cylinders (CYL): -0.75D, -1.25D, -1.75D
Axis (AXIS): 10°, 20°, 70°, 80°, 90°, 100°, 110°, 160°, 170°, 180°

1-DAY ACUVUE® MOIST Brand MULTIFOCAL Contact Lenses are hemispherical shells of the following dimensions:

Diameter (DIA): 14.3 mm
Center Thickness: 0.084 mm to 0.207 mm (varies with power)
Base Curve (BC): 8.4 mm
Powers (D): +6.00D to -9.00D (in 0.25D increments)
Near ADD Powers
(MAX ADD): Low Near ADD (LOW): +1.25D
Medium Near ADD (MID): +1.75D
High Near ADD (HGH): +2.50D

TRANSMITTANCE CURVES

1-DAY ACUVUE® MOIST Brand Contact Lenses (etafilcon A) Visibility Tinted with UV Blocker vs. 24 yr. old human cornea and 25 yr. old human crystalline lens.

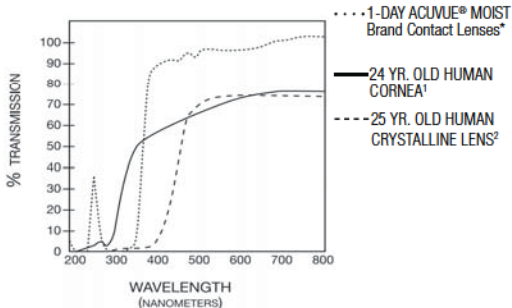

*The data are representative measurements taken through the central 3-5 mm portion for the thinnest marketed lens (~3.00D lens, 0.084 mm center thickness).

¹ Lerman, S., Radiant Energy and the Eye, MacMillan, New York, 1980, p. 58, figure 2-21

² Waxler, M., Hitchins, V.M., Optical Radiation and Visual Health, CRC Press, Boca Raton, Florida, 1986, p. 19, figure 5

WARNING: UV absorbing contact lenses are NOT substitutes for protective UV absorbing eyewear, such as UV absorbing goggles or sunglasses because they do not completely cover the eye and surrounding area. The patient should continue to use UV absorbing eyewear as directed.

ACTIONS

In its hydrated state, the contact lens, when placed on the cornea, acts as a refracting medium to focus light rays on the retina.

The UV Blocking for these lenses averages 97% in the UVB range of 280 nm to 315 nm and 82% in the UVA range of 316 nm to 380 nm for the entire power range.

NOTE: Long-term exposure to UV radiation is one of the risk factors associated with cataracts. Exposure is based on a number of factors such as environmental conditions (altitude, geography, cloud cover) and personal factors (extent and nature of outdoor activities). UV-Blocking contact lenses help provide protection against harmful UV radiation. However, clinical studies have not been done to demonstrate that wearing UV-Blocking contact lenses reduces the risk of developing cataracts or other eye disorders. The Eye Care Professional should be consulted for more information.

INDICATIONS (USES)

1-DAY ACUVUE® MOIST Brand Contact Lenses are indicated for daily disposable wear for the optical correction of refractive ametropia (myopia and hyperopia) in phakic or aphakic persons with non-diseased eyes who may have 1.00D or less of astigmatism.

1-DAY ACUVUE® MOIST Brand Contact Lenses for ASTIGMATISM are indicated for daily disposable wear for the optical correction of refractive ametropia (myopia and hyperopia) in phakic or aphakic persons with non-diseased eyes who may have 0.50D to 3.00D of astigmatism.

1-DAY ACUVUE® MOIST Brand MULTIFOCAL Contact Lenses are indicated for daily disposable wear for the optical correction of distance and near vision in presbyopic phakic or aphakic persons with non-diseased eyes who may have 4.00D of ADD power or less and 0.75D or less of astigmatism.

The lenses contain a UV Blocker to help protect against transmission of harmful UV radiation to the cornea and into the eye.

When prescribed for daily disposable use, no cleaning or disinfection is required. Lenses should be discarded upon removal.

CONTRAINDICATIONS (REASONS NOT TO USE)

DO NOT USE these lenses when any of the following conditions exist:

- Acute or subacute inflammation or infection of the anterior chamber of the eye.
- Any eye disease, injury, or abnormality that affects the cornea, conjunctiva, or eyelids.
- Severe insufficiency of lacrimal secretion (dry eye).
- Corneal hypoesthesia (reduced corneal sensitivity).

- Any systemic disease that may affect the eye or be exaggerated by wearing contact lenses.
- Allergic reactions of ocular surfaces or adnexa that may be induced or exaggerated by wearing contact lenses or use of contact lens solutions.
- Ocular irritation due to allergic reactions which may be caused by use of contact lens solutions (i.e., rewetting drops) that contain chemicals or preservatives (such as mercury, Thimerosal, etc.) to which some people may develop an allergic response.
- Any active corneal infection (bacterial, fungal, protozoal, or viral).
- If eyes become red or irritated.

WARNINGS

Patients should be advised of the following warnings pertaining to contact lens wear:

EYE PROBLEMS, INCLUDING CORNEAL ULCERS, CAN DEVELOP RAPIDLY AND LEAD TO LOSS OF VISION. IF THE PATIENT EXPERIENCES:

- **Eye Discomfort,**
- **Excessive Tearing,**
- **Vision Changes,**
- **Loss of Vision,**
- **Eye Redness, or**
- **Other Eye Problems,**

THE PATIENT SHOULD BE INSTRUCTED TO IMMEDIATELY REMOVE THE LENSES AND PROMPTLY CONTACT THE EYE CARE PROFESSIONAL.

- When prescribed for daily wear, patients should be instructed not to wear their lenses while sleeping. Clinical studies have shown that when lenses are worn overnight, the risk of ulcerative keratitis is greater than among those who do not wear them overnight.³
- Studies have shown that contact lens wearers who are smokers have a higher incidence of adverse reactions than nonsmokers.
- Problems with contact lenses or lens care products could result in serious injury to the eye. Patients should be cautioned that proper use and care of contact lenses and lens care products are essential for the safe use of these products.

- The overall risk of ulcerative keratitis may be reduced by carefully following directions for lens care.

³New England Journal of Medicine, September 21, 1989; 321 (12), pp. 773-783

Specific Instructions for Use and Warnings:

- **Water Activity**
Instruction for Use

Do not expose contact lenses to water while wearing them.

WARNING:

Water can harbor microorganisms that can lead to severe infection, vision loss, or blindness. If lenses have been submersed in water when participating in water sports or swimming in pools, hot tubs, lakes, or oceans, the patient should be instructed to discard them and replace them with a new pair. The Eye Care Professional should be consulted for recommendations regarding wearing lenses during any activity involving water.

PRECAUTIONS

Special Precautions for Eye Care Professionals:

- Due to the small number of patients enrolled in clinical investigation of lenses, all refractive powers, design configurations, or lens parameters available in the lens material are not evaluated in significant numbers. Consequently, when selecting an appropriate lens design and parameters, the Eye Care Professional should consider all characteristics of the lens that can affect lens performance and ocular health, including oxygen permeability, wettability, central and peripheral thickness, and optic zone diameter.

The potential impact of these factors on the patient's ocular health should be carefully weighed against the patient's need for refractive correction; therefore, the continuing ocular health of the patient and lens performance on the eye should be carefully monitored by the prescribing Eye Care Professional.
- Patients who wear these lenses to correct presbyopia using monovision (or modified monovision using 1-DAY ACUVUE® MOIST Brand MULTIFOCAL) may not achieve the best corrected visual acuity for either far or near vision. Visual requirements vary with the individual and should be considered when selecting the most appropriate type of lens for each patient.

- Fluorescein, a yellow dye, should not be used while the lenses are on the eyes. The lenses absorb this dye and become discolored. Whenever fluorescein is used in eyes, the eyes should be flushed with a sterile saline solution that is recommended for in-eye use.
- Eye Care Professionals should instruct the patient to remove lenses immediately if the eyes become red or irritated.

Eye Care Professionals should carefully instruct patients about the following care regimen and safety precautions.

Handling Precautions:

- Before leaving the Eye Care Professional's office, the patient should be able to promptly remove the lenses or should have someone else available who can remove the lenses for him or her.
- DO NOT use if the sterile blister package is opened or damaged.
- Always wash and rinse hands before handling lenses. Do not get cosmetics, lotions, soaps, creams, deodorants, or sprays in the eyes or on the lenses. It is best to put on lenses before putting on makeup.
- DO NOT touch contact lenses with the fingers or hands if the hands are not free of foreign materials, as microscopic scratches of the lenses may occur, causing distorted vision and/or injury to the eye.
- Carefully follow the handling, insertion, removal, and wearing instructions in the Patient Instruction Guide for these lenses and those prescribed by the Eye Care Professional.
- Always handle lenses carefully and avoid dropping them.
- Never use tweezers or other tools to remove lenses from the lens container. Slide the lens up the side of the bowl until it is free of the container.
- Do not touch the lens with fingernails.

Lens Wearing Precautions:

- If the lens sticks (stops moving) on the eye, follow the recommended directions in "Care for Sticking (Non-Moving) Lenses." The lens should move freely on the eye for the continued health of the eye. If non-movement of the lens continues, the patient should be instructed to immediately consult his or her Eye Care Professional.
- Never wear lenses beyond the period recommended by the Eye Care Professional.

- The patient should be advised to never allow anyone else to wear their lenses. They have been prescribed to fit their eyes and to correct their vision to the degree necessary. Sharing lenses greatly increases the chance of eye infections.
- If aerosol products, such as hairspray, are used while wearing lenses, exercise caution and keep eyes closed until the spray has settled.
- Avoid all harmful or irritating vapors and fumes while wearing lenses.

Lens Care Precautions:

- The patient should be informed that no cleaning or disinfection is needed when lenses are worn for daily disposable wear. Patients should always dispose of lenses when removed and have spare lenses or spectacles available.

Other Topics to Discuss with Patients:

- Always contact the Eye Care Professional before using any medicine in the eyes.
- Certain medications, such as antihistamines, decongestants, diuretics, muscle relaxants, tranquilizers, and those for motion sickness may cause dryness of the eye, increased lens awareness, or blurred vision. Should such conditions exist, proper remedial measures should be prescribed.
- Oral contraceptive users could develop visual changes or changes in lens tolerance when using contact lenses. Patients should be cautioned accordingly.
- As with any contact lens, follow-up visits are necessary to assure the continuing health of the patient's eyes. The patient should be instructed as to a recommended follow-up schedule.

Who Should Know That the Patient is Wearing Contact Lenses?

- Patients should inform all doctors (Health Care Professionals) about being a contact lens wearer.
- Patients should always inform their employer of being a contact lens wearer. Some jobs may require use of eye protection equipment or may require that the patient not wear contact lenses.

ADVERSE REACTIONS

The patient should be informed that the following problems may occur when wearing contact lenses:

- The eye may burn, sting, and/or itch.
- There may be less comfort than when the lens was first placed on the eye.
- There may be a feeling of something in the eye (foreign body, scratched area).
- There may be the potential for some temporary impairment due to peripheral infiltrates, peripheral corneal ulcers, or corneal erosion. There may be the potential for other physiological observations, such as local or generalized edema, corneal neovascularization, corneal staining, injection, tarsal abnormalities, iritis, and conjunctivitis, some of which are clinically acceptable in low amounts.
- There may be excessive watering, unusual eye secretions, or redness of the eye.
- Poor visual acuity, blurred vision, rainbows or halos around objects, photophobia, or dry eyes may also occur if the lenses are worn continuously or for too long a time.

The patient should be instructed to conduct a simple 3-part self-examination at least once a day. They should ask themselves:

- How do the lenses feel on my eyes?
- How do my eyes look?
- Have I noticed a change in my vision?

If the patient reports any problems, he or she should be instructed to **IMMEDIATELY REMOVE THE LENS**. If the problem or discomfort stops, the patient should discard the lens and place a new fresh lens on the eye.

If after inserting the new lens, the problem continues, the patient should be directed to **IMMEDIATELY REMOVE THE LENS AND CONTACT HIS OR HER EYE CARE PROFESSIONAL**.

The patient should be advised that when any of the above symptoms occur, a serious condition such as infection, corneal ulcer, neovascularization, or iritis may be present. He or she should be instructed to seek immediate professional identification of the problem and prompt treatment to avoid serious eye damage.

GENERAL FITTING GUIDELINES

A. Patient Selection

Patients selected to wear these lenses should be chosen based on:

- Motivation to wear lenses
- Ability to follow instructions regarding lens wear
- General health
- Ability to adequately handle and care for the lenses
- Ability to understand the risks and benefits of lens wear

Patients who do not meet the above criteria should not be provided with contact lenses.

B. Pre-fitting Examination

Initial evaluation of the patient should begin with a thorough case history to determine if there are any contraindications to contact lens wear. During the case history, the patient's visual needs and expectations should be determined as well as an assessment of their overall ocular, physical, and mental health.

Preceding the initial selection of trial contact lenses, a comprehensive ocular evaluation should be performed that includes, but is not limited to, the measurement of distance and near visual acuity, distance and near refractive prescription (including determining the preferred reading distance for presbyopes), keratometry, and biomicroscopic evaluation.

Based on this evaluation, if it is determined that the patient is eligible to wear these lenses, the Eye Care Professional should proceed to the lens fitting instructions as outlined below.

C. Initial Power Determination

A spectacle refraction should be performed to establish the patient's baseline refractive status and to guide in the selection of the appropriate lens power. Remember to compensate for vertex distance if the refraction is greater than $\pm 4.00D$.

D. Base Curve Selection (Trial Lens Fitting)

The following trial lenses should be selected for patients regardless of keratometry readings. However, corneal curvature measurements should be performed to establish the patient's baseline ocular status.

- 1-DAY ACUVUE® MOIST: 8.5 mm/14.2 mm
- 1-DAY ACUVUE® MOIST for ASTIGMATISM: 8.5 mm/14.5 mm
- 1-DAY ACUVUE® MOIST MULTIFOCAL: 8.4 mm/14.3 mm

The trial lens should be placed on each of the patient's eyes and evaluated after the patient has adjusted to the lenses.

1. Criteria of a Properly Fit Lens

A properly fit lens will center and completely cover the cornea (i.e., no limbal exposure), have sufficient movement to provide tear exchange under the contact lens with the blink, and be comfortable. The lens should move freely when manipulated digitally with the lower lid, and then return to its properly centered position when released.

2. Criteria of a Flat Fitting Lens

A flat fitting lens may exhibit one or more of the following characteristics: decentration, incomplete corneal coverage (i.e., limbal exposure), excessive movement with the blink and/or edge standoff. If the lens is judged to be flat fitting, it should not be dispensed to the patient.

3. Criteria of a Steep Fitting Lens

A steep fitting lens may exhibit one or more of the following characteristics: insufficient movement with the blink, conjunctival indentation, and resistance when pushing the lens up digitally with the lower lid. If the lens is judged to be steep fitting, it should not be dispensed to the patient.

If the initial trial base curve is judged to be flat or steep fitting, the alternate base curve, if available, should be trial fit and evaluated after the patient has adjusted to the lens. The lens should move freely when manipulated digitally with the lower lid, and then return to a properly centered position when released. If resistance is encountered when pushing the lens up, the lens is fitting tightly and should not be dispensed to the patient.

E. Final Lens Power (Spherical)

A spherical over-refraction should be performed to determine the final lens power after the lens fit is judged acceptable. The spherical over-refraction should be combined with the trial lens power to determine the final lens prescription. The patient should experience good visual acuity with the correct lens power unless there is excessive residual astigmatism.

Example 1	
Diagnostic lens:	-2.00D
Spherical over-refraction:	-0.25D
Final lens power:	-2.25D
Example 2	
Diagnostic lens:	-2.00D
Spherical over-refraction:	+0.25D
Final lens power:	-1.75D

If vision is acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If the fit is acceptable, dispense the lenses and instruct the patient to return in one week for reassessment (see **PATIENT MANAGEMENT** section).

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

TORIC FITTING GUIDELINES

Although most aspects of the fitting procedure are identical for all types of soft contact lenses, including toric lenses, there are some additional steps and/or rules to follow to assure the proper fit of toric lenses.

The only new steps you must follow in prescribing 1-DAY ACUVUE® MOIST for ASTIGMATISM are that you must determine the stability, repeatability, and drift angle of the lens axis so that you can prescribe the correct lens axis for the patient.

A. How to Determine Lens Cylinder and Axis Orientation

1. Locate the Orientation Marks

To help determine the proper orientation of the toric lens, you'll find two primary marks approximately 1 mm from the lens edge representing the vertical position on opposite ends of the lens at 6 and 12 o'clock (Fig. 1). Because of the lens' ballasting system, either mark can represent the vertical position – there is no "top" and "bottom" as in a prism-ballasted lens. You don't need to view both marks to assess orientation; simply look for the 6 o'clock mark as you would with a prism-ballasted lens.



Figure 1

You'll need a slit lamp biomicroscope with a 1 to 2 mm parallelepiped beam to highlight the marks when the lens is fitted to the eye. There are a number of techniques you can use to improve the visibility of the 6 o'clock mark. Using a parallelepiped beam and medium magnification (10x or 15x), slowly pan down the lens, looking just below the direct illumination at the retroluminated area. Backlighting the mark this way should make it more visible. Sometimes manipulating the lower lid may be necessary to uncover the mark.

2. Observe Lens Rotation and Stability

Observe the position and stability of the "bottom" mark. It usually stabilizes at the 6 o'clock position. If it does, calculation of the lens power will be straightforward. The 6 o'clock position is not a "must"; however, the absolute requirement is that the axis position be stable and repeatable.

The mark may stabilize somewhat left or right (drift) of the vertical meridian and still enable you to fit a toric lens for that eye, as long as the lens always returns to the same "drift axis" position after settling. The deviation can be compensated for in the final prescription. Your objective is to ensure that whatever position the initial lens assumes near 6 o'clock, this position must be stable and repeatable. With full eye movement or heavy blink, you may see the marks swing away, but they must return quickly to the original stable position. If the lens does not return quickly, you may need to select a different lens.

3. Assessing Rotation

Imagine the eye as a clock dial and every hour represents a 30° interval. If the orientation mark of the initial lens stabilizes somewhat left or right of the vertical position, the final lens will orient on the eye with the same deviation. You can use an axis reticule in the slit lamp or use a line-scribed lens in a spectacle trial frame to measure or estimate the "drift angle" of the cylinder axis.

To compensate for this "drift," measure or estimate the "drift," then add or subtract it from the refractive axis to determine the correct cylinder axis. Use the LARS (Left Add, Right Subtract) method to determine which direction to compensate.

B. Final Lens Power

When the diagnostic lens has its axis aligned in the same meridian as the patient's refractive axis, a spherocylindrical over-refraction may be performed and visual acuity determined. However, in the case of crossed axes, such as when the diagnostic lens axis is different from the spectacle cylinder axis, it is not advisable to perform a full spherocylindrical over-refraction because of the difficulty in computing the resultant power. A spherical over-refraction without cylinder refraction may be performed.

If the required cylinder correction falls between two available cylinder powers, it is recommended to prescribe the lower cylinder power lens. See below for instructions on how to determine the final lens power.

1. For the Sphere

If sphere alone or combined sphere and cylinder Rx > 4.00D, compensate for vertex distance. If sphere alone or combined sphere and cylinder Rx $\leq \pm 4.00$ D, vertex compensation is not necessary.

2. For the Cylinder

Adjust the axis by the drift angle using the LARS method. Choose a cylinder that is ≤ 0.50 D from the refractive cylinder.

3. Case Examples

Example 1

Manifest (spectacle) refraction:

O.D. -2.50D / -1.25D x 180° 20/20

O.S. -2.00D / -1.00D x 180° 20/20

Choose a diagnostic lens for each eye with axis 180°. Place the lens on each eye and allow a minimum of 3 minutes for it to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, recheck until stable.

Check the orientation of the axis mark. If the bottom axis mark is in the 6 o'clock position on both eyes, choose the appropriate cylinder as listed previously. If the lens has not yet stabilized, recheck until stable.

Here is the Rx prescribed:

O.D. -2.50D / -1.25D x 180°

O.S. -2.00D / -0.75D x 180°

Example 2

Manifest (spectacle) refraction:

O.D. -3.00D / -1.00D x 90° 20/20

O.S. -4.75D / -2.00D x 90° 20/20

Choose diagnostic lenses of -3.00D / -0.75D x 90° for the right eye and -4.50D / -1.75D x 90° for the left eye, the nearest lenses available to the spherical power and axis needed. For the left eye, since the manifest refraction called for -4.75D, compensating for vertex distance the sphere is reduced by 0.25D to -4.50D. The cylinder power will be -1.75D. Place the lens on each eye and allow a minimum of 3 minutes for it to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, recheck until stable.

Right Eye

The orientation mark on the right lens rotates left from the 6 o'clock position by 10° and remains stable in this position. Compensation for this rotation should be done as follows:

Compensate the 10° axis drift by adding it to the manifest refraction axis.

Here is the Rx prescribed:

O.D. -3.00D / -0.75D x 100°

Left Eye

The orientation mark on the left lens rotates right from the 6 o'clock position by 10° and remains stable in this position. Compensation for this rotation should be done as follows:

Compensate for the 10° axis drift by subtracting it from the manifest refraction axis.

Here is the Rx prescribed:

O.S. -4.50D / -1.75D x 80°

If vision is acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If fit is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (see

PATIENT MANAGEMENT section).

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

MULTIFOCAL FITTING GUIDELINES

A. Presbyopic Needs Assessment & Patient Education

Multifocal contact lenses may produce compromise to vision under certain circumstances and the patient should understand that they might not find their vision acceptable in specific situations (i.e., reading a menu in a dim restaurant, driving at night in rainy/foggy conditions, etc.). Therefore, caution should be exercised when the patient is wearing the correction for the first time until they are familiar with the vision provided in visually challenging environments. Occupational and environmental visual demands should be considered. If the patient requires critical visual acuity and stereopsis, it should be determined by trial whether this patient can function adequately with 1-DAY ACUVUE® MOIST MULTIFOCAL. Wearing these lenses may not be optimal for activities such as:

- Visually demanding situations such as operating potentially dangerous machinery or performing other potentially hazardous activities; and
- Driving automobiles (e.g., driving at night). Patients who cannot meet their state driver's license requirements with the 1-DAY ACUVUE® MOIST MULTIFOCAL should be advised to not drive with this correction, OR may require that additional over-correction be prescribed.

1-DAY ACUVUE® MOIST MULTIFOCAL is not recommended for patients who have -1.00D or greater of refractive cylinder as this level of uncorrected cylinder may lead to additional visual compromise. These lenses are available in the following ADD powers:

- Lens "LOW" = low near ADD lens (Max ADD +1.25)
- Lens "MID" = medium near ADD lens (Max ADD +1.75)
- Lens "HGH" = high near ADD lens (Max ADD +2.50)

B. Initial Power Determination

A spectacle refraction should be performed to establish the patient's baseline refractive status and to guide in the selection of the appropriate lens power. Remember to compensate for vertex distance if the refraction is greater than $\pm 4.00D$. Determine the spherical equivalent distance prescription for a multifocal patient. Determine the eye dominance using one of the methods below:

Method 1 Determine which eye is the "sighting eye." Have the patient point to an object at the far end of the room. Cover one eye. If the patient is still pointing directly at the object, the eye being used is the dominant (sighting) eye.

Method 2 Determine which eye does not accept added plus power. Place a +1.00D hand-held trial lens in front of one eye and then the other while the distance refractive error correction is in place for both eyes while the patient is viewing the distance visual acuity chart. The eye with the plus over it that the patient notices the greatest reduction in vision is determined to be the dominant eye.

C. Select the Initial Trial Lens

1. For each eye, select the trial lens distance power that is closest to the patient's distance spherical equivalent. Remember to compensate for vertex distance if the refraction is greater than $\pm 4.00D$.
2. Select the near power of the lens based on the patient's ADD range as follows:
 - ADD: +0.75D to +1.25D use a low near ADD (LOW) lens on each eye
 - ADD: +1.50D to +1.75D use a medium near ADD (MID) lens on each eye
 - ADD: +2.00D to +2.50D use a medium near ADD (MID) on the dominant eye and a high near ADD (HGH) lens on the non-dominant eye
3. Allow the lenses to settle for a minimum of 10 minutes.
4. Assess distance and near vision binocularly and monocularly.
5. Demonstrate the vision under various lighting conditions (normal and decreased illumination) and at distance, intermediate, and near.
6. Make adjustments in power as necessary based on the distance over-refraction. The use of hand-held trial lenses is recommended. Check the impact on distance and near vision.
7. If vision is still unacceptable, make adjustments in power as necessary (see "Multifocal Troubleshooting" below). If distance and near vision are acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If fit is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (see **PATIENT MANAGEMENT** section).

D. Multifocal Troubleshooting

Unacceptable Near Vision

If it has been determined that no change is required based on the over-refraction, then add +0.25D to the spherical power of the non-dominant eye.

Unacceptable Distance Vision

If it has been determined that no change is required based on the over-refraction, then make the changes as listed below:

- If the patient is wearing two "LOW" ADD lenses, change the dominant eye to a 1-DAY ACUVUE® MOIST sphere lens with a power equal to the spherical equivalent distance prescription.
- If the patient is wearing two "MID" ADD lenses, change the ADD power in the dominant eye to the "LOW" ADD power.
- If the patient is wearing a "MID" ADD lens in the dominant eye and a "HIGH" ADD lens in the non-dominant eye, change the non-dominant eye to a "MID" ADD lens and add +0.25D to the distance power.

E. Adaptation

Visually demanding situations should be avoided during the initial wearing period. A patient may at first experience some mild blurred vision, dizziness, headaches and a feeling of slight imbalance. You should explain the adaptational symptoms to the patient. These symptoms may last for a brief minute or for several weeks. The longer these symptoms persist, the poorer the prognosis for successful adaptation.

To help in the adaptation process, the patient can be advised to first use the lenses in a comfortable, familiar environment such as in the home.

Some patients feel that automobile driving performance may not be optimal during the adaptation process. This is particularly true when driving at night. Before driving a motor vehicle, it may be recommended that the patient be a passenger first to make sure that their vision is satisfactory for operating an automobile. During the first several weeks of wear (when adaptation is occurring), it may be advisable for the patient to only drive during optimal driving conditions. After adaptation and success with these activities, the patient should be able to drive under other conditions with caution.

All patients should be supplied with a copy of the PATIENT

INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

MONOVISION FITTING GUIDELINES

A. Patient Selection

1. Monovision Needs Assessment

For a good prognosis, the patient should have adequately corrected distance and near visual acuity in each eye. The amblyopic patient or the patient with significant astigmatism (greater than 1.00D) in one eye may not be a good candidate for monovision correction with these lenses.

Occupational and environmental visual demands should be considered. If the patient requires critical vision (visual acuity and stereopsis), it should be determined by trial whether this patient can function adequately with monovision correction. Monovision contact lens wear may not be optimal for activities such as:

- Visually demanding situations such as operating potentially dangerous machinery or performing other potentially hazardous activities; and
- Driving automobiles (e.g., driving at night). Patients who cannot meet their state driver's license requirements with monovision correction should be advised to not drive with this correction, OR may require that additional over-correction be prescribed.

2. Patient Education

All patients do not function equally well with monovision correction. Patients may not perform as well for certain tasks with this correction as they have with spectacles (multifocal, bifocal, trifocal, readers, progressives). Each patient should understand that monovision, as well as other presbyopic alternatives, can create a vision compromise that may reduce visual acuity and depth perception for distance and near tasks. Therefore, caution should be exercised when the patient is wearing the correction for the first time until they are familiar with the vision provided in visually challenging environments (e.g., reading a menu in a dimly lit restaurant, driving at night in rainy/foggy conditions, etc.). During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision, and straight ahead and upward gaze that monovision contact lenses provide.

B. Eye Selection

1. Ocular Preference Determination Methods

Generally, the non-dominant eye is corrected for near vision. The following two methods for eye dominance can be used.

Method 1 Determine which eye is the "sighting eye." Have the patient point to an object at the far end of the room. Cover one eye. If the patient is still pointing directly at the object, the eye being used is the dominant (sighting) eye.

Method 2 Determine which eye will accept the added power with the least reduction in vision. Place a hand-held trial lens equal to the spectacle near ADD in front of one eye and then the other while the distance refractive error correction is in place for both eyes. Determine whether the patient functions best with the near ADD lens over the right or left eye.

2. Other Eye Selection Methods

Other methods include the "Refractive Error Method" and the "Visual Demands Method."

Refractive Error Method

For anisometropic correction, it is generally best to fit the more hyperopic (less myopic) eye for distance and the more myopic (less hyperopic) eye for near.

Visual Demands Method

Consider the patient's occupation during the eye selection process to determine the critical vision requirements. If a patient's gaze for near tasks is usually in one direction, correct the eye on that side for near.

Example: A secretary who places copy to the left side of the desk will function best with the near lens on the left eye.

C. Special Fitting Characteristics

1. Unilateral Vision Correction

There are circumstances where only one contact lens is required. As an example, an emmetropic patient would only require a near lens, whereas a bilateral myope would require corrective lenses on both eyes.

Examples:

A presbyopic emmetropic patient who requires a +1.75D ADD would have a +1.75D lens on the near eye and the other eye left without correction.

A presbyopic patient requiring a +1.50D ADD who is -2.50D myopic in the right eye and -1.50D myopic in the left eye may have the right eye corrected for distance and the left eye uncorrected for near.

2. Near ADD Determination

Always prescribe the lens power for the near eye that provides optimal near acuity at the midpoint of the patient's habitual reading distance. However, when more than one power provides optimal reading performance, prescribe the least plus (most minus) of the powers.

3. Trial Lens Fitting

A trial fitting is performed in the office to allow the patient to experience monovision correction. Lenses are fit according to the **GENERAL FITTING GUIDELINES** for base curve selection described in this Package Insert.

Case history and a standard clinical evaluation procedure should be used to determine the prognosis. Determine the distance correction and the near correction. Next, determine the near ADD. With trial lenses of the proper power in place, observe the reaction to this mode of correction.

Allow the lenses to settle for about 20 minutes with the correct power lenses in place. Walk across the room and have the patient look at you. Assess the patient's reaction to distance vision under these circumstances. Then have the patient look at familiar near objects such as a watch face or fingernails. Again assess the reaction. As the patient continues to look around the room at both near and distance objects, observe the reactions. Only after these vision tests are completed, should the patient be asked to read print. Evaluate the patient's reaction to large print (e.g., typewritten copy) at first and then graduate to newsprint and finally smaller type sizes.

After the patient's performance under the above conditions is completed, tests of visual acuity and reading ability under conditions of moderately dim illumination should be attempted.

An initial unfavorable response in the office, while indicative of a guarded prognosis, should not immediately rule out a more extensive trial under the usual conditions in which a patient functions.

4. Adaptation

Visually demanding situations should be avoided during the initial wearing period. A patient may at first experience some mild blurred vision, dizziness, headaches, and a feeling of slight imbalance. You should explain the adaptational symptoms to the patient. These symptoms may last for a brief minute or for several weeks. The longer these symptoms persist, the poorer the prognosis for successful adaptation.

To help in the adaptation process, the patient can be advised to first use the lenses in a comfortable, familiar environment such as in the home.

Some patients feel that automobile driving performance may not be optimal during the adaptation process. This is particularly true when driving at night. Before driving a motor vehicle, it may be recommended that the patient be a passenger first to make sure that their vision is satisfactory for operating an automobile. During the first several weeks of wear (when adaptation is occurring), it may be advisable for the patient to only drive during optimal driving conditions. After adaptation and success with these activities, the patient should be able to drive under other conditions with caution.

D. Other Suggestions

The success of the monovision technique may be further improved by having your patient follow the suggestions below:

- Have a third contact lens (distance power) to use when critical distance viewing is needed.
- Have a third contact lens (near power) to use when critical near viewing is needed.
- Have supplemental spectacles to wear over the monovision contact lenses for specific visual tasks may improve the success of monovision correction. This is particularly applicable for those patients who cannot meet state driver's licensing requirements with monovision correction.
- Make use of proper illumination when carrying out visual tasks.

Monovision fitting success can be improved by the following suggestions:

- Reverse the distance and near eyes if a patient is having trouble adapting.
- Refine the lens powers if there is trouble with adaptation. Accurate lens power is critical for presbyopic patients.
- Emphasize the benefits of clear near vision, and straight ahead and upward gaze with monovision.

The decision to fit a patient with monovision correction is most appropriately left to the Eye Care Professional in conjunction with the patient after carefully considering the patient's needs.

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

PATIENT MANAGEMENT

- Follow the accepted standard of care in fitting and following up with your patient, e.g., American Optometric Association standard of care.
- Schedule the appropriate follow-up examination.
- Preferably, at the follow-up visits, lenses should have been worn for at least six hours.
- Provide the patient with a copy of the PATIENT INSTRUCTION GUIDE for these lenses, which can be found at www.acuvue.com. REVIEW THESE INSTRUCTIONS WITH THE PATIENT SO THAT HE OR SHE CLEARLY UNDERSTANDS THE PRESCRIBED WEARING AND REPLACEMENT SCHEDULES.

WEARING SCHEDULE

The wearing schedule should be determined by the Eye Care Professional. Regular checkups, as determined by the Eye Care Professional, are also extremely important.

Patients tend to over wear the lenses initially. The Eye Care Professional should emphasize the importance of adhering to the initial maximum wearing schedule. Maximum wearing time should be determined by the Eye Care Professional based upon the patient's physiological eye condition, because individual response to contact lenses varies.

The maximum suggested wearing time for these lenses is:

DAY	HOURS
1	6-8
2	8-10
3	10-12
4	12-14
5 and after	all waking hours

REPLACEMENT SCHEDULE

These lenses are indicated for daily disposable wear and should be discarded upon removal.

When disposed of after a single daily use, these lenses may reduce the risk of developing giant papillary conjunctivitis.⁴

When worn as a daily disposable lens, these lenses may provide improved comfort for many patients who experience mild discomfort and itching associated with allergies during contact lens wear, compared to lenses replaced at intervals of greater than 2 weeks.

Clinical research has shown that when worn on a daily disposable basis, these lenses may provide improved comfort for 2 out of 3 patients who reported suffering from discomfort associated with allergies during contact lens wear.

⁴The CLAO Journal, July 1999, Volume 25, Number 3

LENS CARE DIRECTIONS

The Eye Care Professional should review with patients that no cleaning or disinfection is needed with daily disposable lenses. Patients should always dispose of lenses when they are removed and have replacement lenses or spectacles available.

For complete information concerning contact lens handling and care, refer to the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

Care for Sticking (Non-Moving) Lenses

During removal, if the lens sticks to the eye, the patient should be instructed to apply a few drops of the recommended lubricating or rewetting solution

directly to the eye and wait until the lens begins to move freely on the eye before removing it. If non-movement of the lens continues after a few minutes, the patient should **immediately** consult the Eye Care Professional.

EMERGENCIES

The patient should be informed that if chemicals of any kind (household products, gardening solutions, laboratory chemicals, etc.) are splashed into the eyes, the patient should: **FLUSH EYES IMMEDIATELY WITH TAP WATER AND IMMEDIATELY CONTACT THE EYE CARE PROFESSIONAL OR VISIT A HOSPITAL EMERGENCY ROOM WITHOUT DELAY.**

HOW SUPPLIED

Each UV-absorbing sterile lens is supplied in a foil-sealed plastic package containing buffered saline solution with povidone. The plastic package is marked with the following:

- **1-DAY ACUVUE® MOIST:** base curve, power, diameter, lot number, and expiration date
- **1-DAY ACUVUE® MOIST for ASTIGMATISM:** base curve, power, diameter, cylinder, axis, lot number, and expiration date
- **1-DAY ACUVUE® MOIST MULTIFOCAL:** base curve, power, diameter, ADD power, lot number, and expiration date

REPORTING OF ADVERSE REACTIONS

All serious adverse experiences and adverse reactions observed in patients wearing these lenses or experienced with these lenses should be reported to:

Johnson & Johnson Vision Care, Inc.
7500 Centurion Parkway
Jacksonville, FL 32256
USA
Tel: 1-800-843-2020
www.acuvue.com

Johnson & Johnson Vision Care, Inc.
7500 Centurion Parkway
Jacksonville, FL 32256
USA
Tel: 1-800-843-2020
www.acuvue.com



©Johnson & Johnson Vision Care, Inc. 2017
In Canada: Johnson & Johnson Vision Care division of Johnson & Johnson Inc.
In USA: Johnson & Johnson Vision Care, Inc.
Printed in USA
Revision date: 07/17
Revision number: M-07-17-02

1-DAY ACUVUE® MOIST and LACREON® are Trademarks of
Johnson & Johnson Vision Care, Inc.

APPENDIX D: BINOCULAR OVER REFRACTION

Binocular Over-refraction Technique

1. Place trial frame on subject
2. Add +1.00 D sphere to OS
3. Add + 0.50DS OD and check VA
 - if VA remained unchanged or improved, repeat step 3
 - if VA decreased, add minus until best VA first achieved *note: add minus for 0.5 seconds to avoid reflex accommodation.
4. Record VA
5. Change +1.00 D sphere to OD
6. Repeat steps 3 and 4

APPENDIX E: PRESBYOPIC SYMPTOMS QUESTIONNAIRE

Presbyopic Symptoms Questionnaire

1. Do you notice that you often have to hold things farther away so that you can read them?
2. Do you notice that you often have difficulty focusing on near objects (i.e., experiencing blurry vision when looking at things close-up)?
3. Do you often have headaches or eyestrain, or feel fatigued, when reading or conducting other near activities?
4. Do you often have difficulty reading small or fine prints, such as phone books, medicine bottles or package labels, etc.?
5. Do you often have difficulty reading under dim or low light?

APPENDIX F: OCULAR DOMINANCE

OCULAR DOMINANCE TEST

+1.00 D LENS TEST

- Step 1 Place the subjects best sphero-cylindrical distance refraction in a trial frame.
- Step 2 Have the subject view a BVA line of letters.
- Step 3 With both eyes open alternate a +1.00 D trial lens between the right and left eye and ask the subject to indicate over which eye does the lens cause the line of letters to appear more blurred. The eye that the greatest blur is reported is the distance dominant eye. If the subject indicates that the amount of blur is about the same between the two eyes then record as neither eye dominant.

SIGHTING OCULAR DOMINANCE

- Step 1 Ask the subject to extend both arms out and use his/her hands to form a triangle. The subject will be asked to keep both eyes open, and look through the triangle at a small object on the wall (e.g., a light switch or doorknob).
- Step 2 Occlude the subject's left eye, then right eye. While alternating the occluder from the subject's eyes, ask the subject when they see the object.

If the subject sees the object when the left eye is covered, the subject is *right eye* dominant.

If the subject sees the object when the right eye is covered, the subject is *left eye* dominant.

If the subject sees the object with both eyes, the opening between the hands may be too large. Therefore, ask the subject to make a smaller opening and repeat the procedure.

APPENDIX G: TEST LENS FITTING GUIDE

Step 1.

Choose the first lens based on the best spherical equivalent refraction and ADD power for both eyes. Select the first lens per table 1 below.

Table 1. Initial Lens Selection

	ADD							
	+0.75	+1.00	+1.25	+1.50	+1.75	+2.00	+2.25	+2.50
Dominant Eye	LOW	LOW	LOW	MID	MID	MID	MID	MID
Non-Dominant Eye	LOW	LOW	LOW	MID	MID	HGH	HGH	HGH

Assess the subject's vision at distance and near after the lens has settled (10 minutes). If the vision is acceptable continue with the fit assessment and dispensing as per the protocol.

If the vision is not acceptable, ensure that the proper initial lens power was selected by performing a distance over-refraction with +/- 0.25D trial lenses (or flippers) to determine if a change in the initial lens power is required (note: the over-refraction should be performed outside of the phoropter in normal room illumination). Recheck both distance and near vision with the over-refraction in place. If a change in the initial lens power is not required refer to the fitting steps listed below in step 2 (table 2).

Step 2.

Table 2. Lens change if required. *

Distance Complaint								
ADD	+0.75	+1.00	+1.25	+1.50	+1.75	+2.00	+2.25	+2.50
Dominant Eye	ACUVUE® OASYS® 2-WEEK Sphere	ACUVUE® OASYS® 2-WEEK Sphere	ACUVUE® OASYS® 2-WEEK Sphere	LOW	LOW	MID	MID	MID
Non-Dominant Eye	LOW	LOW	LOW	MID	MID	MID +	MID +	MID +

Near Complaint								
ADD	+0.75	+1.00	+1.25	+1.50	+1.75	+2.00	+2.25	+2.50
Dominant Eye	LOW	LOW	LOW	MID	MID	MID	MID	MID
Non-Dominant Eye	LOW+	LOW+	LOW+	MID+	MID+	HGH+	HGH+	HGH+

*Note: a + following the contact lens design indicates to add +0.25 D to the distance contact lens power on the non-dominant eye (see example below).

Example: The subject is a +1.75 ADD and has a near complaint and it is determined a change in lens pairs is needed. Referring to table 2 near complaint section, under the +1.75 ADD it states to keep the dominant eye the same (i.e. MID) and add +0.25D to the non-dominant eye (i.e. MID+).

Subjects spherical equivalent distance refraction

OD: +2.50

OS: +3.00 (OS non-dominant eye)

The new lens chosen should be as follows:

OD: +2.50 MID ADD (i.e. no change)

OS: +3.25 MID ADD

Step 3.

If after the above lens modifications have been attempted and the subject's vision is still not satisfactory, and additional optimizations are allowed by the protocol, lens changes may be attempted, based on the Investigator's clinical experience, to determine if acceptable vision can be achieved.

APPENDIX H: CONTROL LENS FITTING GUIDE

Step 1.

Choose the first lens based on the best spherical equivalent refraction and ADD power for both eyes. Select the first lens per table 1 below.

Table 1. Initial Lens Selection

	ADD							
	+0.75	+1.00	+1.25	+1.50	+1.75	+2.00	+2.25	+2.50
Dominant Eye	LOW	LOW	LOW	MID	MID	MID	MID	MID
Non-Dominant Eye	LOW	LOW	LOW	MID	MID	HGH	HGH	HGH

Assess the subject's vision at distance and near after the lens has settled (10 minutes). If the vision is acceptable continue with the fit assessment and dispensing as per the protocol.

If the vision is not acceptable, ensure that the proper initial lens power was selected by performing a distance over-refraction with +/- 0.25D trial lenses (or flippers) to determine if a change in the initial lens power is required (note: the over-refraction should be performed outside of the phoropter in normal room illumination). Recheck both distance and near vision with the over-refraction in place. If a change in the initial lens power is not required refer to the fitting steps listed below in step 2 (table 2).

Step 2.

Table 2. Lens change if required. *

Distance Complaint								
ADD	+0.75	+1.00	+1.25	+1.50	+1.75	+2.00	+2.25	+2.50
Dominant Eye	1-Day ACUVUE® Moist	1-Day ACUVUE® Moist	1-Day ACUVUE® Moist	LOW	LOW	MID	MID	MID
Non-Dominant Eye	LOW	LOW	LOW	MID	MID	MID +	MID +	MID +

Near Complaint								
ADD	+0.75	+1.00	+1.25	+1.50	+1.75	+2.00	+2.25	+2.50
Dominant Eye	LOW	LOW	LOW	MID	MID	MID	MID	MID
Non-Dominant Eye	LOW+	LOW+	LOW+	MID+	MID+	HGH+	HGH+	HGH+

*Note: a + following the contact lens design indicates to add +0.25 D to the distance contact lens power on the non-dominant eye (see example below).

Example: The subject is a +1.75 ADD and has a near complaint and it is determined a change in lens pairs is needed. Referring to table 2 near complaint section, under the +1.75 ADD it states to keep the dominant eye the same (i.e. MID) and add +0.25D to the non-dominant eye (i.e. MID+).

Subjects spherical equivalent distance refraction

OD: -2.50

OS: -3.00 (OS non-dominant eye)

The new lens chosen should be as follows:

OD: -2.50 MID ADD (i.e. no change)

OS: -2.75 MID ADD

Step 3.

If after the above lens modifications have been attempted and the subject's vision is still not satisfactory, and additional optimizations are allowed by the protocol, lens changes may be attempted based on the Investigator's clinical experience, to determine if acceptable vision can be achieved.

APPENDIX I:

- LIMBAL & CONJUNCTIVAL (BULBAR) REDNESS
- EXPANDED SODIUM FLUORESCEIN CORNEAL STAINING
- DETERMINATION OF NEAR ADD
- NEAR logMAR VISUAL ACUITY MEASUREMENT PROCEDURE
- LENS FITTING CHARACTERISTICS
- SUBJECT REPORTED OCULAR SYMPTOMS
- DETERMINATION OF DISTANCE SPHEROCYLINDRICAL REFRACTIONS
- BIOMICROSCOPY SCALE
- KERATOMETRY
- DISTANCE AND NEAR VISUAL ACUITY EVALUATION
- ETDRS DISTANCE VISUAL ACUITY MEASUREMENT PROCEDURE
- VISUAL ACUITY CHART LUMINANCE AND ROOM ILLUMINATION TESTING

██████████ LIMBAL AND CONJUNCTIVAL (BULBAR) REDNESS

[REDACTED]

Limbal & Conjunctival (Bulbar) Redness

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED] EXPANDED SODIUM FLUORESCEIN CORNEAL STAINING

[REDACTED]

Expanded Sodium Fluorescein Corneal Staining

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED] DETERMINATION OF NEAR ADDITION

[REDACTED] [REDACTED]

[REDACTED] [REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]

[REDACTED] [REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]

[REDACTED] [REDACTED]
[REDACTED] [REDACTED]
[REDACTED] [REDACTED]
[REDACTED] [REDACTED]

[REDACTED]	
[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED] [REDACTED] [REDACTED] [REDACTED]
[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED] [REDACTED]
[REDACTED]	[REDACTED] [REDACTED] [REDACTED]
[REDACTED]	[REDACTED] [REDACTED] [REDACTED] [REDACTED]
[REDACTED]	[REDACTED] [REDACTED]
[REDACTED]	[REDACTED] [REDACTED] [REDACTED] [REDACTED] [REDACTED] [REDACTED] [REDACTED] [REDACTED]

[REDACTED]

[REDACTED]	
[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]

[REDACTED]
[REDACTED]
[REDACTED]
[REDACTED]

[REDACTED]

[REDACTED]	
[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]
	[REDACTED]
[REDACTED]	[REDACTED]
	[REDACTED]
[REDACTED]	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
[REDACTED]	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]

[REDACTED]	[REDACTED]	
	[REDACTED]	
	[REDACTED]	
	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]
	[REDACTED]	[REDACTED]

[REDACTED]
[REDACTED]
[REDACTED]

[REDACTED]
[REDACTED]
[REDACTED]

[REDACTED]
[REDACTED]

[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]

[illegible]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

NEAR LOGMAR VISUAL ACUITY MEASUREMENT PROCEDURE

[REDACTED]

Near LogMAR Visual Acuity Measurement Procedure

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]

		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]
		[REDACTED]	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED] LENS FITTING CHARACTERISTICS

[REDACTED]

Lens Fitting Characteristics

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]			
[REDACTED]			
[REDACTED]		[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]


[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]





SUBJECT REPORTED OCULAR SYMPTOMS/PROBLEMS

[REDACTED]

Subject Reported Ocular Symptoms/Problems

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

**[REDACTED] DETERMINATION OF DISTANCE SPHEROCYLINDRICAL
REFRACTIONS**

Journal of Management Inquiry 23(1)

11/11/2019

© 2006 The Authors

██████████

110

[illegible]

[illegible][illegible]

BIOMICROSCOPY SCALE

[REDACTED]

Biomicroscopy Scale

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[REDACTED]		[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[illegible][illegible][illegible]

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	

[REDACTED]		[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	

[REDACTED]

[REDACTED]

[REDACTED]		[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	

[REDACTED]		[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	

--	--	--	--	--	--

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED] KERATOMETRY PROCEDURE

[REDACTED]

Keratometry Procedure

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED] DISTANCE AND NEAR VISUAL ACUITY EVALUATION

[REDACTED]

	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]

	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]

[REDACTED]

	[REDACTED]
	[REDACTED]
	[REDACTED]
	[REDACTED]

[REDACTED]

	[REDACTED]
	[REDACTED]

[REDACTED]

	[REDACTED]
	[REDACTED]
	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

**[REDACTED] DISTANCE LOGMAR VISUAL ACUITY MEASUREMENT
PROCEDURE**

[REDACTED]

[REDACTED]

- [REDACTED]
 - [REDACTED]
 - [REDACTED]
 - [REDACTED]
 - [REDACTED]
 - [REDACTED]
 - [REDACTED]
 - [REDACTED]
 - [REDACTED]
 - [REDACTED]

[REDACTED]

[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED] [REDACTED] [REDACTED]
[REDACTED]	[REDACTED] [REDACTED] [REDACTED] [REDACTED]
[REDACTED]	[REDACTED] [REDACTED] [REDACTED] [REDACTED] <ul style="list-style-type: none">[REDACTED][REDACTED] [REDACTED] <ul style="list-style-type: none">[REDACTED][REDACTED] [REDACTED] <ul style="list-style-type: none">[REDACTED][REDACTED] [REDACTED] <ul style="list-style-type: none">[REDACTED] [REDACTED] [REDACTED]
[REDACTED]	[REDACTED] [REDACTED]

Page 2 of 3

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

**██████████ VISUAL ACUITY CHART LUMINANCE AND ROOM ILLUMINATION
TESTING**

[illegible]

[REDACTED]		[REDACTED]	
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]
[REDACTED]	[REDACTED]	[REDACTED]	[REDACTED]

[REDACTED]

Category	Sub-category	Value	Category	Sub-category	Value
Category 1	Sub-category 1.1	10	Category 2	Sub-category 2.1	10
	Sub-category 1.2	20		Sub-category 2.2	20
	Sub-category 1.3	30		Sub-category 2.3	30
	Sub-category 1.4	40		Sub-category 2.4	40
	Sub-category 1.5	50		Sub-category 2.5	50
	Sub-category 1.6	60		Sub-category 2.6	60
	Sub-category 1.7	70		Sub-category 2.7	70
	Sub-category 1.8	80		Sub-category 2.8	80
	Sub-category 1.9	90		Sub-category 2.9	90
	Sub-category 1.10	100		Sub-category 2.10	100

[illegible]

PROTOCOL COMPLIANCE INVESTIGATOR(S) SIGNATURE PAGE

CR-6267 Clinical Evaluation of a Reusable Multifocal Optical Design in a Presbyopic Population

Version and Date: 2.0 Amendment 1 22 June 2018

I have read and understand the protocol specified above and agree on its content.

I agree to conduct this study according to ISO 14155,¹ GCP and ICH guidelines,² the Declaration of Helsinki,³ United States (US) Code of Federal Regulations (CFR),⁴ and the pertinent individual country laws/regulations and to comply with its obligations, subject to ethical and safety considerations. The Principal Investigator is responsible for ensuring that all clinical site personnel, including Sub-Investigators adhere to all ICH² regulations and GCP guidelines regarding clinical trials during and after study completion.

I will assure that no deviation from, or changes to the protocol will take place without prior agreement from the Sponsor and documented approval from the Institutional Review Board (IRB), except where necessary to eliminate an immediate hazard(s) to the trial participants.

I am responsible for ensuring that all clinical site personnel including Sub-Investigators adhere to all ICH² regulations and GCP guidelines regarding clinical trials during and after study completion.

All clinical site personnel involved in the conduct of this study have completed Human Subjects Protection Training.

I agree to ensure that all clinical site personnel involved in the conduct of this study are informed about their obligations in meeting the above commitments.

I shall not disclose the information contained in this protocol or any results obtained from this study without written authorization.

Principal
Investigator:

Signature

Date

Name and Professional Position (Printed)

Institution/Site:

Institution/Site Name

Institution/Site Address