

CLINICAL INVESTIGATION PLAN FOR THE ZENITH® LOW PROFILE AAA ENDOVASCULAR GRAFT

Zenith® Low Profile AAA Endovascular Graft Clinical Study

Version: 08-013-07
Version Date: 15 April 2014

Sponsor and Manufacturer:

Cook Incorporated
750 Daniels Way
Bloomington, IN 47404 USA

Alternate Manufacturer:

William A. Cook Australia Pty Ltd
95 Brandl Street, Brisbane Technology Park
Eight Mile Plains, Brisbane, QLD 4113 AUSTRALIA

CLINICAL INVESTIGATION PLAN SIGNATURE PAGE

This clinical trial will be conducted in compliance with the clinical investigation plan, ISO 14155, ICH GCP, 21 CFR 812, and other applicable requirements as appropriate.

Sponsor Contact

Signature

DD/Mon/YYYY

Printed Name

Title

Coordinating Clinical Investigator

I hereby confirm that I approve of this Clinical Investigation Plan and agree to comply with its terms as laid out in this document.

Signature

DD/Mon/YYYY

Printed Name

Title

CLINICAL INVESTIGATION PLAN SIGNATURE PAGE, CON'T

Principal Clinical Investigator

I hereby confirm that I approve of this Clinical Investigation Plan and agree to comply with its terms as laid out in this document.

Signature

DD/Mon/YYYY

Printed Name

Title

CONFIDENTIALITY STATEMENT

This document shall be treated as a confidential document for the sole information and use of the clinical investigation team and the Ethics Committee/IRB.

TABLE OF CONTENTS

1.0	General Information	7
1.1	Sponsor and Manufacturer	7
1.2	Data Coordinating Center/Monitor	7
1.3	Study Administration	7
1.4	Investigators	8
1.5	Insurance	8
1.6	Monitoring Arrangements	8
1.7	Data Management and Quality Assurance	8
2.0	Approvals and Agreements	9
3.0	Clinical Investigation Plan Overview	9
4.0	Objectives of the Clinical Investigation	10
4.1	Objective	10
4.2	Claims and Intended Performance that are to be Verified	11
4.3	Specific Hypothesis to be Accepted or Rejected by Statistical Data	11
5.0	Device Description and Intended Purpose	13
5.1	Device Identification	13
5.2	Intended Purpose	14
5.3	General Device Description	15
5.4	Photographs of Device	15
5.5	Instructions for Use and Implantation	16
5.6	Summary of Necessary Training and Experience	17
5.7	Description of the Necessary Medical or Surgical Procedures	17
6.0	Preliminary Investigations and Justification	17
6.1	Literature Review	17
6.2	Non-clinical Testing	17
6.3	Previous Clinical Experience	17
7.0	Risk Analysis and Risk Assessment	17
7.1	Risks and Foreseeable Adverse Device Effects	17
7.2	Methods to Minimize Risks	19
8.0	Design of the Clinical Investigation	19
8.1	Type of Investigation	19
8.2	Rationale	19
8.3	Measures to be Taken to Avoid or Minimize Bias	19
8.4	Variables to be Measured to Demonstrate Achievement of Endpoints	19
8.5	Inclusion/Exclusion Criteria	20
8.6	Patient Consent	23
8.7	Point of Enrollment	23
8.8	Methods	24
8.9	Criteria and Procedures for Study Termination	25
8.10	Sample Size	26
8.11	Period of Use for the Device or its Control	26

8.12	Limitations of the Investigation	26
8.13	Safety Monitoring	26
9.0	Statistical Considerations	27
9.1	Sample Size Calculations	27
9.2	Performance Goals	28
9.3	Site-level Poolability	28
9.4	Missing Data	29
9.5	Future Use of Study Data	29
10.0	Emergency Situations	30
11.0	Deviations from Clinical Investigation Plan	30
12.0	Procedure for Reporting Adverse Events and Adverse Device Effects	30
13.0	Ethical Considerations	31
13.1	Declaration of Helsinki II	31
13.2	Ethical Approval	31
14.0	Early Termination or Suspension of the Investigation	32
15.0	Publication Policy	32
16.0	Data Collection	32
17.0	Data Reporting	32

Attachments

Written Procedures for Monitoring Studies	Attachment 1
Definitions	Attachment 2

1.0 General Information

1.1 Sponsor and Manufacturer

Sponsor and Manufacturer

Cook Incorporated

750 Daniels Way

Bloomington, IN 47404 USA

Contact: [REDACTED]

Telephone: [REDACTED]

Fax: [REDACTED]

E-mail: [REDACTED]

Alternate Manufacturer

William A. Cook Australia Pty Ltd

95 Brandl Street, Brisbane Technology Park

Eight Mile Plains, Brisbane, QLD 4113 AUSTRALIA

Contact: [REDACTED]

Telephone: [REDACTED]

Fax: [REDACTED]

E-mail: [REDACTED]

1.2 Data Coordinating Center/Monitor

MED Institute, Inc.

1 Geddes Way

West Lafayette, IN 47906

Contact: [REDACTED]

Telephone: [REDACTED]

Fax: [REDACTED]

E-mail: [REDACTED]

1.3 Study Administration

This study will be conducted in compliance with global regulations (e.g., ICH GCP, ISO 14155, 21 CFR 812, and other regulations as applicable).

1.4 Investigators

Contact information for the Global Principal Investigator and principal investigators will be provided in the investigator file. The contact information and qualifications for the Global Principal Investigator, principal investigators and coordinating investigators, and core laboratory will be updated and maintained by the Data Coordinating Center.

1.5 Insurance

The devices are covered by the sponsor's product liability insurance. A clinical study insurance policy will be taken out according to local requirements.

1.6 Monitoring Arrangements

The conduct of the clinical study will be supervised through a process of centralized and on-site monitoring. The data coordinating center will remotely monitor the study for data completeness and for adverse events. On-site monitoring will be implemented as necessary throughout the course of the study. The investigator/institution will provide direct access to source data/documents for study-related monitoring, audits, Ethics Committee/IRB review and regulatory inspection. Written procedures for monitoring the investigation are maintained by the monitor and are provided in Attachment 1.

Name and Address of the Monitor:

MED Institute, Inc. or designee
1 Geddes Way
West Lafayette, IN 47906

Contact:

Telephone:

Fax:

E-mail:



1.7 Data Management and Quality Assurance

The principal investigator or appropriately trained designee at each investigative site will complete standardized, data collection forms in an electronic data capturing (EDC) system (see section 16). The completed data forms and other patient documents pertaining to the study will be reviewed, processed, and stored by the sponsor. Data will be reviewed for missing data, data consistency, and reasonableness of responses. Discrepancies will be resolved through a

formal query process involving direct contact with investigators or research coordinators. The data coordinating center is responsible for database management, data verification, data archiving, and data retention

Pertinent imaging (pre-procedure, procedural, and follow-up) will be sent to MED Institute, who will coordinate shipment of imaging for independent analysis.

As needed to assist the sponsor in its research (e.g., during evaluation of an adverse event), data will be accessible to the sponsor, the participating investigators, the manufacturer, and companies or individuals the sponsor authorizes.

MED Institute, Inc., the data coordinating center, maintains a Safe Harbor Privacy Policy that describes the privacy principles followed with respect to the transfer of personal information from member states in Europe to the United States.

2.0 Approvals and Agreements

The sponsor, Global Principal Investigator, and the principal clinical investigators for each site shall agree to this document and any modifications. A justification for any modifications will be documented. Approval and agreement will be indicated by signing and dating the appropriate document.

3.0 Clinical Investigation Plan Overview

This clinical investigation is designed as a prospective non-randomized study enrolling up to 120 patients to receive the Zenith® Low Profile AAA Endovascular Graft main body in conjunction with the Zenith® Spiral-Z® AAA Iliac Leg Graft at up to 40 global clinical sites with a maximum enrollment of up to 24 patients per individual site. The objective of the study is to evaluate the safety and effectiveness of the Zenith Low Profile AAA Endovascular Graft used in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft. Freedom from major adverse events (MAEs) at 30 days and device success at 12 months for this treatment cohort will be compared to their respective performance goals derived from the results of the Zenith® AAA Endovascular Graft clinical study.

Any patient with an abdominal aortic, aortoiliac, or iliac aneurysm and suitable for treatment with the Zenith Low Profile AAA Endovascular Graft with the 16 Fr or

17 Fr H&L-B One-Shot™ Introduction System in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft with the Z-Trak® Introduction System is eligible for enrollment in the study. The study flow diagram is presented in Figure 1.

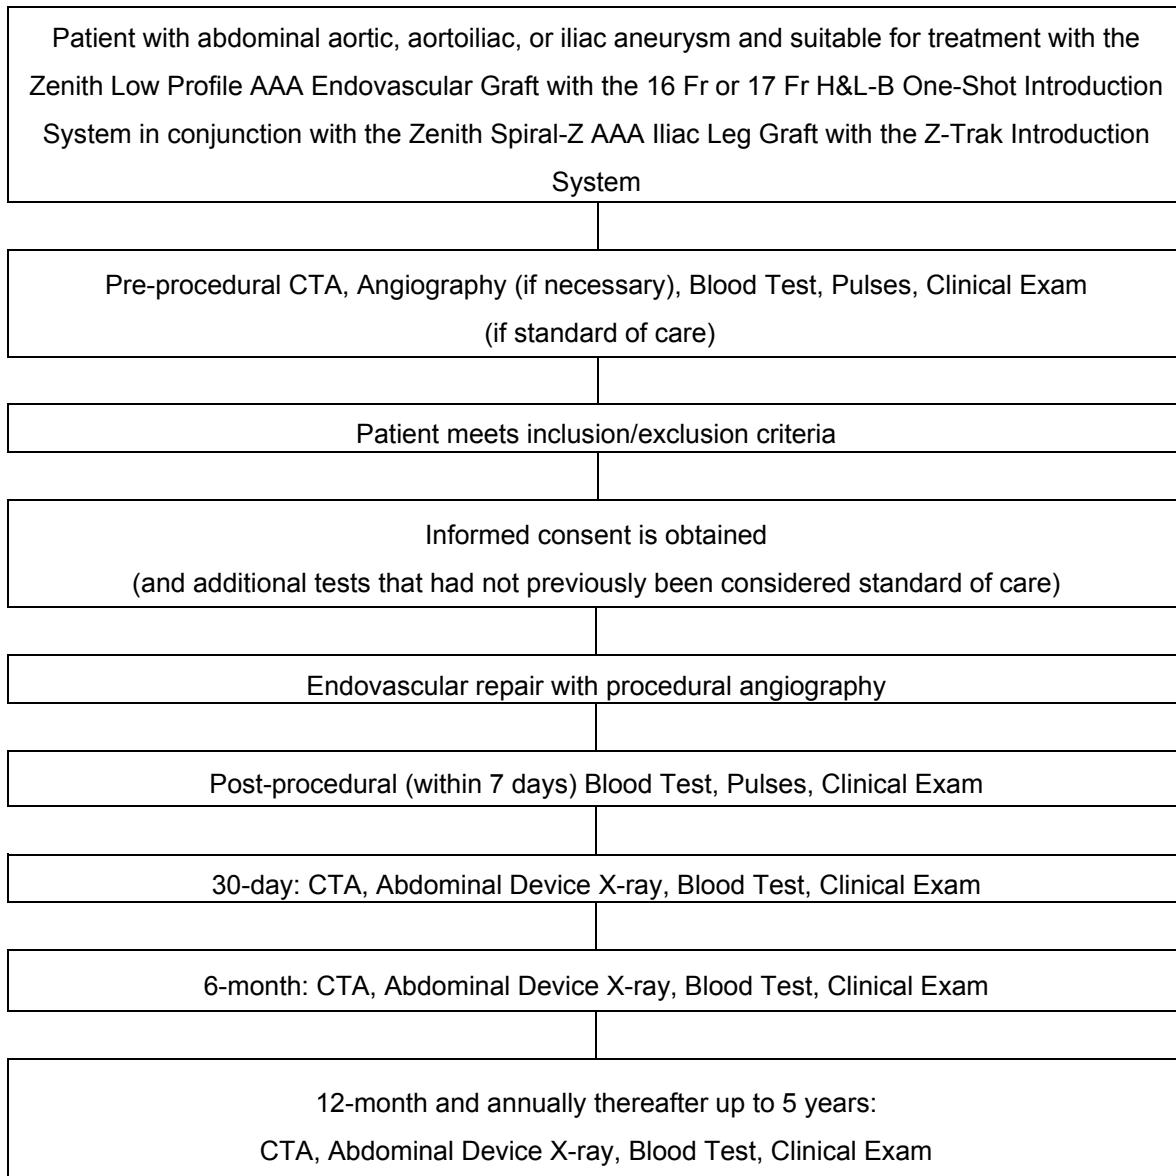


Figure 1. Study flow diagram

4.0 Objectives of the Clinical Investigation

4.1 Objective

The objective of the study is to evaluate the safety and effectiveness of the Zenith Low Profile AAA Endovascular Graft used in conjunction with the Zenith

Spiral-Z AAA Iliac Leg Graft. The safety endpoint will be freedom from MAEs at 30 days and the effectiveness endpoint will be device success at 12 months.

4.2 Claims and Intended Performance that are to be Verified

The following data points will be evaluated to verify device performance:

- Device success (including technical success)
- Procedural times
- Access method (percutaneous, cutdown, or conduit usage) employed during the procedure
- Clinical utility measures
- Morbidity, including Major Adverse Events (MAEs) as well as events distal to the graft limb (e.g., arterial thrombosis)
- Reinterventions-
- Endoleak, change in aneurysm size, migration, device patency, device integrity

4.3 Specific Hypotheses to be Accepted or Rejected by Statistical Data

The safety endpoint of 30-day freedom from MAEs will be analyzed on a per patient basis. The analysis requires that the agreed upon performance goal of 88%, which was derived from the 30-day freedom from MAE rate for patients treated with the currently approved Zenith AAA Endovascular Graft, be met. The performance goal will be said to have been met provided that the null hypothesis is rejected in favor of the alternate with a one-tailed exact binomial test at the 0.025-level. Given that $\pi_{MAE(30)}$ is the probability that a randomly selected patient experienced freedom from MAEs at 30 days, the null and alternate hypotheses are as follows.

Null Hypothesis: The 30-day freedom from MAEs for patients treated with the Zenith Low Profile AAA Endovascular Graft in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft does not meet the performance goal (88%).

$$H_0: \pi_{MAE(30)} < 88\%$$

Alternate Hypothesis: The 30-day freedom from MAEs for patients treated with the Zenith Low Profile AAA Endovascular Graft in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft meets the performance goal (88%).

$$H_A: \pi_{MAE(30)} \geq 88\%$$



Similarly, the effectiveness endpoint of 12-month device success will be analyzed on a per patient basis. The analysis requires that the agreed upon performance goal of 83%, which was derived from the 12-month device success rate for patients treated with the currently approved Zenith AAA Endovascular Graft, be met. The performance goal will be said to have been met provided that the null hypothesis is rejected in favor of the alternate with a one-tailed exact binomial test at the 0.025-level. Given that $\pi_{DS(12)}$ is the probability that a randomly selected patient experienced device success at 12 months, the null and alternate hypotheses are as follows.

Null Hypothesis: The 12-month device success for patients treated with the Zenith Low Profile AAA Endovascular Graft in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft does not meet the performance goal (83%).

$$H_0: \pi_{DS(12)} < 83\%$$

Alternate Hypothesis: The 12-month device success for patients treated with the Zenith Low Profile AAA Endovascular Graft in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft meets the performance goal (83%).

$$H_A: \pi_{DS(12)} \geq 83\%$$



5.0 Device Description and Intended Purpose

5.1 Device Identification

The name of the device is the Zenith Low Profile AAA Endovascular Graft which is used in conjunction with the commercially available Zenith Spiral-Z AAA Iliac Leg Graft.

The following main body (Table 5.1-1), iliac leg (Table 5.1-2), and ancillary device sizes (Tables 5.1-3 and 5.1-4) will be available for the study:

Table 5.1-1. Zenith Low Profile AAA Endovascular Graft Main Body Graft Size Availability*

ZALB-22-70	ZALB-24-70	ZALB-26-70	ZALB-28-70	ZALB-30-70	ZALB-32-70	ZALB-36-70
ZALB-22-84	ZALB-24-84	ZALB-26-84	ZALB-28-84	ZALB-30-84	ZALB-32-84	ZALB-36-84
ZALB-22-98	ZALB-24-98	ZALB-26-98	ZALB-28-98	ZALB-30-98	ZALB-32-98	ZALB-36-98
ZALB-22-108	ZALB-24-108	ZALB-26-108	ZALB-28-108	ZALB-30-108	ZALB-32-108	ZALB-36-108
ZALB-22-118	ZALB-24-118	ZALB-26-118	ZALB-28-118	ZALB-30-118	ZALB-32-118	ZALB-36-118
ZALB-22-128	ZALB-24-128	ZALB-26-128	ZALB-28-128	ZALB-30-128	ZALB-32-128	ZALB-36-128

* Graft sizes are ZALB-XX-YY where XX mm is the proximal graft diameter and YY mm is the length from the proximal graft edge to the distal end of the contralateral leg.

Table 5.1-2. Zenith Spiral-Z AAA Iliac Leg Graft Size Availability*

ZSLE-9-39	ZSLE-11-39	ZSLE-13-39	ZSLE-16-39	ZSLE-20-39	ZSLE-24-39
ZSLE-9-56	ZSLE-11-56	ZSLE-13-56	ZSLE-16-56	ZSLE-20-56	ZSLE-24-56
ZSLE-9-74	ZSLE-11-74	ZSLE-13-74	ZSLE-16-74	ZSLE-20-74	ZSLE-24-74
ZSLE-9-90	ZSLE-11-90	ZSLE-13-90	ZSLE-16-90	ZSLE-20-90	ZSLE-24-90
ZSLE-9-107	ZSLE-11-107	ZSLE-13-107			
ZSLE-9-122	ZSLE-11-122	ZSLE-13-122			

* Graft sizes are ZSLE-XX-YY where XX mm is the distal graft diameter and YY mm is the working length (from the distal edge of the overlap zone to the distal edge of the graft material).

Table 5.1-3. Zenith Low Profile AAA Endovascular Graft Main Body Extension Graft Size

Availability*

ZLBE-22-45	ZLBE-24-45	ZLBE-26-45	ZLBE-28-45	ZLBE-30-45	ZLBE-32-45	ZLBE-36-45
ZLBE-22-58	ZLBE-24-58	ZLBE-26-58	ZLBE-28-58	ZLBE-30-58	ZLBE-32-58	ZLBE-36-58

* Graft sizes are ZLBE-XX-YY where XX mm is the proximal graft diameter and YY mm is the graft length.

Table 5.1-4. Zenith Low Profile AAA Endovascular Graft Converter Graft Size Availability*

ZLC-24-66	ZLC-28-66	ZLC-32-66	ZLC-36-66
-----------	-----------	-----------	-----------

* Graft sizes are ZLC-XX-YY where XX mm is the proximal graft diameter and YY mm is the graft length.

Devices under investigation will be tracked by the clinical site throughout the course of the clinical study. This includes information such as lot numbers, quantity, and disposition of devices. Additionally, information such as the quantity, size(s), and lot number(s) of devices used in patients will be recorded on Case Report Forms (CRFs).

5.2 Intended Purpose

The Zenith Low Profile AAA Endovascular Graft with the Zenith Spiral-Z AAA Iliac Leg Graft and ancillary components are indicated for the endovascular treatment of patients with abdominal aortic, aorto-iliac, or iliac aneurysms having morphology suitable for endovascular repair, including:

- Iliac/femoral anatomy that is suitable for access with a 16 Fr (6.0 mm nominal sheath O.D.) or 17 Fr (6.5 mm nominal sheath O.D.) introduction system;
- Non-aneurysmal infrarenal aortic segment (neck) proximal to the aneurysm:
 - with a length of at least 15 mm,
 - with a diameter measured outer wall to outer wall of no greater than 32 mm and no less than 18 mm,
 - with an angle less than 60 degrees relative to the long axis of the aneurysm, and
 - with an angle less than 45 degrees relative to the axis of the suprarenal aorta; and
- Iliac artery distal fixation site greater than 10 mm in length and 7.5-20 mm in diameter (measured outer wall to outer wall).

5.3 General Device Description

A general device description, including any materials that will be in contact with tissues or body fluids can be located in the Clinical Investigator Brochure. The device does not contain medicinal products, human and/or animal tissues or their derivatives, or other biologically active substances.

5.4 Photographs of Device

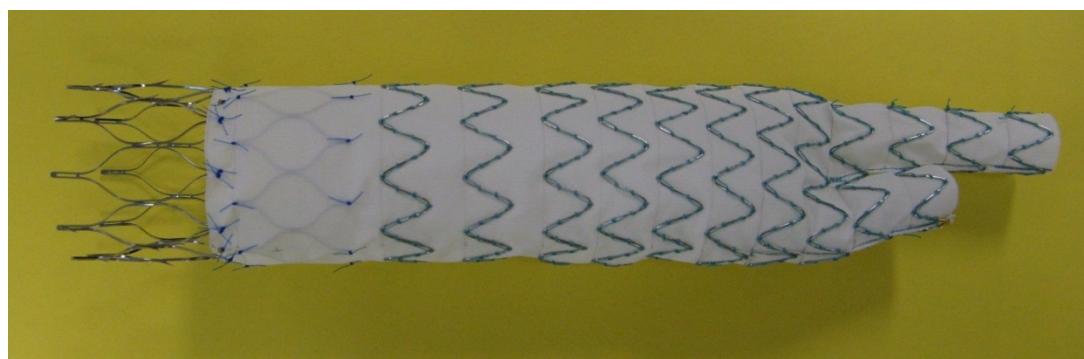


Figure 2. Zenith Low Profile AAA Endovascular Graft Main Body

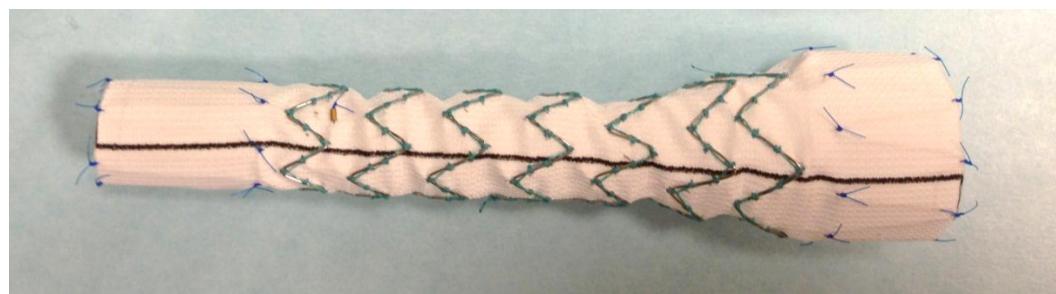


Figure 3. Zenith Spiral-Z AAA Iliac Leg Graft



Figure 4. Zenith Low Profile AAA Endovascular Graft Introduction System

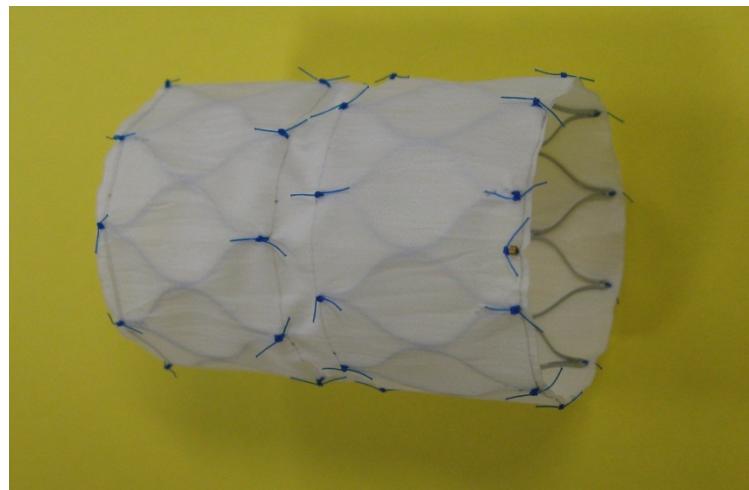


Figure 5. Zenith Low Profile AAA Endovascular Graft Main Body Extension

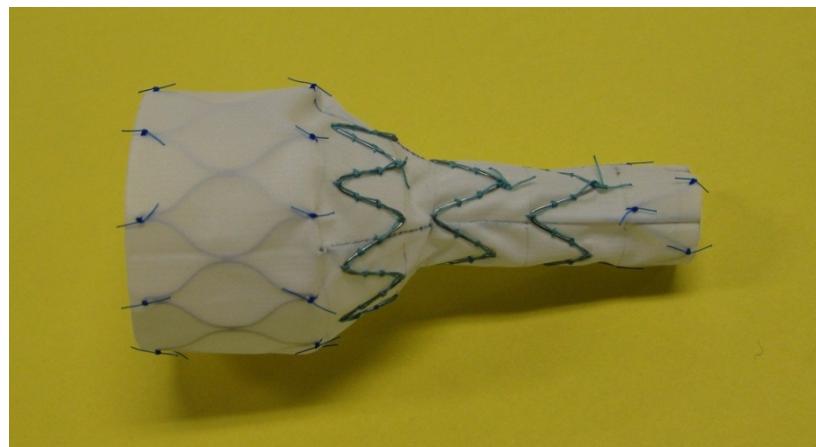


Figure 6. Zenith Low Profile AAA Endovascular Graft Converter

The Zenith Iliac Plug, which is commercially available, may be used in conjunction with the Zenith Low Profile AAA Endovascular Graft Converter to convert the patient to an aortouni-iliac configuration, if necessary.

5.5 Instructions for Use and Implantation

Please reference the manufacturer's Instructions for Use for complete instructions including implantation, storage and handling requirements, preparation for use, pre-use checks for safety and performance, and precautions to be taken after use.

5.6 Summary of Necessary Training and Experience

The Zenith Low Profile AAA Endovascular Graft and Zenith Spiral-Z AAA Iliac Leg Graft should be deployed by investigators trained and experienced in endovascular procedures. Please refer to the manufacturer's Instructions for Use for a complete summary of the necessary training and experience required for use of these devices.

5.7 Description of the Necessary Medical or Surgical Procedures

Please refer to the manufacturer's Instructions for Use for a complete description of the procedures involved in the use of these devices.

6.0 Preliminary Investigations and Justification

6.1 Literature Review

Please refer to the Clinical Investigator Brochure for a complete literature review and evaluation.

6.2 Non-clinical Testing

Non-clinical tests were conducted in accordance with Good Laboratory Practice requirements, or performed in compliance with verified methods and Standard Operating Procedures to maintain the integrity of the results. *In vitro* testing has established reasonable safety of the device for the duration of the study and in the trial population to be studied. Please refer to the Clinical Investigator Brochure for a summary of non-clinical testing.

6.3 Previous Clinical Experience

Please refer to the Clinical Investigator Brochure for a complete description of the previous clinical experiences with these devices and other similar devices.

7.0 Risk Analysis and Risk Assessment

Please refer to the Clinical Investigator Brochure for a complete risk analysis.

7.1 Risks and Foreseeable Adverse Device Effects

Risks of adverse events are likely to be similar to those reported in recent studies of other endovascular AAA grafts. Adverse events associated either with the Zenith Low Profile AAA Endovascular Graft, the Zenith Spiral-Z AAA Iliac Leg Graft, or the implantation procedure that may occur and require intervention include, but are not limited to:

- Amputation
- Anesthetic complications and subsequent attendant problems (e.g., aspiration)
- Aneurysm enlargement
- Aneurysm rupture and death
- Aortic damage, including perforation, dissection, bleeding, rupture and death
- Arterial or venous thrombosis and/or pseudoaneurysm
- Arteriovenous fistula
- Bleeding, hematoma, or coagulopathy
- Bowel complications (e.g., ileus, transient ischemia, infarction, necrosis)
- Cardiac complications and subsequent attendant problems (e.g., arrhythmia, myocardial infarction, congestive heart failure, hypotension, hypertension)
- Claudication (e.g., buttock, lower limb)
- Death
- Edema
- Embolization (micro and macro) with transient or permanent ischemia or infarction
- Endoleak
- Endoprostheses: improper component placement; incomplete component deployment; component migration; suture break; occlusion; infection; stent fracture; graft material wear; dilatation; erosion; puncture; perigraft flow; barb separation and corrosion
- Fever and localized inflammation
- Genitourinary complications and subsequent attendant problems (e.g., ischemia, erosion, fistula, incontinence, hematuria, infection)
- Graft or native vessel occlusion
- Hepatic failure
- Impotence
- Infection of the aneurysm, device or access site, including abscess formation, transient fever and pain
- Lymphatic complications and subsequent attendant problems (e.g., lymph fistula)
- Neurologic local or systemic complications and subsequent attendant problems (e.g., stroke, transient ischemic attack, paraparesis, paralysis)
- Pulmonary/respiratory complications and subsequent attendant problems (e.g., pneumonia, respiratory failure, prolonged intubation)

- Renal complications and subsequent attendant problems (e.g., artery occlusion, contrast toxicity, insufficiency, failure)
- Surgical conversion to open repair
- Vascular access site complications, including infection, pain, hematoma, pseudoaneurysm, or arteriovenous fistula
- Vascular spasm or vascular trauma (e.g., iliofemoral vessel dissection, bleeding, rupture, death)
- Vessel damage
- Wound complications and subsequent attendant problems (e.g., dehiscence, infection)

7.2 Methods to Minimize Risks

The device design, non-clinical testing, clinical study design, and the Instructions for Use are intended to minimize the risks associated with the endovascular procedures.

8.0 Design of the Clinical Investigation

8.1 Type of Investigation

The current investigation is a prospective, non-randomized, non-blinded study.

8.2 Rationale

The assessment of safety will be based on freedom from MAEs at 30 days and the assessment of effectiveness will be based on device success at 12 months.

8.3 Measures to be Taken to Avoid or Minimize Bias

This study is not randomized or blinded, as it is intended to prospectively collect information regarding the safety and effectiveness of the Zenith Low Profile AAA Endovascular Graft in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft. Similar inclusion/exclusion criteria will be used during patient selection for the current patient cohort compared to that for the Zenith AAA Endovascular Graft clinical study, which was the basis for the chosen performance goals.

8.4 Variables to be Measured to Demonstrate Achievement of Endpoints

To evaluate deployment characteristics and procedural outcome, the following data points will be collected intra-operatively:

- 1) Assessment of system performance including: deployment issues, ease of insertion, visualization, and ease of removal
- 2) Complications (if any)
- 3) Ancillary equipment needed
- 4) Adjunctive maneuvers including: balloon dilation of iliac arteries, additional stents required, and additional surgical procedures
- 5) Findings of completion assessment: minimum iliac leg graft lumen diameter, device patency, endoleak, and kinks

In addition, the results of the endovascular repair will be assessed by clinical and/or imaging evaluation at the time of graft insertion, within 7 days post-procedure, at 30 days [REDACTED], 6 months [REDACTED], 12 months [REDACTED] [REDACTED], 2 years [REDACTED], 3 years [REDACTED], 4 years [REDACTED] [REDACTED], and 5 years [REDACTED] according to the post-operative study schedule below. [REDACTED]
[REDACTED]

Study Schedule						
	Pre-op	Intra-op	Post-procedure	30-Day	6-Month	12-Month ⁵
Clinical Exam	X		X	X	X	X
Pulses	X		X			
Blood Test ¹	X		X	X	X	X
CTA	X ²			X ⁴	X ⁴	X ⁴
Abdominal Device X-ray				X	X	X
Angiography	X ³	X				

1 Blood test for serum creatinine.
2 Imaging should be performed within 6 months prior to implant procedure.
3 Required only to resolve any uncertainties in anatomical measurements necessary for graft sizing.
4 A non-contrast CT in conjunction with a duplex ultrasound may be used for those patients experiencing renal failure or who are otherwise unable to undergo contrast enhanced CT scan.
5 Yearly thereafter through 5 years.

8.5 Inclusion/Exclusion Criteria

Patients must meet at least one of the inclusion criteria below to be enrolled in the study. General and medical exclusion criteria will be assessed during the initial patient evaluation by conducting a history and physical examination. Anatomical exclusion criteria will be assessed using a variety of imaging

techniques that are routinely performed during the evaluation of abdominal aortic aneurysms. Sectional imaging will be performed by CT scan.

Angiography and intravascular ultrasound will be performed as needed to further assess inclusion/exclusion criteria.

Assessment of entry criteria will be based upon data available pre-operatively. Data obtained peri-operatively and post-operatively (including the results from core lab analysis of pre-procedure imaging) may contradict pre-operative assessment. However, such contradiction is not considered a protocol violation and should not be construed as evidence of inadequate or inaccurate pre-operative assessment with respect to the enrollment criteria or evidence of inappropriate enrollment. Enrollment is to be based upon best available pre-operative data. Therefore, some criteria relate to subjective assessment while other criteria are considered absolute and able to be determined definitively. Variability in assessment between centers, investigators and observers is expected with several criteria.

8.5.1 Inclusion Criteria

A patient is deemed suitable for inclusion in the study if the patient has at least one of the following AND is suitable for treatment with the Zenith Low Profile AAA Endovascular Graft with the 16 Fr (for 22 – 32 mm diameter grafts) or 17 Fr (for 36 mm diameter graft) H&L-B One-Shot Introduction System in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft with the Z-Trak Introduction System:

- 1) Aortic or aortoiliac aneurysm with a diameter ≥ 5.0 cm for males or ≥ 4.5 cm for females
- 2) Iliac aneurysm with a diameter ≥ 3.0 cm
- 3) Aneurysm with a history of growth ≥ 0.5 cm per year.

8.5.2 Exclusion Criteria

Patients must be excluded from the study if any of the following conditions are true:

General Exclusion Criteria

- 1) Less than 18 years of age
- 2) Other current conditions (e.g., cancer, systemic infection) that may cause the patient to be noncompliant with the clinical investigation plan, that may confound the results, or that is associated with a life expectancy less than 2 years
- 3) Pregnant or breastfeeding or planning on becoming pregnant within 60 months
- 4) Unwilling to comply with the follow-up schedule
- 5) Inability or refusal to give informed consent
- 6) Less than 30 days beyond primary endpoint for other investigative drug or device study

Medical Exclusion Criteria

- 1) Known sensitivities or allergies to nitinol (nickel, titanium), polyester, polypropylene, gold, stainless steel, or solder (tin, silver)
- 2) History of anaphylactic reaction to contrast material that cannot be adequately premedicated
- 3) Leaking/ruptured or symptomatic aneurysm
- 4) Uncorrectable coagulopathy
- 5) Planned interventional or surgical procedure that is unrelated to AAA repair within 30 days before or after AAA repair

Anatomical Exclusion Criteria

- 1) Significant occlusive disease, tortuosity, or calcification
- 2) Proximal neck <15 mm in length
- 3) Proximal neck, measured outer wall to outer wall on a sectional image (CT) > 32 mm in diameter or <18 mm in diameter
- 4) Proximal neck angulated more than 60 degrees relative to the long axis of the aneurysm
- 5) Immediate suprarenal neck angulated more than 45 degrees relative to the immediate infrarenal neck
- 6) Proximal seal site with inverted funnel shape (change in neck diameter > 10% over the first 15 mm of proximal neck length)
- 7) Proximal seal site with circumferential thrombus/atheroma
- 8) Aortic diameter, measured inner wall to inner wall on a sectional image (CT), < 20 mm just proximal to the aortoiliac bifurcation

- 9) Iliac/femoral anatomy that is unsuitable for access with the 16 Fr (6.0 mm nominal sheath O.D.) or 17 Fr (6.5 mm nominal sheath O.D.) introduction system
- 10) Iliac artery diameter, measured outer wall to outer wall on a sectional image (CT), > 20 mm or < 7.5 mm at distal fixation site
- 11) Iliac artery distal fixation site < 10 mm in length
- 12) Indispensable inferior mesenteric artery (IMA)
- 13) Inability to maintain at least one patent hypogastric artery
- 14) Renal artery stenosis > 80% (and serum creatinine > 2.0 mg/dl)
- 15) Unsuitable arterial anatomy

8.6 Patient Consent

Patients who meet all of the inclusion criteria and none of the exclusion criteria will be invited to participate in this study. All patients eligible for entry will have the clinical study explained to them, as well as potential risks and benefits of their participation in the study. Each patient who agrees to participate will be required to sign and date an informed consent document prior to the procedure or any study-specific testing. If approved by the local Ethics Committee/IRB, a legally authorized representative may provide consent on behalf of the patient.

If new information is obtained after a patient receives treatment with the device, patients who have not exited the study will be informed about the new information, and will be reconsented at the discretion of the investigator and/or the site's Ethics Committee/IRB.

8.7 Point of Enrollment

Point of enrollment will be based on the intent-to-treat population, and is defined to include any patient for which the treatment procedure is initiated. More specifically, once a procedure has begun (i.e., cutdown or percutaneous access initiated), this patient would be included in the intent-to-treat population. The patient's informed consent will be obtained and assessment of the patient's conformance to the inclusion/exclusion criteria will occur prior to the procedure.

8.8 Methods

8.8.1. Medication

The hospital's standard protocol should be followed with respect to medication.

8.8.2. Pre-procedure

Grafts are sized based on the findings from preoperative radiologic studies, including computerized tomography (CT) or conventional angiography. Refer to the Instructions for Use for details regarding the suggested imaging studies to be obtained and sizing guidelines.

8.8.3. Procedure

Standard techniques for placement of arterial access sheaths, guiding catheters, angiographic catheters and wire guides should be employed during use of the Zenith Low Profile AAA Endovascular Graft and the Zenith Spiral-Z AAA Iliac Leg Graft. The Zenith Low Profile AAA Endovascular Graft and the Zenith Spiral-Z AAA Iliac Leg Graft are compatible with 0.035 inch diameter wire guides.

Refer to institutional protocols relating to anesthesia, anticoagulation and monitoring of vital signs. Refer to the Instructions for Use for complete details regarding use of the Zenith Low Profile AAA Endovascular Graft and the Zenith Spiral-Z AAA Iliac Leg Graft. Fluoroscopic guidance and angiography should be used throughout the procedure to verify positioning of the devices with respect to the patient's anatomy.

The iliac leg graft should overlap with the main body limb by at least one stent, as inadequate overlap (< 1 stent) may increase the risk for migration and/or endoleak. Excessive overlap of the iliac leg graft with the main body (leg component more than 10 mm above the main body bifurcation) may restrict flow and thereby increase the risk of limb thrombosis. Additionally, the proximal edge of the ipsilateral leg graft should align closely with that of the contralateral leg graft (i.e., the ends of both graft legs should be at the same height relative to the graft bifurcation).

If the distal seal of the iliac leg graft lands in a location different from that used to select the graft size, undersizing or excessive oversizing could result. Excessive oversizing may result in flow restriction with higher risk of limb thrombosis and

should be treated appropriately at the time of procedure (e.g., with adjunctive balloon dilatation and/or stent placement).

Pre-existing regions of stenosis/narrowing less than approximately 20 mm ID in the aorta or 7-8 mm ID in the iliac arteries may increase the risk for limb thrombosis if left untreated. Dilatation of these regions with a noncompliant balloon and/or stent placement may be necessary to help assure continued graft patency. The completion angiogram (with stiff wire guides removed) should be reviewed carefully to determine whether further treatment in these regions is necessary (e.g., adjunctive balloon dilatation/stent placement). Failure to remove the stiff wire guide prior to the angiogram could mask any limb kinking or narrowing that might occur when the wire guide is removed.

Both graft leg lumens should be evaluated carefully in multiple views at the completion of the procedure to assess for any narrowing and to document the minimum graft lumen ID. Patients with a graft leg lumen less than approximately 5 mm ID may be at increased risk for limb thrombosis. Intervention (e.g., noncompliant balloon dilatation and/or stent placement) should be considered to help assure continued graft patency.

8.8.4. Peri-operative Care

The endovascular method does not require any departure from the usual peri-operative management of patients undergoing aneurysm repair.

8.8.5. Post-operative Treatment of Endoleaks

Type I and type III endoleaks warrant immediate treatment. Type II endoleaks should be treated at the physician's discretion, depending on aneurysm behavior and size, endoleak source, and time from implantation. If the aneurysm is enlarging, treatment by embolization or ligation should be considered. Type III endoleaks should be treated with additional ballooning or prostheses.

8.9 Criteria and Procedures for Study Termination

A patient's follow-up in the study will end after:

- 1) Failure to deploy the device + 30 days;
- 2) Conversion to open surgical technique + 30 days;
- 3) Patient withdrawal or lost to follow-up;

- 4) Patient death;
- 5) Closure of the investigation; or
- 6) Completion of all scheduled clinical and imaging visits through 5 years.

No medical care related to the clinical study will be provided for the subjects after study completion.

8.10 Sample Size

This investigation will enroll a maximum of 120 subjects at a maximum of 40 investigative sites. Patient recruitment is expected to be completed within 12 months of initiating the study. Follow-up data will continue to be collected for 5 years after graft deployment for each patient in the study, making the study duration at least 72 months.

8.11 Period of Use for the Device or its Control

The 5-year follow-up period of the clinical investigation should permit the demonstration of performance over a period of time sufficient to represent a realistic test of the performance of the device and allow identification and risk assessment of any associated adverse device effects over that period.

8.12 Limitations of the Investigation

This study is inherently limited by the number of patients who will be excluded due to general, medical, and anatomical exclusion criteria. Additional challenges of the study include the anticipated comorbidities likely to be found in patients with aortic, aortoiliac, or iliac aneurysms, which may confound data analysis. Additional confounding elements of the study might include the lower incidence of AAA in women, with the anticipation of fewer women than men being enrolled in the study.

8.13 Safety Monitoring

Safety monitoring will include collecting data regarding adverse events. Section 7, Risk Analysis, lists the potential adverse events associated with this study.

A Data Safety Monitoring Board (DSMB) consisting of independent physicians and at least one independent statistician, who are not investigators in the study, nor have a perceived conflict of interest with the conduct and administration of

the study, will be convened on a regular basis to evaluate the study progress and review adverse events.

An independent Clinical Events Committee (CEC) will be established to adjudicate clinical events reported during the study. This adjudication will be performed according to standard operating procedures to assess whether the events were due to a pre-existing condition, procedure-related, technique-related, and/or device-related. In addition, a core lab will be established to independently review available imaging.

Regular scheduled monitoring, including on-site visits, will be conducted, in part, for identification of adverse events and assurance that they are correctly reported to the DSMB, CEC, and Ethics Committees/IRBs.

In addition, incidences of intra-operative conversion to open surgical aneurysm repair, access failure, and intra-operative type I or type III endoleak will be evaluated by the sponsor on a case-by-case basis. If a potential safety issue is identified, the sponsor may delay additional enrollment until further investigation into the incident is performed.

9.0 Statistical Considerations

9.1 Sample Size Calculations

Evaluation of the safety hypothesis, 30-day freedom from MAEs, requires 46 patients to determine whether the performance goal of 88% has been met. Evaluation of the effectiveness hypothesis, 12-month device success, requires 59 patients to determine whether the performance goal of 83% has been met. Cook intends to enroll 120 patients to account for patients who withdraw or are lost to follow-up, and also to provide added enhanced statistical certainty as well as the same number of patients as agreed to for a previous similar study.

Sample size calculations for the safety and effectiveness hypotheses can be performed with the following assumptions. Using performance goals of 88% for freedom from MAEs and 83% for device success, with an expected rate of 99.2% for freedom from MAEs and 93.5% for device success, an exact binomial calculation, $\alpha=0.025$, power=0.80 and a one-sided test, 46 patients for freedom

from MAEs and 59 patients for device success are required to demonstrate that the Zenith Low Profile AAA Endovascular Graft in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft meets the stated performance goals.

9.2 Performance Goals

The performance goals used for the hypotheses in section 4.3 and the sample size calculations in section 9.1 were derived from the pivotal study of the Zenith AAA Endovascular Graft. The 30-day freedom from MAEs was 98.3% and the 12-month device success was 93.0% in the pivotal study of the Zenith AAA Endovascular Graft. Therefore, the performance goals of 88% for freedom from MAEs and 83% for device success, respectively, have been determined.

9.3 Site-level Poolability

Poolability of data from multiple sites will be verified by examining the safety and efficacy measures as well as important patient baseline characteristics among sites. Site-level poolability will be considered appropriate provided that these measures are similar among sites.



9.4 Missing Data

Missing data will be addressed using three primary strategies: 1) estimating missing data with the best available data, 2) case deletion, and 3) multiple imputation.

The first strategy may be used for missing imaging data. Previous clinical trial experience suggests that some portion of the imaging data may not meet the criteria for accurate measurements by the core laboratory. However, it is recognized that the treating physician uses this information to provide the best possible care for the patient. Therefore, it is reasonable to substitute any missing core laboratory measurements with the corresponding measurements made by the treating physician (or his/her staff). In addition, the absence or presence of clinical sequelae may provide the required missing core laboratory assessment of device performance. This strategy is a best approximation of the missing data value.

The second strategy is case deletion. If the amount of missing data does not result in a reduction of analyzable patients to a number that is below that required for sufficient statistical power of the endpoints, then case deletion will be the method of choice for that analysis.

The third method is multiple imputation. This method will be used to predict missing endpoint or covariate data. It may be that the study endpoints may depend upon certain covariates. Therefore, it may be possible to model study endpoints, given a series of related covariates. This model-based imputation exercise may provide estimates of the missing data that can be utilized in estimating event rates and confidence bounds.

9.5 Future Use of Study Data

The data collected in this study may be used to justify additional studies of variations on the Zenith Low Profile AAA Endovascular Graft including, but not limited to, design variations. It is anticipated that the safety and effectiveness

data obtained may serve as prior information in the analysis of the safety and effectiveness of future variations of the Zenith Low Profile AAA Endovascular Graft.

10.0 Emergency Situations

Patients will not be treated with the Zenith Low Profile AAA Endovascular Graft in conjunction with the Zenith Spiral-Z AAA Iliac Leg Graft in emergency situations where prior consent of the patient is not possible.

11.0 Deviations from Clinical Investigation Plan

Investigators are not allowed to deviate from this Clinical Investigation Plan without prior authorization by the sponsor except under emergency situations when necessary to preserve the rights, safety, or well-being of study patients.

Deviations or noncompliances will be recorded together with an explanation. Deviations or noncompliances that impact the rights, welfare, or safety of patients shall be reported to the sponsor and Ethics Committee/IRB as required and as soon as possible. If appropriate, corrective and preventive actions will be discussed by the sponsor, investigator, and/or the Ethics Committee/IRB to determine a suitable course of action.

When available, the reasons for withdrawal and discontinuation of any patient from the investigation shall be recorded. If such discontinuation is because of problems with safety or lack of effectiveness of the device, that patient shall still be followed-up in the investigation, if possible.

12.0 Procedure for Reporting Adverse Events and Adverse Device Effects

Events known to be related to pre-existing conditions or existing at admission are not considered adverse events (e.g., prior medically-treated cardiac arrhythmia with no change in status during the endovascular procedure). Additionally, common standard of care practices are not considered adverse events (e.g., centers located at high geographical altitudes that discharge all patients on home oxygen therapy regardless of procedure).

All adverse events (i.e., device-related and non-device-related) are to be reported using the appropriate case report form (Adverse Event/Complication

form). In cases of adverse device effects (adverse event with relation to the study device) or serious adverse events, completed forms should be submitted to the Data Coordinating Center as soon as possible upon knowledge of the event.

MED Institute, Inc.
1 Geddes Way
West Lafayette, IN 47906
Telephone: [REDACTED]
Fax: [REDACTED]

The Data Coordinating Center will notify the sponsor/manufacturer accordingly. In accordance with applicable requirements, the investigator will notify the local Ethics Committee/IRB, while the sponsor/manufacturer will notify the regulatory authority. Furthermore, if the sponsor determines that the device presents a potential risk to the study patients, all investigators in the study will be notified. Clinical sites will be responsible for following their normal reporting process (e.g., to manufacturer, to regulatory authority) for any problems with the commercially available devices. Refer to section 7.1 for a list of potential adverse events related to this study.

13.0 Ethical Considerations

13.1 Declaration of Helsinki

The investigation shall be performed according to the ethical principles that have their origin in the Declaration of Helsinki and in accordance with ISO 14155, ICH GCP, and 21 CFR 812.

13.2 Ethical Approval

The investigator is responsible for obtaining approval of this clinical investigation by the relevant Ethics Committee/IRB, and the clinical study will not begin until a favorable opinion of the Ethics Committee/IRB has been obtained. The sponsor must be provided with a copy of this approval before delivery of any study device. The investigator is responsible for complying with the requirements imposed by his/her Ethics Committee/IRB and/or regulatory authority. Furthermore, the investigator will ensure that local regulations concerning data protection are followed.

14.0 Early Termination or Suspension of the Investigation

The sponsor reserves the right to terminate/suspend the study at any point should they believe that important harmful events might result from its continuation. If a decision is made to terminate the study, all patients already treated will be followed according to the study follow-up schedule. Subjects may withdraw from the study at any time without penalty or loss of benefits. The subject should notify the investigator of his/her desire to withdraw. The investigator may also decide to withdraw a subject from the study at any time on the basis of medical judgement. In any case, the reasons for withdrawal will be documented, when available.

15.0 Publication Policy

Publication and presentation policies are outlined in the study contractual documents.

16.0 Data Collection

Patient data will be collected and entered by trained personnel at the clinical site onto electronic Case Report Forms (eCRFs) through an electronic data capturing (EDC) system. This is a secure, web-based system, allowing those with permission to access data from any location at any time. Source data are to be retained for data entered into the EDC system. Data obtained and simultaneously entered into the EDC system may also serve as source documentation.

Site personnel are required to undergo data entry training and will have unique login names and passwords in order to enter patient data. In accordance with 21 CFR Part 11, the EDC system creates a secure, computer-generated, time stamped audit trail to record the date and time of operator entries and actions that create, modify, or delete electronic records.

17.0 Data Reporting

Progress reports and a final report at the conclusion of the clinical investigation will be submitted by the investigators and sponsor to the regulatory bodies and Ethics Committees/IRBs as required by local regulations.

Attachment 1
Written Procedures for Monitoring Studies

1. **What is the primary purpose of the study?** (Please check one box)

5

100% of the time, the system is able to correctly identify the target word in the sentence. This is a significant improvement over the baseline system, which only achieves 50% accuracy.

For more information, contact the Office of the Vice President for Research and Economic Development at 319-273-2500 or research@uiowa.edu.

For more information, contact the Office of the Vice President for Research and Economic Development at 319-273-2500 or research@uiowa.edu.

For more information, contact the Office of the Vice President for Research and Economic Development at 515-294-6450 or research@iastate.edu.

Digitized by srujanika@gmail.com

100% of the time, the *labeled* and *unlabeled* data are drawn from the same underlying distribution.

THE JOURNAL OF CLIMATE

11. **What is the primary purpose of the *Journal of Clinical Endocrinology and Metabolism*?**

113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
559
560
561
562
563
564
565
566
567
568
569
569
570
571
572
573
574
575
576
577
578
579
579
580
581
582
583
584
585
586
587
588
589
589
590
591
592
593
594
595
596
597
598
599
599
600
601
602
603
604
605
606
607
608
609
609
610
611
612
613
614
615
616
617
618
619
619
620
621
622
623
624
625
626
627
628
629
629
630
631
632
633
634
635
636
637
638
639
639
640
641
642
643
644
645
646
647
648
649
649
650
651
652
653
654
655
656
657
658
659
659
660
661
662
663
664
665
666
667
668
669
669
670
671
672
673
674
675
676
677
678
679
679
680
681
682
683
684
685
686
687
688
689
689
690
691
692
693
694
695
696
697
698
699
699
700
701
702
703
704
705
706
707
708
709
709
710
711
712
713
714
715
716
717
718
719
719
720
721
722
723
724
725
726
727
728
729
729
730
731
732
733
734
735
736
737
738
739
739
740
741
742
743
744
745
746
747
748
749
749
750
751
752
753
754
755
756
757
758
759
759
760
761
762
763
764
765
766
767
768
769
769
770
771
772
773
774
775
776
777
778
779
779
780
781
782
783
784
785
786
787
788
789
789
790
791
792
793
794
795
796
797
798
799
799
800
801
802
803
804
805
806
807
808
809
809
810
811
812
813
814
815
816
817
818
819
819
820
821
822
823
824
825
826
827
828
829
829
830
831
832
833
834
835
836
837
838
839
839
840
841
842
843
844
845
846
847
848
849
849
850
851
852
853
854
855
856
857
858
859
859
860
861
862
863
864
865
866
867
868
869
869
870
871
872
873
874
875
876
877
878
879
879
880
881
882
883
884
885
886
887
888
889
889
890
891
892
893
894
895
896
897
898
899
899
900
901
902
903
904
905
906
907
908
909
909
910
911
912
913
914
915
916
917
918
919
919
920
921
922
923
924
925
926
927
928
929
929
930
931
932
933
934
935
936
937
938
939
939
940
941
942
943
944
945
946
947
948
949
949
950
951
952
953
954
955
956
957
958
959
959
960
961
962
963
964
965
966
967
968
969
969
970
971
972
973
974
975
976
977
978
979
979
980
981
982
983
984
985
986
987
988
989
989
990
991
992
993
994
995
996
997
998
999
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2159
2160
2161
2162
2163
2164
2165
2166

For more information, contact the Office of the Vice President for Research and Economic Development at 515-294-6450 or research@iastate.edu.

For more information, contact the Office of the Vice President for Research and Economic Development at 515-294-6450 or research@iastate.edu.

© 2013 Pearson Education, Inc.

© 2019 Pearson Education, Inc.

For more information, contact the Office of the Vice President for Research and the Office of the Vice President for Student Affairs.

Term	Percentage
Organic	~65%
Non-GMO	~75%
Artificial preservatives	~85%
Organic food	~90%
Organic produce	~90%
Organic meat	~90%
Organic dairy	~90%
Organic eggs	~90%
Organic flour	~90%
Organic sugar	~90%
Organic oil	~90%
Organic coffee	~90%
Organic tea	~90%
Organic cosmetics	~90%
Organic personal care products	~90%
Organic household cleaning products	~90%

Category	Number of Samples
0	1000
1	1000
2	1000
3	1000
4	0
5	1000
6	1000
7	1000
8	1000
9	1000
10	0

Attachment 2
Definitions

Proximal Neck: Infrarenal aortic segment from the lowest level of the distal-most renal artery intended to remain patent, to the proximal end of the aneurysmal aorta.

Calcification: Calcification will be graded based upon the following:
None: Absence of calcification;
Mild: Less than 40% circumferential calcification;
Moderate: 40-70% circumferential calcification; or
Severe: Greater than 70% circumferential calcification.

Tortuosity of Iliac Arteries: Tortuosity will be graded based upon the following:
None: No tortuosity;
Mild: Minimal tortuosity (less than one turn involving either external or common iliac artery);
Moderate: Single turn involving either external or common iliac artery; or
Severe: Compound turns involving external and common iliac arteries.

Occlusive Disease of Iliacs: Occlusive disease will be graded based upon the following:

None: Absence of occlusive disease;
Mild: Some disease, focal with less than 30% narrowing;
Moderate: Between 30-50% narrowing not requiring interventional techniques to meet entry criteria; or
Severe: Greater than 50% narrowing or any patient requiring angioplasty prior to endograft delivery.

New York Heart Association Classification:

- 1 Patient with cardiac disease but without resulting limitations of physical activity. Ordinary physical activity

does not cause undue fatigue, palpitation, or dyspnea.

- 2 Patients with cardiac disease resulting in slight limitation of physical activity. They are comfortable at rest, ordinary physical activity results in fatigue, palpitation, or dyspnea.
- 3 Patients with cardiac disease resulting in marked limitation of physical activity. They are comfortable at rest, less than ordinary physical activity causes fatigue, palpitation, or dyspnea.
- 4 Patients with cardiac disease resulting in inability to carry out any physical activity without discomfort. Symptoms of cardiac insufficiency may be present even at rest. If any physical activity is undertaken, discomfort is increased.

Disabling Chronic Obstructive Pulmonary

Disease (COPD): Having a forced expiratory volume (FEV₁) <1.0 liter or receiving home oxygen therapy.

Intractable

Hypertension: Having a systolic arterial pressure >160 mmHg despite receiving medication.

MI (Non-Q-Wave): Investigator identified patients having clinical evidence of a myocardial infarction with elevated peak CK values greater than or equal to three times the upper limit of normal with elevated CK-MB (above the institution's upper limit of normal) in the absence of new pathological Q-waves or clinical evidence of a myocardial infarction with troponin greater than three times the upper limit of normal, as determined by the investigator.

MI (Q-Wave): Post-procedure presence of new Q-waves greater than 0.04 seconds in at least two EKG leads.

Renal Failure: Acute or progressive renal insufficiency leading to the need for dialysis or hemofiltration.

Renal Insufficiency: A rise in serum creatinine of more than 30% above the pre-procedure level, resulting in a serum creatinine level >2.0 mg/dl that does not spontaneously resolve (does not include those patients with a pre-procedure serum creatinine >2.0 mg/dl).

Embolization: Clinical evidence of ischemic tissue remote from the operative field, presumably caused by thrombus dislodged from the aneurysmal sac, aortic neck, or adjacent vessels, including ischemia of the kidneys, pelvis (IIA) or lower limbs. This is, of course, distinct from intentional pre-operative, operative, or post-operative embolization procedures.

Graft Limb Occlusion: The presence of thrombus within one, or both, of the graft limbs (including any legs and extensions) creating complete occlusion with no blood flow through the graft limb.

Graft Lumen Diameter: The diameter measured inner wall to inner wall within the endograft.

Type I Endoleak: A peri-prosthetic leak occurring at the proximal and/or distal fixation zones.

Type II Endoleak: A leak caused by retrograde flow from patent lumbar or inferior mesenteric arteries or other collateral vessels.

Type III Endoleak: A leak caused by a defect in the graft fabric, or inadequate seal of modular graft components.

Type IV Endoleak: A leak caused by graft fabric porosity, often resulting in a generalized blush of contrast within the aneurysm sac.

Endoleak (early): Any endoleak observed within 30 days of device deployment.

Endoleak (late): Any endoleak observed later than 30 days after device deployment that was not documented during the first 30 days post-deployment.

Radiographic Migration

(stent-graft): Antegrade or retrograde movement of the stent-graft ≥ 10 mm at the level of the renal arteries as compared to the position on the first post-operative CT scan.

Clinical Utility

Measures: Duration of procedural intubation; days to resumption of oral fluids; days to resumption of normal diet; days to resumption of normal bowel function; days to ambulation; duration of ICU stay; days to discharge.

Clinically Significant Migration

(stent-graft): Antegrade or retrograde movement of the stent-graft requiring surgical or endovascular intervention.

Barb Separation: Radiographic evidence of detachment of barbs from the stent strut as confirmed by the CEC.

Stent/attachment System

Fracture/break: Fracture or breakage of any portion of the stent or attachment system including metallic fracture or breakage of any suture material used to construct the stent or secure the stent or attachment system to the graft material as confirmed by the CEC.

Technical Success: Successful access of the aneurysm site and deployment of the Zenith Low Profile AAA Endovascular Graft and the Zenith Spiral-Z AAA Iliac Leg Graft in the intended location. The endovascular graft must be patent at the

time of deployment completion as evidenced by intraoperative angiography.

Device Success

(12-month):

Technical Success, with none of the following at 12 months:

- Type I or type III endoleaks requiring re-intervention;
- Graft limb occlusion;
- Aneurysm rupture or conversion to open surgical repair; or
- Aneurysm enlargement greater than 0.5 cm.

Major Adverse Events: All-cause death, Q-wave MI, renal failure requiring dialysis, paralysis, stroke, bowel ischemia, re-intubation.

Serious Adverse

Event:

An adverse event that led to death, led to a serious deterioration in the health of the subject that resulted in a life-threatening illness or injury, resulted in a permanent impairment of a body structure or a body function, required in-patient hospitalization or prolongation of existing hospitalization, resulted in medical or surgical intervention to prevent permanent impairment to body structure or a body function, led to fetal distress, fetal death, a congenital abnormality or birth defect.