

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

Evaluation of Prototype Lenses with Experimental UV/HEV Blocker

Protocol CR-6437

Version: 1.0

Date: 18 March 2021

Investigational Products: senofilcon A with and without a new ultraviolet (UV) / high energy visible (HEV) light blocker

Keywords: Sphere R&D platform, ACUVUE® OASYS 1-DAY, senofilcon A (C3), UV/HEV-blocker, daily wear, daily disposable, dispensing, CLUE vision, CLUE comfort, CLUE handling, subjective performance

Statement of Compliance to protocol, GCP and applicable regulatory guidelines:

This trial will be conducted in compliance with the protocol, ISO 14155,¹ the International Council for Harmonization Good Clinical Practice E6(R2) (ICH GCP),² the Declaration of Helsinki,³ and all applicable regulatory requirements.

Confidentiality Statement:

This document contains confidential information, which should not be copied, referred to, released or published without written approval from Johnson & Johnson Vision Care, Inc. The information may not be disclosed to others except to the extent necessary to obtain Institutional Review Board/Independent Ethics Committee approval and informed consent, or as required by International, Federal and State Laws, as applicable. Persons to whom this information is disclosed must be informed that this information is privileged and confidential and that it should not be further disclosed without the written permission of Johnson & Johnson Vision Care, Inc. Any supplemental information that may be added to this document is also confidential and proprietary to Johnson & Johnson Vision Care, Inc. and must be kept in confidence in the same manner as the contents of this document.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

TABLE OF CONTENTS

PROTOCOL TITLE, NUMBER, VERSION AND DATE.....	6
SPONSOR NAME AND ADDRESS.....	6
MEDICAL MONITOR.....	6
AUTHORIZED SIGNATURES.....	7
CHANGE HISTORY.....	8
SYNOPSIS.....	9
COMMONLY USED ABBREVIATIONS AND DEFINITIONS OF TERMS	14
1. INTRODUCTION AND BACKGROUND	16
1.1. Name and Descriptions of Investigational Products	16
1.2. Intended Use of Investigational Products.....	16
1.3. Summary of Findings from Nonclinical Studies.....	16
1.4. Summary of Known Risks and Benefits to Human Subjects.....	16
1.5. Relevant Literature References and Prior Clinical Data Relevant to Proposed Clinical Study	17
2. STUDY OBJECTIVES, ENDPOINTS AND HYPOTHESES	17
2.1. Objectives.....	17
2.2. Endpoints.....	18
2.3. Hypotheses	19
3. TARGETED STUDY POPULATION	20
3.1. General Characteristics	20
3.2. Inclusion Criteria.....	20
3.3. Exclusion Criteria.....	21
3.4. Enrollment Strategy.....	22
4. STUDY DESIGN AND RATIONALE	23
4.1. Description of Study Design	23
4.2. Study Design Rationale.....	23
4.3. Enrollment Target and Study Duration	23
5. TEST ARTICLE ALLOCATION AND MASKING	24
5.1. Test Article Allocation.....	24
5.2. Masking.....	25
5.3. Procedures for Maintaining and Breaking the Masking.....	25
6. STUDY INTERVENTION.....	25

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

6.1. Identity of Test Articles.....	25
6.2. Ancillary Supplies/Products.....	26
6.3. Administration of Test Articles.....	27
6.4. Packaging and Labeling	27
6.5. Storage Conditions	27
6.6. Collection and Storage of Samples	27
6.7. Accountability of Test Articles	28
7. STUDY EVALUATIONS	28
7.1. Time and Event Schedule.....	28
7.2. Detailed Study Procedures	29
VISIT 1	29
VISIT 2	34
VISIT 3	39
FINAL EVALUATION.....	40
7.3. Unscheduled Visits.....	41
7.4. Laboratory Procedures	43
8. SUBJECTS COMPLETION/WITHDRAWAL.....	43
8.1. Completion Criteria.....	43
8.2. Withdrawal/Discontinuation from the Study	43
9. PRE-STUDY AND CONCOMITANT INTERVENTION/MEDICATION	44
9.1. Systemic Medications	44
10. DEVIATIONS FROM THE PROTOCOL	46
11. STUDY TERMINATION	47
12. PROCEDURE FOR HANDLING PRODUCT QUALITY COMPLAINTS	48
13. ADVERSE EVENTS.....	49
13.1. Definitions and Classifications.....	49
13.2. Assessing Adverse Events.....	52
13.2.1. Causality Assessment.....	52
13.2.2. Severity Assessment.....	52
13.3. Documentation and Follow-Up of Adverse Events	53
13.4. Reporting Adverse Events.....	54
13.4.1. Reporting Adverse Events to Sponsor	54

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

13.4.2. Reporting Adverse Events to the Responsible IEC/IRB and Health Authorities	55
13.5. Event of Special Interest	55
13.6. Reporting of Pregnancy.....	56
14. STATISTICAL METHODS.....	56
14.1. General Considerations	56
14.2. Sample Size Justification	56
14.3. Analysis Populations	60
14.4. Level of Statistical Significance.....	60
14.5. Primary Analysis.....	60
14.6. Secondary Analysis.....	61
14.7. Other Exploratory Analysis.....	61
14.8. Interim Analysis	64
14.9. Procedure for Handling Missing Data and Drop-Outs.....	64
14.10. Procedure for Reporting Deviations from Statistical Plan.....	64
15. DATA HANDLING AND RECORD KEEPING/ARCHIVING.....	64
15.1. Electronic Case Report Form/Data Collection.....	64
15.2. Subject Record	65
15.3. Trial Registration on ClinicalTrials.gov.....	66
16. DATA MANAGEMENT.....	66
16.1. Access to Source Data/Document.....	66
16.2. Confidentiality of Information	66
16.3. Data Quality Assurance.....	66
16.4. Data Monitoring Committee (DMC).....	67
17. CLINICAL MONITORING	67
18. ETHICAL AND REGULATORY ASPECTS	67
18.1. Study-Specific Design Considerations.....	67
18.2. Investigator Responsibility.....	67
18.3. Independent Ethics Committee or Institutional Review Board (IEC/IRB).....	68
18.4. Informed Consent.....	69
18.5. Privacy of Personal Data.....	69
19. STUDY RECORD RETENTION.....	70
20. FINANCIAL CONSIDERATIONS	71

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

21. PUBLICATION.....	71
22. REFERENCES	72
APPENDIX A: PATIENT REPORTED OUTCOMES (STUDY QUESTIONNAIRES)	74
APPENDIX B: PATIENT INSTRUCTION GUIDE	96
APPENDIX C: PACKAGE INSERT (APPROVED PRODUCT).....	97
APPENDIX D: [REDACTED]	126
[REDACTED] Limbal and Conjunctival (Bulbar) Redness	127
[REDACTED] Expanded Sodium Fluorescein Corneal Staining.....	134
[REDACTED] Lens Fitting Characteristics.....	141
[REDACTED] Subject Reported Ocular Symptoms/Problems	147
[REDACTED] Front and Back Surface Lens Deposit Grading Procedure	149
[REDACTED] Determination of Distance Spherocylindrical Refractions.....	154
[REDACTED] Biomicroscopy Scale.....	160
[REDACTED] Distance and Near Visual Acuity Evaluation.....	166
[REDACTED] Patient Reported Outcomes.....	171
[REDACTED] White Light Lens Surface Wettability	173
APPENDIX E: IRIS COLOR	175
APPENDIX F: STARTING LENS POWER.....	177
APPENDIX G: GUIDELINES FOR COVID-19 RISK MITIGATION	179
PROTOCOL COMPLIANCE INVESTIGATOR(S) SIGNATURE PAGE	191

LIST OF TABLES

Table 1: Enrollment Strategy Overall	22
Table 2: Duration of Study Visits	23
Table 3: Test Articles.....	25
Table 4: Ancillary Supplies	26
Table 5: Time and Events	28
Table 6: Unscheduled Visit Procedures	41
Table 7: Disallowed systemic medications.....	45
Table 8: Disallowed systemic antihistamines	46
Table 9: Examples of major and minor protocol deviations.....	46
Table 12: Sample Size Estimates.....	59

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

LIST OF FIGURES

Figure 1: Study Flowchart 13

PROTOCOL TITLE, NUMBER, VERSION AND DATE

Title: Evaluation of Prototype Lenses with Experimental UV/HEV Blocker

Protocol Number: CR-6437

Version: 1.0

Date: 18 March 2021

SPONSOR NAME AND ADDRESS

Johnson & Johnson Vision Care, Inc. (JJVC)
7500 Centurion Parkway
Jacksonville, FL 32256

MEDICAL MONITOR



The Medical Monitor must be notified by the clinical institution/site by e-mail or telephone within 24 hours of learning of a Serious Adverse Event. The Medical Monitor may be contacted during business hours for adverse event questions. General study related questions should be directed towards your assigned clinical research associate.

The Medical Monitoring Plan is maintained as a separate document and included in the Trial Master File.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

AUTHORIZED SIGNATURES

The signatures below constitutes the approval of this protocol and the attachments and provide the necessary assurances that this trial will be conducted according to all stipulations of the protocol, including all statements regarding confidentiality, and according to local legal and regulatory requirements and applicable U.S. federal regulations,⁴ ISO 14155,¹ ICH guidelines,² and the Declaration of Helsinki.³

Author/Study Responsible Clinician	<i>See Electronic Signature Report</i> [REDACTED]	DATE
Clinical Operations Manager	<i>See Electronic Signature Report</i> [REDACTED]	DATE
Biostatistician	<i>See Electronic Signature Report</i> [REDACTED]	DATE
Biostatistics Reviewer	<i>See Electronic Signature Report</i> [REDACTED]	DATE
Data Management	<i>See Electronic Signature Report</i> [REDACTED]	DATE
Medical Safety Officer	<i>See Electronic Signature Report</i> [REDACTED]	DATE
Reviewer	<i>See Electronic Signature Report</i> [REDACTED]	DATE
Approver	<i>See Electronic Signature Report</i> [REDACTED]	DATE

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

CHANGE HISTORY

Version	Originator	Description of Change(s) and Section Number(s) Affected	Date
1.0	[REDACTED]	Original Protocol	18 Mar 2021

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

SYNOPSIS

Protocol Title	Evaluation of Prototype Lenses with Experimental UV/HEV Blocker
Sponsor	JJVC, 7500 Centurion Parkway, Jacksonville, FL 32256
Clinical Phase	Clinical trial phase: Confirmatory Design control phase: Confirmatory phase 3
Trial Registration	This study will be registered on ClinicalTrials.gov.
Test Article(s)	<p>Investigational Product:</p> <ul style="list-style-type: none"> • senofilcon A C3 containing a new UV/HEV blocker with propylene glycol (PG) hydration <p>Approved Product:</p> <ul style="list-style-type: none"> • Production ACUVUE® OASYS 1-Day (senofilcon A C3)
Wear and Replacement Schedules	<p>Wear Schedule: daily disposable</p> <p>Replacement Schedule: daily</p>
Objectives	The purpose of this investigation is to evaluate the short-term, clinical performance of prototype contact lenses with experimental UV/HEV-blocker produced on a commercial manufacturing line. Subjective responses will comprise the primary and secondary endpoints.
Study Endpoints	<p>Primary endpoint:</p> <ol style="list-style-type: none"> 1. CLUE overall comfort score at 2-week follow-up <p>Secondary endpoints:</p> <ol style="list-style-type: none"> 1. CLUE overall quality of vision score at 2-week follow-up 2. CLUE overall handling score at 2-week follow-up <p>Other observations: preferences to habitual lens, preference between Test and Control lenses, purchase intent, outdoor performance, indoor performance, driving performance, digital performance, cosmetic acceptance.</p>
Study Design	<p>This is a bilateral, 2-week dispensing, randomized, controlled, subject-masked, 2×2 crossover study. Each subject will be bilaterally fitted with a Test or Control lens in random fashion for a wear period of two weeks each. There will be a total of 3 visits:</p> <ol style="list-style-type: none"> 1. Visit 1: Screening, baseline evaluation and lens fit #1 2. Visit 2: 2-week follow-up, lens fit #2 3. Visit 3: 2-week follow-up, Final evaluation

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

	See the flow chart at the end of the synopsis table for the schematic of the study visits and procedures of main observations (Figure 1)
Sample Size	Approximately 230 subjects in total (enrolling ~115 to start with the Test lens and ~115 to start with the Control lens) will be targeted to be enrolled in this study, with the aim to complete approximately 200 subjects (~100 in each of the 2 lens wear sequences).
Study Duration	Subject enrollment will last 8 weeks per site. Once enrolled, subjects will be in the study for approximately 4 weeks, making the entire study approximately 12 weeks in duration.
Anticipated Study Population	Subjects will be male and female of any race and ethnicity, age 18 through 39, habitual wearers of spherical silicone hydrogel contact lenses within the power range of -1.00 through -6.00 D. Subjects will be targeted in a 7:3 ratio based on habitual lens wear (7 habitual daily disposable wearers versus 3 habitual daily wear reusable wearers).
Eligibility Criteria - Inclusion	<p>Potential subjects must satisfy all of the following criteria to be enrolled in the study:</p> <p>Inclusion Criteria after Screening The subject must:</p> <ol style="list-style-type: none"> 1. Read, understand, and sign the STATEMENT OF INFORMED CONSENT and receive a fully executed copy of the form. 2. Appear able and willing to adhere to the instructions set forth in this clinical protocol. 3. Be between 18 and 39 (inclusive) years of age at the time of screening. 4. By self-report, habitually wear spherical silicone hydrogel soft contact lenses in both eyes in a daily reusable or daily disposable wear modality (i.e. not extended wear modality). Habitual wear is defined as a minimum of 6 hours of wear per day, for a minimum of 5 days per week during the past 30 days. 5. Have a habitual contact lens prescription that is current within the prior 6 months, and they must have worn that prescription for at least 2 weeks prior to entering the study. <p>Inclusion Criteria following Baseline Evaluation</p>

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

	<ol style="list-style-type: none"> 6. The subject's vertex corrected spherical equivalent distance refraction must be in the range of -1.00 through -6.00 D (except -5.00 D) in both eyes. 7. The subject's refractive cylinder must be 1.00 D or less. 8. The subject must have best corrected visual acuity of 20/25 or better in each eye.
Eligibility Criteria – Exclusion	<p>Potential subjects who meet any of the following criteria will be excluded from participating in the study:</p> <p>Exclusion Criteria after Screening: The subject must not:</p> <ol style="list-style-type: none"> 1. Be currently pregnant or lactating. 2. Have any ocular or systemic allergies or diseases that may interfere with contact lens wear. 3. Have any autoimmune disease or use of medication, which may interfere with contact lens wear. Habitual medications used by successful soft contact lens wearers are considered acceptable. 4. Have any previous, or planned, ocular or interocular surgery (e.g., radial keratotomy, PRK, LASIK, etc.). 5. Be currently wearing lenses in a monovision, multi-focal, toric, or extended wear modality. 6. Have participated in a contact lens or lens care product clinical trial within 14 days prior to study enrollment 7. Be an employee (e.g., Investigator, Coordinator, Technician) or immediate family member of an employee (including partner, child, parent, grandparent, grandchild or sibling of the employee or their spouse) of the clinical site. 8. Have a history of binocular vision abnormality or strabismus. 9. Have any infectious disease (e.g., hepatitis, tuberculosis) or contagious immunosuppressive diseases (e.g., HIV) by self-report. <p>Exclusion Criteria following Baseline Evaluation The subject must not:</p> <ol style="list-style-type: none"> 10. Have any Grade 3 or greater slit lamp findings (e.g., edema, corneal neovascularization, corneal staining,


Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

	<p>tarsal abnormalities, conjunctival injection) on the FDA classification scale, any previous history or signs of a contact lens-related corneal inflammatory event (e.g., past peripheral ulcer or round peripheral scar), or any other ocular abnormality that may contraindicate contact lens wear.</p> <ol style="list-style-type: none"> 11. Have any ocular infection. 12. Have any corneal distortion resulting from previous hard or rigid gas permeable contact lens wear. 13. Have entropion, ectropion, extrusions, chalazia, recurrent styes, glaucoma, history of recurrent corneal erosions, or aphakia.
Disallowed Medications/Interventions	Use of any prescription or over-the-counter (OTC) medications that may affect contact lens wear from 24 hours prior to receiving the study product through the study period of ~28 days. Habitual medications taken by successful soft contact lens wearers are generally considered acceptable (see Section 9.1 for details regarding disallowed systemic medications). Note that habitual medications should be taken throughout the study period.
Measurements and Procedures	Subjective questionnaires (CLUE and MRD/GSI) will comprise the primary and secondary outcome measures with physiological responses being monitored.
Microbiology or Other Laboratory Testing	None
Study Termination	The occurrence of an Unanticipated Adverse Device Effect (UADE) or Serious Adverse Event (SAE) for which a causal relationship to a test article cannot be ruled out, will result in stopping further dispensing investigational product. In the event of a UADE or SAE, the Sponsor Medical Monitor may unmask the treatment regimen of subject(s) and may discuss this with the Principal Investigator before any further subjects are enrolled.
Ancillary Supplies/ Study-Specific Materials	Preservative free rewetting drops/artificial tears or saline. ACUVUE™ RevitaLens will be used to transport any problematic lenses back to the Sponsor.
Principal Investigator(s) and Study Institution(s)/Site(s)	A full list of Principal Investigators, clinical sites, and institutions is kept separately from the Study Protocol and is included in the study Trial Master File.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

Figure 1: Study Flowchart

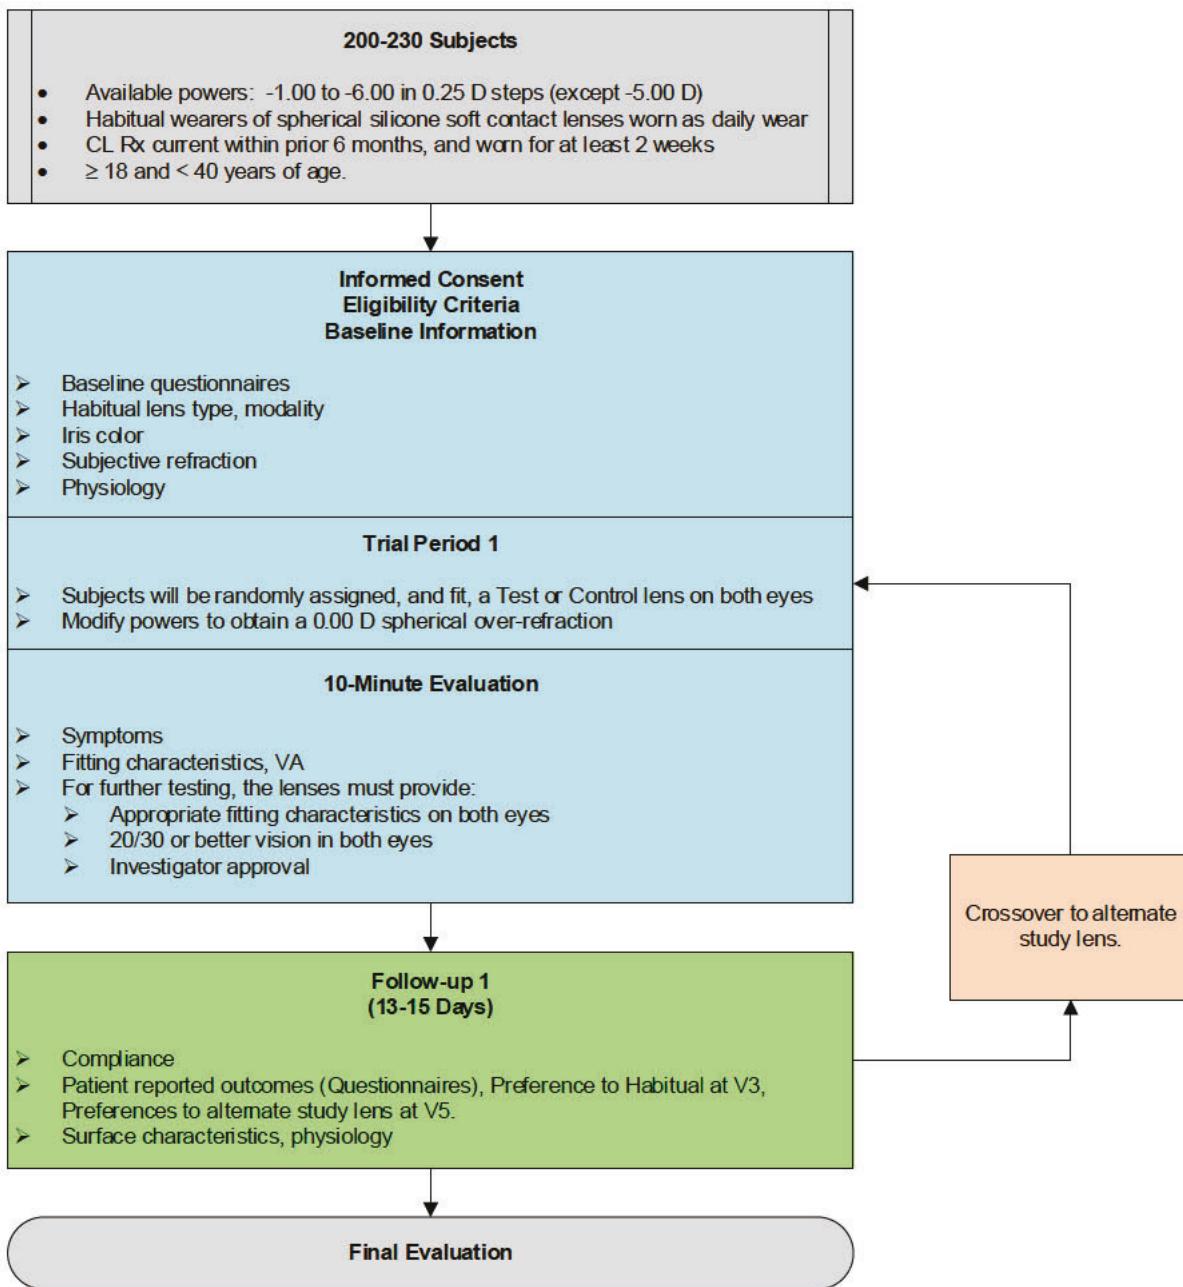

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

COMMONLY USED ABBREVIATIONS AND DEFINITIONS OF TERMS

ADD	Plus Power Required For Near Use
ADE	Adverse Device Effect
AE	Adverse Event/Adverse Experience
BCVA	Best Corrected Visual Acuity
BSCVA	Best Spectacle Corrected Visual Acuity
CFR	Code of Federal Regulations
CLUE	Contact Lens User Experience
COAS	Complete Ophthalmic Analysis System
COM	Clinical Operations Manager
CRA	Clinical Research Associate
CRF	Case Report Form
CRO	Contract Research Organization
CT	Center Thickness
	
D	Diopter
DMC	Data Monitoring Committee
eCRF	Electronic Case Report Form
EDC	Electronic Data Capture
ETDRS	Early Treatment Diabetic Retinopathy Study
FDA	Food and Drug Administration
GCP	Good Clinical Practice
HIPAA	Health Insurance Portability and Accountability Act
IB	Investigator's Brochure
ICF	Informed Consent Form
ICH	International Conference on Harmonization
IDE	Investigational Device Exemption
IEC	Independent Ethics Committee
IRB	Institutional Review Board
ISO	International Organization for Standardization
ITT	Intent-to-Treat
JJVC	Johnson & Johnson Vision Care, Inc.
LC	Limbus Center
LogMAR	Logarithm of Minimal Angle of Resolution
MedDRA [®]	Medical Dictionary for Regulatory Activities
MOP	Manual of Procedures
NIH	National Institutes of Health
OD	Right Eye
OHRP	Office for Human Research Protections
OHSR	Office for Human Subjects Research
OS	Left Eye
OU	Both Eyes
PD	Protocol Deviation
PHI	Protected Health Information

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

PI	Principal Investigator
PIG	Patient Instruction Guide
PQC	Product Quality Complaint
PRO	Patient Reported Outcome
QA	Quality Assurance
QC	Quality Control
SAE	Serious Adverse Event/Serious Adverse Experience
SAP	Statistical Analysis Plan
SAS	Statistical Analysis System
SD	Standard Deviation
SOP	Standard Operating Procedure
UADE	Unanticipated Adverse Device Effect
USADE	Unanticipated Serious Adverse Device Effect
VA	Visual Acuity

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

1. INTRODUCTION AND BACKGROUND

The range of high energy visible (HEV) light is roughly defined in the literature, with references stating 380-500 nm⁵, 400-500 nm⁶ and others stating 430-510 nm.⁷ This region of the electromagnetic spectrum has special meaning to the eye. It is light that we can see, but yet can have negative and positive effects on the eye. At the shorter wavelength end of the range, around 435±20 nm,⁸ the light has enough energy to cause premature damage to the retinal pigment epithelium and has been linked to macular degeneration. The shorter wavelengths are also scattered more than longer wavelengths (Rayleigh scattering), which create the blue sky and “blue haze” that we see when looking at distant objects. At the longer wavelength end of the range, around 480±20 nm,⁹ the light is responsible for regulating our circadian rhythms and pupillary light reflexes.

Ophthalmic devices that block the shorter HEV wavelengths while transmitting the longer wavelengths might experience an immediate visual improvement through better chromatic contrast, while benefitting in the long-term through enhanced retinal protection. This study will investigate, for the first time, the prototype Test lenses manufactured on a commercial line.

1.1. Name and Descriptions of Investigational Products

This study will test a senofilcon A (C3) design prototype with new UV/HEV blocker against a commercially available marketed product ACUVUE OASYS® Brand Contact Lenses 1-Day with HydraLuxe™ Technology (AO1D). Further details about the test articles are found in section 6 of this protocol. Note that the new UV/HEV blocker was previously identified as Theia I.

1.2. Intended Use of Investigational Products

The intended use of the investigative product is for correcting myopia and for improving the visual experience by improving contrast. During the study, each test article will be worn bilaterally in daily wear, daily disposable modality for at least 6 hours per day and 5 days per week for approximately two weeks. The subject will wear both test articles in a cross-over study design.

1.3. Summary of Findings from Nonclinical Studies

All previous pre-clinical findings were deemed satisfactory prior to proceeding with clinical trials on humans. For the most comprehensive nonclinical information regarding senofilcon A (C3) – based lens with new UV/HEV blocker, refer to the latest version of the Investigator’s Brochure.¹⁰

1.4. Summary of Known Risks and Benefits to Human Subjects

The risks of wearing soft contact lenses are well known and are described in the Investigator’s Brochure and Informed Consent. The material safety testing/lens release criteria was

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

determined based on the Risk Assessment. Benefits to the subjects include the correction of their refractive error with the potential of improved contrast in HEV environments.

For the most comprehensive risk and benefit information regarding the senofilcon A (C3) with new UV/HEV-blocker, refer to the latest version of the Investigator's Brochure.¹⁰

1.5. Relevant Literature References and Prior Clinical Data Relevant to Proposed Clinical Study

The package insert for the AO1D Control lens can be found in the appendices. Prior clinical data of the new UV/HEV-blocker is summarized in the Investigator's Brochure.

The literature is absent of any articles pertaining to soft contact lenses containing HEV-blocker. Articles that pertain to "blue-blocking" spectacles and intraocular lenses do exist with a sampling shown here:

1. Mainster MA. Violet and blue light blocking intraocular lenses: photoprotection versus photoreception. *British Journal of Ophthalmology*. 2006;90(6):784-792.
2. Braunstein RE. A Blue-Blocking Intraocular Lens Should Be Used in Cataract Surgery. *Archives of Ophthalmology*. 2005;123(4):547.
3. Glazer-Hockstein C, Dunaief JL. Could Blue Light-Blocking Lenses Decrease the Risk of Age-Related Macular Degeneration? *Retina*. 2006;26(1):1-4.
4. Kimberly B, James R P. AMBER LENSES TO BLOCK BLUE LIGHT AND IMPROVE SLEEP: A RANDOMIZED TRIAL. *Chronobiology International*. 2009;26(8):1602-1612.
5. Hayashi K. Visual function in patients with yellow tinted intraocular lenses compared with vision in patients with non-tinted intraocular lenses. *British Journal of Ophthalmology*. 2006;90(8):1019-1023.
6. Schmoll C, Khan A, Aspinall P, et al. New light for old eyes: comparing melanopsin-mediated non-visual benefits of blue-light and UV-blocking intraocular lenses. *British Journal of Ophthalmology*. 2013;98(1):124-128.

2. STUDY OBJECTIVES, ENDPOINTS AND HYPOTHESES

2.1. Objectives

The purpose of this investigation is to evaluate the short-term, clinical performance of prototype contact lenses with experimental UV/HEV-blocker produced on a commercial manufacturing line. Subjective responses will comprise the primary and secondary endpoints. The results may be used to support marketing claims or help understand market readiness of the Test lens.

Primary Objective(s)

The primary objective is to evaluate the clinical performance of the senofilcon A material, with and without a UV/HEV filter, when both are manufactured on commercial production lines.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

2.2. Endpoints

Primary Endpoint:

1. CLUE overall quality of vision score at 2-week follow-up

Secondary Endpoints:

1. CLUE overall comfort score at 2-week follow-up
2. CLUE overall handling score at 2-week follow-up

Subjective over quality of vision, overall comfort and handling scores will be assessed using Contact Lens User Experience (CLUE) questionnaire.¹¹ CLUE is a validated patient-reported outcomes questionnaire to assess patient-experience attributes of soft, disposable contact lenses (comfort, vision, handling, and packaging) in a contact-lens wearing population in the US, ages 18-65. Scores follow a normal distribution with a population average score of 60 (SD 20), where higher scores indicate a more favorable/positive response. A 5-point increase in an average CLUE score translates into 10% shift in the distribution of scores for population of soft disposable contact lens wearers.

Other Exploratory Endpoints:

Items evaluating visual clarity:

- Clarity of vision indoors in bright light (MIS00623)
- Clarity of vision indoors in dim light (MIS00624)
- Clarity of vision in bright sunlight (MIS00612)
- Clarity of distance vision (i.e. looking at things that are more than 5 feet away, such as street signs) (P3_0006_p10)

Items evaluating driving performance:

- Ability to see comfortably while driving at night (MIS01980)
- Ability to see comfortably while driving during the day (MIS01981)
- My vision was clear enough to allow me to drive at night (V056_1)
- With these lenses, I felt very confident to drive at night (V086_2)

Items evaluating digital device performance:

- Reduction in the feeling of tired eyes from using a computer or other digital device (MIS02001)
- Ability to see comfortably while using a computer or other digital device (MIS01982)

Preference items:

- Overall opinion (PREf6_1_1)
- Overall comfort (PREf6_2_1)
- Overall vision (PREf6_3_1)
- Comfort throughout the day (PREf6_5_1)
- Comfort at the end of the day (PREf6_6_1)
- Comfort from activity to activity (PREf6_7_1)

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

- Clarity of vision from activity to activity (PREf6_8_1)
- Overall preference while using computer screens & digital devices (PREf6_4_1)

All other exploratory endpoints (items) are evaluated using Likert scales. The response set for preference items include: Strongly prefer the first set of study lenses, Slightly prefer the first set of study lenses, No preference, Slightly prefer the second set of study lenses, and Strongly prefer the second set of study lenses. Study lens preference will be derived based on subject's responses and the sequence of lens wear.

2.3. Hypotheses

Primary Hypothesis

1. Test lens will be non-inferior to the Control lens at the 2-week follow-up evaluation with respect to CLUE Vision. A non-inferiority margin of -5 points will be used.

Secondary Hypotheses

1. Test lens will be non-inferior to the Control lens at the 2-week follow-up evaluation with respect to CLUE comfort. A non-inferiority margin of -5 points will be used.
2. Test lens will be non-inferior to the Control lens at the 2-week follow-up evaluation with respect to CLUE Handling. A non-inferiority margin of 5 points will be used.

All primary and secondary hypotheses must be met to satisfy the objective of the study. Other exploratory endpoints will be assessed in support of the primary and secondary endpoints; other exploratory hypotheses will be evaluated only when all primary and secondary hypotheses are met.

Other Exploratory Hypotheses

1. The Test lens will be superior to the Control lens with respect to the proportion of subjects with "Excellent" response to the statement "Clarity of vision indoors in bright light" at the 2-week follow-up visit.
2. The Test lens will be superior to the Control lens with respect to the proportion of subjects with higher ratings to the following individual CLUE or MRD items at the 2-week follow-up evaluation:
 - 1) Clarity of distance vision (i.e. looking at things that are more than 5 feet away, such as street signs). (P3_0006_p10)
 - 2) Clarity of vision in bright sunlight. (MIS00612)
 - 3) Ability to see comfortably while driving at night (MIS01980)
 - 4) Ability to see comfortably while driving during the day (MIS01981)
 - 5) Clarity of vision indoors in bright light. (MIS00623)
 - 6) Reduction in the feeling of tired eyes from using a computer or other digital device. (MIS02001)

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

- 7) Ability to see comfortably while using a computer or other digital device. (MIS01982)
- 8) My vision was clear enough to allow me to drive at night (V056_1)
- 9) With these lenses, I felt very confident to drive at night (V086_2)
- 10) Clarity of vision indoors in dim light (MIS00624)

3. The Test lens will be superior to the Control lens with respect to the following preference questions at the 2-week follow-up evaluation:

- 1) Overall opinion (PREf6_1_1)
- 2) Overall comfort (PREf6_2_1)
- 3) Overall vision (PREf6_3_1)
- 4) Comfort throughout the day (PREf6_5_1)
- 5) Comfort at the end of the day (PREf6_6_1)
- 6) Comfort from activity to activity (PREf6_7_1)
- 7) Clarity of vision from activity to activity (PREf6_8_1)
- 8) Overall preference while using computer screens & digital devices (PREf6_4_1)

Study lens preferences to habitual lens, study lens purchase intent, acceptable lens fit rates, surface characteristics, biomicroscopy findings, and other characteristics of both study lenses will be descriptively summarized with tables and/or graphs.

3. TARGETED STUDY POPULATION

3.1. General Characteristics

Approximately 115 subjects will be targeted to start with the Test lens and approximately 115 will be targeted to start with the Control lens. Within each of these two starting groups, the intent is to complete 100 (200 total subjects). Enrolled subjects will be habitual wearers of silicone hydrogel spherical contact lenses. All subjects will be the age of ≥ 18 and < 40 . Subjects will wear the study contact lenses approximately two weeks each on a daily wear (DW) daily disposable (DD) basis for a total study duration of approximately 28 days (4 weeks) per subject.

3.2. Inclusion Criteria

Potential subjects must satisfy all of the following criteria to be enrolled in the study:

Inclusion Criteria after Screening

The subject must:

1. Read, understand, and sign the STATEMENT OF INFORMED CONSENT and receive a fully executed copy of the form.
2. Appear able and willing to adhere to the instructions set forth in this clinical protocol.
3. Be between 18 and 39 (inclusive) years of age at the time of screening.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

4. By self-report, habitually wear spherical silicone hydrogel soft contact lenses in both eyes in a daily reusable or daily disposable wear modality (i.e. not extended wear modality). Habitual wear is defined as a minimum of 6 hours of wear per day, for a minimum of 5 days per week during the past 30 days.
5. Have a habitual contact lens prescription that is current within the prior 6 months, and they must have worn that prescription for at least 2 weeks prior to entering the study.

Inclusion Criteria following Baseline Evaluation

6. The subject's vertex corrected spherical equivalent distance refraction must be in the range of -1.00 through -6.00 D (except -5.00 D) in both eyes.
7. The subject's refractive cylinder must be 1.00 D or less.
8. The subject must have best corrected visual acuity of 20/25 or better in each eye.

3.3. Exclusion Criteria

Potential subjects who meet any of the following criteria will be excluded from participating in the study:

Exclusion Criteria after Screening:

The subject must not:

1. Be currently pregnant or lactating.
2. Have any ocular or systemic allergies or diseases that may interfere with contact lens wear.
3. Have any autoimmune disease or use of medication, which may interfere with contact lens wear. Habitual medications used by successful soft contact lens wearers are considered acceptable.
4. Have any previous, or planned, ocular or interocular surgery (e.g., radial keratotomy, PRK, LASIK, etc.).
5. Be currently wearing lenses in a monovision, multi-focal, toric, or extended wear modality.
6. Have participated in a contact lens or lens care product clinical trial within 14 days prior to study enrollment
7. Be an employee (e.g., Investigator, Coordinator, Technician) or immediate family member of an employee (including partner, child, parent, grandparent, grandchild or sibling of the employee or their spouse) of the clinical site.
8. Have a history of binocular vision abnormality or strabismus.
9. Have any infectious disease (e.g., hepatitis, tuberculosis) or contagious immunosuppressive diseases (e.g., HIV) by self-report.

Exclusion Criteria following Baseline Evaluation

The subject must not:

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

10. Have any Grade 3 or greater slit lamp findings (e.g., edema, corneal neovascularization, corneal staining, tarsal abnormalities, conjunctival injection) on the FDA classification scale, any previous history or signs of a contact lens-related corneal inflammatory event (e.g., past peripheral ulcer or round peripheral scar), or any other ocular abnormality that may contraindicate contact lens wear.
11. Have any ocular infection.
12. Have any corneal distortion resulting from previous hard or rigid gas permeable contact lens wear.
13. Have entropion, ectropion, extrusions, chalazia, recurrent styes, glaucoma, history of recurrent corneal erosions, or aphakia.

3.4. Enrollment Strategy

Study subjects will be recruited from the Institution/clinical site's subject database and/or utilizing Independent Ethics Committee (IEC) or Institutional Review Board (IRB) approved materials.

The overall goal is to enroll approximately 230 eligible subjects and complete 200 that are evenly distributed between those that begin with the Test lens and those that begin with the Control lens (Table 1).

Table 1: Enrollment Strategy Overall

Overall Enrollment	Strata	Test/Control	Control/Test	Total
Randomized	Overall	114~116	114~116	228~232
	Habitual Daily Disposable	80~81	80~81	160~162
	Habitual Daily Wear Reusable	34~35	34~35	68~70
Completed	Overall	100	100	200
	Habitual Daily Disposable	70	70	140
	Habitual Daily Wear Reusable	30	30	60

Approximately 11-12 sites are expected to enroll approximately 20 subjects each with each subject wearing the Test lens and the Control lens during the study. Habitual wearers of daily disposable lenses will be preferentially targeted in a 7:3 ratio over habitual wearers of daily wear reusable lenses within each site (i.e., 7 habitual wearers of daily disposable lenses versus 3 habitual wearers of daily wear reusable lenses).

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

4. STUDY DESIGN AND RATIONALE

4.1. Description of Study Design

This study is a controlled, randomized, subject-masked, 2 treatments \times 2 periods crossover, 2-week dispensing, bilateral evaluation where the study lenses are worn for a minimum of 5 days per week and 6 hours per day worn. At study closure, participants will have no further access to the Test lenses.

4.2. Study Design Rationale

The purpose of this study is to evaluate the performance of a new UV/HEV-blocker in a 2 \times 2 crossover design. Crossover designs are a well-established study design in which subjects are exposed to multiple treatments during different time periods. This design is cost effective and more efficient since it eliminates part of the inter-subject variability from the treatment comparisons. Subjects will be randomized into the two lens wear sequences: Test/Control or Control/Test. Randomization removes potential for systematic error or bias and balances both the known and unknown confounding factors that may affect the study outcomes. A potential limitation of crossover design is the carry-over effect from the previous treatment. A wash-out period is not considered in this study since the wearing time of 2 weeks in each period is considered long enough to minimize the presence of the carry-over effect. In case a significant carry-over effect is observed, only the first period of the data will be analyzed.

4.3. Enrollment Target and Study Duration

This study will have an enrollment target of 230 subjects, with a target of at least 200 to complete. The study will be conducted at up to 11 clinical sites, where the enrollment target for each site will be approximately 20 subjects. A subject will be considered enrolled upon signing of the informed consent form.

There will be 3 visits in total per subject; total study duration including the enrollment period is expected to be approximately 12 weeks. Subjects who are discontinued prior to the final evaluation may be replaced at the discretion of the study sponsor. The investigation will end at the time that the study data is hard locked.

Table 2: Duration of Study Visits

Visit	Description	\approx Duration
1	Informed consent, eligibility criteria, baseline data, trial fitting 1, dispense lenses. Study lenses to be worn 13-15 days to first follow-up visit.	2.0 hours
2	13-15 day follow-up for the study lens, subjective responses, preference to habitual, VA, fitting characteristics, surface characteristics, physiology. Trial fitting 2, dispense lenses. Study lenses to be worn 13-15 days to first follow-up visit.	2.0 hours

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

3	13-15 day follow-up for the study lens, subjective responses, preference between study lenses, VA, fitting characteristics, surface characteristics, physiology, Final Evaluation.	1.0 hours
---	--	-----------

5. TEST ARTICLE ALLOCATION AND MASKING

5.1. Test Article Allocation

Use of the test articles will be randomized using a lens fitting schedule supplied by the study biostatistician. The clinical site will follow the lens fitting schedule provided and will complete enrollment according to the randomization list and will not pre-select or pre-assign subjects.

Randomly-permuted block randomization will be used to avoid bias in the assignment of subjects to treatment and to enhance the validity of statistical comparisons across treatment groups. A computer-generated randomization scheme will be used to randomly assign subjects, in blocks of 2, to one of the two possible lens wear sequences (Test/Control or Control/Test). The randomization will be stratified by site and type of habitual lens wear (daily disposable and daily wear reusable). The ratio of habitual wearers of daily disposable lenses to habitual wearers of daily wear reusable lenses is 7:3 within each study site (7 habitual wearers of daily disposable lenses versus 3 habitual wearers of daily wear reusable lenses). See Table 1. The random scheme will be generated using the PROC PLAN procedure from Statistical Analysis System (SAS) Software Version 9.4 or higher (SAS Institute, Cary, NC)¹².

Randomization will be performed at visit 1. The following must have occurred prior to randomization:

- Informed consent must have been obtained.
- The subject must have met all eligibility criteria.
- The subject's screening and baseline information must have been collected.

The following steps should be followed to maintain randomization codes:

1. Investigator or designee (documented on the Delegation Log) will consult the lens fitting schedule to obtain the test article assignment for that subject prior to dispensing.
2. Investigator or designee will record the subject's number on the appropriate line of the lens fitting schedule.
3. Investigator or designee will pull the appropriate test articles from the study supply. All test articles that are opened, whether dispensed (placed/fit on eye or dispensed outside the clinical site) or not, must be recorded on the Test Article Accountability Log in the "Dispensed" section.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

5.2. Masking

This is a subject-masked trial. The investigators may be aware of the study lenses based on a slight difference in lens color (the Test lenses will be slightly more turquoise in color than the Control lens).

Masking will be used to reduce potential bias. Subjects will be unaware of the identity of the investigational product, although they might notice a slight difference in lens color between Test and Control. Investigators and clinical site personnel involved in the data collection will not be masked as to the identity of the investigational product.

Under normal circumstances, the mask should not be broken until all subjects have completed the study and the database is finalized. Otherwise, the mask should be broken only if specific emergency treatment/course of action would be dictated by knowing the treatment status of the subject. In such cases, the Investigator may, in an emergency, contact the medical monitor. In the event the mask is broken, the Sponsor must be informed as soon as possible. The date, time, and reason for the unmasking must be documented in the subject record. The Investigator is also advised not to reveal the study treatment assignment to the clinical site or Sponsor personnel.

Subjects who have had their treatment assignment unmasked are expected to return for all remaining scheduled evaluations. Subjects who are discontinued will be replaced.

5.3. Procedures for Maintaining and Breaking the Masking

The identity of the study lenses will be masked to the subjects by over labeling the blister pack of the study lens. The label will contain the study number, lot number, sphere power, expiration date and the randomization codes.

The test articles mask shall not be broken unless information concerning the lens type is necessary for the urgent medical treatment of a subject. The Sponsor must be notified before the mask is broken.

6. STUDY INTERVENTION

6.1. Identity of Test Articles

The following contact lenses will be used in this study:

Table 3: Test Articles

	Control	Test
Manufacturer	JJVC	JJVC
Name	AV OASYS 1-DAY	TRP-200
Hydration	PG	PG

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

	Control	Test
Material	senofilcon A (C3)	senofilcon A (C3)
Packaging Form	Sterile blister pack	Sterile blister pack
Nominal Water Content (%)	38	38
Nominal Dk (edge corrected)	103	103
Nominal Modulus	101	101
Inversion Indicator	123	123
Nominal Base Curve/Diameter @ 22°C (mm)	8.5 / 14.3	8.5 / 14.3
Nominal Center Thickness @ -3.00 D (mm)	0.070	0.085
Nominal Powers (D)	-1.00 to -6.00 in 0.25 steps, except -5.00	-1.00 to -6.00 in 0.25 steps, except -5.00
UV/HEV-Blocker	NA	Yes

At least 873 lenses per SKU per study lens will be made available based on the following factors: sample size, bilateral wear, daily replacement, 2-week duration, safety margin of 2X, and US distribution model for the range of lenses -1.00 through -6.00 D.

6.2. Ancillary Supplies/Products

The following solutions will be used in this study. Note that RevitaLens will be used primarily to transport potential problematic lenses back to the Sponsor.

Table 4: Ancillary Supplies

	Solution			
Solution Name/Description	Acuvue™ RevitaLens Multipurpose Solution	Single use Eye-Cept® Rewetting Drops	LaciPure Saline Solution	ScleralFil Preservative Free Saline Solution
Manufacturer	Johnson & Johnson Vision	Optics Laboratory	Menicon	Bausch & Lomb
Preservative	alexidine dihydrochloride 0.00016% and polyquaternium-1 0.0003%	None	None	None

Lens cases and fluorescein strips (either 0.6 mg or 1.0 mg) will be supplied for use as needed.

Clinical Study Protocol


Johnson & Johnson Vision Care, Inc.

6.3. Administration of Test Articles

Test articles will be dispensed to subject meeting all eligibility requirements, including any dispensing requirements set forth in this clinical protocol. Subjects will be dispensed an adequate supply of test articles to complete the study. Lost or damaged test articles may be replaced at the discretion of the Investigator and/or the Sponsor.

6.4. Packaging and Labeling

The test articles will be packaged in blisters as the primary packaging. The test article will be over-labeled to mask the subject to the identity of the lens. The test articles will be in investigational cartons sealed with plastic bags as the secondary packaging form. The sample study label is shown below. The sample study label is shown below. The information represented on the label below is sample information only and is not representative of the actual study lens information.

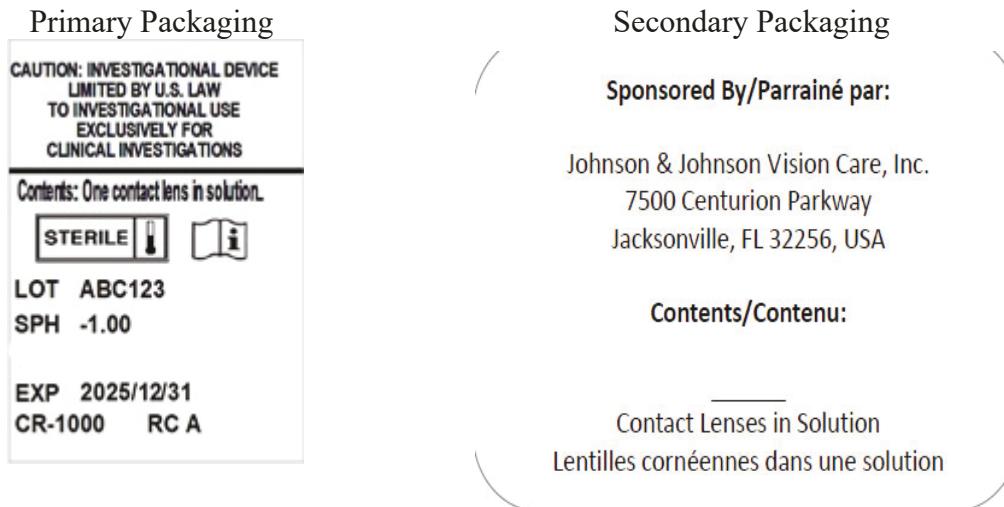

6.5. Storage Conditions

Test articles will be maintained at ambient temperatures at the clinical site. Test articles must be kept under secure conditions.

6.6. Collection and Storage of Samples

Subjects will dispose of their worn lenses on a daily basis. When possible, any lens or test article associated with an Adverse Events and/or a Product Quality Complaint must be retained and stored in a glass vial with moderate RevitaLens solution pending directions from the sponsor for potential return back to JJVC.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

6.7. Accountability of Test Articles

JJVC will provide the Investigator with sufficient quantities of study articles and supplies to complete the investigation. The Investigator is asked to retain all lens shipment documentation for the test article accountability records.

Test articles must be kept in a locked storage cabinet, accessible only to those assigned by the Investigator for dispensing. The Investigator may delegate this activity to authorized study site personnel listed on the Site Delegation Log. All test articles must be accounted. This includes:

1. What was dispensed for the subject for trial fitting, to wear out of the office, or issued for the subject to replace appropriately between visits.
2. What was returned to the Investigator unused, including expired or malfunctioning product.
3. The number and reason for unplanned replacements.

The Investigator will collect all unused test articles from the subjects at the end of the subject's participation. Subject returned unused test articles must be separated from the clinical study inventory of un-dispensed test articles and must be labeled with the subject number and date of return. Following final reconciliation of test articles by the monitor, the Investigator or monitor will return all unused test articles to JJVC.

If there is a discrepancy between the shipment documents and the contents, contact the study monitor immediately.

7. STUDY EVALUATIONS

7.1. Time and Event Schedule

Table 5: Time and Events

Visit Information	Visit 1 Screening, Baseline, Treatment 1	Visit 2 2-week FU Treatment 1, Treatment 2 Fitting	Visit 3 2-week FU Treatment 2 Final Evaluation
Time Point		14 days after Visit 1 (+/- 1 day)	14 days after Visit 2 (+/- 1 day)
Estimated Visit Duration	2.0 hours	2.0 hours	1.0 hours
Statement of Informed Consent	x		
Demographics	x		

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit Information	Visit 1 Screening, Baseline, Treatment 1	Visit 2 2-week FU Treatment 1, Treatment 2 Fitting	Visit 3 2-week FU Treatment 2 Final Evaluation
Time Point		14 days after Visit 1 (+/- 1 day)	14 days after Visit 2 (+/- 1 day)
Estimated Visit Duration	2.0 hours	2.0 hours	1.0 hours
Medical History/Concomitant Medications	X	X	X
Habitual Contact Lens Information	X		
Inclusion/Exclusion Criteria	X		
Study Questionnaires Baseline	X		
Entrance Visual Acuity	X	X	X
Slit Lamp Biomicroscopy	X	X	X
Expanded Conjunctival Redness	X	X	X
Expanded Corneal Staining	X	X	X
Iris Color	X		
Subjective Spherocylindrical Refraction	X		X
Lens Selection	X	X	
Lens Insertion & Settling	X	X	
Visual Acuity and Over Refraction	X	X	
Lens Power Modification (if applicable)	X	X	
Subject Reported Ocular Symptoms	X	X	X
Study Questionnaires Fitting	X	X	
Lens Fit Assessment	X	X	X
Lens Wettability	X	X	X
Surface characteristics	X	X	X
Lens dispensing information and criteria	X	X	
Patient instructions	X		
Study Questionnaires FU		X	X
Exit Acuity	X	X	X
Final Evaluation			X

7.2. Detailed Study Procedures

VISIT 1

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

The subjects must enter the visit wearing their habitual contact lenses.

Visit 1: Screening		
Step	Procedure	Details
1.1	Statement of Informed Consent	<p>Each subject must read, understand, and sign the Statement of Informed Consent before being enrolled into the study. The Principal Investigator or his/her designee conducting the informed consent discussion must also sign the consent form.</p> <p>Note: The subject must be provided a signed copy of this document.</p>
1.2	Demographics	Record the subject's year of birth, gender, race and ethnicity.
1.3	Medical History and Concomitant Medications	Questions regarding the subjects' medical history and concomitant medications.
1.4	Habitual Lenses	Questions regarding the subject's habitual lens type, modality, parameters, and duration (days per week, months worn SCLs).
1.5	Habitual Wear Time	Record the average wearing time and comfortable wearing time.
1.6	SCL Rx Confirmation	<p>The investigator confirms:</p> <ol style="list-style-type: none"> 1. The subject is wearing a SCL Rx that has been confirmed current (up-to-date) within the prior 6 months. 2. The subject has worn the up-to-date SCL Rx for at least 2 weeks.
1.7	Eligibility after Screening	<p>All responses to Screening Inclusion Criteria questions must be answered "yes" and all responses to Exclusion Criteria must be answered "no" for the subject to be considered eligible.</p> <p>If subject is deemed to be ineligible after screening, proceed to Final Evaluation and complete Subject Disposition. Refraction and Biomicroscopy forms are not required.</p>

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 1: Baseline		
Step	Procedure	Details
1.8	Baseline Questionnaire	<p>The subject will respond to the following Baseline Questionnaires based on their habitual lenses:</p> <ol style="list-style-type: none"> 1. CLUE Baseline 2. GSI Background 3. Activity History
1.9	Entrance Visual Acuity	Record the distance Snellen visual acuity (OD, OS, and OU) to the nearest letter with their habitual contact lens correction in place. Subjects must read the smallest line until at least 50% of the letters are read incorrectly.
1.10	Remove Habitual Lens	The subject's habitual lenses will be removed and stored in their own lens case. If they forgot to bring their lens case, one will be provided to them.
1.11	Slit Lamp Biomicroscopy	<p>The FDA Slit Lamp Classification Scale (████████) will be used to grade the findings and determine eligibility. Limbal and Bulbar Conjunctival Hyperemia findings (████████) and Corneal Staining Assessment (████████) will also be collected for internal purposes.</p> <p>If any of the slit lamp findings on the FDA scales are Grade 3 or higher, the subject may not continue at this time, but may return up to one additional time to determine eligibility. If discontinued a final examination must be completed.</p> <p>If the clearance of the fluorescein needs to be expedited, rewetting drops or saline may be instilled.</p>
1.12	Iris Color	The investigator will record the subject's iris color based on the scale provided.
1.13	Subjective Spherical-Cylindrical Refraction	Complete subjective spherical-cylindrical refraction and record the resultant distance visual acuity (OD, OS, and OU) to the nearest letter.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 1: Baseline		
Step	Procedure	Details
1.14	Eligibility after Baseline	<p>All responses to Inclusion Criteria questions must be answered “yes” and all responses to Exclusion Criteria questions must be answered “no” for the subject to be considered eligible.</p> <p>If subject is deemed to be ineligible after baseline, proceed to Final Evaluation and complete all forms.</p>

Visit 1: Treatment 1 Lens Fitting		
Step	Procedure	Details
1.15	Lens Selection	<p>Assign the study lens based on the randomization scheme.</p> <p>Select the contact lens power based on subjective spherocylindrical refraction</p> <p>[REDACTED]</p> <p>[REDACTED]</p> <p>Record the test condition.</p>
1.16	Lens Insertion	<p>The Investigator or the subject inserts the study lenses. Record the time of lens insertion.</p> <p>Check for lens damage under the slit lamp before proceeding with lens settling.</p> <p>Replace damaged lenses if applicable.</p>
1.17	Lens Settling	Allow the study lenses to settle for a minimum of 5 minutes.
1.18	Subjective Best Sphere Over Refraction	Perform subjective best sphere refraction over the study lenses with a phoropter (adopt the maximum plus to maximum visual acuity (MPMVA) approach and record the best corrected <u>distance</u> visual acuity to the nearest letter (OD, OS, and OU).
1.19	Lens Power Modification (if applicable)	<p>Adjust the lens power if the subject’s best sphere over-refraction is not plano.</p> <p>One power modification is allowed per eye.</p> <p>Subject’s requiring the -5.00 D power to achieve a plano spherical over-refraction of</p>

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 1: Treatment 1 Lens Fitting		
Step	Procedure	Details
		one or both eyes will be discontinued from the study.
1.20	Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.
1.21	Post-Fit Questionnaire	Subjects will respond to the GSI Post-fit Questionnaire.
1.22	Subjective Lens Fit Assessment	<p>Evaluate overall lens fit acceptance (acceptable or unacceptable) based on centration, movement and other fitting characteristics.</p> <p>An unacceptable fit is deemed by one of the following criteria:</p> <ul style="list-style-type: none"> • limbal exposure at primary gaze or with extreme eye movement • edge lift • excessive movement in primary and up gaze • insufficient movement in all three of the following conditions: primary gaze, up gaze, and Josephson push up <p>Note: if lens fit is unacceptable subject will be discontinued from the study.</p>
1.23	White Light Lens Surface Wettability	Record the white light lens wettability of both lenses.
1.24	Surface Deposits	Record any front and back surface lens deposits.
1.25	Visual Acuity	Record the distance visual acuity with the contact lenses (OD, OS, and OU) to the nearest letter. Smaller lines must be shown until the subject incorrectly identifies at least 50% of the letters.
1.26	Continuance	<p>For the subject to continue in the study, they must meet all three of the following criteria:</p> <ol style="list-style-type: none"> 1. Visual acuity is 20/30 or better OD and OS 2. The lens fit is acceptable OD and OS

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 1: Treatment 1 Lens Fitting		
Step	Procedure	Details
		<p>3. Investigator approval. If the Investigator does not approve the dispensing of the first study lens, then the study is terminated for that subject.</p>
1.27	Dispense	<p>The lenses will be dispensed for 13-15 days</p> <ol style="list-style-type: none"> 1. The subjects should wear their lenses similar to the inclusion criteria: ≥ 6 hours per day, ≥ 5 days per week. 2. The lenses will be worn as daily wear daily disposable only. 3. All subjects will be provided a bottle of ACUVUE RevitaLens to return any problematic lenses to the investigational site. 4. Rewetting drops are permitted if needed. 5. A patient instruction booklet will be provided. <p>Note 1: Ensure that the subject has enough lenses to last them to their next scheduled visit with no extras. In the event a lens is lost or damaged, and the subject has run out of lenses, the subject will return to the investigator site for replacement.</p> <p>Note 2: The subject's habitual contact lenses cannot be worn at any time during the study.</p>

VISIT 2

The follow-up will occur 13-15 days after Visit 1. The subjects must enter the visit wearing their study contact lenses.

Visit 2: Treatment 1 Follow-Up		
Step	Procedure	Details
2.1.	Adverse Events and Concomitant Medications Review	Review any changes to the subject's medical history or concomitant medications from the previous study visit. Record any changes, and any adverse events.
2.2.	Wearing Time	Record the average wearing time and comfortable wearing time.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 2: Treatment 1 Follow-Up		
Step	Procedure	Details
2.3.	Compliance	Confirm compliance with the prescribed wear schedule. Outdoor and total hours will also be collected.
2.4.	Return unworn lenses	Collect any unworn study lenses from the subject.
2.5.	Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.
2.6.	Follow-Up Questionnaire	Subjects will respond to the following questionnaires: 1. CLUE Follow-up 2. GSI Product Performance 3. Lens preference to habitual
2.7.	Visual Acuity	Record the distance Snellen visual acuity with the contact lenses (OD, OS, and OU) to the nearest letter. Subjects must read the smallest line until at least 50% of the letters are read incorrectly.
2.8.	Subjective Lens Fit Assessment	Evaluate overall lens fit acceptance (acceptable or unacceptable) based on centration, movement and other fitting characteristics. An unacceptable fit is deemed by one of the following criteria: 1. limbal exposure at primary gaze or with extreme eye movement 2. edge lift 3. excessive movement in primary and up gaze 4. insufficient movement in all three of the following conditions: primary gaze, up gaze, and Josephson push up <u>Note:</u> if lens fit is unacceptable subject will be discontinued from the study.
2.9.	Surface Deposits	Record any front and back surface lens deposits.
2.10.	Wettability Characteristics	Record the white light lens wettability of both lenses.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 2: Treatment 1 Follow-Up		
Step	Procedure	Details
2.11.	Lens Removal	Both lenses will be removed and discarded.
2.12.	Slit Lamp Biomicroscopy	<p>FDA Slit Lamp Classification Scale will be used to grade the findings. If no slit lamp finding is noted on the EDC form it is considered as a zero "0" grade for all observations listed.</p> <p>Note: If the subject has Grade 3 or 4 slit lamp findings on the FDA scale, then they must be followed as an adverse event.</p> <p>Adverse events must be reported to the JJVC monitors immediately.</p> <p>Limbal and Bulbar Conjunctival Hyperemia findings (████████) and Corneal Staining Assessment (████████) will be emphasized using a more detailed scale.</p> <p>After the slit lamp examination, at the discretion of the Investigator, rinse the subject's eyes thoroughly with rewetting drops or saline.</p>

Visit 2: Treatment 2 Lens Fitting		
Step	Procedure	Details
2.13.	Lens Selection	<p>Assign the study lens based on the randomization scheme.</p> <p>Select the contact lens power based on subjective sphero-cylindrical refraction ██████████ or final contact lens power of previous study lens.</p> <p>Record the test condition.</p>
2.14.	Lens Insertion	<p>The Investigator or the subject inserts the study lenses. Record the time of lens insertion.</p> <p>Check for lens damage under the slit lamp before proceeding with lens settling.</p> <p>Replace damaged lenses if applicable.</p>

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 2: Treatment 2 Lens Fitting		
Step	Procedure	Details
2.15.	Lens Settling	Allow the study lenses to settle for a minimum of 5 minutes.
2.16.	Subjective Best Sphere Over Refraction	Perform subjective best sphere refraction over the study lenses with a phoropter (adopt the maximum plus to maximum visual acuity (MPMVA) approach and record the best corrected <u>distance</u> visual acuity to the nearest letter (OD, OS, and OU).
2.17.	Lens Power Modification (if applicable)	Adjust the lens power if the subject's best sphere over-refraction is not plano. One power modification is allowed per eye. Subject's requiring the -5.00 D power to achieve a plano spherical over-refraction of one or both eyes will be discontinued from the study.
2.18.	Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.
2.19.	Post-Fit Questionnaire	Subjects will respond to the GSI Post-fit Questionnaire.
2.20.	Subjective Lens Fit Assessment	<p>Evaluate overall lens fit acceptance (acceptable or unacceptable) based on centration, movement and other fitting characteristics.</p> <p>An unacceptable fit is deemed by one of the following criteria:</p> <ul style="list-style-type: none"> • limbal exposure at primary gaze or with extreme eye movement • edge lift • excessive movement in primary and up gaze • insufficient movement in all three of the following conditions: primary gaze, up gaze, and Josephson push up <p>Note: if lens fit is unacceptable subject will be discontinued from the study.</p>
2.21.	White Light Lens Surface Wettability	Record the white light lens wettability of both lenses.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 2: Treatment 2 Lens Fitting		
Step	Procedure	Details
2.22.	Surface Deposits	Record any front and back surface lens deposits.
2.23.	Visual Acuity	Record the distance visual acuity with the contact lenses (OD, OS, and OU) to the nearest letter. Smaller lines must be shown until the subject incorrectly identifies at least 50% of the letters.
2.24.	Continuance	<p>For the subject to continue in the study, they must meet all three of the following criteria:</p> <ol style="list-style-type: none"> 1. Visual acuity is 20/30 or better OD and OS 2. The lens fit is acceptable OD and OS 3. Investigator approval. If the Investigator does not approve the dispensing of the first study lens, then the study is terminated for that subject.
2.25.	Dispense	<p>The lenses will be dispensed for 13-15 days</p> <ol style="list-style-type: none"> 1. The subjects should wear their lenses similar to the inclusion criteria: ≥ 6 hours per day, ≥ 5 days per week. 2. The lenses will be worn as daily wear daily disposable only. 3. All subjects will be provided a bottle of ACUVUE RevitaLens to return any problematic lenses to the investigational site. 4. Rewetting drops are permitted if needed. <p>Note 1: Ensure that the subject has enough lenses to last them to their next scheduled visit with no extras. In the event a lens is lost or damaged, and the subject has run out of lenses, the subject will return to the investigator site for replacement.</p> <p>Note 2: The subject's habitual contact lenses cannot be worn at any time during the study.</p>

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

VISIT 3

The follow-up will occur 13-15 days after Visit 2. The subjects must enter the visit wearing their study contact lenses.

Visit 3: Treatment 2 Follow-Up			
Step	Procedure	Details	
3.1.	Adverse Events and Concomitant Medications Review	Review any changes to the subject's medical history or concomitant medications from the previous study visit. Record any changes, and any adverse events.	
3.2.	Wearing Time	Record the average wearing time and comfortable wearing time.	
3.3.	Compliance	Confirm compliance with the prescribed wear schedule. Outdoor and total hours will also be collected.	
3.4.	Return unworn lenses	Collect any unworn study lenses from the subject.	
3.5.	Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire.	
3.6.	Follow-Up Questionnaire	Subjects will respond to the following questionnaires: 1. CLUE Follow-up 2. GSI Product Performance 3. Lens preference to alternate study lens	
3.7.	Visual Acuity	Record the distance Snellen visual acuity with the contact lenses (OD, OS, and OU) to the nearest letter. Subjects must read the smallest line until at least 50% of the letters are read incorrectly.	
3.8.	Subjective Lens Fit Assessment	Evaluate overall lens fit acceptance (acceptable or unacceptable) based on centration, movement and other fitting characteristics. An unacceptable fit is deemed by one of the following criteria: 1. limbal exposure at primary gaze or with extreme eye movement 2. edge lift 3. excessive movement in primary and up gaze	

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Visit 3: Treatment 2 Follow-Up		
Step	Procedure	Details
		<p>4. insufficient movement in all three of the following conditions: primary gaze, up gaze, and Josephson push up</p> <p>Note: if lens fit is unacceptable subject will be discontinued from the study.</p>
3.9.	Surface Deposits	Record any front and back surface lens deposits.
3.10.	Wettability Characteristics	Record the white light lens wettability of both lenses.
3.11.	Lens Removal	Both lenses will be removed and discarded.
3.12.	Slit Lamp Biomicroscopy	<p>FDA Slit Lamp Classification Scale will be used to grade the findings. If no slit lamp finding is noted on the EDC form it is considered as a zero "0" grade for all observations listed.</p> <p>Note: If the subject has Grade 3 or 4 slit lamp findings on the FDA scale, then they must be followed as an adverse event.</p> <p>Adverse events must be reported to the JJVC monitors immediately.</p> <p>Limbal and Bulbar Conjunctival Hyperemia findings (████████) and Corneal Staining Assessment █████ will be emphasized using a more detailed scale.</p> <p>After the slit lamp examination, at the discretion of the Investigator, rinse the subject's eyes thoroughly with rewetting drops or saline.</p>

FINAL EVALUATION

The final evaluation will ordinarily take place immediately following the last scheduled follow-up visit per the study protocol. It may also take place at any point the subject discontinues the study or is terminated from the study.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Final Evaluation		
Step	Procedure	Details
F.1	Final Exam Form	Indicate if the subject completed the study successfully. If subject discontinued from the study, indicate the reason.
F.2	Subjective spherocylindrical Refraction	Perform bare-eye subjective spherocylindrical refraction with a phoropter and record the best corrected <u>distance</u> visual acuity to the nearest letter (OD, OS, and OU).

7.3. Unscheduled Visits

If, during the investigation, a subject requires an unscheduled visit to the clinical site, the following information will be collected at a minimum:

- Chief complaint prompting the visit. If the reason is an adverse event, the applicable eCRF for the adverse event must be completed and subject record completed as appropriate
- Date and time of the visit and all procedures completed at the unscheduled visit
- Review of adverse event and concomitant medications
- Documentation of any test article dispensed or collected from the subject, if applicable
- Slit lamp findings (using the Slit Lamp Classification Scale)

If the Investigator withdraws a subject from the study, the final study visit case report forms must be completed indicating the reason(s) why the subject was withdrawn. The subject record must be completed documenting the date and primary reason for withdrawal and the study CRA notified.

Any ocular and non-ocular Adverse Events that are ongoing at the time of the study visit will be followed by the Investigator, within licensure, until they have resolved, returned to pretreatment status, stabilized, or been satisfactorily explained. If further treatment i.e., beyond licensure is required, the subject will be referred to the appropriate health care provider.

The following information will be collected during an unscheduled visit (Table 6).

Table 6: Unscheduled Visit Procedures

Step	Procedure	Details
U.1	Reason for unscheduled visit	Indicate if the <u>only</u> reason for the visit is that the subject requires additional test articles. If the reason is other than

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Step	Procedure	Details	
		resupply of previously dispensed lenses, specify the reason for the visit.	
U.2	Chief Complaints (if applicable)	Record the subject's chief complaints for reasons for the unscheduled visit	
U.3	Adverse Events and Concomitant Medications Review (if applicable)	Review any changes to the subject's medical history or concomitant medications from the previous study visit. Record any changes, and any adverse events.	
U.4	Entrance VA (if applicable)	Record the entrance distance visual acuity (OD, OS and OU) to the nearest letter.	
U.5	Subjective Sphero-cylindrical Refraction (if applicable)	The investigator will complete a subjective refraction (sphere and cylinder) and record the resultant distance visual acuity OD, OS, and OU to the nearest letter.	
U.6	Slit Lamp Biomicroscopy (if applicable)	<p>FDA Slit Lamp Classification Scale will be used to grade the findings. If no slit lamp finding is noted on the EDC form it is considered as a zero "0" grade for all observations listed.</p> <p>Note: If the subject has Grade 3 or 4 slit lamp findings on the FDA scale, then they must be followed as an adverse event. Adverse events must be reported to the JJVC monitors immediately.</p> <p>Limbal and Bulbar Conjunctival Hyperemia findings (████████) and Corneal Staining Assessment (████████) will be emphasized using a more detailed scale.</p> <p>After the slit lamp examination, at the discretion of the Investigator, rinse the subject's eyes thoroughly with rewetting drops or saline.</p>	
U.7	Dispensing (if applicable)	Additional lenses may be dispensed if one is lost or torn during the wearing period.	

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

Step	Procedure	Details	
U.8	Exit Visual Acuity (if applicable)	Record the subject's exit distance visual acuity (OD, OS and OU) to the nearest letter.	

Note: If the only reason for the unscheduled visit is that the subject requires additional test articles, only the dispensing information needs to be recorded.

7.4. Laboratory Procedures

Not Applicable.

8. SUBJECTS COMPLETION/WITHDRAWAL

8.1. Completion Criteria

Subjects are considered to have completed the study if they:

- provided informed consent.
- they are eligible.
- have not withdrawn/discontinued from the study for any reason described in section 8.2.
- completed all visits through the final visit 3
- If all visits were completed but an additional visit is considered necessary for subject care, follow the requirements for unscheduled visits in section 7.3.

8.2. Withdrawal/Discontinuation from the Study

A subject will be withdrawn from the study for any of the following reasons:

- Subject withdrawal of consent.
- Subject not compliant to protocol such as study lens wear time or habitual lens wear while enrolled in the study.
- Subject lost to follow-up.
- Subject no longer meets eligibility criteria (e.g. the subject becomes pregnant).
- Subject develops significant or serious adverse events necessitating discontinuation of study lens wear.
- Subjects who have experienced a Corneal Infiltrative Event (CIE).
- Investigator's clinical judgment regarding the subject safety reasons (that it is in the best interest of the subject to stop treatment).
- Subject missed two consecutive study visits.
- Subject not compliant with study lens wear schedule (i.e. wears study lenses less than at least 6 hours per day for at least 5 days a week over the 2 week wear period)
- Subject not successfully dispensed due to lack of efficacy and safety including poor vision, poor comfort or unacceptable fit.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

For discontinued subjects, the Investigator will:

- Complete the current visit (scheduled or unscheduled).
- Complete the Final Evaluation, indicating the reason that the subject was discontinued from the study.
- Record the spherocylindrical refraction with best corrected distance visual acuity.
- Collect used test article(s) (worn or brought to the visit) from the subject and discard them, unless otherwise stated in section 7.2.
- Collect all unused test article(s) from the subject.
- Make arrangements for subject care, if needed, due to their study participation

Additional subjects will be enrolled if a subject discontinues from the study prematurely.

In cases where a subject is lost to follow-up, every possible effort must be made to contact the subject and determine the reason for discontinuation/withdrawal. The measures taken to follow up must be documented including two written attempts and a certified letter (or equivalent) as the final attempt.

9. PRE-STUDY AND CONCOMITANT INTERVENTION/MEDICATION

Concomitant medications will be documented during screening and updated during the study.

- Disallowed medications for this study include: medications that may interfere with contact lens wear (see section 9.1). Habitual medications used by successful soft contact lens wearers are considered acceptable.
- Concomitant therapies that are disallowed include: NA

9.1. Systemic Medications

Certain systemic medications are known to have a higher likelihood to interfere with contact lens wear, chiefly by disrupting the tear film.

A summary of disallowed systemic medications is shown in Table 7. Subjects with a history of taking these medications will be allowed to enroll only if:

- The medications have been taken on a continual, routine basis for at least 6 months, and
- The subject has demonstrated successful contact lens wear during this time.

Or:

- The subject was taking the medication on a temporary basis and ceased taking that medication at least 2 weeks prior to signing the informed consent (this is considered sufficient time for the medication to have left the body prior to enrollment).

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Subjects with a history of taking medications listed in Table 7 on a long-term, routine basis for less than 6 months will not be allowed to participate in the study.

Table 7: Disallowed systemic medications

Class of Drug	Common Indication(s)	Common Examples
Estrogens (not including contraceptive medication)	Menopause, osteoporosis, vaginitis	Vagifem, Estrace, Climara, Vivelle-Dot, Premarin, Minivelle, etc.
Anticholinergics	Irritable bowel syndrome, Parkinson's disease, peptic ulcer, cystitis, nasal congestion, cold symptoms, overactive bladder, COPD	Bentyl, Spiriva, Atrovent, Hyosyne, Levsin, Symax Fastab, Symax SL, Homax SL, Cogentin, Transderm Scop, etc.
Beta-blockers	Hypertension, angina, heart attack, migraine, atrial fibrillation, adrenal cancer, essential tumor, glaucoma	Toprol XL, Lopressor, Tenormin, Propranolol, Timoptic, Trandate, Inderal LA, etc.
Psychotropics	Antipsychotic (schizophrenia, mania), antidepression, antiobsessive, antianxiety, mood stabilizer, stimulants (ADHD)	Zoloft, Celexa, Prozac, Lexapro, Effexor, Cymbalta, Ativan, Xanax, Desyrel, Wellbutrin, etc.
Vitamin A analogs	Cystic acne	Isotretinoin

Examples of disallowed systemic antihistamines are given in Table 8. Subjects with a history of taking systemic antihistamines will be allowed to enroll only if:

- They have taken antihistamines continuously for at least 2 weeks, and
- They have demonstrated successful wear while taking the medication

Or:

- They stopped taking the medication for at least 2 weeks prior to enrollment.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Table 8: Disallowed systemic antihistamines

Class of Drug	Common Indication(s)	Common Examples
Antihistamines	Allergic rhinitis, sedation, hives, allergic conjunctivitis, skin allergy, itching, motion sickness	Hydroxyzine, Promethagan, Phenadoz, Vistaril, Claritin, Zyrtec, Astepro, Astelin, Optivar, Allegra, Benadryl, etc.

10. DEVIATIONS FROM THE PROTOCOL

Investigator will notify study sponsor upon identification of a protocol deviation. Protocol deviations must be reported to the sponsor within 24 hours after discovery of the protocol deviation. The Investigator will report deviations per IRB/IEC requirements. All deviations will be tracked, and corrective actions implemented as appropriate.

If it becomes necessary for the Investigator to implement a deviation in order to eliminate an immediate hazard to the trial subject, the Investigator may implement the deviation immediately without notification to the sponsor. Within 24 hours after the implemented deviation, the Investigator must notify and provide the rationale to the Sponsor and, as required, the IEC/IRB.

If the deviation potentially impacts the safety of patient or changes the technical integrity of the study, then it must be reported to IEC/IRB. This is a "Major Deviation". Deviations that contradict the information contained in the Informed Consent/Assent forms will be considered Major Deviations.

Minor deviations have no substantive effect on patient safety or technical integrity of the study. They are often logistical in nature.

Protocol waivers are prohibited.

Table 9 lists examples of deviations that will constitute major and minor protocol deviations for this study.

Table 9: Examples of major and minor protocol deviations

Deviation category	Major deviation	Minor deviation
Out-of-window visit	Visit attended 2 days or more than out of visit window defined in study procedures	Visit attended 1 day or fewer out of visit window defined in study procedures
Unanswered PRO questions	For questionnaires where data is related to a primary or	For questionnaires where data is related to a primary or

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Deviation category	Major deviation	Minor deviation
	secondary endpoint, 2 or more PRO questions are unanswered (i.e., left blank).	secondary endpoint, 1 or fewer PRO questions are unanswered (i.e., left blank). For questionnaires where data where data is not related to a primary or secondary endpoint, any PRO questions are unanswered (i.e., left blank).
Insufficient wear of study lenses	Subject does not wear study lenses for at least 6 hours on at least 5 days of a study lens wear period.	NA

In the case of a major protocol deviation, the decision of whether or not the subject will be excluded from the Per-Protocol analysis population will be made at the time of cohort review.

11. STUDY TERMINATION

If more than 2 subjects in the investigational soft contact lens group develop serious expected (e.g., definite or probable MK) or unexpected device related adverse events, the study will be suspended. Upon review and consultation with IRB, and JJVC Safety Review committee, the study may be terminated. This potential stopping rule is established based on our trial involving approximately 200 subjects wearing the investigational soft contact lens for up to 3 years with an assumed MK rate that is below 0.2% per patient-year. The rate of 0.2% per patient year is the established rate for extended wear lenses in adults, which was requested by the FDA as a criterion for evaluating a contact lens for pediatric use in an FDA response to a pre-IDE submission. To be conservative, 200 independent patient years were used in the calculation. The probability of observing 2 cases or more incidents of MK is 0.061, and 3 cases or more incidents of MK is 0.007 (given an MK rate of 0.2% per patient year).

The occurrence of one or more Unanticipated Serious Adverse Device Effect (USADE), or any SAE where the relationship to study agent cannot be ruled out, may result in stopping further dispensing of test article. In the event of a USADE or SAE, the Sponsor may unmask the treatment regimen for the subject(s) and will discuss this with the Investigator before any further subjects are enrolled.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

The Sponsor will determine when a study will be stopped. The Principal Investigator always has the discretion to initiate stopping the study based on patient safety or if information indicates the study's results are compromised.

JJVC reserves the right to terminate the study at any time for any reason. Additionally, the IEC/IRB reserves the right to terminate the study if an unreasonable risk is determined. The study can be terminated by the Principal Investigator at the individual clinical site due to specific clinical observations, if in their opinion, after a discussion with JJVC, it is determined that it would be unwise to continue at the clinical site.

JJVC (and the IEC/IRB and DMC, if applicable) will evaluate all adverse events. If it is determined that an adverse event presents an unreasonable risk, the investigation, or that part of the investigation presenting the risk, will be terminated as soon as possible.

Should the study be terminated (either prematurely or as scheduled), the Investigator will notify the IEC/IRB and Regulatory Authority as required by local regulatory requirements.

12. PROCEDURE FOR HANDLING PRODUCT QUALITY COMPLAINTS

A Product Quality Complaint (PQC) refers to any written, electronic, or oral communication that alleges deficiencies related to the identity, quality, durability, reliability, safety, effectiveness or performance of test articles after they have been released for clinical trial use.

Potential complaints may come from a variety of sources including but not limited to subjects, clinical research associates (CRA), clinical operations managers (COM), medical monitors, and site personnel, etc. The following are not considered product quality complaints:

- Subject satisfaction inquiries reported via "Subjective Questionnaires" and "Patient Reported Outcomes (PRO)."
- Clinical test articles that are stored improperly or damaged after receipt at the investigational site.
- Lens replacements that occur due to drops/fall-outs.
- Damage deemed by clinicians or clinical staff to be caused by handling by the user, and not indicative of a quality deficiency (i.e. tears, rips, etc.), only in situations where there is no deficiency alleged by the subject.

Within 24 hours of site personnel becoming aware that a PQC has occurred, the PQC must be recorded in the EDC system, which will trigger an automatic email notification to the appropriate COM/CRA and Clinical QA representative. In cases where the EDC system in use is not configured to send automatic notifications or when an EDC system is not used, the COM/CRA is responsible for notifying Clinical QA upon discovery that a PQC has occurred.

Upon receipt of the EDC notification, the COM/CRA will contact the study site to collect additional information which will include:

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

- Date the complaint was received/recorded in the EDC System (Date of Sponsor Awareness).
- Who received the complaint.
- Study number.
- Clinical site information (contact name, site ID, telephone number).
- Lot number(s).
- Unique Subject Identifier(s).
- Indication of who first observed complaint (site personnel or subject).
- OD/OS indication, along with whether the lens was inserted.
- Any related AE number if applicable.
- Detailed complaint description (scheduled/unscheduled visit, wear time, symptoms, resolution of symptoms, etc.).
- Eye Care Provider objective (slit lamp) findings if applicable.
- Confirmation of product availability for return (and tracking information, if available), or rationale if product is not available for return

Once a complaint is received, it will be assessed by the COM, CRA, or trained site personnel to determine if it is an Adverse Event/Serious Adverse Event (AE/SAE). If the complaint results in an AE/SAE, the COM/CRA, or trained site personnel will follow section 13 of this protocol. If the AE/SAE was potentially the result of a product quality related deficiency, these procedures also applies and will be executed in parallel.

In some cases, a PQC form may be generated in EDC by the site in error. In this event, the PQC forms will be marked “Intentionally Left Blank” or “ILB”. Justification for ILB must be documented.

13. ADVERSE EVENTS

13.1. Definitions and Classifications

Adverse Event (AE) – An AE is “any untoward medical occurrence, unintended disease or injury, or untoward clinical signs (including abnormal laboratory findings) in subjects, users or other persons, whether or not related to the investigational medical device.”

Note: This definition includes events related to the investigational medical device or the comparator, and to the procedures involved. For users or other persons, this definition is restricted to events related to investigational medical devices.¹

An AE includes any condition (including a pre-existing condition) that:

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

1. Was not present prior to the study, but appeared or reappeared following initiation of the study.
2. Was present prior to the study but worsened during the study. This would include any condition resulting from concomitant illnesses, reactions to concomitant medications, or progression of disease states.

Note: Pregnancy must be documented as an adverse event and must be reported to the clinical monitor and to the Sponsor immediately upon learning of the event.

Serious Adverse Event (SAE) – An SAE is any adverse event that led to any of the following:

- Death
- Serious deterioration in the health of the subject that resulted in any of the following:
- Life-threatening illness or injury
- Permanent or persistent impairment of a body structure or a body function
- Hospitalization or prolongation of patient hospitalization
- Medical or surgical intervention to prevent life-threatening illness or injury or permanent impairment to a body structure or a body function.
- Chronic disease
- Foetal distress, foetal death or a congenital physical or mental impairment of birth defect.

Diagnoses and conditions that are considered Ocular Serious Adverse Events include, but not limited to:

- Microbial Keratitis (MK)
- Iritis (including cells in the anterior chamber)
- Permanent decrease in best spectacle corrected visual acuity equivalent to 2 acuity lines or greater
- Central Corneal Opacity
- Central Corneal Neovascularization
- Uveitis
- Endophthalmitis
- Hypopyon
- Hyphemia
- Penetration of Bowman's Membrane
- Persistent Epithelial Defect
- Limbal cell Damage leading to Conjunctivalization

Significant Adverse Events – are defined as events that are symptomatic and warrant discontinuation (temporary or permanent) of the contact lens wear

Diagnoses and conditions that are considered Ocular Significant Adverse Events include, but not limited to the following:

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

- Contact Lens Induced Peripheral Ulcer (CLPU)
- Significant Infiltrative Events (SIE)
- Superior Epithelial Arcuate Lesions (SEALs)
- Any Temporary Loss of > 2 Lines of BSCVA
- Other grade 3 or higher corneal findings, such as abrasions or edema
- Non-contact lens related corneal events - e.g. Epidemic Keratoconjunctivitis (EKC)
- Asymptomatic Corneal Scar
- Any corneal event which necessitates temporary lens discontinuation > 2 weeks

Non-Significant Adverse Events – are defined as those events that are usually asymptomatic and usually do not warrant discontinuation of contact lens wear but may cause a reduction in wear time. However, the Investigator may choose to prescribe treatment as a precautionary measure.

Diagnoses and conditions that are considered Ocular Non-Significant Adverse Events include, but not limited to the following:

- Non-significant Infiltrative Event (NSIE)
- Contact Lens Papillary Conjunctivitis (CLPC)
- Superficial Punctate Keratitis (SPK)
- Conjunctivitis: Bacterial, Viral, Allergic
- Blepharitis
- Meibomianitis
- Contact Dermatitis
- Localized Allergic Reactions
- Any corneal event not explicitly defined as serious or significant adverse event, which necessitates temporary lens discontinuation < 2 weeks

Adverse Device Effect (ADE) – An ADE is an “adverse event related to the use of an investigational medical device.”

Note 1: This definition includes adverse events resulting from insufficient or inadequate instructions for use, deployment, implantation, installation, or operation, or any malfunction of the investigational medical device.

Note 2: This definition includes any event resulting from use error or from intentional misuse of the investigational medical device.¹

Unanticipated Adverse Device Effect (UADE) – A UADE is any serious adverse effect on health or safety or any life-threatening problem or death caused by, or associated with, the test article, if that effect, problem, or death was not previously identified in nature, severity, or degree of incidence in the investigational plan, Investigator’s Brochure or protocol, or any

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

other unanticipated serious problem associated with the test article that relates to the rights, safety and welfare of subjects.

13.2. Assessing Adverse Events

In conjunction with the medical monitor, the Investigator will evaluate adverse events to ensure the events are categorized correctly. Elements of categorization will include:

- Seriousness/Classifications (see definition in section 13.1).
- Causality or Relatedness – i.e. the relationship between the test article, study treatment or study procedures and the adverse event (not related, unlikely related, possibly related, or related - see definition in section 13.2.1).
- Adverse Event Severity – Adverse event severity is used to assess the degree of intensity of the adverse event (mild, moderate, or severe - see definition in section 0).
- Outcome – not recovered or not resolved, recovering or resolving, recovered or resolved with sequelae, recovered or resolved, death related to adverse event, or unknown.
- Actions Taken – none, temporarily discontinued, permanently discontinued, or other.

13.2.1. Causality Assessment

Causality Assessment – A determination of the relationship between an adverse event and the test article. The test article relationship for each adverse event should be determined by the investigator using these explanations:

- Not Related- An adverse event that is not related to the use of the test article, study treatment or study procedures.
- Unlikely Related – An adverse event for which an alternative explanation is more likely, e.g. concomitant treatment, concomitant disease(s), or the relationship of time suggests that a causal relationship is not likely.
- Possibly Related – An adverse event that might be due to the use of the test article, or to the study treatment or study procedures. An alternative explanation, e.g. concomitant treatment, concomitant disease(s), is inconclusive. The relationship in time is reasonable. Therefore, the causal relationship cannot be excluded.
- Related – An adverse event that is listed as a possible adverse effect (device) or adverse reaction (drug) and cannot be reasonably explained by an alternative explanation, e.g. concomitant treatment of concomitant disease(s). The relationship in time is very suggestive, e.g. it is confirmed by de-challenge and re-challenge.

13.2.2. Severity Assessment

Severity Assessment – A qualitative assessment of the degree of intensity of an adverse event as determined by the Investigator or reported to him/her by the subject. The assessment of severity is made irrespective of test article, study treatment or study procedure relationship or seriousness of the event and should be evaluated according to the following scale:

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

- Mild – Event is noticeable to the subject but is easily tolerated and does not interfere with the subject’s daily activities.
- Moderate – Event is bothersome, possible requiring additional therapy, and may interfere with the subject’s daily activities.
- Severe – Event is intolerable, necessitates additional therapy or alteration of therapy and interferes with the subject’s daily activities.

13.3. Documentation and Follow-Up of Adverse Events

The recording and documenting of adverse events (ocular and non-ocular) begin when the subjects are exposed to the test article, study treatment or study procedure. Adverse events reported before the use of test article, start of study treatment, or study procedures will be recorded as medical history. However, if the condition deteriorates at any time during the study it will be recorded and reported as an AE. Untoward medical events reported after the subject’s exit from the study will be recorded as adverse events at the discretion of the Investigator.

Upon finding an adverse event, the Principal Investigator will document the condition in the subject record and in the eCRFs and complete the Adverse Event eCRF.

Complete descriptions of all adverse events must be available in the subject record. All Adverse Events including local and systemic reactions not meeting the criteria for “serious adverse events” shall be captured on the appropriate case report form or electronic data system. All adverse events occurring while the subject is enrolled in the study must be documented appropriately regardless of relationship.

It is the Investigator’s responsibility to maintain documentation of each reported adverse event. All adverse events will be followed in accordance with applicable licensing requirements. Such documentation will include the following:

- Adverse event (diagnosis not symptom).
- Drawings or photographs (where appropriate) that detail the finding (e.g., size, location, and depth, etc.).
- Date the clinical site was notified.
- Date and time of onset.
- Date and time of resolution.
- Adverse event classification, severity, and relationship to test articles, as applicable.
- Treatment regimen instituted (where appropriate), including concomitant medications prescribed, in accordance with applicable licensing requirements.
- Any referral to another health care provider if needed.
- Outcome, ocular damage (if any).
- Likely etiology.
- Best corrected visual acuity at the discovery of the event and upon conclusion of the event, if the AE is related to the visual system.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

Upon discovery of an AE that is deemed ‘possibly related’ or ‘related’ to the test article or study procedures (whether related to the visual system or not), an AE review form [REDACTED] must be completed. Additional dated and initialed entries should be made at follow-up evaluations. Separate forms must be completed for each eye if the AE is bilateral.

In addition, if an infiltrate(s) is present, he/she will complete the Corneal Infiltrate Assessment eCRF. Where necessary, a culture of the corneal lesion will be collected to determine if the infection is microbial in nature. If cultures are collected, the date of culture collection and laboratory utilized will be recorded.

Changes in the severity of an AE shall be documented to allow an assessment of the duration of the event at each level of intensity to be performed. Adverse events characterized as intermittent require documentation of the onset and duration of each episode. Changes in the assessment of relationship to the Test Article shall also be clearly documented.

Subjects who present with an adverse event shall be followed by the Investigator, within licensure, until all signs and symptoms have returned to pre-treatment status, stabilized, or been satisfactorily resolved. If further treatment beyond licensure is required, the patient will be referred to the appropriate health care provider. The Investigator will use his/her clinical judgment as to whether a subject reporting with an adverse event will continue in the study. If a subject is discontinued from the study, it will be the responsibility of the Investigator to record the reason for discontinuation. The Investigator will also document the adverse event appropriately and complete the Adverse Event eCRF. Any subjects with ongoing adverse events related to the test article, study treatment or study procedures, as of the final study visit date, should be followed to resolution of the adverse event or until referral to an appropriate health care provider, as recommended by the Investigator. Non-ocular adverse events that are not related to the test article, study treatment, or study procedures may be recorded as “ongoing” without further follow-up.

13.4. Reporting Adverse Events

The Investigator will notify the Sponsor of an adverse event by e-mail, facsimile, or telephone as soon as possible and no later than 24 hours from discovery for any serious /significant adverse events, and 2 days from discovery for any non-significant adverse event. In addition, a written report will be submitted by the Principal Investigator to the IEC/IRB according to their requirements (section 13.4.2). The report will comment whether the adverse event was considered to be related to the test article, study treatment or study procedures.

13.4.1. Reporting Adverse Events to Sponsor

Serious/Significant Adverse Events

The Investigator will inform the sponsor of all serious/significant adverse events occurring during the study period as soon as possible by e-mail or telephone, but no later than 24 hours following discovery of the event. The Investigator is obligated to pursue and obtain information requested by the Sponsor in addition to that information reported on the eCRF. All

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

subjects experiencing a serious/significant adverse event must be followed up and all outcomes must be reported.

When medically necessary, the Investigator may break the randomization code to determine the identity of the treatment that the subject received. The Sponsor and study monitor should be notified prior to unmasking the test articles.

In the event of a serious/significant adverse event, the Investigator must:

- Notify the Sponsor immediately.
- Obtain and maintain in the subject's records all pertinent medical information and medical judgment for colleagues who assisted in the treatment and follow-up of the subject.
- Provide the Sponsor with a complete case history which includes a statement as to whether the event was or was not related to the use of the test article.
- Notify the IEC/IRB as required by the IEC/IRB reporting procedure according to national regulations.

Unanticipated (Serious) Adverse Device Effect (UADE)

In the event of an Unanticipated (Serious) Adverse Device Effect (UADE), the Investigator will submit a report of the UADE to the Sponsor and IEC/IRB as soon as possible, but no later than 24 hours after the Investigator first learns of the effect. This report is in addition to the immediate notification mentioned above.

The Sponsor must conduct an evaluation of the UADE and must report the results of the evaluation to FDA, the IEC/IRB and participating Investigators within 10 working days after the Sponsor first receives notification of the effect.

Non-Serious Adverse Events

All non-serious adverse events, including non-serious adverse device effects, will be reported to the sponsor by the Investigator no later than 2 days from discovery.

13.4.2. Reporting Adverse Events to the Responsible IEC/IRB and Health Authorities

Adverse events that meet the IEC/IRB requirements for reporting must be reported within the IEC/IRB's written guidelines. Each clinical site will refer to and follow any guidelines set forth by their Approving IEC/IRB. Each clinical site will refer to and follow any guidelines set forth by their local governing Health Authorities.

The Sponsor will report applicable Adverse Events to the local health authorities according the written guidelines, including reporting timelines.

13.5. Event of Special Interest

None

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

13.6. Reporting of Pregnancy

Subjects reporting pregnancy (by self-report) during the study will be discontinued after the event is recorded as an Adverse Event. Once discontinued, pregnant participants and their fetuses will not be monitored for study related purposes. Pregnant participants are not discontinued from contact lens or solution related studies for safety concerns, but due to general concerns relating to pregnancy and contact lens use. Specifically, pregnant women are discontinued due to fluctuations in refractive error and/or visual acuity that occur secondary to systemic hormonal changes, and not due to unforeseen health risks to the mother or fetus.

14. STATISTICAL METHODS

14.1. General Considerations

A general description of the statistical methods to be implemented in this clinical trial is outlined below. More details will be included in the stand-alone Statistical Analysis Plan (SAP). The SAP will be developed and finalized prior to database lock.

All data summaries and statistical analyses will be performed using the Statistical Analysis System (SAS) software Version 9.4 or higher (SAS Institute, Cary, NC)¹³. Throughout the analysis of data, the results for each subject/eye will be used when available for summarization and statistical analysis. Unscheduled visits will be summarized separately and will be excluded from the statistical analysis.

Summary tables (descriptive statistics and/or frequency tables) will be provided for all baseline variables, efficacy variables and safety variables as appropriate. Continuous variables will be summarized with descriptive statistics (n, mean, standard deviation [SD], median, minimum and maximum). Frequency count and percentage of subjects or eyes within each category will be provided for categorical data.

14.2. Sample Size Justification

This study is designed and powered to demonstrate non-inferiority of the Test lens compared to the Control lens with respect to CLUE overall quality of vision, CLUE overall comfort and handling at the 2-week follow-up evaluation. Sample size was calculated for these primary and secondary endpoints to achieve a minimum statistical power of 80% with a 2-sided type I error of 0.05 based on historical data from [REDACTED]. The same type of Test and Control lenses were investigated in [REDACTED] with the same 2×2 crossover design; Test lenses in [REDACTED] were made from the pilot line while Test lenses in the current study are produced from the manufacturing line. Table 10 below presents the descriptive statistics of CLUE scores at the 2-week follow-up evaluation observed from [REDACTED]¹⁴

In addition to the primary and secondary endpoints mentioned above, sample size was also calculated to see what is the required number of subjects for achieving a statistical power of approximately 80% to demonstrate superiority of the Test lens compared to the Control lens

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

with respect to clarity of vision in doors in bright light (proportion of subjects with “Excellent” response) and overall preference while using computer screens & digital devices (i.e., exploratory hypotheses of two individual items) at the 2-week follow-up evaluation. Table 11 below displays the descriptive statistics of these two individual items at the 2-week follow-up evaluation observed from [REDACTED].¹⁴

Table 10: Descriptive Summary of CLUE Scores at 2-week Follow-up from [REDACTED] – Completed Per Protocol Subjects

Domain	Test [Mean(SD)]	Control [Mean(SD)]
CLUE Vision	69.4 (19.95)	65.7 (21.38)
CLUE Comfort	68.0 (22.08)	64.5 (23.21)
CLUE Handling	69.7 (21.20)	70.0 (20.84)

SD = standard deviation

Table 11: Descriptive Summary of Two Individual Items at 2-week Follow-up from [REDACTED] – Completed Per Protocol Subjects

Item	Response Category	Test n(%)	Control n(%)
Clarity of vision indoors in bright light	Not Applicable	1 (0.6)	2 (1.1)
	Excellent	98 (55.1)	81 (45.5)
	Very Good	50 (28.1)	58 (32.6)
	Good	24 (13.5)	28 (15.7)
	Fair	4 (2.2)	7 (3.9)
	Total	178	178
Item	Response Category	Total n(%)	
Overall preference while using computer screens & digital devices	Strongly prefer the AO1D	26 (14.6)	
	Slightly prefer the AO1D	13 (7.3)	
	No Preference	59 (33.1)	
	Slightly prefer the IP-RTY1-PG	35 (19.7)	
	Strongly prefer the IP-RTY1-PG	45 (25.3)	
	Total	178	

CLUE Overall Quality of Vision

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

Sample size for CLUE overall quality of vision was calculated using a linear mixed model-based power analysis method assuming no difference between the Test and Control lenses.¹⁵ An unstructured (UN) covariance matrix, which was used to model the covariance between measurements on the same subjects across study periods, was estimated from the analysis of [REDACTED] historical data.¹⁴ Parameters in the UN covariance matrix were freely estimated for the two habitual lens groups. For sample size calculation CLUE vision scores were analyzed using a linear mixed model with lens as a fixed effect and the estimated UN covariance matrix and tested for non-inferiority using a non-inferiority margin of -5 points. Below is the variance-covariance matrix used in the sample size calculation for CLUE overall quality of vision.

Habitual daily disposable lens wearers:
$$\begin{bmatrix} 210.12 & 55.2899 \\ 55.2899 & 367.06 \end{bmatrix}$$

Habitual daily reusable lens wearers:
$$\begin{bmatrix} 276.46 & 125.78 \\ 125.78 & 118.44 \end{bmatrix}$$

CLUE Overall Comfort

Sample size for CLUE overall comfort was calculated using a linear mixed model-based power analysis method¹⁶ assuming no difference between Test and Control. An unstructured (UN) covariance matrix, which was used to model the covariance between measurements on the same subjects across study periods, was estimated from the analysis of [REDACTED] historical data.¹⁴ Parameters in the UN covariance matrix were freely estimated for different habitual lens groups. For sample size calculation CLUE comfort scores were analyzed using a linear mixed model with lens as a fixed effect and the estimated UN covariance matrix and tested for non-inferiority using a non-inferiority margin of -5 points. Below is the variance-covariance matrix used in the sample size calculation for CLUE comfort.

Habitual daily disposable lens wearers:
$$\begin{bmatrix} 351.71 & -19.9976 \\ -19.9976 & 487.88 \end{bmatrix}$$

Habitual daily reusable lens wearers:
$$\begin{bmatrix} 384.67 & 230.69 \\ 230.69 & 442.74 \end{bmatrix}$$

CLUE Overall Handling

Sample size for CLUE overall handling was calculated using a linear mixed model-based power analysis method¹⁶ assuming no difference between the Test and Control lenses. A unstructured (UN) covariance matrix, which was used to model the covariance between measurements on the same subjects across study periods, was estimated from the analysis of [REDACTED] historical data. Parameters in the UN covariance matrix were freely estimated for different habitual lens groups. For sample size calculation CLUE handling scores were analyzed using a linear mixed model with lens as a fixed effect and the estimated UN covariance matrix and tested for non-inferiority using a non-inferiority margin of -5 points. Below is the variance-covariance matrix used in the sample size calculation for CLUE overall handling.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

Habitual daily disposable lens wearers:
$$\begin{bmatrix} 255.02 & 95.4223 \\ 95.4223 & 418.37 \end{bmatrix}$$

Habitual reusable lens wearers:
$$\begin{bmatrix} 425.78 & 201.18 \\ 201.18 & 261.21 \end{bmatrix}$$

Clarity of vision indoors in bright light

Clarity of vision indoors in bright light will be evaluated at 2-week follow-up using a 5-point Likert scale (1: Excellent, 2: Very Good, 3: Good, 4: Fair and 5: Poor) with a “Not Applicable” response option. Responses to clarity of vision indoors in bright light will be converted into a binary variable for the purpose of analysis (Excellent = 1 and others = 0) and “Not Applicable” will not be included in the analysis. Indicated by historical data from [REDACTED], the correlation between measurements from different periods within the same subject was about 0.45 and the proportion of subjects with an “Excellent” response was about 0.55 and 0.45 for the Test and Control lenses, respectively. Assumptions for correlation and proportions were made based on these observations and a total of 2000 replicating trials were simulated. The simulated binary data were analyzed using a generalized linear mixed model with a logit link function and tested for statistical superiority. Sample size was estimated for a minimum statistical power of 80%.

Overall preference while using computer screens & digital devices

Responses to overall preference while using computer screens & digital devices will be collapsed into three categories for the purpose of analysis (Prefer Test, No Preference, and Prefer Control). Indicated by historical data from [REDACTED], the percentage of subjects preferring Test lens was assumed to be 0.4, the percentage of subjects preferring Control lens was assumed to be 0.2, the percentage of subjects with no preference was assumed to be 0.4. A total of 2000 replicating trials were simulated. The simulated multinomial data were analyzed using a generalized linear regression model with a generalized logit link function and tested for statistical superiority (preference ratio of preferring Test to Control). Sample size was estimated for a minimum statistical power of 80%.

Table 10: Sample Size Estimates

Endpoint		Hypothesis	Sample size	Power
Primary	CLUE Vision	Non-inferiority	100	91.3%
Secondary	CLUE Handling	Non-inferiority	160	90.5%
	CLUE Comfort	Non-inferiority	200	81.4%
Exploratory	Clarity of vision indoors in bright light	Superiority	200	79.2%
	Overall preference while using computer screens & digital devices	Superiority	150	81.2%

As indicated in Table 12 above, the sample size chosen for this study was primarily driven by the secondary endpoint of CLUE overall comfort in order to achieve a statistical power of at

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

least 80% for the primary and secondary endpoints. The plan is to enroll approximately 230 eligible subjects with a target of 200 to complete the study. During the enrollment period, the subject dropout rate will be closely monitored, if an unexpectedly high dropout rate is observed, then the targeted total enrollment number may be increased accordingly to ensure that a minimum of 200 subjects complete the study. With 200 subjects to complete this study was also powered (a statistical power of approximately 80% or above) to demonstrate superiority of the Test lens compared to the Control lens with respect to clarity of vision in doors in bright light (proportion of subjects with “Excellent” response) and overall preference while using computer screens & digital devices at the 2-week follow-up evaluation.

14.3. Analysis Populations

Safety Population:

All subjects who were administered any test article excluding subjects who drop out prior to administering any test article. At least one observation should be recorded.

Per-Protocol Population:

All subjects who have successfully completed all visits and did not substantially deviate from the protocol as determined by the trial cohort review committee prior to database hard lock (Per-Protocol Population). Justification of excluding subjects with protocol deviations in the Per-Protocol Population set will be documented in a memo to file.

Intent-to-Treat (ITT) Population:

All randomized subjects regardless of actual treatment and subsequent withdrawal from study or deviation from protocol. At least one observation should be recorded.

14.4. Level of Statistical Significance

All planned analysis for this study will be conducted with a two-sided type I error rate of 5%. The primary and secondary hypotheses will be tested with a type I error of 5% individually. All primary and secondary hypotheses need to be met in order to analyze other exploratory hypotheses and each exploratory hypothesis will be tested individually at the two-sided type I error rate of 5%.

14.5. Primary Analysis

The primary endpoint is CLUE overall quality of vision. Non-inferiority of Test compared to Control with respect to CLUE vision will be assessed on the Per-protocol population (PP).

CLUE Overall Quality of Vision

CLUE vision scores will be analyzed using a linear mixed model to compare the Test and Control lenses at the 2-week follow-up evaluation. The model will include baseline CLUE vision scores, lens type, lens sequence, and period as fixed effects and site as a random effect (G-side). Other subject characteristics such as age, gender, race, iris category, and subject group based on habitual lens wear (habitual daily disposable and habitual daily wear reusable)

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

will be included as fixed covariates when appropriate. The covariance of residuals between measurement from different periods within the same subject (R-side) will be modeled using Unstructured (UN) covariance structure. If the model does not converge, then other covariance structures, such as compound Symmetry (CS) covariance structure, will be considered. Heterogeneous residuals covariance structures across habitual lens groups will be considered when appropriate. A log-likelihood ratio test will be used to test for the homogeneity between the residual covariance structures. The Kenward and Roger method (Kenward & Roger, 1997)¹⁷ will be used for the denominator degree of freedom.

Hypothesis Testing

The null and alternative hypotheses for testing non-inferiority of the Test lens relative to the Control lens with respect to CLUE vision scores are as follows:

$$\begin{aligned} H_0: \mu_T - \mu_C &\leq -5 \\ H_A: \mu_T - \mu_C &> -5 \end{aligned}$$

Where, μ_T represents the mean CLUE vision score for the Test lens and μ_C represents the mean CLUE vision score for the Control lens. Non-inferiority will be declared if the lower bound of the 2-sided 95% confidence interval of the difference (Test – Control) is greater than -5. If non-inferiority of the Test lens over Control lens is met, then superiority will be assessed on the ITT population. If the lower bound is greater than 0, then superiority of the Test lens over the Control lens will be established.

14.6. Secondary Analysis

The secondary endpoints include CLUE overall comfort and CLUE overall handling. The non-inferiority analysis on CLUE comfort and handling will be conducted on the PP population.

CLUE Overall Comfort

CLUE overall comfort scores will be analyzed using the same model as the primary endpoint of CLUE vision and tested in the same manner.

CLUE Overall Handling

CLUE overall handling scores will be analyzed using the same model as the primary endpoint of CLUE vision and tested in the same manner.

14.7. Other Exploratory Analysis

The following other exploratory endpoints will be assessed in support of primary and secondary endpoints and will be conducted on the ITT population. Exploratory hypotheses will be assessed only when all primary and secondary hypotheses are met.

Clarity of Vision Indoors in Bright Light

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

To test superiority of the Test lens compared to the Control with respect to the proportion of subjects with “Excellent” response to the statement “clarity of vision indoors in bright light”, responses will be converted into a binary variable for the purpose of analysis (Excellent = 1 and others = 0) and “Not applicable” response will not be considered in the analysis. The dichotomized item responses will be analyzed using a generalized linear mixed model with a binomial distribution and the logit as the link function. The model will include lens type, sequence, and period as fixed effects and site as a random effect (G-side). Other subject characteristics such as age, gender, race, subject group based on habitual lens wear, and iris category will be included as fixed covariates when appropriate. The covariance of residuals between measurements from different periods within the same subject (R-side) will be modeled using Unstructured (UN) covariance structure. If the model does not converge, then other covariance structures, such as compound Symmetry (CS) covariance structure, will be considered. Heterogeneous residuals covariance structures across habitual lens groups will be considered when appropriate. A log-likelihood ratio test will be used to test for the homogeneity between the residual covariance structures.

Hypothesis Testing

The null and alternative hypotheses for testing superiority of the Test lens relative to the Control lens with respect to clarity of vision indoors at bright light are as follows:

$$H_0: OR \leq 1.0$$
$$H_A: OR > 1.0$$

Where OR represents the odds ratio of having “Excellent” rating for the Test lens compared to the Control at the 2-week follow-up. Superiority will be declared if the lower bound of the 2-sided 95% confidence interval is above 1.0.

Individual CLUE or MRD questions:

- 1) Clarity of distance vision (i.e. looking at things that are more than 5 feet away, such as street signs). (P3_0006_p10)
- 2) Clarity of vision in bright sunlight. (MIS00612)
- 3) Ability to see comfortably while driving at night (MIS01980)
- 4) Ability to see comfortably while driving during the day (MIS01981)
- 5) Clarity of vision indoors in bright light. (MIS00623)
- 6) Reduction in the feeling of tired eyes from using a computer or other digital device. (MIS02001)
- 7) Ability to see comfortably while using a computer or other digital device. (MIS01982)
- 8) My vision was clear enough to allow me to drive at night (V056_1)
- 9) With these lenses, I felt very confident to drive at night (V086_2)
- 10) Clarity of vision indoors in dim light (MIS00624)

All individual CLUE and MRD items are assessed using 5-point Likert scales. “Not applicable” responses will not be considered in the analysis. Item responses will be reverse coded as needed so that higher values indicate more positive/favorable ratings for study lenses.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

To compare the proportion of subjects with higher ratings for the Test lens to the proportion of subjects with higher ratings for the Control lens, the outcome variable will be derived by comparing the within-subject ratings for Test and Control: (1) if the rating of the Test is higher than the rating of the Control ($\text{Test} - \text{Control} > 0$), then the derived nominal outcome variable will be “Higher rating for Test”; (2) if the rating of the Control is higher than the rating of the Test ($\text{Test} - \text{Control} < 0$), then the derived outcome will be “Higher rating for Control”; and (3) if ratings for Test and Control are the same ($\text{Test} - \text{Control} = 0$), then the derived outcome will be “Same Rating”. The derived outcome will be analyzed using a generalized linear mixed model with a multinomial distribution and the generalized logit as the link function. The analysis model will include lens sequence as a fixed effect and site as a random effect (G-sided). Other subject characteristics such as gender, race, subject group based on habitual lens wear, and iris category will be included as fixed covariates when appropriate.

Hypothesis Testing

The null and alternative hypotheses for testing superiority of the Test lens relative to the Control lens with respect to the proportion of subjects with higher ratings are as follows:

$$H_0: PR \leq 1.0$$
$$H_A: PR > 1.0$$

Where PR represents the proportion ratio of higher rating for Test to higher rating for Control at the 2-week follow-up evaluation. Superiority will be declared if the lower bound of the 2-sided 95% confidence interval is above 1.0.

Preference Questions:

- 1) Overall opinion (PREf6_1_1)
- 2) Overall comfort (PREf6_2_1)
- 3) Overall vision (PREf6_3_1)
- 4) Comfort throughout the day (PREf6_5_1)
- 5) Comfort at the end of the day (PREf6_6_1)
- 6) Comfort from activity to activity (PREf6_7_1)
- 7) Clarity of vision from activity to activity (PREf6_8_1)
- 8) Overall preference while using computer screens & digital devices (PREf6_4_1)

Responses to preference items will be collapsed into three categories for the purpose of analysis (Prefer Test, No Preference, and Prefer Control). The collapsed item responses will be analyzed using a generalized linear mixed model with a multinomial distribution and the generalized logit as the link function. The analysis model will include lens sequence as a fixed effect and site as a random effect (G-sided). Other subject characteristics such as gender, race, subject group based on habitual lens wear, and iris category will be included as fixed covariates when appropriate.

Hypothesis Testing

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

The null and alternative hypotheses for testing superiority of the Test lens relative to the Control lens with respect to subjective preference are as follows:

$$H_0: PR \leq 1.0$$
$$H_A: PR > 1.0$$

Where PR represents the preference ratio of preferring the Test lens to preferring the Control lens (proportion of subjects preferring Test to proportion of subjects preferring Control) at the 2-week follow-up. Superiority will be declared if the lower bound of the 2-sided 95% confidence interval is above 1.0.

Study lens preferences to habitual lens, study lens purchase intent, acceptable lens fit rates, surface characteristics, biomicroscopy findings, and other characteristics of both study lenses will be descriptively summarized with tables and/or graphs. Post-hoc analyses may be conducted at the discretion of the study responsible clinician.

14.8. Interim Analysis

An interim analysis will be conducted after 50% of the subjects (about 100 subjects) complete 2-week follow-up evaluation in the second study period. The interim analysis will consist of descriptive summaries for questionnaire data. The results will be reviewed with historical data with Test lenses from the pilot line before the design validation study is initiated. The results will be communicated to the project team.

14.9. Procedure for Handling Missing Data and Drop-Outs

Subject dropout is expected to be one of the main reasons of missing data in this clinical trial. Past clinical trials don't provide the evidence that subject dropout is systematic or not-at-random. To evaluate the impact of missing data, sensitivity analysis will be conducted using multiple imputation methods if the proportion of subject dropout is greater than the 15%. The SAS/STAT procedures PROC MI and PROC MIANALYZE will be utilized with a parametric regression method used to make at least 20 imputations.

14.10. Procedure for Reporting Deviations from Statistical Plan

The analysis will be conducted according to that specified in above sections. There are no known reasons for which it is planned to deviate from these analysis methods. If for any reason a change is made, the change will be documented in the study report along with a justification for the change.

15. DATA HANDLING AND RECORD KEEPING/ARCHIVING

15.1. Electronic Case Report Form/Data Collection

The data for this study will be captured on electronic case report forms (eCRFs) using the Bioclinica EDC system. An authorized data originator will enter study data into the eCRFs

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

using the EDC system. Data collected on equipment that is not captured in EDC will be formatted to the specification of the JJVC database manager and sent to JJVC for analysis.

External data sources for this study include: Not Applicable

The clinical data will be recorded on dedicated eCRFs specifically designed to match the study procedures for each visit. Only specifically delegated staff can enter data on a CRF. Once completed, the eCRFs will be reviewed for accuracy and completeness and signed by the Investigator. The sponsor or sponsor's representatives will be authorized to gain access to the subject recordation for the purposes of monitoring and auditing the study.

Edit checks, electronic queries, and audit trails are built into the system to ensure accurate and complete data collection. Data will be transmitted from the clinical site to a secure central database as forms are completed or updated, ensuring information accuracy, security, and confidentiality. After the final database lock, the Investigator will be provided with Individual Patient Profiles (IPP) including the full audit trail on electronic media in PDF format for all of the study data. The IPP must be retained in the study files as a certified copy of the source data for the study.

The content and structure of the eCRFs are compliant with ISO14155:2011.¹

15.2. Subject Record

At a minimum, subject record should be available for the following:

- subject identification
- eligibility
- study identification
- study discussion
- provision of and date of informed consent
- visit dates
- results of safety and efficacy parameters as required by the protocol
- a record of all adverse events
- follow-up of adverse events
- medical history and concomitant medication
- test article receipt/dispensing/return records
- date of study completion
- reason for early discontinuation of test article or withdrawal from the study, if applicable

The subject record is the eCRF or an external record. The author of an entry in the subject record must be identifiable. The first point of entry is considered to be the source record.

Adverse event notes must be reviewed and initialed by the Investigator.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

15.3. Trial Registration on ClinicalTrials.gov

This study will be registered on ClinicalTrials.gov by the Sponsor.

16. DATA MANAGEMENT

16.1. Access to Source Data/Document

The Investigator/Institution will permit trial-related monitoring, audits, IEC/IRB review and regulatory inspection(s) by providing direct access to source data/documents. Should the clinical site be contacted for an audit by an IEC/IRB or regulatory authority, JJVC must be contacted and notified in writing within 24 hours.

16.2. Confidentiality of Information

Information concerning the investigational product and patent application processes, scientific data or other pertinent information is confidential and remains the property of JJVC. The Investigator may use this information for the purposes of the study only. It is understood by the Investigator that JJVC will use information developed in this clinical study in connection with the development of the investigational product and therefore may disclose it as required to other clinical investigators and to regulatory agencies. In order to allow the use of the information derived from this clinical study, the Investigator understands that he/she has an obligation to provide complete test results and all data developed during this study to the Sponsor.

16.3. Data Quality Assurance

Steps will be taken to ensure the accuracy and reliability of data, include the selection of qualified investigators and appropriate clinical sites and review of protocol procedures with the Principal Investigator. The Principal Investigator, in turn, must ensure that all Sub-Investigators and clinical site personnel are familiar with the protocol and all study-specific procedures and have appropriate knowledge of the study article.

Training on case report form completion will be provided to clinical site personnel before the start of the study. The Sponsor will review case report forms for accuracy and completeness remotely during the conduct of the study, during monitoring visits, and after transmission to data management. Any data discrepancies will be resolved with the Investigator or designee, as appropriate.

Quality Assurance representatives from JJVC may visit clinical sites to review data produced during the study and to access compliance with applicable regulations pertaining to the conduct of clinical trials. The clinical sites will provide direct access to study-related source data/documents and reports for the purpose of monitoring and auditing by JJVC and for inspection by local and regulatory authorities.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

16.4. Data Monitoring Committee (DMC)

Not Applicable

17. CLINICAL MONITORING

The study monitors will maintain close contact with the Principal Investigator and the Investigator's designated clinical site personnel. The monitor's responsibilities will include:

- Ensuring that the investigation is being conducted according to the protocol, any subsequent versions, and regulatory requirements are maintained.
- Ensuring the rights and wellbeing of subjects are protected.
- Ensuring adequate resources, including facilities, laboratories, equipment, and qualified clinical site personnel.
- Ensuring that protocol deviations are documented with corrective action plans, as applicable.
- Ensuring that the clinical site has sufficient test article and supplies.
- Clarifying questions regarding the study.
- Resolving study issues or problems that may arise.
- Reviewing of study records and source documentation verification in accordance with the monitoring plan.

18. ETHICAL AND REGULATORY ASPECTS

18.1. Study-Specific Design Considerations

Potential subjects will be fully informed of the risks and requirements of the study and, during the study, subjects will be given any new information that may affect their decision to continue participation. Subjects will be told that their consent to participate in the study is voluntary and may be withdrawn at any time with no reason given and without penalty or loss of benefits to which they would otherwise be entitled. Only subjects who are fully able to understand the risks, benefits, and potential adverse events of the study, and provide their consent voluntarily will be enrolled.

18.2. Investigator Responsibility

The Principal Investigator is responsible for ensuring that the clinical study is performed in accordance with the signed agreement, the investigational plan, section 4 of the ICH E6(R2) guidelines on Good Clinical Practice (GCP),² and applicable regulatory requirements. GCP is an international ethical and scientific quality standard for designing, conducting, recording, and reporting studies that involve the participation of human subjects. Compliance with this standard provides public assurance that the rights, safety, and well-being of study subjects are protected, consistent with the principles of the Declaration of Helsinki 64th WMA General Assembly 2013³ and that the clinical study data are credible. The Investigator must maintain

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

clinical study files in accordance with section 8 of the ICH E6(R2) guidelines on Good Clinical Practice (GCP),² and applicable regulatory requirements.

18.3. Independent Ethics Committee or Institutional Review Board (IEC/IRB)

Before the start of the study, the Investigator (or Sponsor when applicable) will provide the IEC/IRB with current and complete copies of the following documents (where applicable):

- Final protocol.
- Sponsor-approved informed consent form (and any other written materials to be provided to the subjects)
- Investigator's Brochure (or equivalent information).
- Sponsor-approved subject recruitment materials.
- Information on compensation for study-related injuries or payment to subjects for participation in the study.
- Investigator's curriculum vitae, clinical licenses, or equivalent information (unless not required, as documented by IEC/IRB).
- Information regarding funding, name of the Sponsor, institutional affiliations, other potential conflicts of interest, and incentives for subjects.
- Any other documents that the IEC/IRB requests to fulfill its obligation.

This study will be undertaken only after IEC/IRB has given full approval of the final protocol, the informed consent form, applicable recruiting materials, and subject compensation programs, and the Sponsor has received a copy of this approval. This approval letter must be dated and must clearly identify the documents being approved.

During the study, the Investigator (or Sponsor when applicable) will send the following documents to the IEC/IRB for their review and approval, where appropriate:

- Protocol revisions
- Revision(s) to informed consent form and any other written materials to be provided to subjects
- If applicable, new or revised subject recruitment materials approved by the Sponsor
- Revisions to compensation for study-related injuries or payment to subjects for participation in the study
- Investigator's Brochure revisions
- Summaries of the status of the study (at least annually or at intervals stipulated in guidelines of the IEC/IRB)
- Reports of adverse events that are serious, unanticipated, and associated with the test articles, according to the IRB's requirements
- New information that may adversely affect the safety of the subjects or the conduct of the study
- Major protocol deviations as required by the IEC/IRB
- Report of deaths of subjects under the Investigator's care

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

- Notification if a new Investigator is responsible for the study at the clinical site
- Any other requirements of the IEC/IRB

For protocol revisions that increase subject risk, the revisions and applicable informed consent form revisions must be submitted promptly to the IEC/IRB for review and approval before implementation of the change(s).

At least once a year, the IEC/IRB will review and reapprove this clinical study. This request should be documented in writing.

At the end of the study, the Investigator (or Sponsor where required) will notify the IEC/IRB about the study completion. Documentation of this notification must be retained at the clinical site and a copy provided to the CRO or Sponsor as applicable.

18.4. Informed Consent

Each subject or their representative, must give written consent according to local requirements after the nature of the study has been fully explained. The consent form must be signed before performance of any study-related activity. The consent form that is used must be approved by both the Sponsor and by the reviewing IEC/IRB. The informed consent is in accordance with principles that originated in the Declaration of Helsinki,³ current ICH GCP² and ISO 14155¹ guidelines, applicable regulatory requirements, and Sponsor Policy.

Before entry into the study, the Investigator or an authorized member of the clinical site personnel must explain to potential subject the aims, methods, reasonably anticipated benefits, and potential hazards of the study, and any discomfort it may entail. Subjects will be informed that their participation is voluntary and that they may withdraw consent to participate at any time.

The subject will be given sufficient time to read the informed consent form and the opportunity to ask questions. After this explanation and before entry into the study, consent should be appropriately recorded by means of the subject's dated signature. After having obtained the consent, a copy of the informed consent form must be given to the subject.

18.5. Privacy of Personal Data

The collection, processing and disclosure of personal data and medical information related to the Study Subject, and personal data related to Principal Investigator and any clinical site personnel (e.g., name, clinic address and phone number, curriculum vitae) is subject to compliance with the Health Information Portability and Accountability Act (HIPAA) in the United States¹⁸ and other applicable personal data protection and security laws and regulations. Appropriate measures will be employed to safeguard these data, to maintain the confidentiality of the person's related health and medical information, to properly inform the concerned persons about the collection and processing of their personal data, to grant them reasonable access to their personal data and to prevent access by unauthorized persons.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

All information obtained during the course of the investigation will be regarded as confidential. All personal data gathered in this trial will be treated in strictest confidence by Investigators, monitors, Sponsor's personnel and IEC/IRB. No data will be disclosed to any third party without the express permission of the subject concerned, with the exception of Sponsor personnel (monitor, auditor), IEC/IRB and regulatory organizations in the context of their investigation related activities that, as part of the investigation will have access to the CRFs and subject records.

The collection and processing of personal data from subjects enrolled in this study will be limited to those data that are necessary to investigate the efficacy, safety, quality, and utility of the investigational product(s) used in this study.

These data must be collected and processed with adequate precautions to ensure confidentiality and compliance with applicable data privacy protection laws and regulations.

The Sponsor ensures that the personal data will be:

- processed fairly and lawfully.
- collected for specified, explicit, and legitimate purposes and not further processed in a way incompatible with these purposes.
- adequate, relevant, and not excessive in relation to said purposes.
- accurate and, where necessary, kept current.

Explicit consent for the processing of personal data will be obtained from the participating subject before collection of data. Such consent should also address the transfer of the data to other entities and to other countries.

The subject has the right to request through the Investigator access to his personal data and the right to request rectification of any data that are not correct or complete. Reasonable steps should be taken to respond to such a request, taking into consideration the nature of the request, the conditions of the study, and the applicable laws and regulations.

Appropriate technical and organizational measures to protect the personal data against unauthorized disclosures or access, accidental or unlawful destruction, or accidental loss or alteration must be put in place. Sponsor personnel whose responsibilities require access to personal data agree to keep the identity of study subjects confidential.

19. STUDY RECORD RETENTION

In compliance with the ICH GCP guidelines,² the Investigator/Institution will maintain all CRFs and all subject records that support the data collected from each subject, as well as all study documents as specified in ICH GCP² and all study documents as specified by the applicable regulatory requirement(s). The Investigator/Institution will take measures to prevent accidental or premature destruction of these documents.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

Essential documents must be retained until at least two (2) years after the last approval of a marketing application in an ICH region and until there are no pending or contemplated marketing applications in an ICH region or until at least two (2) years have elapsed since the formal discontinuation of clinical development of the investigational product. These documents will be retained for a longer period if required by the applicable regulatory requirements or instructed by the Sponsor. It is the responsibility of the Sponsor to inform the Investigator/Institution as to when these documents no longer need to be retained.

If the responsible Investigator retires, relocates, or for other reasons withdraws from the responsibility of keeping the study records, custody must be transferred to a person who will accept the responsibility. The Sponsor must be notified in writing of the name and address of the new custodian. Under no circumstance shall the Investigator relocate or dispose of any study documents before having obtained written approval from the Sponsor.

If it becomes necessary for the Sponsor or the appropriate regulatory authority to review any documentation relating to this study, the Investigator must permit access to such reports.

If the Investigator has a question regarding retention of study records, he/she should contact JJVC.

20. FINANCIAL CONSIDERATIONS

Remuneration for study services and expenses will be set forth in detail in the Clinical Research Agreement. The Research Agreement will be signed by the Principal Investigator and a JJVC management representative prior to study initiation.

JJVC reserves the right to withhold remuneration for costs associated with protocol violations such as:

- Continuing an ineligible subject in the study.
- Scheduling a study visit outside the subject's acceptable visit range.

JJVC reserves the right to withhold final remuneration until all study related activities have been completed, such as:

- Query resolution.
- Case Report Form signature.
- Completion of any follow-up action items.

21. PUBLICATION

This is a multicenter study. The participating institution and Principal Investigators for this study agree that, should this study results be published, the first publication of the results of this study shall be made in conjunction with the presentation of a joint, multicenter publication

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

of the study results with the investigators and the institutions from all appropriate sites contributing data, analyses and comments.

22. REFERENCES

1. ISO 14155:2011: Clinical Investigation of Medical Devices for Human Subjects — Good Clinical Practice. Available at <https://www.iso.org/standard/45557.html>
2. International Conference on Harmonization Good Clinical Practice E6 (ICH-GCP). Available at <http://www.ich.org/products/guidelines/efficacy/article/efficacy-guidelines.html>
3. Declaration of Helsinki - Ethical principles for Medical Research Involving Human Subjects. Available at <https://www.wma.net/policies-post/wma-declaration-of-helsinki-ethical-principles-for-medical-research-involving-human-subjects/>
4. United States (US) Code of Federal Regulations (CFR). . Available at <https://www.gpo.gov/fdsys/browse/collectionCfr.action?collectionCode=CFR>
5. Gallas J, Eisner M. Eye protection from sunlight damage. *Comprehensive Series in Photosciences*. 2001;3:427-455.
6. Kim H, Kim HS, Jung CH, Yoon I. Monitor Calibration Approach to Reducing High Energy Visible Light from White Light-Emitting Diode. *Science & Engineering Research Support Society*. 2015;87:151-154.
7. Rai V, Dayan N, B. M-K. A Comparative eEvaluation of Photo-toxic Effect of Fractionated Melanin and Chlorpromazine Hydrochloride on Human (Dermal Fibroblasts and Epidermal Keratinocytes) and Mouse Cell Line/s (fibroblast Balb/c 3T3). *Toxicology in Vitro*. 2016;25(2):538-544.
8. Smick K. *Blue Light Hazard: New Knowledge, New Approaches to Maintaining Ocular Health*. Report of a roundtable sponsored by Essilor of America;2013.
9. Panda S. Illumination of the Melanopsis Signaling Pathway. *Science & Engineering Research Support Society*. 2005;307(5709):600-604.
10. Buch J. *Investigator Brochure* [REDACTED] (VIS-CSIB-006348) *Evaluation of Prototype Lenses with Experimental UV/HEV Blocker*. December 03, 2019
11. Wirth RJ, Edwards MC, Henderson M, Henderson T, Olivares G, Houts CR. Development of the Contact Lens User Experience: CLUE Scales. *Optometry and vision science : official publication of the American Academy of Optometry*. 2016;93(8):801-808.
12. SAS Institute Inc. *2016 SAS/STAT® 14.3 User's Guide*. Cary, NC: SAS Institute Inc.
13. (NCT02402127) *Lubricity Post Wear – Competitive Lens Pilot*. 2016
14. Buch J. *Clinical Study Report* [REDACTED] (VIS-CSRP-006381) *Evaluation of Prototype Lenses with Experimental UV/HEV Blocker*. February 08, 2021


Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.


15. Stroup W. *Generalized Mixed Models: Modern Concepts, Methods and Applications*. Boca Raton CRC Press; 2013
16. Stroup WW. *Mixed model procedures to assess power, precision, and sample sizes*. . Alexandria, VA.: American Statistical Association; 1999.
17. Kenward MG, Roger JH. Small Sample Inference for Fixed Effects from Restricted Maximum Likelihood. *Biometrics*. 1997;53(3):983–997.
18. Health Information Portability and Accountability Act (HIPAA). Available at: <https://www.hhs.gov/hipaa/for-professionals/privacy/index.html>.

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**


APPENDIX A: PATIENT REPORTED OUTCOMES (STUDY QUESTIONNAIRES)

































**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

APPENDIX B: PATIENT INSTRUCTION GUIDE

The Patient Instruction Guide (PIG) will be provided separately.

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

APPENDIX C: PACKAGE INSERT (APPROVED PRODUCT)

ACUVUE® OASYS 1-Day with HydraLuxe™

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

**IMPORTANT: Please read carefully and keep this
information for future use.**

This Package Insert and Fitting Guide is intended for the
Eye Care Professional, but should be made available to
patients upon request.

The Eye Care Professional should provide the patient
with the appropriate instructions that pertain to the
patient's prescribed lenses. Copies are available for
download at www.acuvue.com.



ACUVUE OASYS® Brand Contact Lenses 1-Day
with HydraLuxe™ Technology

ACUVUE OASYS® Brand Contact Lenses 1-Day
with HydraLuxe™ Technology for ASTIGMATISM

senofilcon A Soft (hydrophilic) Contact Lenses
Visibility Tinted with UV Blocker
for Daily Disposable Wear



CAUTION: U.S. Federal law restricts this device to
sale by or on the order of a licensed practitioner.

~~CONFIDENTIAL~~

Page 98 of 191

SYMBOLS KEY

The following symbols may appear on the label or carton:

SYMBOL	DEFINITION
	Consult Instructions for Use
	Manufactured by or in
	Date of Manufacture
	Use By Date (expiration date)
	Batch Code
	Sterile Using Steam or Dry Heat
	Single-Use
DIA	Diameter
BC	Base Curve
D	Diopter (lens power)
CYL	Cylinder
AXIS	Axis
	Quality System Certification Symbol
	UV-Blocking
	Fee Paid for Waste Management
	CAUTION: U.S. Federal law restricts this device to sale by or on the order of a licensed practitioner
	Lens Orientation Correct
	Lens Orientation Incorrect (Lens Inside Out)

DESCRIPTION

ACUVUE OASYS® Brand Contact Lenses 1-Day and ACUVUE OASYS® Brand Contact Lenses 1-Day for ASTIGMATISM are soft (hydrophilic) contact lenses made with HydraLuxe™ Technology. They are available as spherical or toric lenses respectively.

These lenses are made of a silicone hydrogel material containing an internal wetting agent, visibility tint, and UV absorbing monomer and are tinted blue using Reactive Blue Dye #4 to make the lenses more visible for handling.

A benzotriazole UV absorbing monomer is used to block UV radiation. The transmittance characteristics for these lenses are less than 1% in the UVB range of 280 nm to 315 nm and less than 10% in the UVA range of 316 nm to 380 nm for the entire power range.

Lens Properties:

The physical/optical properties of the lens are:

• Specific Gravity (calculated):	0.98 - 1.12
• Refractive Index:	1.42
• Light Transmission:	85% minimum
• Surface Character:	Hydrophilic
• Water Content:	38%
• Oxygen Permeability:	

VALUE

122×10^{-11} (cm²/sec)
(ml O₂/ml x mm Hg) at 35°C

103×10^{-11} (cm²/sec)
(ml O₂/ml x mm Hg) at 35°C

METHOD

Fatt (boundary corrected, non-edge corrected)

Fatt (boundary corrected, edge corrected)

Lens Parameters:

• Diameter Range:	12.0 mm to 15.0 mm
• Center Thickness:	varies with power
• Base Curve Range:	7.85 mm to 10.00 mm
• Spherical Power Range:	-20.00D to +20.00D
• Cylinder Power Range:	-0.25D to -10.00D
• Axis Range:	2.5° to 180°

AVAILABLE LENS PARAMETERS

ACUVUE OASYS® Brand 1-Day with HydraLuxe™ Technology are hemispherical shells of the following dimensions:

Diameter:

14.3 mm

Center Thickness:

0.085 mm to 0.221 mm (varies with power)

Base Curve:

8.5 mm, 9.0 mm

Powers:

-0.50D to -6.00D (in 0.25D increments)

-6.50D to -12.00D (in 0.50D increments)

+0.50D to +6.00D (in 0.25D increments)

+6.50D to +8.00D (in 0.50D increments)

ACUVUE OASYS® Brand 1-Day with HydraLuxe™ Technology for ASTIGMATISM are hemitoric shells of the following dimensions:

Diameter:

14.3 mm

Center Thickness:

0.075 mm to 0.172 mm (varies with power)

Base Curve:

8.5 mm

Powers:

+0.00D to -6.00D (in 0.25D increments)

Cylinders: -0.75D, -1.25D, -1.75D, -2.25D*

Axis: 10° to 180° in 10° increments

*-2.25D cylinder is available in 10°, 20°, 70°, 80°, 90°, 100°, 110°, 160°, 170°, 180° axes only.

+0.25D to +4.00D (in 0.25D increments)


-6.50D to -9.00D (in 0.50D increments)

Cylinders: -0.75D, -1.25D, -1.75D

Axis: 10°, 20°, 70°, 80°, 90°, 100°, 110°, 160°, 170°, 180°

TRANSMITTANCE CURVES

ACUVUE OASYS® 1-Day with HydraLuxe™ Technology (senofilcon A) Visibility Tinted with UV Blocker vs. 24 yr. old human cornea and 25 yr. old human crystalline lens.

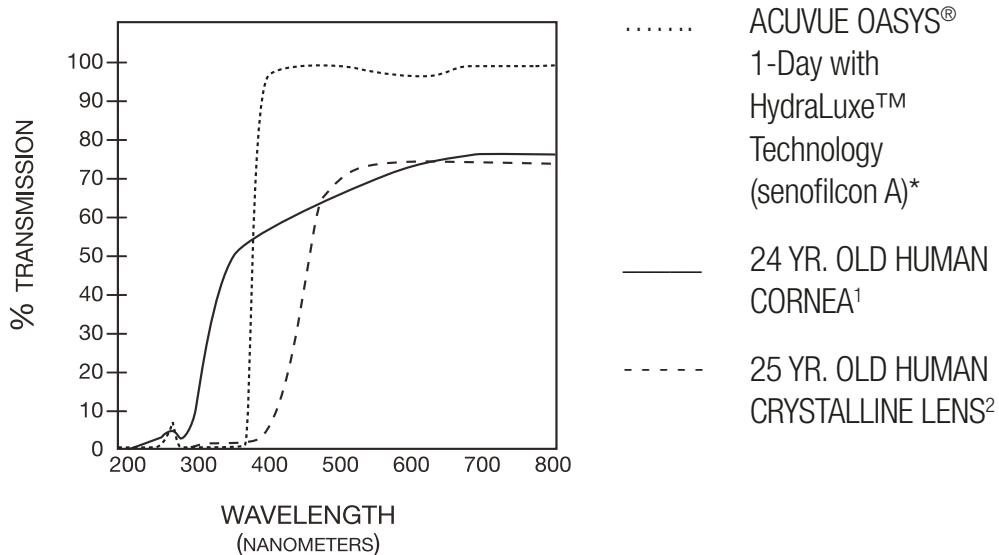

* The data was obtained from measurements taken through the central 3-5 mm portion for the thinnest marketed lens (-9.00D lens, 0.075 mm center thickness).

¹Lerman, S., Radiant Energy and the Eye, MacMillan, New York, 1980, p. 58, figure 2-21

²Waxler, M., Hitchins, V.M., Optical Radiation and Visual Health, CRC Press, Boca Raton, Florida, 1986, p. 19, figure 5

WARNING: UV absorbing contact lenses are NOT substitutes for protective UV absorbing eyewear, such as UV absorbing goggles or sunglasses because they do not completely cover the eye and surrounding area. The patient should continue to use UV absorbing eyewear as directed.

ACTIONS

In its hydrated state, the contact lens, when placed on the cornea, acts as a refracting medium to focus light rays onto the retina.

The transmittance characteristics for these lenses are less than 1% in the UVB range of 280 nm to 315 nm and less than 10% in the UVA range of 316 nm to 380 nm for the entire power range.

NOTE: Long-term exposure to UV radiation is one of the risk factors associated with cataracts. Exposure is based on a number of factors such as environmental conditions (altitude, geography, cloud cover) and personal factors (extent and nature of outdoor activities). UV-Blocking contact lenses help provide protection against harmful UV radiation. However, clinical studies have not been done to demonstrate that wearing UV-Blocking contact lenses reduces the risk of developing cataracts or other eye disorders. The Eye Care Professional should be consulted for more information.

INDICATIONS (USES)

ACUVUE OASYS® Brand Contact Lenses 1-Day with HydraLuxe™ Technology are indicated for daily disposable wear for the optical correction of refractive ametropia (myopia and hyperopia) in phakic or aphakic persons with non-diseased eyes who may have 1.00D or less of astigmatism.

ACUVUE OASYS® Brand Contact Lenses 1-Day with HydraLuxe™ Technology for ASTIGMATISM are indicated for daily disposable wear for the optical correction of refractive ametropia (myopia and hyperopia) in phakic or aphakic persons with non-diseased eyes who may have 0.50D to 3.00D of astigmatism.

These lenses contain a UV Blocker to help protect against transmission of harmful UV radiation to the cornea and into the eye.

CONTRAINDICATIONS (REASONS NOT TO USE)

DO NOT USE these contact lenses when any of the following conditions exist:

- Acute or subacute inflammation or infection of the anterior chamber of the eye.
- Any eye disease, injury or abnormality that affects the cornea, conjunctiva, or eyelids.
- Severe insufficiency of lacrimal secretion (dry eye).

- Corneal hypoesthesia (reduced corneal sensitivity).
- Any systemic disease that may affect the eye or be exaggerated by wearing contact lenses.
- Allergic reactions of ocular surfaces or adnexa that may be induced or exaggerated by wearing contact lenses or use of contact lens solutions.
- Ocular irritation due to allergic reactions which may be caused by use of contact lens solutions (i.e., rewetting drops) that contain chemicals or preservatives (such as mercury, Thimerosal, etc.) to which some people may develop an allergic response.
- Any active corneal infection (bacterial, fungal, protozoal, or viral).
- If eyes become red or irritated.

WARNINGS

Patients should be advised of the following warnings pertaining to contact lens wear:

EYE PROBLEMS, INCLUDING CORNEAL ULCERS, CAN DEVELOP RAPIDLY AND LEAD TO LOSS OF VISION; IF THE PATIENT EXPERIENCES:

- **Eye Discomfort,**
- **Excessive Tearing,**
- **Vision Changes,**
- **Loss of Vision,**
- **Eye Redness,**
- **Or Other Eye Problems,**

THE PATIENT SHOULD BE INSTRUCTED TO IMMEDIATELY REMOVE THE LENSES AND PROMPTLY CONTACT THE EYE CARE PROFESSIONAL.

- When prescribed for daily wear, patients should be instructed not to wear lenses while sleeping. Clinical studies have shown that the risk of serious adverse reactions is increased when lenses are worn overnight, and that the risk of ulcerative keratitis is greater for

extended wear contact lens users than for daily wear users.³

- Studies have shown that contact lens wearers who are smokers have a higher incidence of adverse reactions than nonsmokers.
- Problems with contact lenses or lens care products could result in serious injury to the eye. Patients should be cautioned that proper use and care of contact lenses and lens care products are essential for the safe use of these products.
- The overall risk of ulcerative keratitis may be reduced by carefully following directions for lens care.

³ New England Journal of Medicine, September 21, 1989; 321 (12), pp. 773-783

Specific Instructions for Use and Warnings:

- **Water Activity**

Instructions for Use

Do not expose contact lenses to water while wearing them.

WARNING:

Water can harbor microorganisms that can lead to severe infection, vision loss or blindness. If lenses have been submersed in water when participating in water sports or swimming in pools, hot tubs, lakes, or oceans, the patient should be instructed to discard them and replace them with a new pair. The Eye Care Professional should be consulted for recommendations regarding wearing lenses during any activity involving water.

PRECAUTIONS

Special Precautions for Eye Care Professionals:

- Due to the small number of patients enrolled in clinical investigation of lenses, all refractive powers, design configurations, or lens parameters available in the lens material are not evaluated in significant numbers. Consequently, when selecting an appropriate lens design and parameters, the Eye Care Professional should consider all characteristics of the lens that can affect lens performance and ocular health, including oxygen permeability, wettability, central and peripheral thickness, and optic zone diameter.

- The potential impact of these factors on the patient's ocular health should be carefully weighed against the patient's need for refractive correction; therefore, the continuing ocular health of the patient and lens performance on the eye should be carefully monitored by the prescribing Eye Care Professional.
- Patients who wear these lenses to correct presbyopia using mono-vision may not achieve the best corrected visual acuity for either far or near vision. Visual requirements vary with the individual and should be considered when selecting the most appropriate type of lens for each patient.
- Fluorescein, a yellow dye, should not be used while the lenses are on the eyes. The lenses absorb this dye and become discolored. Whenever fluorescein is used in eyes, the eyes should be flushed with a sterile saline solution that is recommended for in-eye use.
- Eye Care Professionals should instruct the patient to remove the lenses immediately if the eyes become red or irritated.

Eye Care Professionals should carefully instruct patients about the following care regimen and safety precautions.

Handling Precautions:

- Before leaving the Eye Care Professional's office, the patient should be able to promptly remove the lenses or should have someone else available who can remove the lenses for him or her.
- DO NOT use if the sterile blister package is opened or damaged.
- Always wash and rinse hands before handling lenses. Do not get cosmetics, lotions, soaps, creams, deodorants, or sprays in the eyes or on the lenses. It is best to put on lenses before putting on makeup. Water-based cosmetics are less likely to damage lenses than oil-based products.
- DO NOT touch contact lenses with the fingers or hands if the hands are not free of foreign materials, as microscopic scratches of the lenses may occur, causing distorted vision and/or injury to the eye.
- Carefully follow the handling, insertion, removal, and wearing instructions in the "Patient Instruction Guide" for the prescribed

wearing schedule and those prescribed by the Eye Care Professional.

- Always handle lenses carefully and avoid dropping them.
- Never use tweezers or other tools to remove lenses from the lens container unless specifically indicated for that use. Slide the lens up the side of the bowl until it is free of the container.
- Do not touch the lens with fingernails.

Lens Wearing Precautions:

- If the lens sticks (stops moving) on the eye, follow the recommended directions in "Care for a Sticking (Non-Moving) Lens." The lens should move freely on the eye for the continued health of the eye. If non-movement of the lens continues, the patient should be instructed to immediately consult his or her Eye Care Professional.
- Never wear lenses beyond the period recommended by the Eye Care Professional.
- The patient should be advised to never allow anyone else to wear their lenses. They have been prescribed to fit their eyes and to correct their vision to the degree necessary. Sharing lenses greatly increases the chance of eye infections.
- If aerosol products, such as hair spray, are used while wearing lenses, exercise caution and keep eyes closed until the spray has settled.
- Avoid all harmful or irritating vapors and fumes while wearing lenses.
- Always discard lenses worn as prescribed by the Eye Care Professional.

Lens Care Precautions:

- The patient should be informed that no cleaning or disinfection is needed when lenses are worn for daily disposable wear. Patients should always dispose of lenses when removed and have spare lenses or spectacles available.

Other Topics to Discuss with Patients:

- Always contact the Eye Care Professional before using any medicine in the eyes.
- Certain medications, such as antihistamines, decongestants, diuretics, muscle relaxants, tranquilizers, and those for motion sickness may cause dryness of the eye, increased lens awareness, or blurred vision. Should such conditions exist, proper remedial measures should be prescribed. Depending on the severity, this could include the use of lubricating drops that are indicated for use with soft contact lenses or the temporary discontinuance of contact lens wear while such medication is being used.
- Oral contraceptive users could develop visual changes or changes in lens tolerance when using contact lenses. Patients should be cautioned accordingly.
- As with any contact lens, follow-up visits are necessary to assure the continuing health of the patient's eyes. The patient should be instructed as to a recommended follow-up schedule.

Who Should Know That the Patient is Wearing Contact Lenses?

- Patients should inform all doctors (Health Care Professionals) about being a contact lens wearer.
- Patients should always inform their employer of being a contact lens wearer. Some jobs may require use of eye protection equipment or may require that the patient not wear contact lenses.

ADVERSE REACTIONS

The patient should be informed that the following problems may occur when wearing contact lenses:

- The eye may burn, sting, and/or itch.
- There may be less comfort than when the lens was first placed on the eye.
- There may be a feeling of something in the eye (foreign body, scratched area).
- There may be the potential for some temporary impairment due to CR-6437, v 1 0

peripheral infiltrates, peripheral corneal ulcers, or corneal erosion. There may be the potential for other physiological observations, such as local or generalized edema, corneal neovascularization, corneal staining, injection, tarsal abnormalities, iritis, and conjunctivitis; some of which are clinically acceptable in low amounts.

- There may be excessive watering, unusual eye secretions, or redness of the eye.
- Poor visual acuity, blurred vision, rainbows, or halos around objects, photophobia, or dry eyes may also occur if the lenses are worn continuously or for too long a time.

The patient should be instructed to conduct a simple 3-part self-examination at least once a day. They should ask themselves:

- How do the lenses feel on my eyes?
- How do my eyes look?
- Have I noticed a change in my vision?

If the patient reports any problems, he or she should be instructed to **IMMEDIATELY REMOVE THE LENS**. If the problem or discomfort stops, the patient should discard the lens and place a new fresh lens on the eye.

If after inserting the new lens, the problem continues, the patient should be directed to **IMMEDIATELY REMOVE THE LENS AND CONTACT HIS OR HER EYE CARE PROFESSIONAL**.

The patient should be instructed **NOT** to use a new lens as self-treatment for the problem.

The patient should be advised that when any of the above symptoms occur, a serious condition such as infection, corneal ulcer, neovascularization, or iritis may be present. He or she should be instructed to seek immediate professional identification of the problem and prompt treatment to avoid serious eye damage.

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

GENERAL FITTING GUIDELINES

A. Patient Selection

Patients selected to wear these lenses should be chosen based on:

- Motivation to wear lenses
- Ability to follow instructions regarding lens wear care
- General health
- Ability to adequately handle and care for the lenses
- Ability to understand the risk and benefits of lens wear

Patients who do not meet the above criteria should not be provided with contact lenses.

B. Pre-fitting Examination

Initial evaluation of the patient should begin with a thorough case history to determine if there are any contraindications to contact lens wear. During the case history, the patient's visual needs and expectations should be determined as well as an assessment of their overall ocular, physical, and mental health.

Preceding the initial selection of trial contact lenses, a comprehensive ocular evaluation should be performed that includes, but is not limited to, the measurement of distance and near visual acuity, distance and near refractive prescription (including determining the preferred reading distance for presbyopes), keratometry, and biomicroscopic evaluation.

Based on this evaluation, if it is determined that the patient is eligible to wear these lenses, the Eye Care Professional should proceed to the lens fitting instructions as outlined below.

C. Initial Power Determination

A spectacle refraction should be performed to establish the patient's baseline refractive status and to guide in the selection of the appropriate lens power. Remember to compensate for vertex distance if the refraction is greater than $\pm 4.00\text{D}$.

D. Base Curve Selection (Trial Lens Fitting)

The following trial lenses should be selected for patients regardless of keratometry readings. However, corneal curvature measurements should be performed to establish the patient's baseline ocular status.

IN-CONFIDENTIAL

Page 110 of 191

- ACUVUE OASYS® 1-Day: 8.5 mm/14.3 mm
- ACUVUE OASYS® 1-Day for ASTIGMATISM: 8.5 mm/14.3 mm

The trial lens should be placed on each of the patient's eyes and evaluated after the patient has adjusted to the lenses.

1. Criteria of a Properly Fit Lens

A properly fit lens will center and completely cover the cornea (i.e., no limbal exposure), have sufficient movement to provide tear exchange under the contact lens with the blink, and be comfortable. The lens should move freely when manipulated digitally with the lower lid, and then return to its properly centered position when released.

2. Criteria of a Flat Fitting Lens

A flat fitting lens may exhibit one or more of the following characteristics: decentration, incomplete corneal coverage (i.e., limbal exposure), excessive movement with the blink, and/or edge standoff. If the lens is judged to be flat fitting, it should not be dispensed to the patient.

3. Criteria of a Steep Fitting Lens

A steep fitting lens may exhibit one or more of the following characteristics: insufficient movement with the blink, conjunctival indentation, and resistance when pushing the lens up digitally with the lower lid.

If the lens is judged to be steep fitting, it should not be dispensed to the patient.

If the initial trial base curve is judged to be flat or steep fitting, the alternate base curve, if available, should be trial fit and evaluated after the patient has adjusted to the lens. The lens should move freely when manipulated digitally with the lower lid, and then return to a properly centered position when released. If resistance is encountered when pushing the lens up, the lens is fitting tightly and should not be dispensed to the patient.

E. Final Lens Power (Spherical)

A spherical over-refraction should be performed to determine the final lens power after the lens fit is judged acceptable. The spherical over-refraction should be combined with the trial lens power to determine the final lens prescription. The patient should experience good visual acuity with the correct lens power unless there [REDACTED] ye residual astigmatism.

Example 1	
Diagnostic lens:	-2.00D
Spherical over-refraction:	-0.25D
Final lens power:	-2.25D

Example 2	
Diagnostic lens:	-2.00D
Spherical over-refraction:	+0.25D
Final lens power:	-1.75D

If vision is acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If the fit is acceptable, dispense the lenses and instruct the patient to return in one week for reassessment (see dispensing and follow up information in **PATIENT MANAGEMENT**).

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

TORIC FITTING GUIDELINES

Although most aspects of the fitting procedure are identical for all types of soft contact lenses, including toric lenses, there are some additional steps and/or rules to follow to assure the proper fit of toric lenses.

The only new steps you must follow in prescribing ACUVUE OASYS® 1-Day for ASTIGMATISM are that you must determine the stability, repeatability, and drift angle of the lens axis so that you can prescribe the correct lens axis for the patient.

A. How to Determine Lens Cylinder and Axis Orientation

1. Locate the Orientation Marks

To help determine the proper orientation of the toric lens, you'll find two primary marks approximately 1 mm from the lens edge representing the vertical position on opposite ends of the lens at 6 and 12 o'clock (Fig. 1). Because of the lens' ballasting system, either mark can represent the vertical position – there is no "top" and "bottom" as in a prism-ballasted lens. You don't need to view both marks to assess orientation; simply look for the 6 o'clock mark as you would with a prism-ballasted lens.



Figure 1

You'll need a slit lamp biomicroscope with a 1 to 2 mm parallelepiped beam to highlight the marks when the lens is fitted to the eye. There are a number of techniques you can use to improve the visibility of the 6 o'clock mark. Using a parallelepiped beam and medium magnification (10x or 15x), slowly pan down the lens, looking just below the direct illumination at the retroilluminated area. Backlighting the mark this way should make it more visible. Sometimes manipulating the lower lid may be necessary to uncover the mark.

2. Observe Lens Rotation and Stability

Observe the position and stability of the "bottom" mark. It usually stabilizes at the 6 o'clock position. If it does, calculation of the lens power will be straightforward. The 6 o'clock position is not a "must"; however, the absolute requirement is that the axis position be stable and repeatable.

The mark may stabilize somewhat left or right (drift) of the vertical meridian and still enable you to fit a toric lens for that eye, as long as the lens always returns to the same "drift axis" position after settling. The deviation can be compensated for in the final prescription. Your objective is to ensure that whatever position the initial lens assumes near 6 o'clock, this position must be stable and repeatable. With full eye movement or heavy blink, you may see the marks swing away, but they must return quickly to the original stable position. If the lens does not return quickly, you may need to select a different lens.

3. Assessing Rotation

Imagine the eye as a clock dial and every hour represents a 30° interval. If the orientation mark of the initial lens stabilizes somewhat left or right of the vertical position, the final lens will orient on the eye with the same deviation. You can use an axis reticule in the slit lamp or use a line-scribed lens in a spectacle trial frame to measure or estimate the "drift angle" of the cylinder axis.

To compensate for this "drift", measure or estimate the "drift", then add or subtract it from the refractive axis to determine the correct cylinder axis. Use the LARS (Left Add, Right Subtract) method to determine which direction to compensate.

B. Final Lens Power

When the diagnostic lens has its axis aligned in the same meridian as the patient's refractive axis, a spherocylindrical over-refraction may be performed and visual acuity determined. However, in the case of crossed axes, such as when the diagnostic lens axis is different from the spectacle cylinder axis, it is not advisable to perform a full spherocylindrical over-refraction because of the difficulty in computing the resultant power. A spherical over-refraction without cylinder refraction may be performed.

If the required cylinder correction falls between two available cylinder powers, it is recommended to prescribe the lower cylinder power lens. See below for instructions on how to determine the final lens power.

1. For the Sphere

If sphere alone or combined sphere and cylinder Rx $> \pm 4.00D$, compensate for vertex distance. If sphere alone or combined sphere and cylinder Rx $\leq \pm 4.00D$, vertex compensation is not necessary.

2. For the Cylinder

Adjust the axis by the drift angle using the LARS method. Choose a cylinder that is $\leq 0.50D$ from the refractive cylinder.

3. Case Examples

Example 1

Manifest (spectacle) refraction:
O.D. -2.50D / -1.25D x 180° 20/20
O.S. -2.00D / -1.00D x 180° 20/20

Choose a diagnostic lens for each eye with axis 180°. Place the lens on each eye and allow a minimum of 3 minutes for it to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, recheck until stable.

Check the orientation of the axis mark. If the bottom axis mark is in the 6 o'clock position on both eyes, choose the appropriate cylinder as listed previously. If the lens has not yet stabilized, recheck until stable.

Here is the Rx Prescribed:
O.D. -2.50D / -1.25D x 180°
O.S. -2.00D / -0.75D x 180°

Example 2

Manifest (spectacle) refraction:

O.D. -3.00D / -1.00D x 90° 20/20

O.S. -4.75D / -2.00D x 90° 20/20

Choose diagnostic lenses of -3.00D / -0.75D x 90° for the right eye and -4.50D / -1.75D x 90° for the left eye, the nearest lenses available to the spherical power, cylinder power, and axis needed. For the left eye, since the manifest refraction called for -4.75D, compensating for vertex distance the sphere is reduced by 0.25D to -4.50D. The cylinder power will be -1.75D. Place the lens on each eye and allow a minimum of 3 minutes for it to equilibrate, based on the patient's initial response to the lens. If the lens has not yet stabilized, recheck until stable.

Right Eye

The orientation mark on the right lens rotates left from the 6 o'clock position by 10° and remains stable in this position.

Compensation for this rotation should be done as follows:

Compensate the 10° axis drift by adding it to the manifest refraction axis.

Here is the Rx Prescribed:

O.D. -3.00D / -0.75D x 100°

Left Eye

The orientation mark on the left lens rotates right from the 6 o'clock position by 10° and remains stable in this position.

Compensate for the 10° axis drift by subtracting it from the manifest refraction axis.

Here is the Rx Prescribed:

O.S. -4.50D / -1.75D x 80°

If vision is acceptable, perform a slit lamp examination to assess adequate fit (centration and movement). If fit is acceptable, dispense the lenses instructing the patient to return in one week for reassessment (see dispensing and follow-up information in PATIENT MANAGEMENT).

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

MONOVISION FITTING GUIDELINES

A. Patient Selection

1. Monovision Needs Assessment

For a good prognosis, the patient should have adequately corrected distance and near visual acuity in each eye. The amblyopic patient or the patient with significant astigmatism (greater than 1.00D) in one eye may not be a good candidate for monovision correction with these lenses.

Occupational and environmental visual demands should be considered. If the patient requires critical vision (visual acuity and stereopsis), it should be determined by trial whether this patient can function adequately with monovision correction. Monovision contact lens wear may not be optimal for activities such as:

- visually demanding situations such as operating potentially dangerous machinery or performing other potentially hazardous activities; and
- driving automobiles (e.g., driving at night). Patients who cannot meet state driver's licensing requirements with monovision correction should be advised to not drive with this correction, OR may require that additional over-correction be prescribed.

2. Patient Education

All patients do not function equally well with monovision correction. Patients may not perform as well for certain tasks with this correction as they have with spectacles (multifocal, bifocal, trifocal, readers, progressives). Each patient should understand that monovision, as well as other presbyopic alternatives, can create a vision compromise that may reduce visual acuity and depth perception for distance and near tasks. Therefore, caution should be exercised when the patient is wearing the correction for the first time until they are familiar with the vision provided in visually challenging environments (e.g., reading a menu in a dim restaurant, driving at night in rainy/foggy conditions, etc.). During the fitting process, it is necessary for the patient to realize the disadvantages as well as the advantages of clear near vision and straight ahead and upward gaze that monovision contact lenses provide.

B. Eye Selection

1. Ocular Preference Determination Methods

Generally, the non-dominant eye is corrected for near vision. The following two methods for eye dominance can be used.

Method 1: Determine which eye is the "sighting eye." Have the patient point to an object at the far end of the room. Cover one eye. If the patient is still pointing directly at the object, the eye being used is the dominant (sighting) eye.

Method 2: Determine which eye will accept the added power with the least reduction in vision. Place a hand-held trial lens equal to the spectacle near ADD in front of one eye and then the other while the distance refractive error correction is in place for both eyes. Determine whether the patient functions best with the near ADD lens over the right or left eye.

2. Other Eye Selection Methods

Other methods include the "Refractive Error Method" and the "Visual Demands Method."

Refractive Error Method

For anisometropic correction, it is generally best to fit the more hyperopic (less myopic) eye for distance and the more myopic (less hyperopic) eye for near.

Visual Demands Method

Consider the patient's occupation during the eye selection process to determine the critical vision requirements. If a patient's gaze for near tasks is usually in one direction, correct the eye on that side for near.

Example: A secretary who places copy to the left side of the desk will function best with the near lens on the left eye.

C. Special Fitting Characteristics

1. Unilateral Vision Correction

There are circumstances where only one contact lens is required. As an example, an emmetropic patient would only require a near lens, whereas a bilateral myope would require corrective lenses on

both eyes.

Examples:

A presbyopic emmetropic patient who requires a +1.75D ADD would have a +1.75D lens on the near eye and the other eye left without correction.

A presbyopic patient requiring a +1.50D ADD who is -2.50D myopic in the right eye and -1.50D myopic in the left eye may have the right eye corrected for distance and the left uncorrected for near.

2. Near ADD Determination

Always prescribe the lens power for the near eye that provides optimal near acuity at the midpoint of the patient's habitual reading distance. However, when more than one power provides optimal reading performance, prescribe the least plus (most minus) of the powers.

3. Trial Lens Fitting

A trial fitting is performed in the office to allow the patient to experience monovision correction. Lenses are fit according to the GENERAL FITTING GUIDELINES for base curve selection described in this Package Insert.

Case history and standard clinical evaluation procedure should be used to determine the prognosis. Determine the distance correction and the near correction. Next determine the near ADD. With trial lenses of the proper power in place, observe the reaction to this mode of correction.

Allow the lenses to settle for about 20 minutes with the correct power lenses in place. Walk across the room and have the patient look at you. Assess the patient's reaction to distance vision under these circumstances. Then have the patient look at familiar near objects such as a watch face or fingernails. Again assess the reaction. As the patient continues to look around the room at both near and distance objects, observe the reactions. Only after these vision tests are completed should the patient be asked to read print. Evaluate the patient's reaction to large print (e.g., typewritten copy) at first and then graduate to newsprint and finally smaller type sizes.

After the patient's performance under the above conditions is completed, tests of visual acuity and reading ability under

conditions of moderately dim illumination should be attempted.

An initial unfavorable response in the office, while indicative of a guarded prognosis, should not immediately rule out a more extensive trial under the usual conditions in which a patient functions.

4. Adaptation

Visually demanding situations should be avoided during the initial wearing period. A patient may at first experience some mild blurred vision, dizziness, headaches, and a feeling of slight imbalance. You should explain the adaptational symptoms to the patient. These symptoms may last for a brief minute or for several weeks. The longer these symptoms persist, the poorer the prognosis for successful adaptation.

To help in the adaptation process, the patient can be advised to first use the lenses in a comfortable familiar environment such as in the home.

Some patients feel that automobile driving performance may not be optimal during the adaptation process. This is particularly true when driving at night. Before driving a motor vehicle, it may be recommended that the patient be a passenger first to make sure that their vision is satisfactory for operating an automobile. During the first several weeks of wear (when adaptation is occurring), it may be advisable for the patient to only drive during optimal driving conditions. After adaptation and success with these activities, the patient should be able to drive under other conditions with caution.

D. Other Suggestions

The success of the monovision technique may be further improved by having the patient follow the suggestions below:

- Have a third contact lens (distance power) to use when critical distance viewing is needed.
- Have a third contact lens (near power) to use when critical near viewing is needed.
- Having supplemental spectacles to wear over the monovision contact lenses for specific visual tasks may improve the success of monovision correction. This is particularly applicable for those patients who cannot meet state driver's licensing requirements with monovision correction.
- Make use of proper illumination when carrying out visual tasks.

Monovision fitting success can be improved by the following suggestions:

- Reverse the distance and near eyes if a patient is having trouble adapting.
- Refine the lens powers if there is trouble with adaptation. Accurate lens power is critical for presbyopic patients.
- Emphasize the benefits of clear near vision and straight ahead and upward gaze with monovision.

The decision to fit a patient with monovision correction is most appropriately left to the Eye Care Professional in conjunction with the patient after carefully considering the patient's needs.

All patients should be supplied with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.

PATIENT MANAGEMENT

Dispensing Visit

Each sterile lens is supplied in a foil-sealed plastic package containing buffered saline solution with methyl ether cellulose. To remove the lens from the container, peel back the foil seal, place a finger on the lens, and slide the lens up the side of the bowl of the lens package until it is free of the container.

- Evaluate the physical fit and visual acuity of the lens on each eye.
- Teach the patient how to apply and remove his or her lenses.
- Explain daily disposable lens wear and schedule a follow-up examination.
- **Provide the patient with a copy of the PATIENT INSTRUCTION GUIDE for these lenses. Copies are available for download at www.acuvue.com.**

REVIEW THESE INSTRUCTIONS WITH THE PATIENT SO THAT HE OR SHE CLEARLY UNDERSTANDS THE PRESCRIBED WEARING AND REPLACEMENT SCHEDULES.

Follow-Up Examinations

Follow-up care (necessary to ensure continued successful contact lens wear) should include routine periodic progress examinations, management of specific problems, if any, and a review with the patient of the wear schedule, daily disposable modality and proper lens handling procedures.

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.
Recommended Follow-up Examination Schedule (complications
and specific problems should be managed on an individual patient
basis):

1. One week from the initial lens dispensing to patient
2. One month post-dispensing
3. Every three to six months thereafter

NOTE: Preferably, at the follow-up visits, lenses should be worn for at least six hours.

Recommended Procedures for Follow-up Visits:

1. Solicit and record patient's symptoms, if any.
2. Measure visual acuity monocularly and binocularly at distance and near with the contact lenses.
3. Perform an over-refraction at distance and near to check for residual refractive error.
4. With the biomicroscope, judge the lens fitting characteristics (as described in the **GENERAL FITTING GUIDELINES**) and evaluate the lens surface for deposits and damage.
5. Following lens removal, examine the cornea and conjunctiva with the biomicroscope and fluorescein (unless contraindicated).
 - The presence of vertical corneal striae in the posterior central cornea and/or corneal neovascularization is indicative of excessive corneal edema.
 - The presence of corneal staining and/or limbal-conjunctival hyperemia can be indicative of an unclean lens, a reaction to solution preservatives, excessive lens wear and/or a poorly fitting lens.
 - Papillary conjunctival changes may be indicative of an unclean and/or damaged lens.
6. Periodically perform keratometry and spectacle refractions. The values should be recorded and compared to the baseline measurements.

If any observations are abnormal, use professional judgment to alleviate the problem and restore the eye to optimal conditions. If

IN-CONFIDENTIAL

Page 121 of 191

the criteria for successful fit are not satisfied during any follow-up examinations, repeat the patient's trial fitting procedure and refit the patient.

WEARING SCHEDULE

The wearing schedule should be determined by the Eye Care Professional. Regular checkups, as determined by the Eye Care Professional, are also extremely important.

Patients tend to overwear the lenses initially. The Eye Care Professional should emphasize the importance of adhering to the initial maximum wearing schedule. Maximum wearing time should be determined by the Eye Care Professional based upon the patient's physiological eye condition, because individual response to contact lenses varies.

The maximum suggested wearing time for these lenses is:

Day	Hours
1	6-8
2	8-10
3	10-12
4	12-14
5 and after	all waking hours

REPLACEMENT SCHEDULE

These lenses are indicated for daily disposable wear and should be discarded upon removal.

LENS CARE DIRECTIONS

When lenses are prescribed for daily disposable wear, the Eye Care Professional should provide the patient with appropriate and adequate warnings and instructions for daily disposable lens wear at the time they are dispensed.

The Eye Care Professional should review with patients that no cleaning or disinfection is needed with daily disposable lenses. Patients should always dispose of lenses when they are removed and have spare lenses or spectacles available.

Basic Instructions

- Always wash, rinse, and dry hands before handling contact lenses.
- Do not use saliva or anything other than the recommended solutions for lubricating or rewetting lenses. Do not put lenses in the mouth.
- Eye Care Professionals may recommend a lubricating/rewetting solution which can be used to wet (lubricate) lenses while they are being worn to make them more comfortable.

Care for a Sticking (Non-Moving) Lens

If the lens sticks (stops moving), the patient should be instructed to apply a few drops of the recommended lubricating or rewetting solution directly to the eye and wait until the lens begins to move freely on the eye before removing it. If non-movement of the lens continues after a few minutes, the patient should immediately consult the Eye Care Professional.

EMERGENCIES

The patient should be informed that if chemicals of any kind (household products, gardening solutions, laboratory chemicals, etc.) are splashed into the eyes, the patient should: FLUSH EYES IMMEDIATELY WITH TAP WATER AND IMMEDIATELY CONTACT THE EYE CARE PROFESSIONAL OR VISIT A HOSPITAL EMERGENCY ROOM WITHOUT DELAY.

HOW SUPPLIED

Each UV-blocking sterile lens is supplied in a foil-sealed plastic package containing buffered saline solution with methyl ether cellulose. The plastic package is marked with the following:

- ACUVUE OASYS® 1-Day: base curve, power, diameter, lot number, and expiration date
- ACUVUE OASYS® 1-Day for ASTIGMATISM: base curve, power, diameter, cylinder, axis, lot number, and expiration date

REPORTING OF ADVERSE REACTIONS

All serious adverse experiences and adverse reactions observed in patients wearing these lenses or experienced with these lenses should be reported to:

Johnson & Johnson Vision Care, Inc.
7500 Centurion Parkway
Jacksonville, FL 32256
USA
Tel: 1-800-843-2020
www.acuvue.com

Johnson & Johnson Vision Care, Inc.
7500 Centurion Parkway
Jacksonville, FL 32256
USA
Tel: 1-800-843-2020
www.acuvue.com



20401080

©Johnson & Johnson Vision Care Companies 2016
In Canada: Johnson & Johnson Vision Care, division of Johnson & Johnson, Inc.
In USA: Johnson & Johnson Vision Care, Inc.
Printed in USA.
Revision date: 09/16
Revision number: AO-03-16-13

ACUVUE OASYS® and HydraLuxe™ are Trademarks of
the Johnson & Johnson Vision Care Companies

CR-6437, v 1 0

[REDACTED]

Page 125 of 191

JJVC CONFIDENTIAL

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

APPENDIX D: [REDACTED]

Limbal and Conjunctival (Bulbar) Redness
Expanded Sodium Fluorescein Corneal Staining
Lens Fitting Characteristics
Subject Reported Ocular Symptoms/Problems
Front and Back Surface Lens Deposit Grading Procedure
Determination of Distance Spherocylindrical Refractions
Biomicroscopy Scale
Distance and Near Visual Acuity Evaluation
Patient Reported Outcomes
White Light Lens Surface Wettability

Clinical Study Protocol

Johnson & Johnson Vision Care, Inc.

LIMBAL AND CONJUNCTIVAL (BULBAR) REDNESS

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title:

Limbal & Conjunctival (Bulbar) Redness

Document Type:

Document Number:

Revision Number: 5

[REDACTED]

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Limbal & Conjunctival (Bulbar) Redness

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]


Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Limbal & Conjunctival (Bulbar) Redness

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5




Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Limbal & Conjunctival (Bulbar) Redness

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5



Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Limbal & Conjunctival (Bulbar) Redness

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5




Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Limbal & Conjunctival (Bulbar) Redness

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5



**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

██████████ EXPANDED SODIUM FLUORESCEIN CORNEAL STAINING

Title: Expanded Sodium Fluorescein Corneal Staining

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5



[REDACTED]

Title: **Expanded Sodium Fluorescein Corneal Staining**

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: **5**





Title: Expanded Sodium Fluorescein Corneal Staining

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5




Title: Expanded Sodium Fluorescein Corneal Staining

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5



Title: Expanded Sodium Fluorescein Corneal Staining

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5


[REDACTED]

Title: Expanded Sodium Fluorescein Corneal Staining

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5



**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

LENS FITTING CHARACTERISTICS

Title: **Lens Fitting Characteristics**

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5

[REDACTED]

Title: **Lens Fitting Characteristics**

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

Title: **Lens Fitting Characteristics**

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

Title: Lens Fitting Characteristics

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5

Title: Lens Fitting Characteristics

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5



**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

SUBJECT REPORTED OCULAR SYMPTOMS/PROBLEMS

Title: **Subject Reported Ocular Symptoms/Problems**

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 3

[REDACTED]

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

FRONT AND BACK SURFACE LENS DEPOSIT GRADING PROCEDURE

Title: Front and Back Surface Lens Deposit Grading Procedure

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 4

[REDACTED]

Title: Front and Back Surface Lens Deposit Grading Procedure

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 4

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

Title: Front and Back Surface Lens Deposit Grading Procedure

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 4



Title: **Front and Back Surface Lens Deposit Grading Procedure**

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 4



**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

**[REDACTED] DETERMINATION OF DISTANCE SPHEROCYLINDRICAL
REFRACTIONS**

Title: **Determination of Distance Spherocylindrical Refractive Error**

Document Type: [REDACTED]

Document Number: [REDACTED] Revision Number: 5


[REDACTED]

Title: Determination of Distance Spherocylindrical Refractive Error

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 5




Title:

Determination of Distance Spherocylindrical Refractive Error

Document Type:

Document Number:

Revision Number: 5




Title:

Determination of Distance Spherocylindrical Refractive Error

Document Type:

Document Number:

Revision Number: 5



[REDACTED]

[REDACTED]



Title:

Determination of Distance Spherocylindrical Refractive Error

Document Type:

Document Number:

Revision Number: 5



■ [REDACTED]

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

[REDACTED] BIOMICROSCOPY SCALE

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Biomicroscopy Scale

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 9

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Biomicroscopy Scale

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 9

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]



Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Biomicroscopy Scale

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 9



Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Biomicroscopy Scale

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 9

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.

Title: Biomicroscopy Scale

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 9

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

[REDACTED]

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

DISTANCE AND NEAR VISUAL ACUITY EVALUATION

Title: Distance and Near Snellen Visual Acuity Evaluation

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 4


[REDACTED]

Title: Distance and Near Snellen Visual Acuity Evaluation

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 4



Title: Distance and Near Snellen Visual Acuity Evaluation

Document Type:

Document Number:

Revision Number: 4

1. **What is the primary purpose of the proposed legislation?**

111

■ **Black**

■ [REDACTED]

— 10 —

For more information, visit www.ams.org.

11 of 11

© 2019 Pearson Education, Inc. All Rights Reserved. May not be copied, scanned, or duplicated, in whole or in part. Due to electronic rights, some third party content may be suppressed from the eBook and/or eChapter(s). Editorial review has determined that any suppressed content does not materially affect the overall learning experience. Pearson Education, Inc. reserves the right to remove additional content at any time if subsequent rights restrictions require it.

Title: Distance and Near Snellen Visual Acuity Evaluation

Document Type: [REDACTED]

Document Number: [REDACTED]

Revision Number: 4



**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

PATIENT REPORTED OUTCOMES

Clinical Study Protocol

Title: Patient Reported Outcomes
Document Type:
Document Number: **Revision Number:** 2

Page 10 of 10

11. **What is the primary purpose of the *Journal of Clinical Endocrinology and Metabolism*?**

[REDACTED]

100%

For more information, contact the Office of the Vice President for Research and Economic Development at 515-294-6450 or research@iastate.edu.

100% 

1. **What is the primary purpose of the study?** (Please select one)

[REDACTED]

10.1007/s00339-017-0362-2

For more information, contact the Office of the Vice President for Research and Economic Development at 515-294-6450 or research@iastate.edu.

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

WHITE LIGHT LENS SURFACE WETTABILITY

Clinical Study Protocol


Johnson & Johnson Vision Care, Inc.

A large black rectangular redaction box covers the central portion of the page. On the left side, there are several smaller black redaction boxes of varying sizes, some with horizontal lines extending to the right. On the right side, there are also smaller black redaction boxes and horizontal lines extending to the left. The redaction boxes are solid black and completely obscure the underlying text or images.

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

APPENDIX E: IRIS COLOR

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**



**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

APPENDIX F: STARTING LENS POWER

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

APPENDIX G: GUIDELINES FOR COVID-19 RISK MITIGATION

Title:	Guidelines for COVID-19 Risk Mitigation	
Document Type:		
Document Number:		Revision Number: 5

1.0 PURPOSE

The purpose of this document is to provide guidelines for the re-opening or initiation of clinical study sites participating in Johnson & Johnson Vision Care, Inc. (JJVCI) clinical studies during the COVID-19 pandemic.

2.0 SCOPE

This document provides guidelines for Johnson & Johnson Vision Care (JJVCI) to address the potential risks from COVID-19 to study subjects, investigators, study site staff, and monitors at study sites. The guidance provided in this document is in effect from the date of approval through the date of retirement of this Work Instruction. At a minimum, this Work Instruction will be reviewed and updated on a quarterly basis, as appropriate.

NOTE: Re-opening of sites outside of the US will be evaluated on a country by country basis subject to local health authority guidance.

3.0 DEFINITIONS

American Academy of Optometry (AAO): The American Academy of Optometry is an organization of optometrists based in Orlando, Florida. Its goal is to maintain and enhance excellence in optometric practice, by both promoting research and the dissemination of knowledge. The AAO holds an annual meeting, publishes a monthly scientific journal, gives credentials to optometrists through the fellowship process and publishes position statements.

American Optometric Association (AOA): The American Optometric Association, founded in 1898, is the leading authority on quality care and an advocate for our nation's health, representing more than 44,000 Doctors of Optometry (O.D.), optometric professionals, and optometry students. Doctor of Optometry take a leading role in patient care with respect to eye and vision care, as well as general health and well-being. As primary health care providers, Doctor of Optometry have extensive, ongoing training to examine, diagnose, treat and manage ocular disorders, diseases and injuries and systemic diseases that manifest in the eye. The American Optometric Association is a federation of state, student, and armed forces optometric associations. Through these affiliations, the AOA serves members consisting of optometrists, students of optometry, paraoptometric assistants and technicians. The AOA and its affiliates work to provide the public with quality vision and eye care.

Centers for Disease Control and Prevention (CDC): The Centers for Disease Control and Prevention is a national public health institute in the United States. It is a United States federal agency, under the Department of Health and Human Services, and is headquartered in Atlanta, Georgia.

COVID-19: Current outbreak of respiratory disease caused by a novel coronavirus. The virus has been named "SARS-CoV-2" and the disease it causes has been named "Coronavirus Disease 2019" (COVID-19).

Clinical Study: Voluntary research studies conducted in people and designed to answer specific questions about the safety or effectiveness of drugs, vaccines, other therapies, or new ways of using existing treatments. May also be called clinical trials, studies, research, trials, or protocols.

Clinical Study Site: Location where a clinical study is conducted, such as a doctor's office, university, or laboratory. Clinical studies are conducted by Investigators who are individual(s) responsible for the conduct of the clinical study at a study site. If a study is conducted by a team of individuals, the Investigator is the responsible leader of the team and may be called the Principal Investigator.

Clinical Operations Manager (COM): The Johnson & Johnson Vision Care (JJVCI) individual responsible for the overall management of a clinical trial.

Title:	Guidelines for COVID-19 Risk Mitigation	
Document Type:		
Document Number:		Revision Number: 5

Monitor: An individual designated to oversee the progress of a clinical study and ensure that it is conducted, recorded, and reported in accordance with the protocol, Standard Operating Procedures (SOPs), Good Clinical Practice (GCP), and applicable regulatory requirements.

Medical Safety Officer (MSO): Physician who has primary accountability in their product portfolio for product health and safety, and who serves as an independent medical voice for patient safety.

Safety Management Team (SMT): A cross-functional, collaborative team responsible for review, assessment and evaluation of medical safety data arising from any source throughout the product life cycle.

4.0 GUIDANCE FOR STUDY DOCUMENTS

In alignment with recent health authority guidance, JJVCI is providing recommendations for study-related management in the event of disruption to the conduct of the clinical study. This guidance does not supersede any local or government requirements or the clinical judgement of the investigator to protect the health, safety and well-being of participants and site staff. If, at any time, a participant's safety is considered to be at risk, study intervention will be discontinued, and study follow-up will be conducted as outlined in the protocol.

During the COVID-19 pandemic, the additional risks listed below need to be considered for study participants and study personnel:

4.1 Additional Risks Related to the COVID-19 Pandemic:

- The possible transmission of the Coronavirus infection and consequent complications, beyond the risk of adverse events due to the investigational device and/or procedures.
- The risk may be higher in an optometric clinical study because of the close contact the subject will have with health care professionals during the procedures and assessments (since the investigator must make the measurements close to the subject's face) and, in addition the need for multiple follow-up visits/exams which may expose the subject to other patients and/or healthcare professionals who might be transmitting the virus, even if they do not have symptoms.
- Potential disruptions to the study may be necessary due to current or future pandemic-related emergency restrictions, which may lead to delays in scheduled follow-up visits.
- Subjects experiencing an adverse event related to contact lens wear may receive delayed treatment due to COVID-19 restrictions. In this event, all assessments that can be conducted virtually will be completed by the investigator to determine the best course of treatment for the subject, including an unscheduled visit, up to discontinuation from the study, as appropriate.

If a study subject is found to have contracted COVID-19 during participation in a study, he/she will be discontinued from the study and followed until COVID-19 Adverse Event (AE) resolution.

To help minimize the above potential risks, JJVCI recommend reviewing/complying with local, state, and governmental guidance for COVID-19 risks.

JJVCI will provide the following study specific documents with language pertaining to COVID-19 risks:

4.1.1 Informed Consent:

Will include information concerning the study-associated risks related to the COVID-19 pandemic in bold font and/or boxed on the first page of the Informed Consent document:

Title:	Guidelines for COVID-19 Risk Mitigation
Document Type:	
Document Number:	Revision Number: 5

STUDY ASSOCIATED RISKS RELATED TO COVID-19 (CORONAVIRUS) PANDEMIC

It is important to note that this study will be conducted, at least in part, during the COVID-19 pandemic. As such, additional risks associated with the infection with COVID-19 exist for you. This is particularly important for this study due, in part, to the closeness of the doctor during the study examinations.

The potential effects of the disease are not fully known, at this time, and may include long-term serious health consequences. In severe cases, this may result in hospitalization and/or death. Based on current knowledge from the Centers for Disease Control and Prevention (CDC), those at high-risk for severe illness from COVID-19 include older adults and people with underlying medical conditions.

During this study, all appropriate measures will be taken to minimize risks including the use of personal protective equipment such as masks and gloves, as well as proper sanitization. This is in conformance to guidance from the CDC, local health departments, and the state and county in which the study doctor's office is located. However, these measures may not completely eliminate the risks associated with contracting COVID-19.

If you are found to have contracted COVID-19 or feel ill with flu-like symptoms during participation in the study, you will not be permitted to continue in-office study follow-up visits, but you will receive instructions and your condition will be monitored by the doctor and/or study staff.

4.1.2 COVID-19 Risk Control Checklist (Attachment-B):

Will include COVID-19 risk control methods that are required by a site to conduct JJVCI clinical studies. The risk controls are consistent with CDC, AOA, AAO Guidance. The Principal Investigator will review/sign the study specific checklist prior to the Site Initiation Meeting.

4.1.3 Protocol Compliance Investigator(s) Signature Page:

Will include a statement indicating that the Principal Investigator (PI) agrees to conduct the study in compliance with all local, state, and governmental guidance's for COVID-19 risk mitigation.

I have read the suggested guidance provided by JJVCI pertaining to the COVID-19 risk mitigation, (COVID-19 Work Instruction in the Appendix of this protocol). I agree to conduct this study in compliance with local, state, governmental guidance for COVID-19 risks.

4.1.4 Study Site Initiation Training Slides:

Will include suggestions to help mitigate potential transmission of COVID-19. Suggestions may include maintaining social distancing in the clinical site by staggered scheduling of study patients, wearing proper PPEs, frequent disinfection, and installing shields on the slit lamp and other applicable equipment.

5.0 GUIDANCE FOR REMOTE SUBJECT VISITS

Potential disruptions to the study may be necessary due to current or future pandemic-related emergency restrictions. Possible disruption of the study as a result of COVID-19 control measures may lead to delays in scheduled follow-up visits.

Subjects may be delayed in being seen for study follow up visit(s), for example due to COVID-19 control measures or due to the subject's concerns or fears about COVID-19 risk. When appropriate, the remote assessment will be conducted to the extent possible. Discussions with the subject during remote assessments may include:

Title:

Guidelines for COVID-19 Risk Mitigation

Document Type:

Document Number:

Revision Number: 5

Procedure	Details
Subject Reported Ocular Symptoms	Subjects will respond to a verbal open-ended symptoms questionnaire regarding the test article when applicable and feasible.
Change of Medical History (Adverse Events) and Concomitant Medications / Therapies Review	Record any adverse events or medical history changes from the previous study visit with the subject/parents. Review the subject's concomitant medications/therapies and record any changes from the previous study visit.
Wearing Time and Compliance	Record the average wearing time (including number of hours per day during weekdays and weekends, and number of days per week). Confirm compliance with the prescribed wear schedule. • Record and discuss the lens wear compliance based on the subject's self-report. For example, the subjects will be asked the time of the day the subject typically puts on the study lenses in the morning and takes off in the evening, the number of days per week lenses were worn, and the number of consecutive days the subject didn't wear the study lenses, etc.

The discussion with the subject will be documented in EDC under Tele-Visit and a minor protocol deviation will be noted. If during the telephone consultation, a subject states he/she wishes to discontinue participating in the study, instruct the subject to stop wearing the study lenses and schedule the subject to return to the clinic for a Final Evaluation at the earliest possible time. Subjects should return all unused lenses to the clinic at the last visit.

Changes in study visit schedules, missed visits, or participant discontinuations may lead to missing data, including data related to protocol-specified procedures. Case report forms should capture specific information regarding the basis of missing data, including the relationship to the COVID-19 pandemic.

6.0 STUDY CONDUCT DURING PANDEMIC

It is recognized that the Coronavirus Disease 2019 (COVID-19) pandemic may have an impact on the conduct of this clinical study due to, for example, self-isolation/quarantine by participants and study-site personnel; travel restrictions/limited access to public places, including Optometry Clinics; and changes in clinic procedures required to address the COVID-19 challenge.

Every effort should be made to adhere to protocol-specified assessments for study participants, including follow-up. However, if scheduled visits cannot be conducted in person at the study site it is suggested that assessments be performed to the extent possible remotely/virtually or delayed until such time that on-site visits can be resumed in order to continue participant monitoring in accordance with the protocol where possible. At each contact, participants will be interviewed to collect safety data. Key efficacy endpoint assessments should be performed if required and as feasible.

Modifications to protocol-required assessments may be permitted via COVID-19 Appendix after consultation with the participant, investigator, and the sponsor. Missed assessments/visits will be captured in the clinical trial management system for protocol deviations. Interruptions of test article wear or discontinuations of study interventions and withdrawal from the study should be documented with the prefix "COVID-19-related" in the case report form (CRF).

Title:	Guidelines for COVID-19 Risk Mitigation
Document Type:	
Document Number:	Revision Number: 5

The sponsor will continue to monitor the conduct and progress of the clinical study, and any changes will be communicated to the sites and to the health authorities according to local guidance.

If a participant has tested positive for COVID-19, the investigator should contact the sponsor's responsible medical monitor to discuss initial plans for study intervention and follow-up. The medical monitor will notify the Safety Management Team of any subject(s) that have reported "COVID-19", "Asymptomatic COVID-19", or "Suspected COVID-19" adverse events within 24 hours of the notification.

Modifications made to the study conduct as a result of the COVID-19 pandemic will be summarized in the clinical study report.

COVID-19 screening procedures that may be mandated by local healthcare systems do not need to be reported as an amendment to the protocol even if done during clinical study visits.

6.1 **Monitoring Visits**

When on-site monitoring by the sponsor is not feasible, the sponsor's site monitor will contact the study site to schedule remote visits. In such cases, on-site monitoring visits will resume when feasible, with increased frequency to address the source data verification backlog.

Even with staffing limitations during this COVID-19 pandemic, all routine operations related to clinical trials should be well-documented and archived as part of standard process. When conditions permit, all parties involved in this clinical trial should communicate relevant information in a timely manner so that all relevant parties remain sufficiently informed.

6.1.1 Study Site Initiation:

During the period that this Work Instruction is in effect, Site Initiation Meetings and training of study site staff will be conducted remotely. The JJVCI study team will conduct training via Skype, Zoom, Microsoft Teams or similar software as well as utilize online training materials, as applicable. Study site training will be documented utilizing Site Initiation Report [REDACTED]

On-site visits may be considered when, for example, hands-on training or evaluation of site facilities is required. While on site, the Clinical Research Associate (CRA) will follow all local, state, and governmental policies for COVID-19 Risk Mitigation, including social distancing, wearing of PPE, etc. as applicable for the location of the study site.

6.1.2 Interim Monitoring Visits (if applicable):

During the period that this Work Instruction is in effect, Interim Monitoring On-site visits will be kept to a minimum and include only those tasks that the CRA cannot perform remotely (e.g., source document verification, test article reconciliation, etc.).

To ensure data integrity during the conduct of all JJVC studies, clinical study teams will follow the study specific Clinical Monitoring Plan [REDACTED]

While on site, the CRA will follow all local, state, and governmental policies for COVID-19 Risk Mitigation, including social distancing, wearing of PPE, etc. as applicable for the location of the study site.

Title:	Guidelines for COVID-19 Risk Mitigation	
Document Type:		
Document Number:		Revision Number: 5

6.1.3 Study Site Closure:

During the period that this Work Instruction is in effect, the duration of the Study Site Closure Visit will be limited to tasks that the CRA cannot perform remotely (e.g., source document verification, test article final reconciliation and return, etc.).

Title:	Guidelines for COVID-19 Risk Mitigation
Document Type:	
Document Number:	Revision Number: 5

Attachment A: Study Site Correspondence

XXXX XX, 2020

Re: COVID-19 Mitigation Plan, <<CR-xxxx/protocol title>>

Dear <<Principal Investigator>> and Study Team,

Coronavirus (COVID-19) has impacted several communities and business activities over the past several months. While we work toward the successful conduct of clinical studies, our commitment continues to be the safety of patients, healthcare professionals, and to our communities.

Therefore, we would like to share the following revisions/additions related to the above referenced Johnson & Johnson Vision Care company sponsored clinical trial(s) you are currently working on or considering participation within.

Protocol:

- Guidelines for COVID-19 Risk Mitigation provided in the Appendix section.

Protocol Signature Page:

- Will include a statement indicating the Principal Investigator agrees to conduct the study in compliance with all local, state, and governmental guidelines for COVID-19 risk mitigation.

Informed Consent:

- Will include information concerning the study-associated risks related to the COVID-19 pandemic in bold font and/or boxed on the first page of the Informed consent document.

COVID-19 Risk Control Checklist for Clinical Studies:

- Will include COVID-19 risk control measures that are required to ensure the safety and health of subjects, site staff and monitors during the pandemic.

We want to encourage the need for open lines of communication about potential challenges you may foresee as the result of the current COVID-19 situation. Therefore, we encourage you to regularly connect with your respective Johnson & Johnson clinical study team (Clinical Research Associate (CRA), Lead CRA or Study Managers).

Thank you for your continued engagement, collaboration, and dedication to your study subjects during this challenging time.

Please file this letter in your site file study correspondence.

Title:	Guidelines for COVID-19 Risk Mitigation
Document Type:	
Document Number:	Revision Number: 5

Attachment B: COVID-19 Risk Control Checklist

Study Number

Site Number

Principal Investigator (PI) Name

The following COVID-19 risk control methods are required to conduct Johnson & Johnson Vision Care clinical studies. Please review the following requirements and initial each requirement.

PI Initials	General Site Safety Planning Measures
	Signage within site describing Risk Control methods
	Social Distancing practices throughout site (waiting rooms, lobby, exam rooms, etc.)
	Non-contact thermometer available to assess temperatures of staff and patients
	Training on patient flow and physical distancing in waiting room
	Establish longer time frame between patient appointments to reduce persons in the site
	Staff should receive job-specific training on PPE and demonstrate competency with selection and proper use of PPE and wear at all times during interactions with subjects (e.g., putting on and removing without self-contamination)

PI Initials	Site Staff Daily Safety Measures
	As part of routine practice, site staff should regularly monitor themselves for fever and symptoms of COVID-19, including temperature checks
	Any staff member (including non-study clinic staff and Investigators) showing signs of being sick or testing positive for COVID-19 must not be permitted to work on activity that may expose study related staff and subject and the Sponsor shall be informed NOTE: Inform JJVC in 24 hours of any COVID-19 cases and all potential exposure during the clinical study.
	Ensure that all staff wear a mask Gloves should be required when working directly with patients and changed between each patient
	Have staff thoroughly wash hands for at least 20 seconds or use an alcohol-based hand sanitizer when they arrive, before and after each patient, before eating and after using the bathroom.
	Cleaning and disinfection procedures for exam rooms and instruments or equipment between patients with gloves.
	Cleaning and disinfection procedures for commonly touched surfaces (doors, chairs, computers, phones, etc.) with gloves.

PI Initials	Before a Patient or Study Visit:
	Patients should be asked prior to entering the site about fever and respiratory illness and whether they or a family member have had contact with another person with confirmed COVID-19 in the past 14 days. Patients exhibiting signs of being sick should be rescheduled when their symptoms resolve.
	Instruct patients that companions should remain outside of the facility and not accompany the patient into the facility unless they are a parent/guardian of the patient or if they are a true caregiver and need to assist the patient
	Request the patient to call or text the office upon arrival so entrance to and movement through facility can be coordinated by site staff

Title:	Guidelines for COVID-19 Risk Mitigation
Document Type:	
Document Number:	Revision Number: 5

PI Initials	Patients Entering the site:
	Temperature checks utilizing a non-contact thermometer for all patients and companions entering the site.
	All patients and companions must wear cloth or disposable mask at all times in the site
	Maintain social distancing. Waiting rooms or lobbies should be as empty as possible. Advise seated patients to remain at least 6 feet from one another.
	Communal objects in (e.g. toys, reading materials, etc.) should be removed or cleaned regularly.

I certify that I have read and agree to implement all the listed COVID-19 Risk Control Measures required for the conduct of Johnson & Johnson Vision Care studies.

Principal Investigator Signature and Date

Title:	Guidelines for COVID-19 Risk Mitigation	
Document Type:		
Document Number:		Revision Number: 5

RESOURCE LINKS

US Resource Links

- OSHA Training
<https://www.osha.gov/SLTC/covid-19/controlprevention.html>
- Personal Protective Equipment (PPE) Training
CDC: <https://www.cdc.gov/coronavirus/2019-ncov/hcp/using-ppe.html>
- I&R Training
ACUVUE® LensAssist: <https://www.acuvue.com/lensassist>
- Clinic Preparedness Guides
CDC: <https://www.cdc.gov/coronavirus/2019-ncov/hcp/clinic-preparedness.html>
AOA: <https://aoa.uberflip.com/i/1240437-aoa-guidance-for-re-opening-practices-covid-19/1?m4=>
American Optometric Association: <https://www.aoa.org/optometry-practice-reactivation-preparedness-guide>
- In-Office Disinfection of Multi-Patient Use Diagnostic Contact Lenses
<https://www.gpli.info/wp-content/uploads/2020/03/2020-01-15-in-office-disinfecting-of-diagnostic-lenses.pdf>

OUS Resource Links

- Updates on local regulations in Hong Kong
<https://www.coronavirus.gov.hk/eng/index.html>
- Resumption of optical services in England: Letter from Matt Neligan and Poonam Sharma
<https://www.england.nhs.uk/coronavirus/wp-content/uploads/sites/52/2020/04/C0601-reopening-of-optical-services-letter-17-june-2020.pdf>
- NHS Optical Letter
<https://www.england.nhs.uk/coronavirus/wp-content/uploads/sites/52/2020/04/C0127-optical-letter-1-april-2020.pdf>
- The College of Optometrists primary eye care COVID-19 guidance: Red phase
<https://www.college-optometrists.org/the-college/media-hub/news-listing/coronavirus-covid-19-guidance-for-optometrists.html>
- The College of Optometrists COVID-19: College updates
<https://www.college-optometrists.org/the-college/media-hub/news-listing/coronavirus-2019-advice-for-optometrists.html#CollegeGuidelines>
- Infection Control Guidelines. (n.d.). Retrieved from Canadian Association Of Optometrists: https://opto.ca/sites/default/files/resources/documents/infection_control_guidelines_2016.pdf
- Infection prevention and control for COVID-19: Interim guidance for outpatient and ambulatory care settings. (2020, May 23 May). Retrieved from Government of Canada: <https://www.canada.ca/en/public-health/services/diseases/2019-novel-coronavirus-infection/guidance-documents/interim-guidance-outpatient-ambulatory-care-settings.html>

Title:

Guidelines for COVID-19 Risk Mitigation

Document Type:

Document Number:

Revision Number: 5

- Information for Members On Coronavirus (COVID-19). (n.d.). Retrieved from Canadian Association Of Optometrists:
https://opto.ca/sites/default/files/resources/documents/information_for_members_on_coronavirus.pdf
- Coronavirus (COVID-19) resources for health professionals, including aged care providers, pathology providers and health care managers. (2020, September 24). Retrieved from Australian Government Department of Health:
<https://www.health.gov.au/resources/collections/coronavirus-covid-19-resources-for-health-professionals-including-aged-care-providers-pathology-providers-and-health-care-managers>
- Environmental Cleaning and Disinfection Principles for COVID-19. (n.d.). Retrieved from Australian Government Department of Health:
<https://www.health.gov.au/sites/default/files/documents/2020/03/environmental-cleaning-and-disinfection-principles-for-covid-19.pdf>
- Infection control guidelines and advice. (n.d.). Retrieved from Optometry Australia :
<https://www.optometry.org.au/practice-professional-support/coronavirus-covid-19-what-optometrists-need-to-know/covid-19-clinical-advice/infection-control-guidelines-and-advice/>

**Clinical Study Protocol
Johnson & Johnson Vision Care, Inc.**

PROTOCOL COMPLIANCE INVESTIGATOR(S) SIGNATURE PAGE

Protocol Number and Title: CR-6437 Evaluation of Prototype Lenses with Experimental UV/HEV Blocker

Version and Date: 1.0 18 March 2021

I have read and understand the protocol specified above and agree on its content.

I agree to conduct this study according to ISO 14155,¹ GCP and ICH guidelines,² the Declaration of Helsinki,³ United States (US) Code of Federal Regulations (CFR),⁴ and the pertinent individual country laws/regulations and to comply with its obligations, subject to ethical and safety considerations. The Principal Investigator is responsible for ensuring that all clinical site personnel, including Sub-Investigators adhere to all ICH² regulations and GCP guidelines regarding clinical trials during and after study completion.

I will assure that no deviation from or changes to the protocol will take place without prior agreement from the Sponsor and documented approval from the Institutional Review Board (IRB), except where necessary to eliminate an immediate hazard(s) to the trial participants.

I am responsible for ensuring that all clinical site personnel including Sub-Investigators adhere to all ICH² regulations and GCP guidelines regarding clinical trials during and after study completion.

All clinical site personnel involved in the conduct of this study have completed Human Subjects Protection Training.

I agree to ensure that all clinical site personnel involved in the conduct of this study are informed about their obligations in meeting the above commitments.

I shall not disclose the information contained in this protocol or any results obtained from this study without written authorization.

I have read the suggested guidance provided by JJVCI pertaining to the COVID-19 risk mitigation, (COVID-19 Work Instruction in the Appendix G of this protocol). I agree to conduct this study in compliance with local, state, governmental guidance for COVID-19 risks.

Principal
Investigator:

Signature

Date

Name and Professional Position (Printed)

Institution/Site:

Institution/Site Name

Institution/Site Address